

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081221\
 Data File : PS016388.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2021 19:46
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 02:27:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 02 14:10:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.186	6.765	645.3E6	271.6E6	438.626	520.716
Target Compounds							
5) T	DICAMBA	0.000	6.930	0	2248692	N.D.	1.032
6) T	MCPD	0.000	6.987f	0	2054635	N.D.	1.189
8) T	DICHLORPROP	0.000	7.580	0	2941475	N.D.	5.429
10) T	Pentachlo...	0.000	8.268	0	3228459	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.632	0	13536418	N.D.	4.639
12) T	2,4,5-T	0.000	9.018	0	2825673	N.D.	<MDL
15) T	Picloram	10.956	10.840	10038703	10514005	1.006	2.611 #
16) T	DCPA	11.414	10.766	7419357	3800663	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081221\
Data File : PS016388.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2021 19:46
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 02:27:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
Quant Title : 8080.M
QLast Update : Mon Aug 02 14:10:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

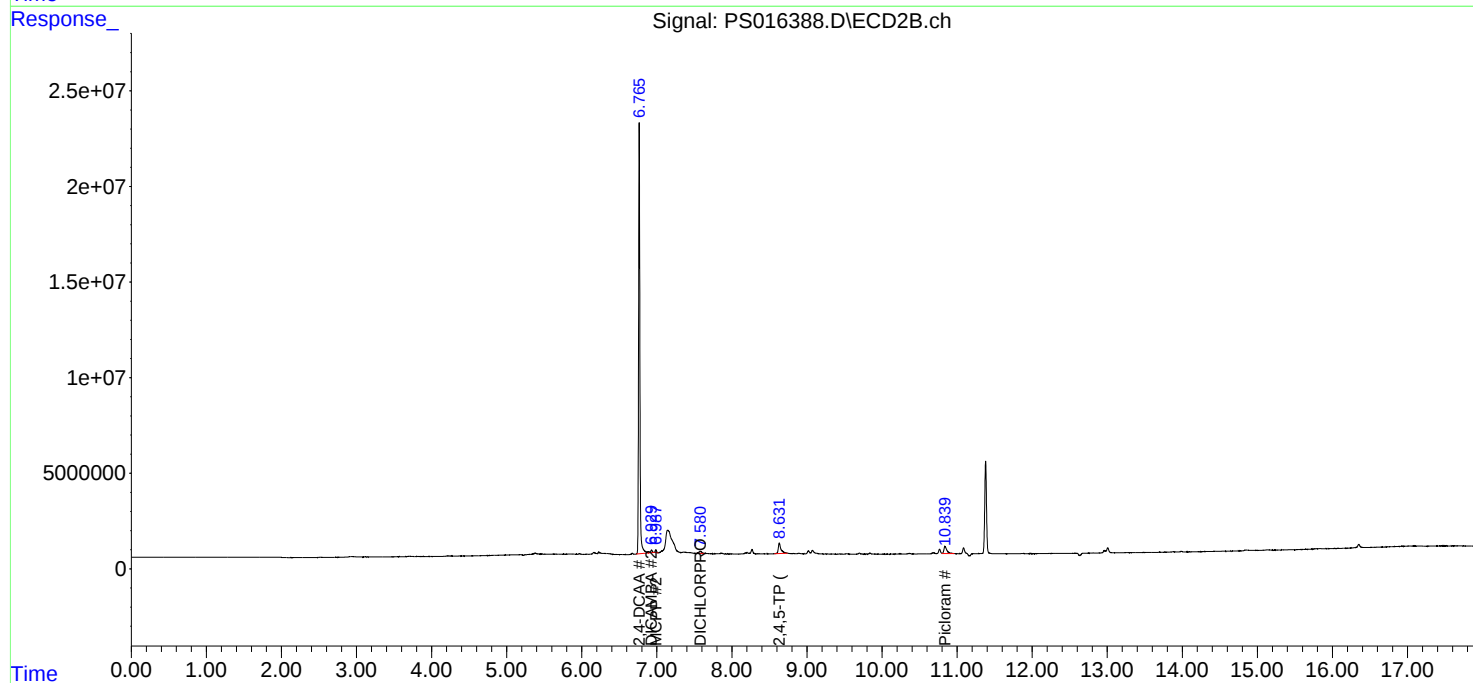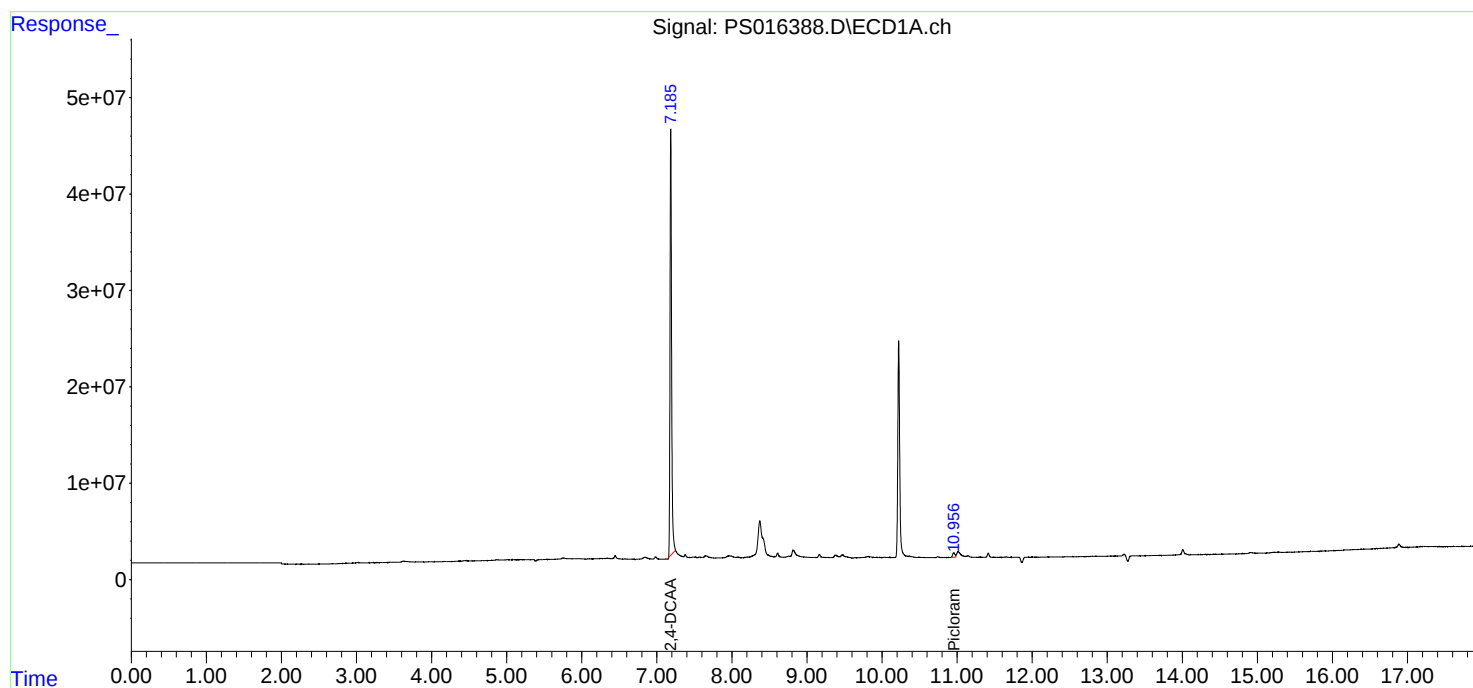


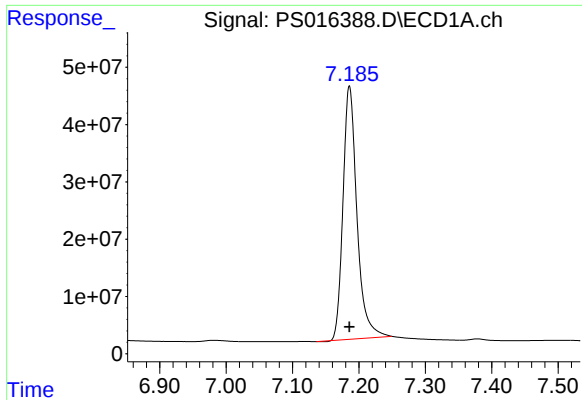

#4 2,4-DCAA


R.T.: 7.186 min
Delta R.T.: 0.000 min
Response: 645265438
Conc: 438.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

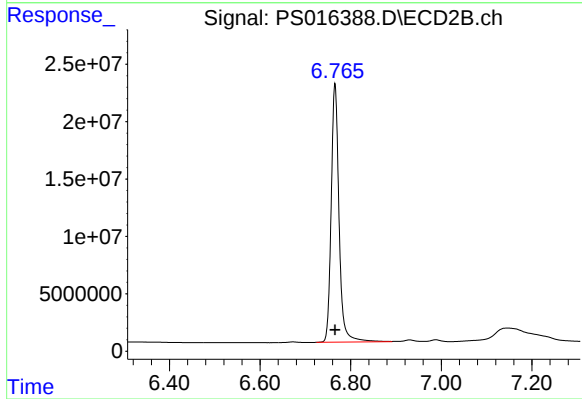


#4 2,4-DCAA

R.T.: 6.765 min
Delta R.T.: 0.000 min
Response: 271618195
Conc: 520.72 ng/ml

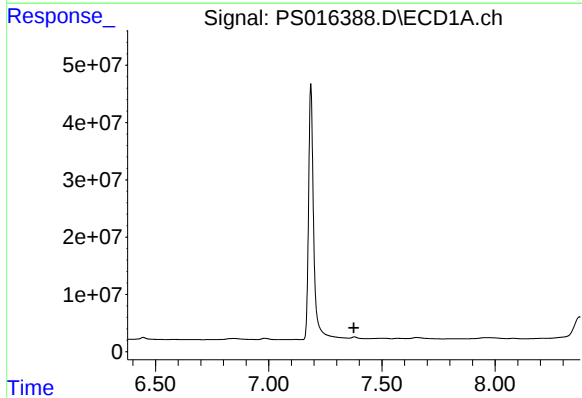


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.377 min
Response: 0
Conc: N.D.

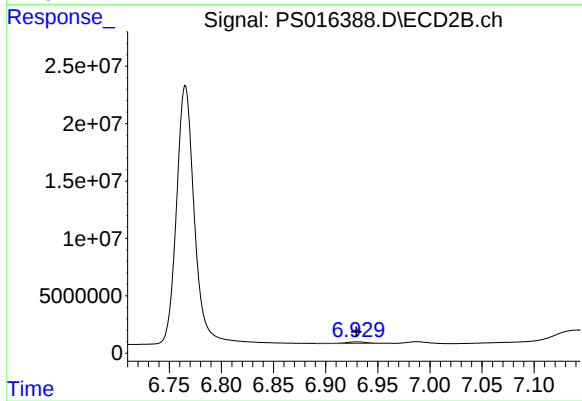

#5 DICAMBA


R.T.: 6.930 min
Delta R.T.: 0.000 min
Response: 2248692
Conc: 1.03 ng/ml

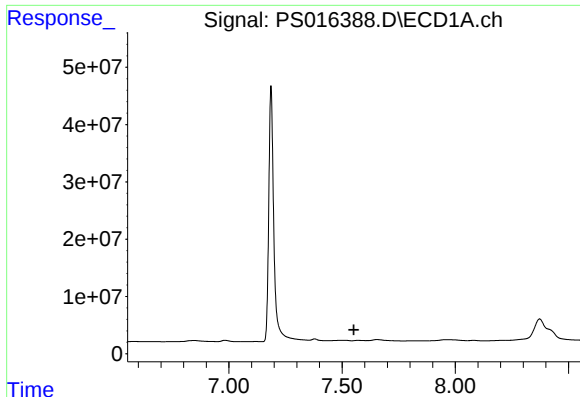

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.552 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

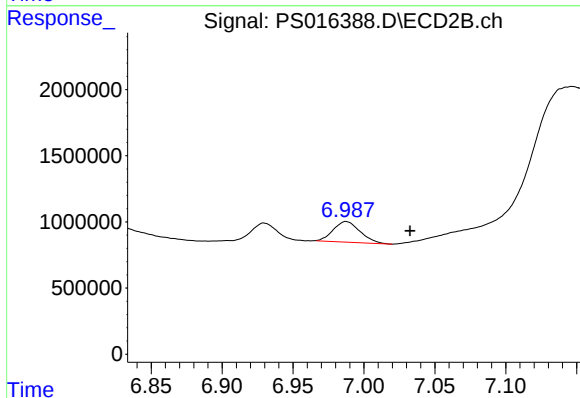


#6 MCP

R.T.: 6.987 min
Delta R.T.: -0.045 min
Response: 2054635
Conc: 1.19 ug/ml

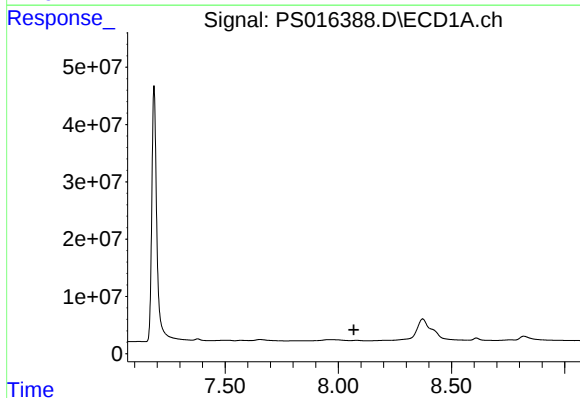


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.069 min
Response: 0
Conc: N.D.

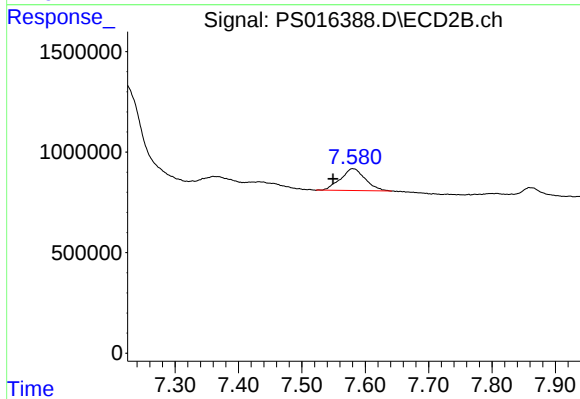

#8 DICHLORPROP


R.T.: 7.580 min
Delta R.T.: 0.031 min
Response: 2941475
Conc: 5.43 ng/ml

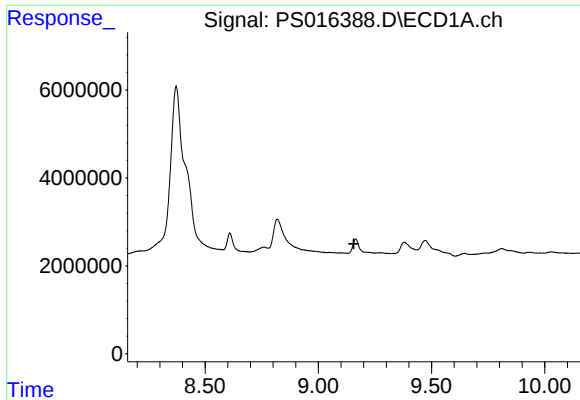

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.157 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

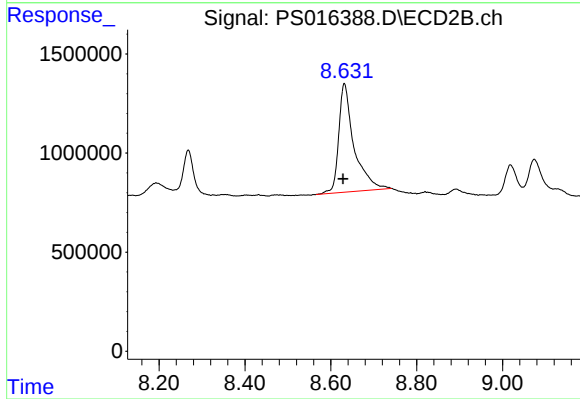


#11 2,4,5-TP (SILVEX)

R.T.: 8.632 min
Delta R.T.: 0.003 min
Response: 13536418
Conc: 4.64 ng/ml

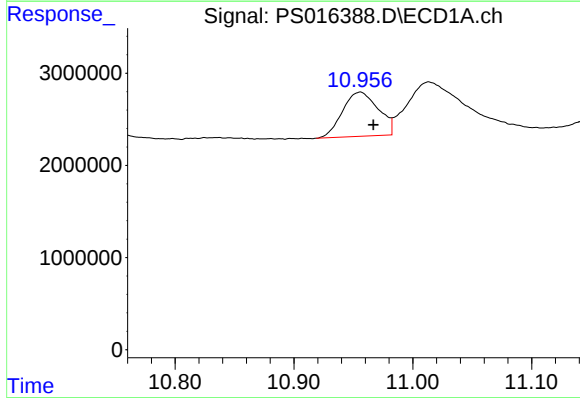

#15 Picloram

R.T.: 10.956 min
Delta R.T.: -0.011 min
Response: 10038703
Conc: 1.01 ng/ml

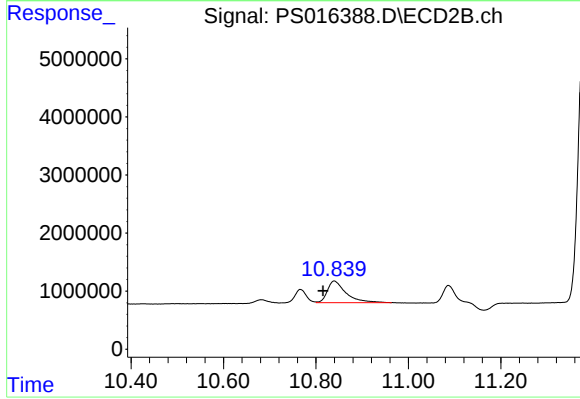

#15 Picloram

R.T.: 10.840 min
Delta R.T.: 0.024 min
Response: 10514005
Conc: 2.61 ng/ml