

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081222\
 Data File : PS020262.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2022 09:45
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 15:16:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
1)	T	Dalapon	2.981	0.000	359531	0	<MDL N.D. #
2)	T	3,5-DICHL...	6.442f	0.000	8689015	0	2.234 N.D. #
3)	T	4-Nitroph...	6.969f	0.000	450780	0	<MDL N.D. #
5)	T	DICAMBA	7.371	6.983f	59901	3161243	<MDL <MDL #
6)	T	MCP	0.000	6.983	0	3161243	N.D. 1.159
7)	T	MCPA	7.677	0.000	705927	0	<MDL N.D. #
9)	T	2,4-D	8.367f	0.000	26633667	0	8.843 N.D. #
10)	T	Pentachlo...	8.633	0.000	224962	0	<MDL N.D. #
11)	T	2,4,5-TP ...	9.092f	0.000	1914041	0	<MDL N.D. #
12)	T	2,4,5-T	9.374f	0.000	34820841	0	1.918 N.D. #
13)	T	2,4-DB	9.967	0.000	1738322	0	<MDL N.D. #
14)	T	DINOSEB	11.170	0.000	758774	0	<MDL N.D. #
15)	T	Picloram	10.942	10.826	24406257	17627229	<MDL 2.336 #
16)	T	DCPA	11.409	0.000	2615655	0	<MDL N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081222\
Data File : PS020262.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2022 09:45
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 15:16:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

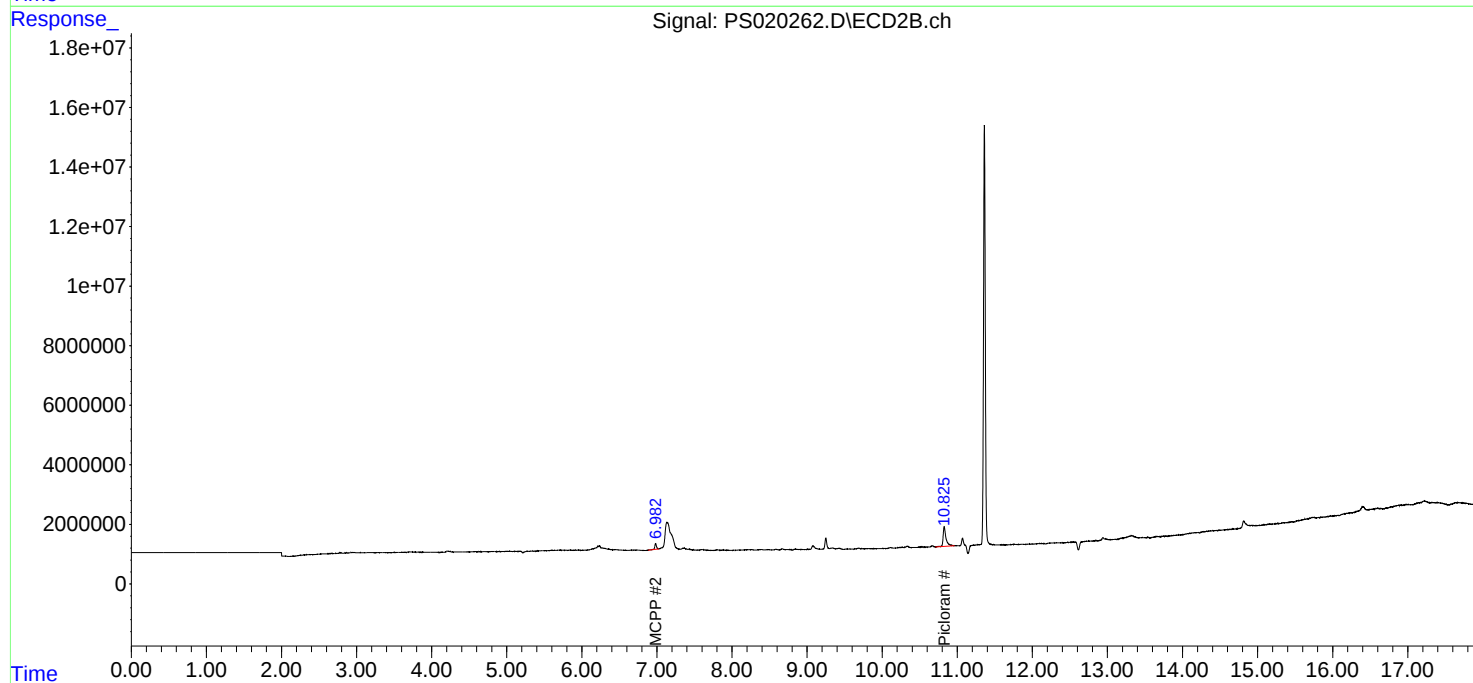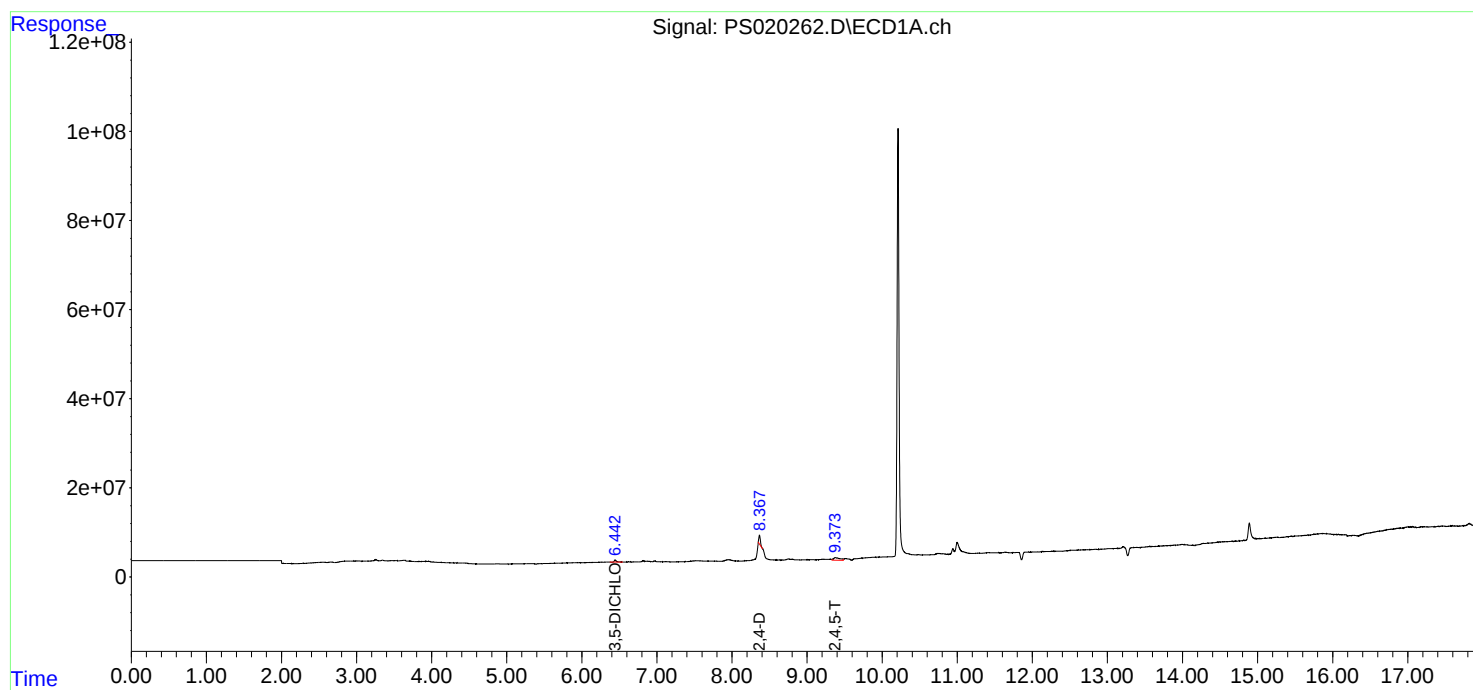


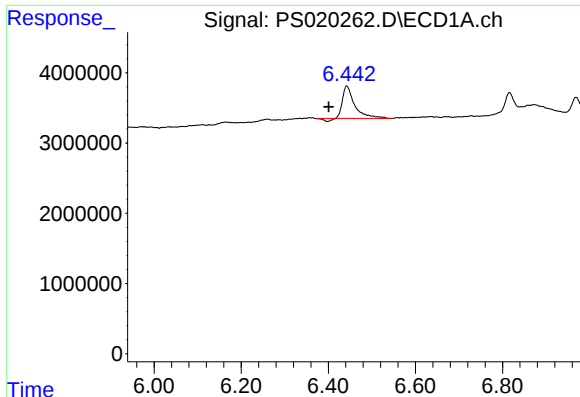

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.442 min
Delta R.T.: 0.041 min
Response: 8689015
Conc: 2.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

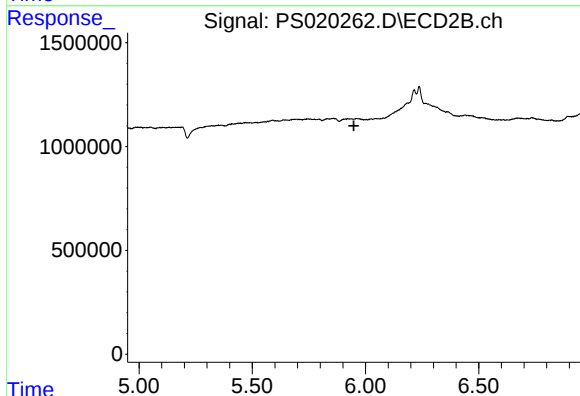


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.949 min
Response: 0
Conc: N.D.

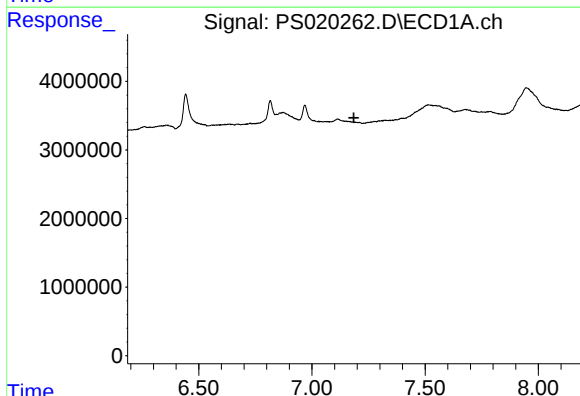


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.186 min
Response: 0
Conc: N.D.

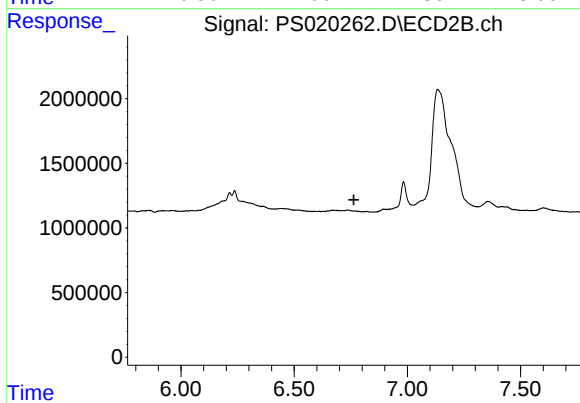

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.763 min
Response: 0
Conc: N.D.

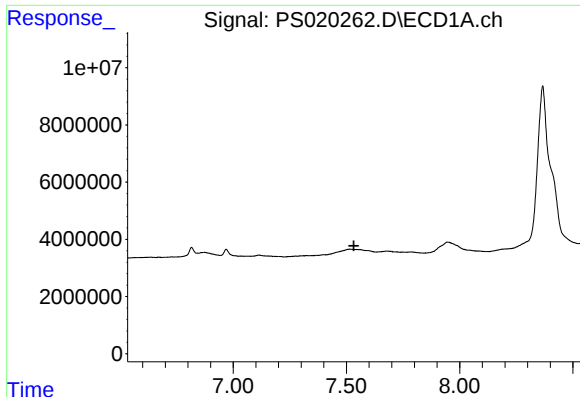

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.533 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

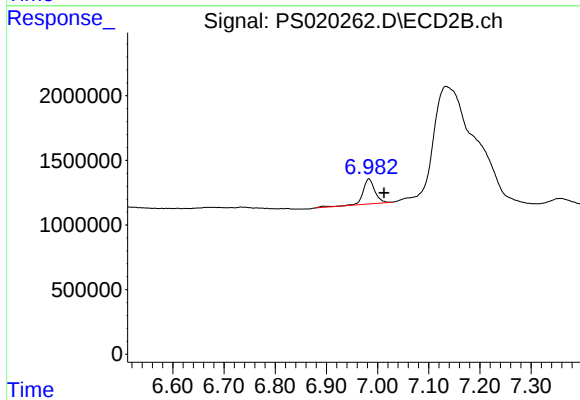


#6 MCP

R.T.: 6.983 min
Delta R.T.: -0.030 min
Response: 3161243
Conc: 1.16 ug/ml

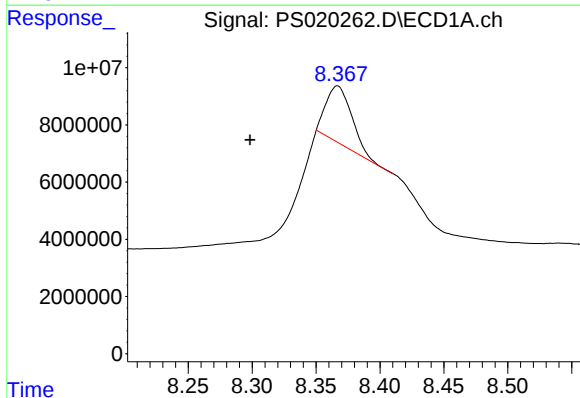


#9 2,4-D

R.T.: 8.367 min
Delta R.T.: 0.068 min
Response: 26633667
Conc: 8.84 ng/ml

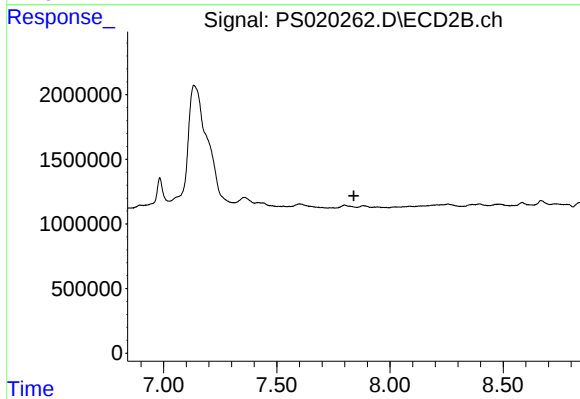

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.840 min
Response: 0
Conc: N.D.

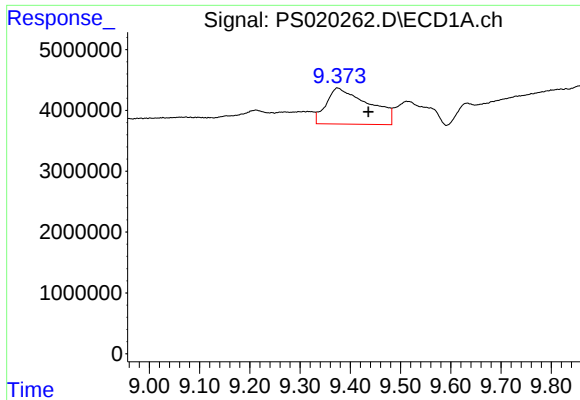

#12 2,4,5-T


R.T.: 9.374 min
Delta R.T.: -0.062 min
Response: 34820841
Conc: 1.92 ng/ml

Instrument :
ECD_S
ClientSampleId :

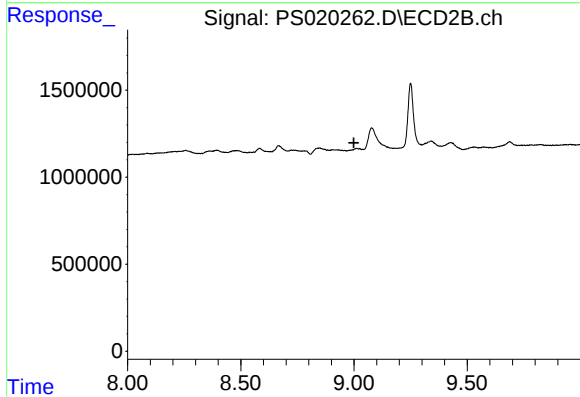


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.999 min
Response: 0
Conc: N.D.

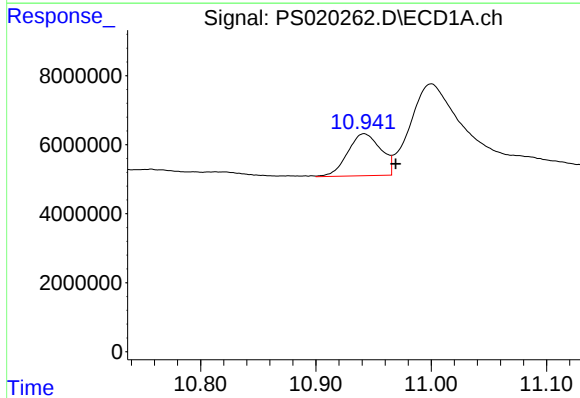

#15 Picloram

R.T.: 10.942 min
Delta R.T.: -0.028 min
Response: 24406257
Conc: N.D.

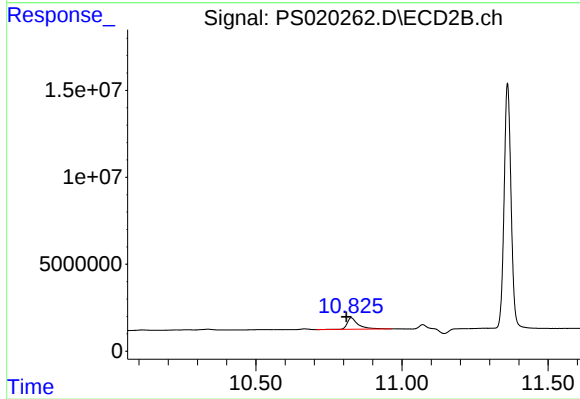

#15 Picloram

R.T.: 10.826 min
Delta R.T.: 0.016 min
Response: 17627229
Conc: 2.34 ng/ml