

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081222\
 Data File : PS020263.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2022 10:09
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 15:16:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.181	6.759	1395.7E6	458.9E6	473.318	563.063
Target Compounds							
1) T	Dalapon	2.986	0.000	99379	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.435	0.000	1997683	0	<MDL	N.D. #
3) T	4-Nitroph...	6.988f	0.000	284790	0	<MDL	N.D. #
5) T	DICAMBA	7.428f	0.000	570696	0	<MDL	N.D. #
6) T	MCP	7.466f	0.000	291669	0	<MDL	N.D. #
7) T	MCPA	7.640f	0.000	3535064	0	<MDL	N.D. #
9) T	2,4-D	8.363f	0.000	10649978	0	3.536	N.D. #
10) T	Pentachlo...	8.543f	0.000	323624	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.160	0.000	1463934	0	<MDL	N.D. #
12) T	2,4,5-T	9.405	0.000	22360369	0	1.232	N.D. #
13) T	2,4-DB	10.006	0.000	1885160	0	<MDL	N.D. #
14) T	DINOSEB	11.182f	0.000	1057657	0	<MDL	N.D. #
15) T	Picloram	10.950	10.836	9523881	11105522	<MDL	1.472 #
16) T	DCPA	11.411	0.000	2144023	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081222\
Data File : PS020263.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2022 10:09
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 15:16:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

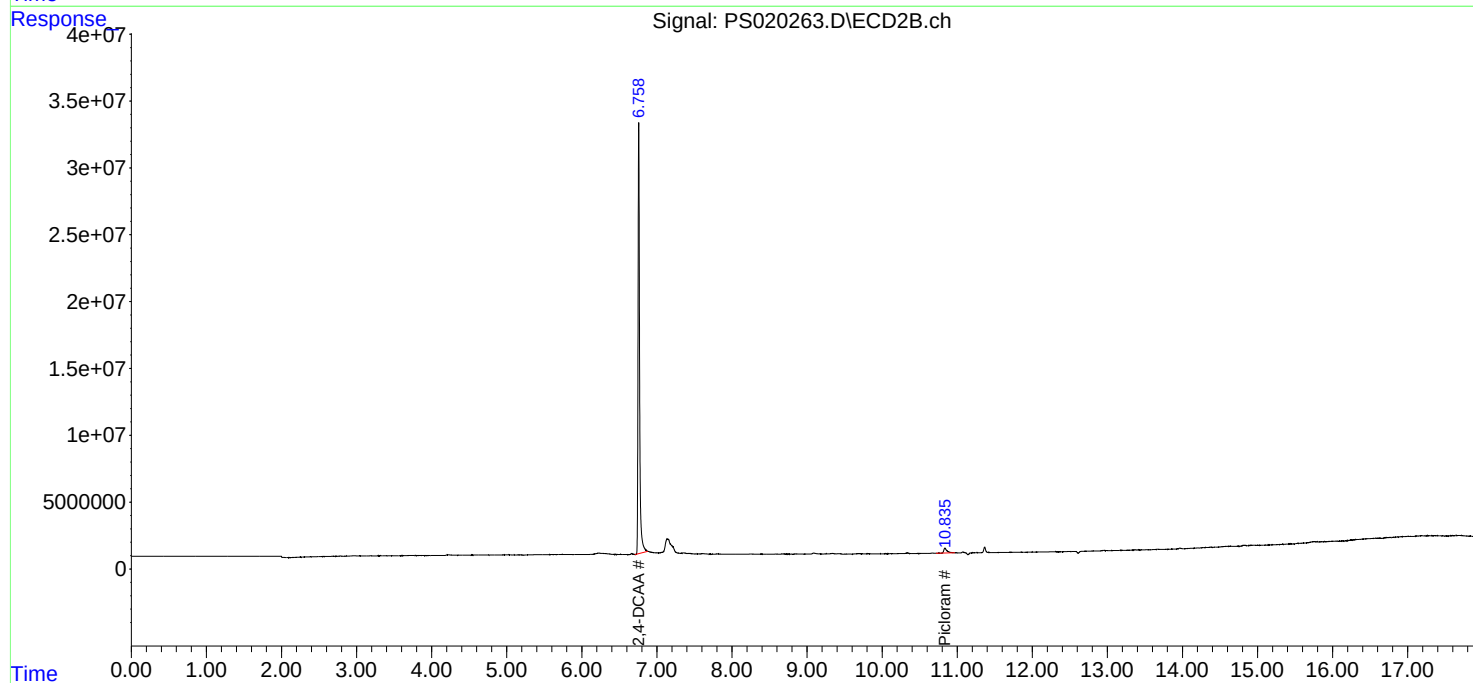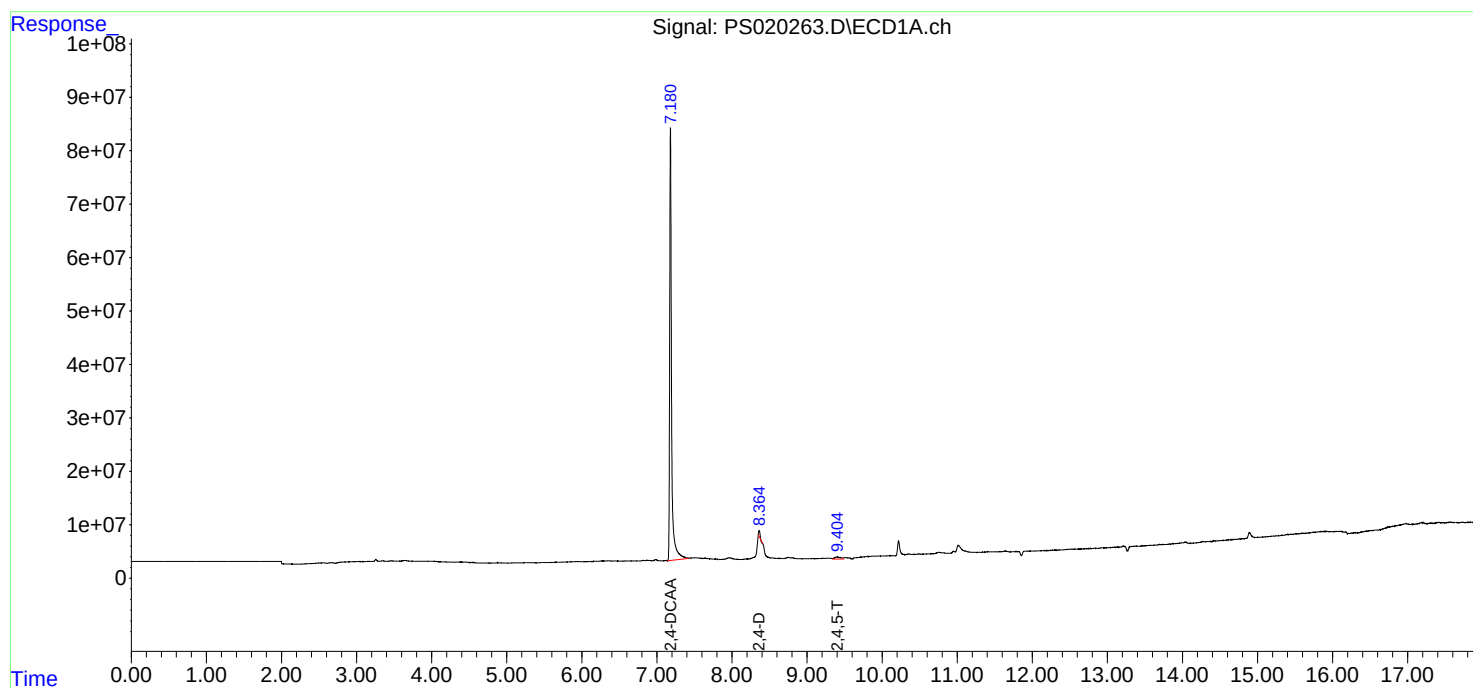


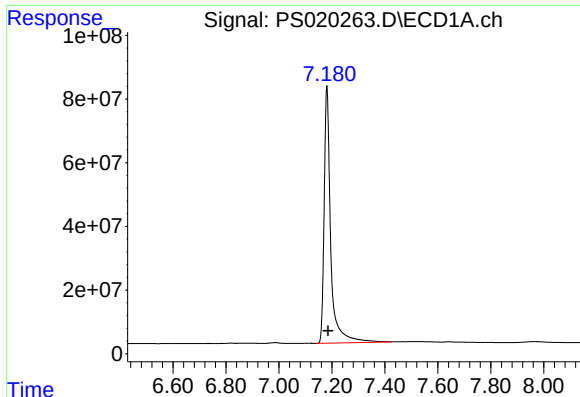

#4 2,4-DCAA


R.T.: 7.181 min
Delta R.T.: -0.005 min
Response: 1395683388
Conc: 473.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

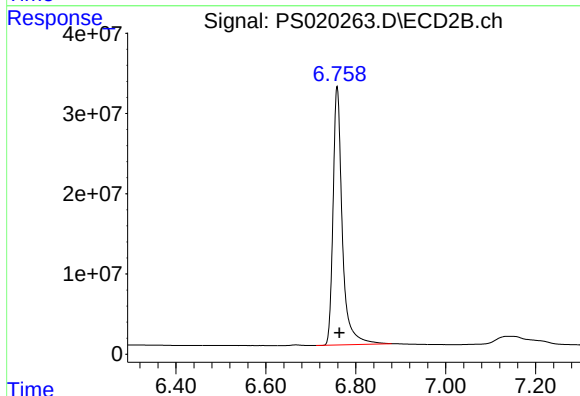


#4 2,4-DCAA

R.T.: 6.759 min
Delta R.T.: -0.005 min
Response: 458871867
Conc: 563.06 ng/ml

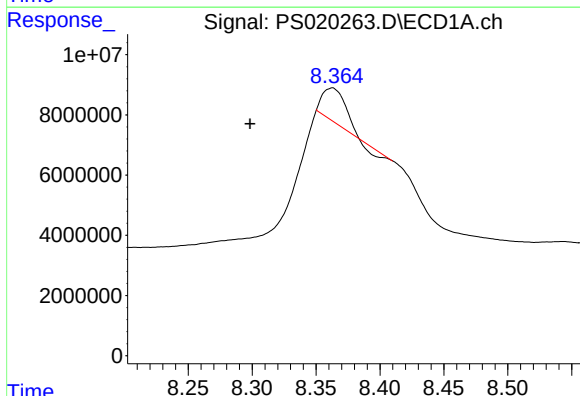


#9 2,4-D

R.T.: 8.363 min
Delta R.T.: 0.064 min
Response: 10649978
Conc: 3.54 ng/ml

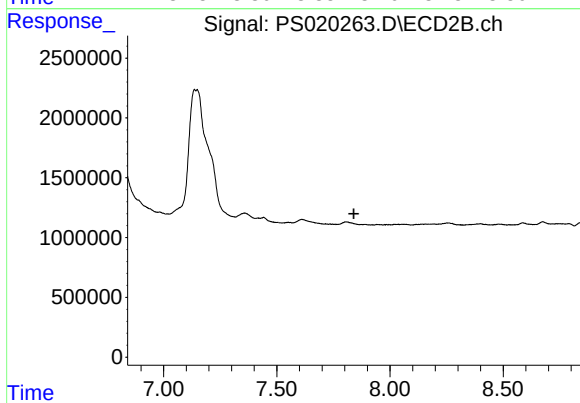

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.840 min
Response: 0
Conc: N.D.

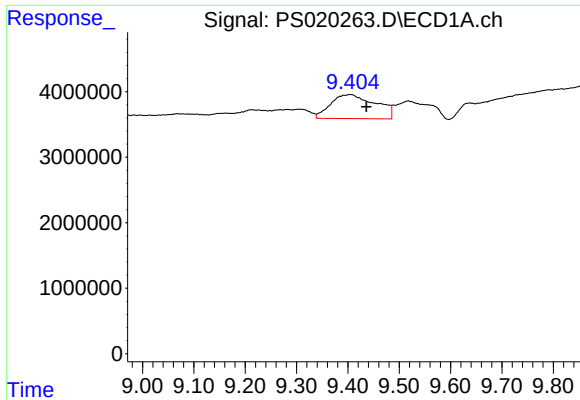

#12 2,4,5-T


R.T.: 9.405 min
Delta R.T.: -0.031 min
Response: 22360369
Conc: 1.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

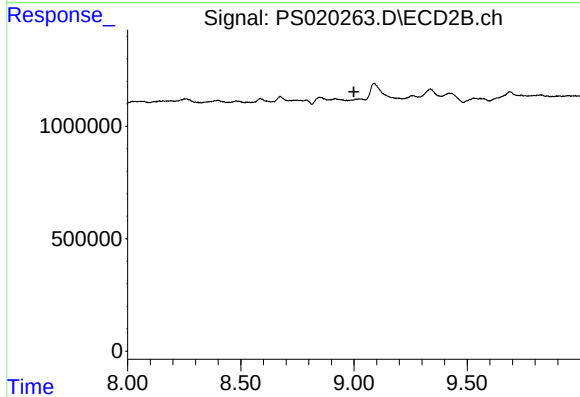


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 8.999 min
Response: 0
Conc: N.D.

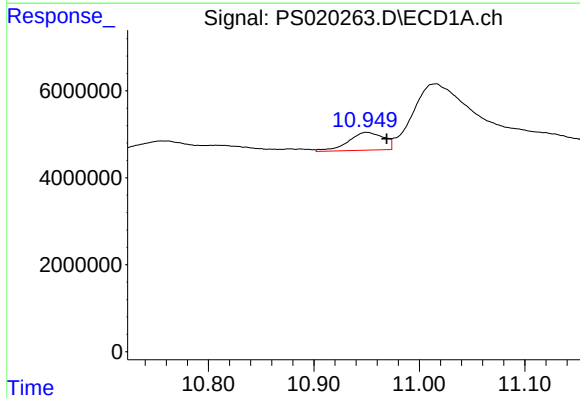

#15 Picloram

R.T.: 10.950 min
Delta R.T.: -0.019 min
Response: 9523881
Conc: N.D.

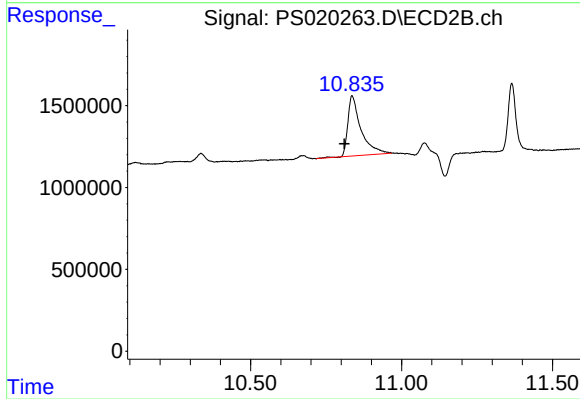

#15 Picloram

R.T.: 10.836 min
Delta R.T.: 0.026 min
Response: 11105522
Conc: 1.47 ng/ml