

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081222\
 Data File : PS020266.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2022 12:00
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 15:17:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
 Quant Title : 8080.M
 QLast Update : Thu Aug 04 02:05:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.181	6.758	1383.5E6	453.8E6	469.171	556.877
Target Compounds							
1) T	Dalapon	3.013	0.000	637839	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.429	0.000	969567	0	<MDL	N.D. #
5) T	DICAMBA	7.367	0.000	11914157	0	1.035	N.D. #
6) T	MCP	7.558	0.000	1155342	0	<MDL	N.D. #
7) T	MCPA	7.643	0.000	2542383	0	<MDL	N.D. #
9) T	2,4-D	8.362f	0.000	10103602	0	3.355	N.D. #
10) T	Pentachlo...	8.600	8.258	3587021	1631996	<MDL	<MDL #
11) T	2,4,5-TP ...	9.154	0.000	3470706	0	<MDL	N.D. #
12) T	2,4,5-T	9.462	0.000	11565325	0	<MDL	N.D. #
13) T	2,4-DB	10.016	0.000	1596256	0	<MDL	N.D. #
14) T	DINOSEB	11.129	0.000	18261684	0	1.148	N.D. #
15) T	Picloram	10.955	10.843	8844048	26413755	<MDL	3.501 #
16) T	DCPA	11.403	10.750	6984333	1168607	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081222\
Data File : PS020266.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2022 12:00
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 15:17:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080322.M
Quant Title : 8080.M
QLast Update : Thu Aug 04 02:05:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

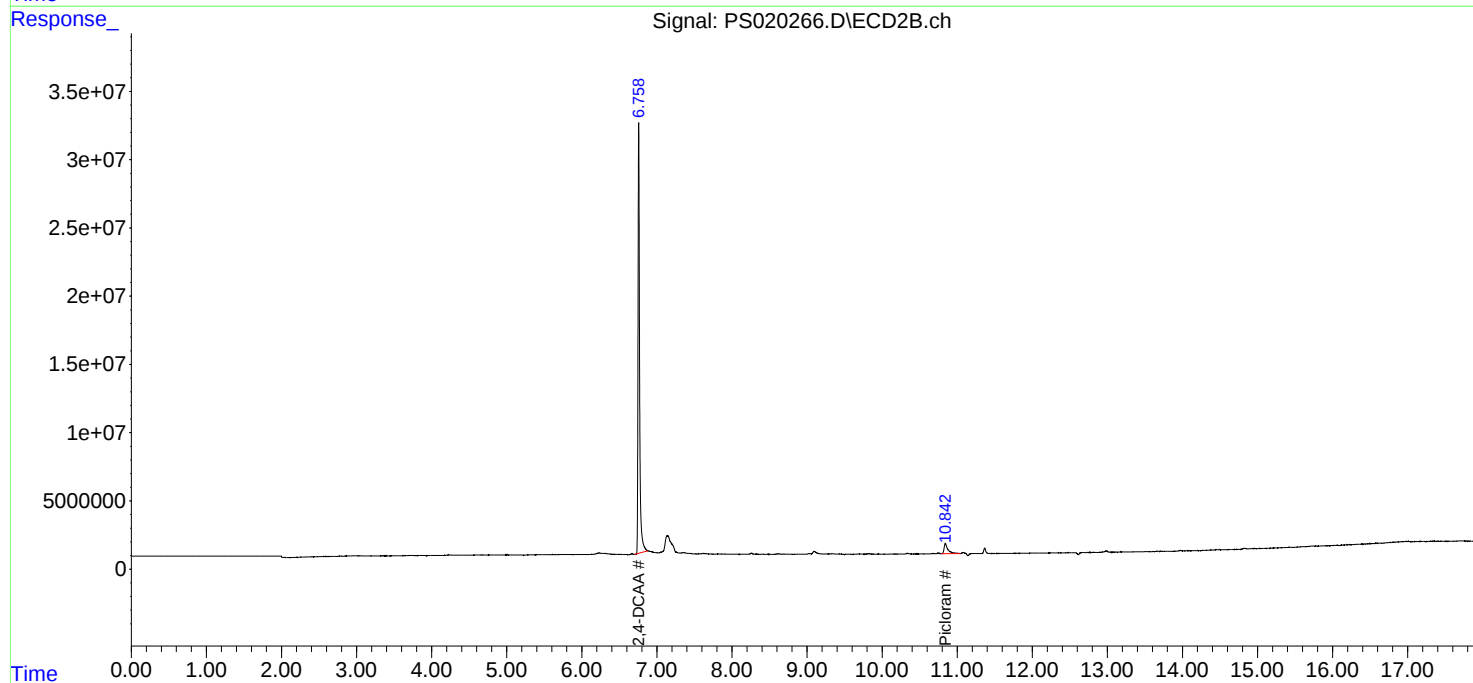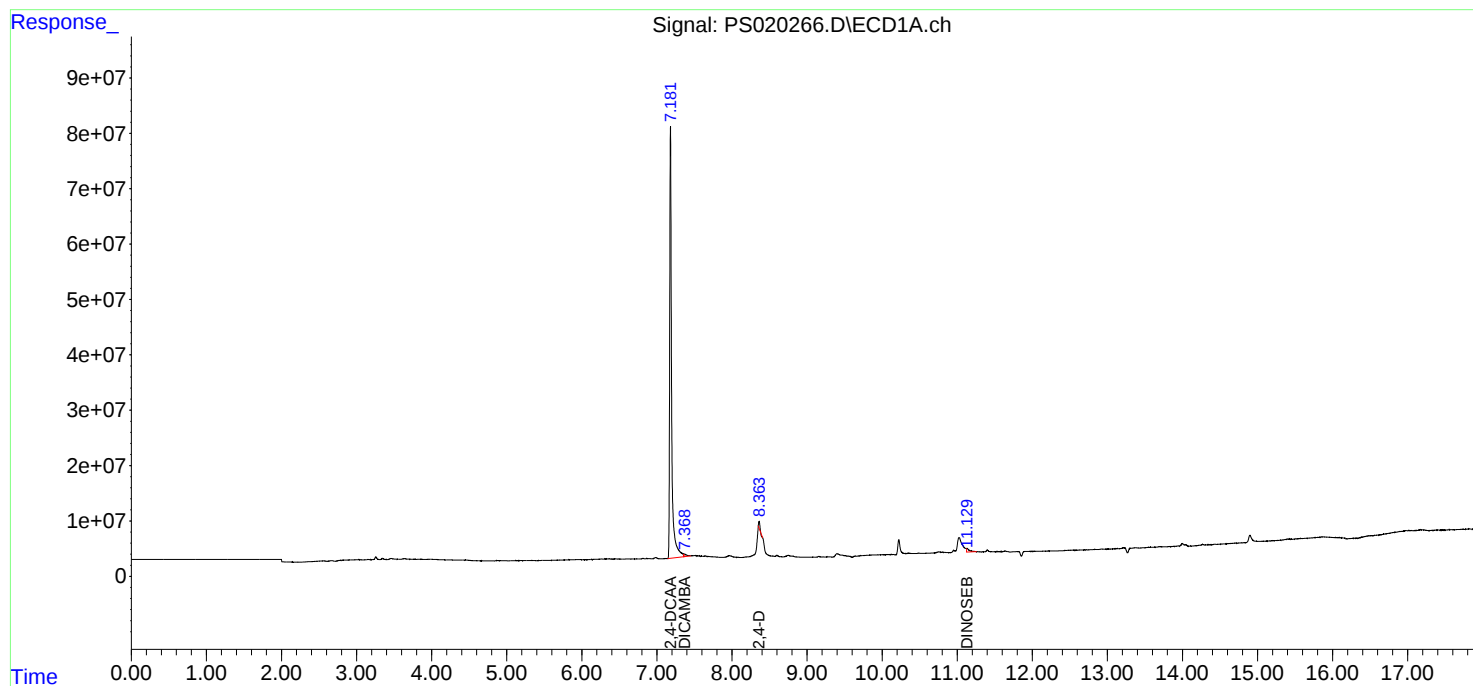


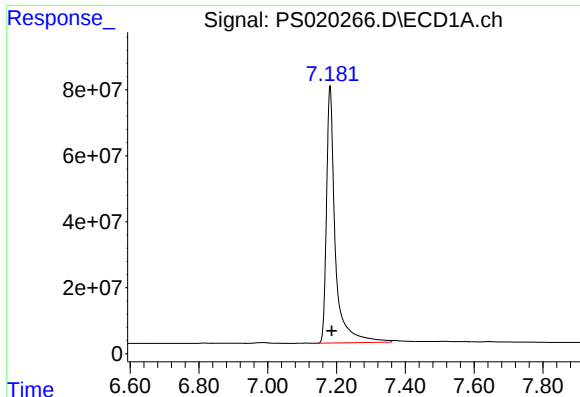

#4 2,4-DCAA


R.T.: 7.181 min
Delta R.T.: -0.005 min
Response: 1383454455
Conc: 469.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

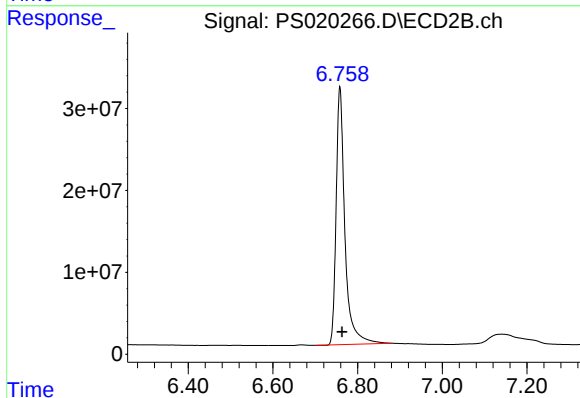


#4 2,4-DCAA

R.T.: 6.758 min
Delta R.T.: -0.005 min
Response: 453830588
Conc: 556.88 ng/ml

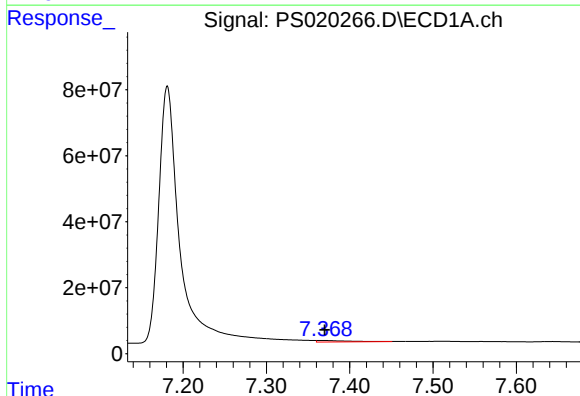


#5 DICAMBA

R.T.: 7.367 min
Delta R.T.: -0.003 min
Response: 11914157
Conc: 1.04 ng/ml

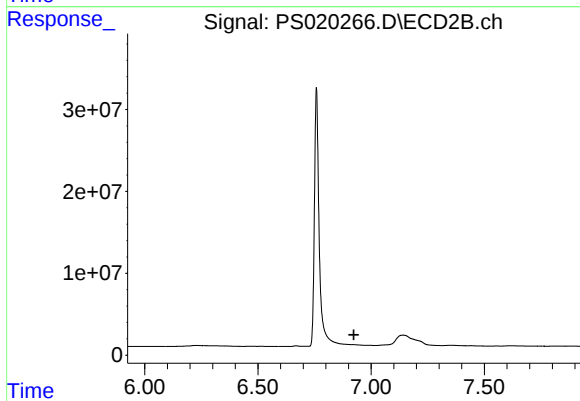

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 6.923 min
Response: 0
Conc: N.D.

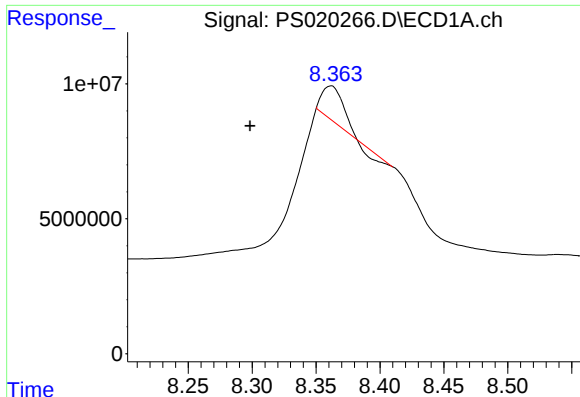

#9 2,4-D


R.T.: 8.362 min
Delta R.T.: 0.063 min
Response: 10103602
Conc: 3.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

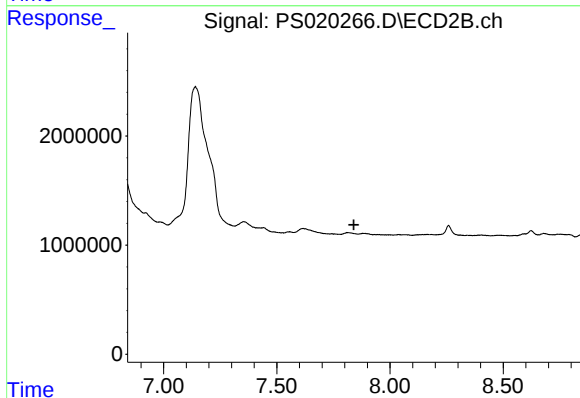


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.840 min
Response: 0
Conc: N.D.

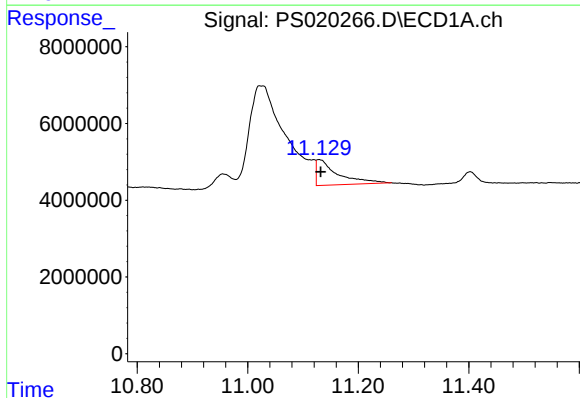


#14 DINOSEB

R.T.: 11.129 min
Delta R.T.: -0.003 min
Response: 18261684
Conc: 1.15 ng/ml

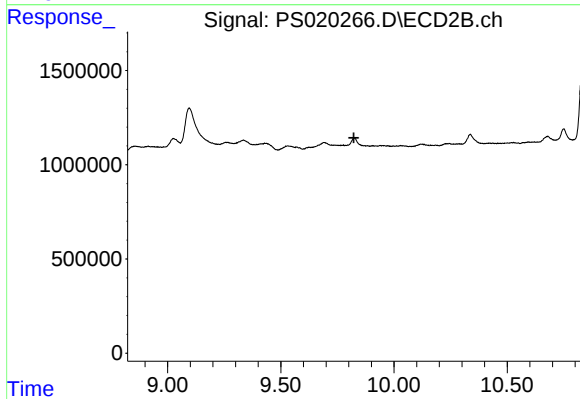

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.823 min
Response: 0
Conc: N.D.

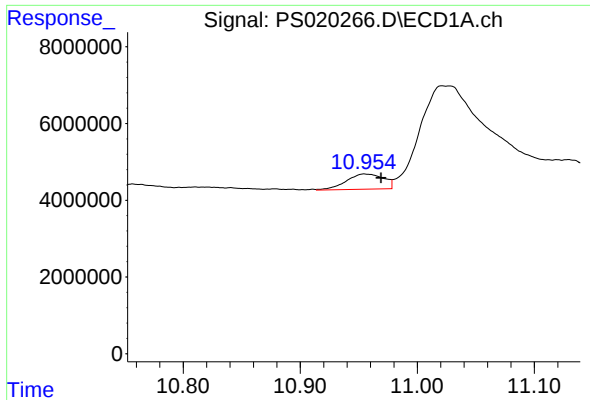

#15 Picloram

R.T.: 10.955 min
Delta R.T.: -0.014 min
Response: 8844048
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

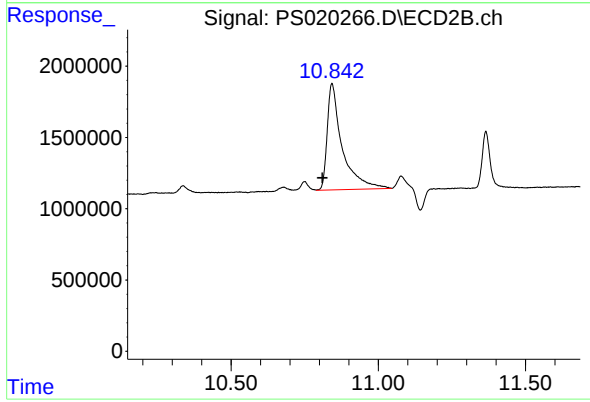

#15 Picloram

R.T.: 10.843 min
Delta R.T.: 0.032 min
Response: 26413755
Conc: 3.50 ng/ml