

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081224\
 Data File : PS027396.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2024 08:50
 Operator : AR\AJ
 Sample : P3520-17
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 OU4-57S-01-080624

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 03:13:46 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080524.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 06 08:10:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.176	7.741	626.2E6	425.1E6	248.979	228.570
Target Compounds							
1) T	Dalapon	0.000	2.663f	0	271.9E6	N.D.	81.489
3) T	4-Nitroph...	6.944f	7.262	55946174	11494908	37.006	9.187 #
5) T	DICAMBA	7.380	7.936	11620670	6112346	1.053	<MDL #
6) T	MCP	7.518f	8.038	23736468	697166	3.119	<MDL #
7) T	MCPA	7.687	8.283	6052620	10115939	<MDL	1.339 #
8) T	DICHLORPROP	8.019f	8.653	20482378	914046	7.741	<MDL #
9) T	2,4-D	0.000	8.982	0	291866	N.D.	<MDL
10) T	Pentachlo...	8.567	9.507	10389179	4517267	<MDL	<MDL #
11) T	2,4,5-TP ...	9.172	9.847f	9005912	3194976	<MDL	<MDL #
12) T	2,4,5-T	9.474f	10.291	6525946	106.3E6	<MDL	8.430 #
13) T	2,4-DB	9.983f	10.839f	128.1E6	4291090	62.461	2.715 #
14) T	DINOSEB	11.205	11.245	177.8E6	251.9E6	15.950	29.574 #
15) T	Picloram	11.008	12.336	200.0E6	66549129	10.372	3.689 #
16) T	DCPA	0.000	12.291	0	12134608	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081224\
Data File : PS027396.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2024 08:50
Operator : AR\AJ
Sample : P3520-17
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
OU4-57S-01-080624

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 03:13:46 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080524.M
Quant Title : 8080.M
QLast Update : Tue Aug 06 08:10:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

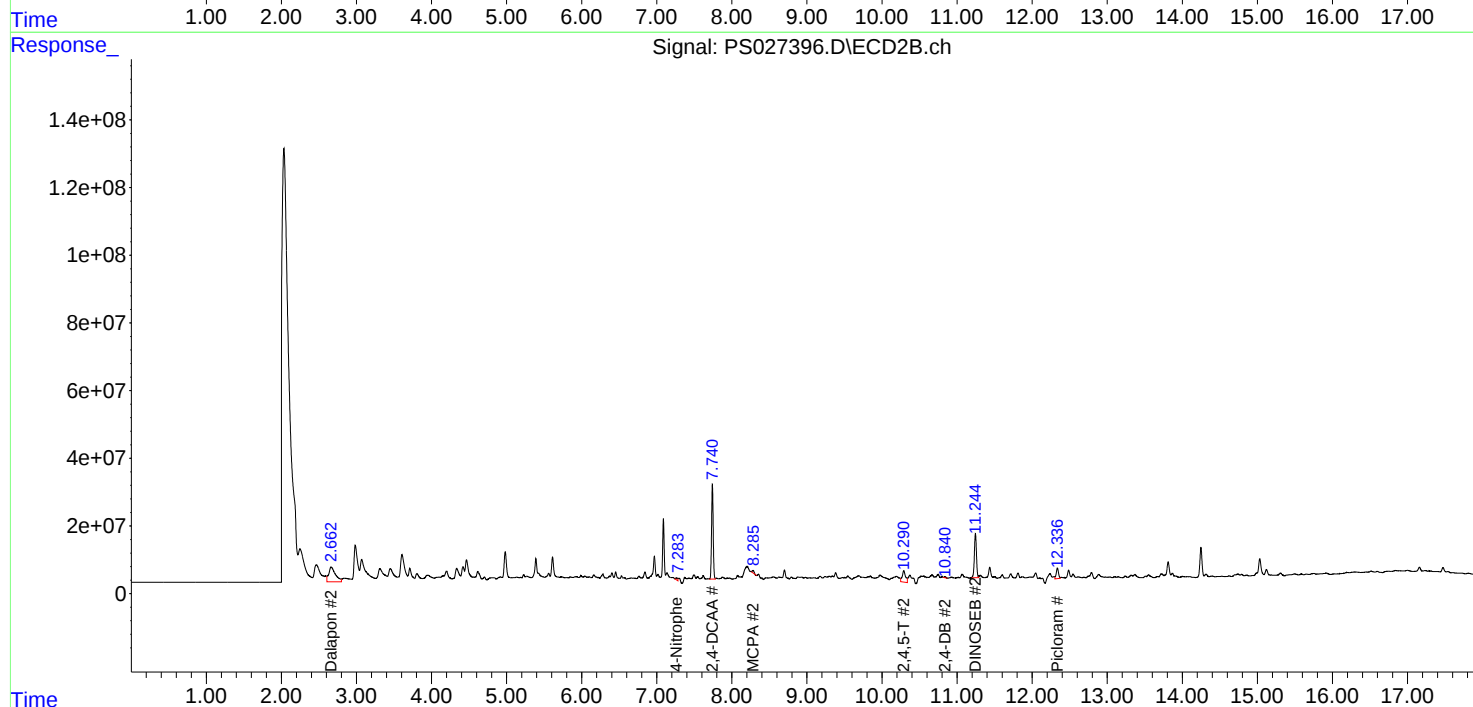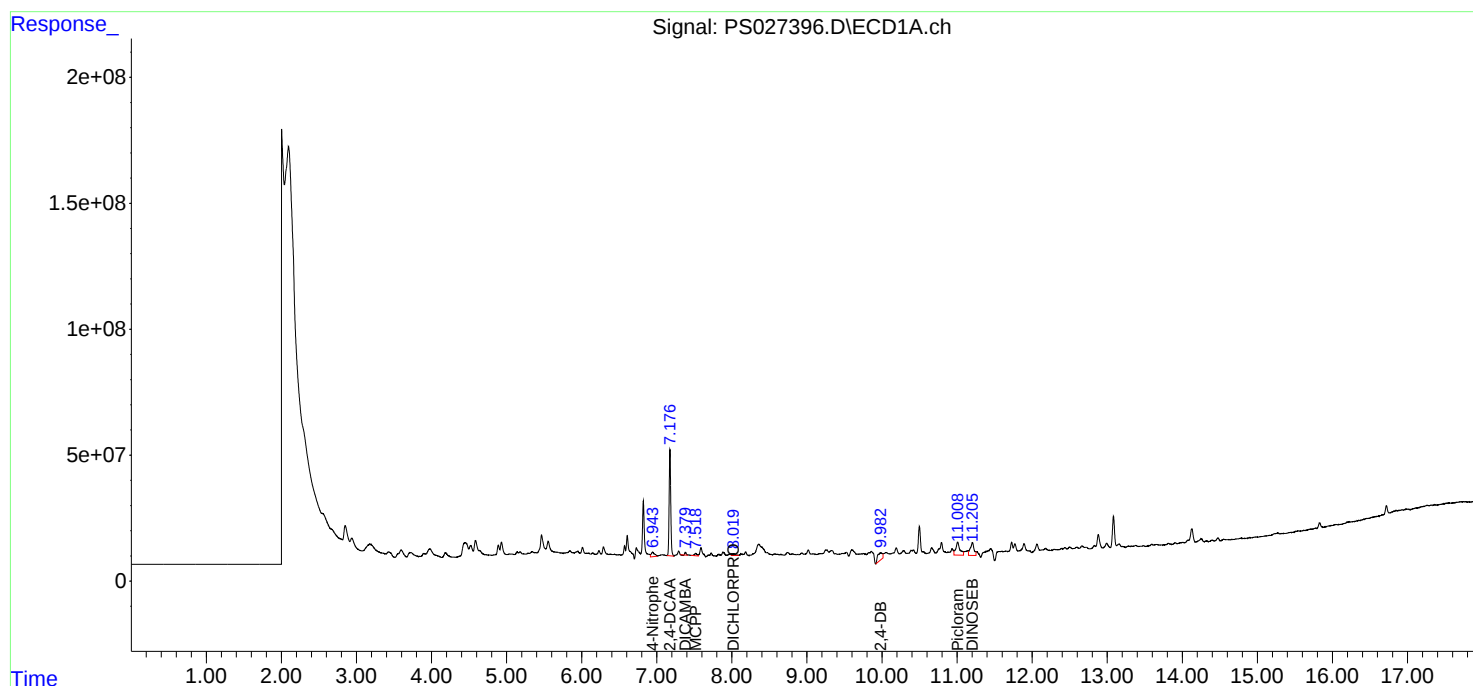

The printer must be in Portrait mode.

Instrument :
ECD_S
ClientSampleId :
OU4-57S-01-080624