

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081224\
 Data File : PS027397.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2024 09:15
 Operator : AR\AJ
 Sample : P3543-01
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 ARS20-0019

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 03:14:02 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080524.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 06 08:10:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.172	7.750	29728495	31229492	11.820	16.792 #
Target Compounds							
1) T	Dalapon	0.000	2.664f	0	308.5E6	N.D.	92.467
3) T	4-Nitroph...	6.942f	7.258	54390724	22574666	35.978	18.043 #
5) T	DICAMBA	0.000	7.931	0	6323461	N.D.	<MDL
6) T	MCP	7.517f	8.030	22621084	2378927	2.973	<MDL #
7) T	MCPA	7.688	0.000	9338093	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	8.701f	0	32545326	N.D.	15.568
9) T	2,4-D	0.000	8.976	0	3583170	N.D.	1.538
10) T	Pentachlo...	8.592	9.528	9442211	4652188	<MDL	<MDL #
11) T	2,4,5-TP ...	9.172	9.846f	12038307	1448468	<MDL	<MDL #
12) T	2,4,5-T	9.453	10.297	19408852	15235052	1.329	1.208
13) T	2,4-DB	10.055f	10.892	23204342	1011853	11.315	<MDL #
14) T	DINOSEB	11.203	11.246	16975344	16474058	1.523	1.934 #
15) T	Picloram	11.010	12.337	43790853	14226720	2.271	<MDL #
16) T	DCPA	11.450f	12.271	14429360	2479996	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081224\
Data File : PS027397.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2024 09:15
Operator : AR\AJ
Sample : P3543-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
ARS20-0019

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 03:14:02 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080524.M
Quant Title : 8080.M
QLast Update : Tue Aug 06 08:10:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

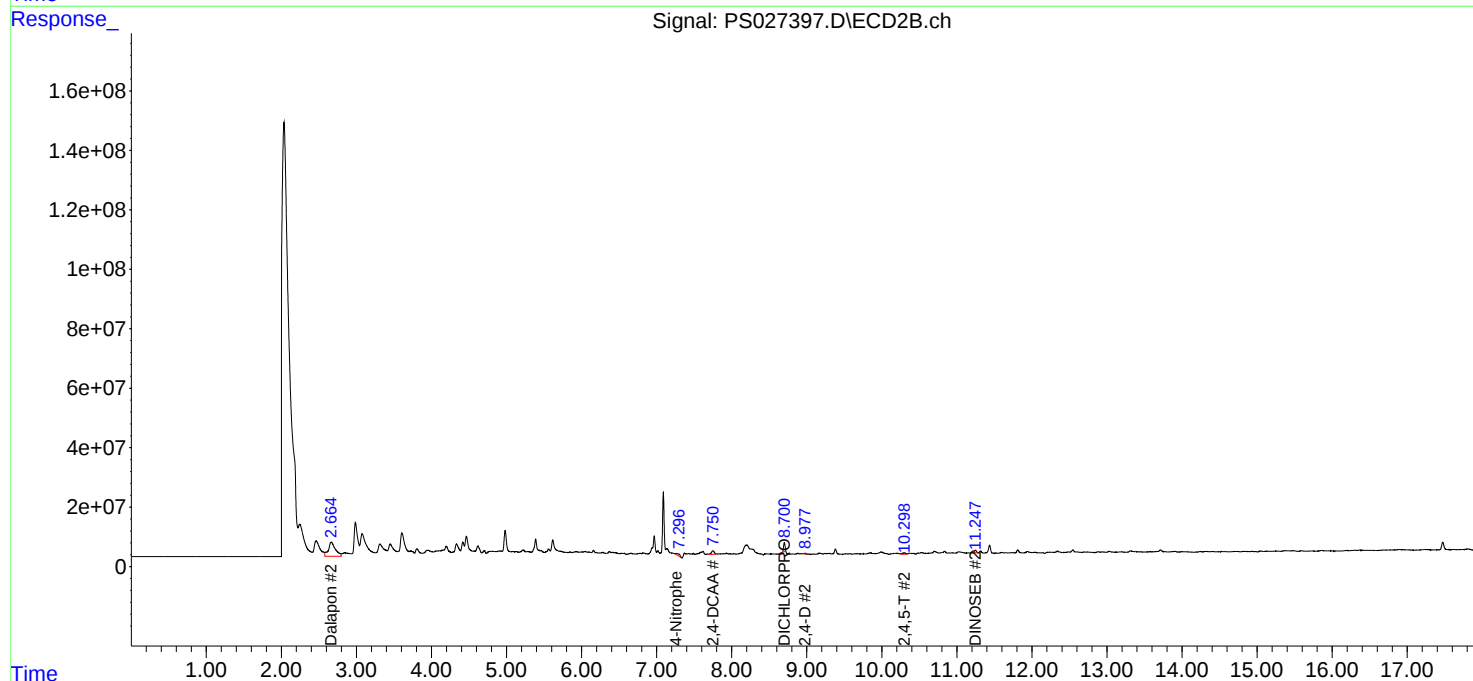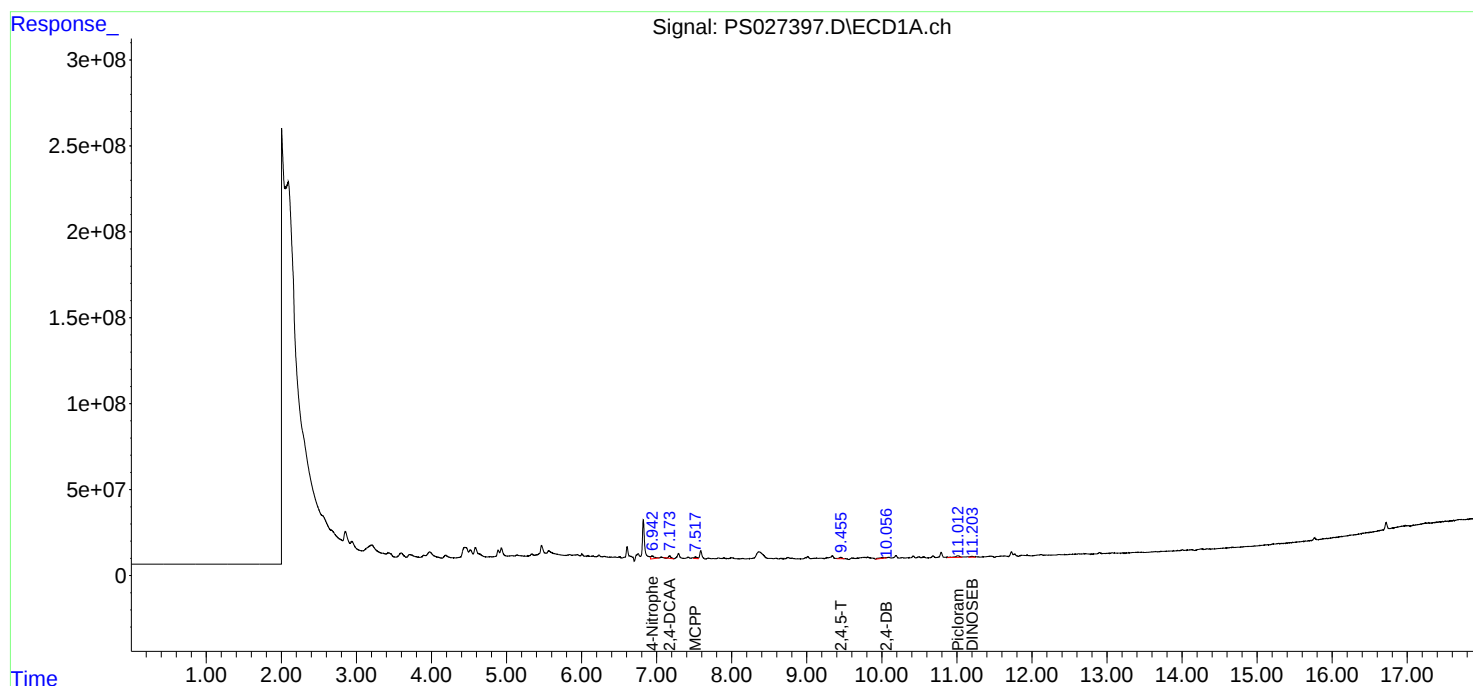

The printer must be in Portrait mode.

Instrument :
ECD_S
ClientSampleId :
ARS20-0019