

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081224\
 Data File : PS027400.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2024 10:28
 Operator : AR\AJ
 Sample : P3548-03
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 RBR200036

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 03:14:37 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080524.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 06 08:10:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.175	7.740	841.6E6	559.7E6	334.623	300.975
Target Compounds							
1) T	Dalapon	0.000	2.654f	0	298.1E6	N.D.	89.333
2) T	3,5-DICHL...	6.386	6.704	-719086	706149	N.D.	<MDL
3) T	4-Nitroph...	6.943f	7.263	52633212	8662397	34.815	6.923 #
5) T	DICAMBA	7.376	7.940	20653678	5643371	1.871	<MDL #
6) T	MCPD	7.540	8.032	26165318	6930011	3.438	1.217 #
7) T	MCPA	7.698	8.278	20366097	5029822	2.102	<MDL #
8) T	DICHLORPROP	8.087	8.654	14141887	1489211	5.345	<MDL #
9) T	2,4-D	8.291	8.974	17016281	3936852	5.968	1.690 #
10) T	Pentachlo...	8.566	9.507	43525741	29588126	1.101	<MDL #
11) T	2,4,5-TP ...	9.166	0.000	12102351	0	<MDL	N.D. #
12) T	2,4,5-T	9.476f	10.289	26210596	117.2E6	1.795	9.297 #
13) T	2,4-DB	10.029	10.898f	58165034	5309086	28.362	3.359 #
14) T	DINOSEB	11.204	11.245	153.6E6	131.6E6	13.785	15.448
15) T	Picloram	11.010	12.333	123.5E6	21514323	6.407	1.193 #
16) T	DCPA	11.448f	12.288	91526377	7731889	5.067	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081224\
Data File : PS027400.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2024 10:28
Operator : AR\AJ
Sample : P3548-03
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
RBR200036

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 03:14:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080524.M
Quant Title : 8080.M
QLast Update : Tue Aug 06 08:10:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

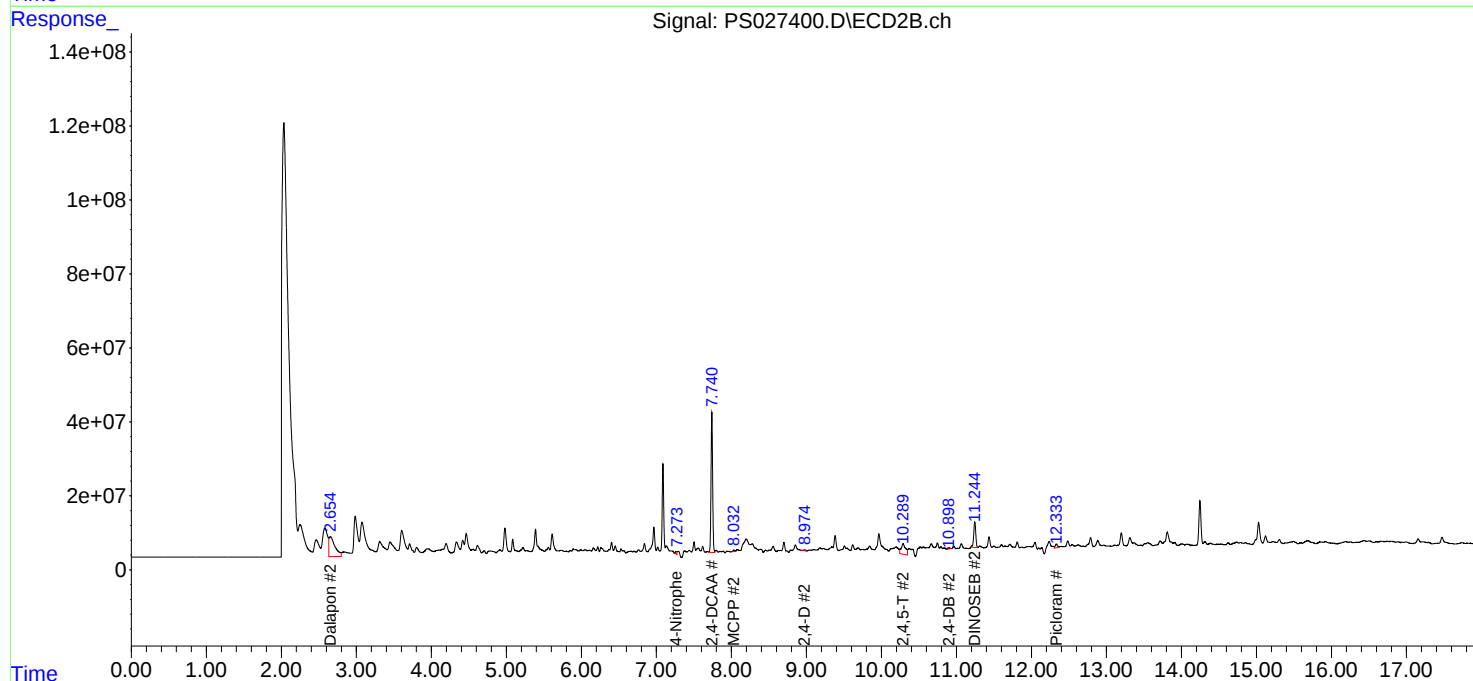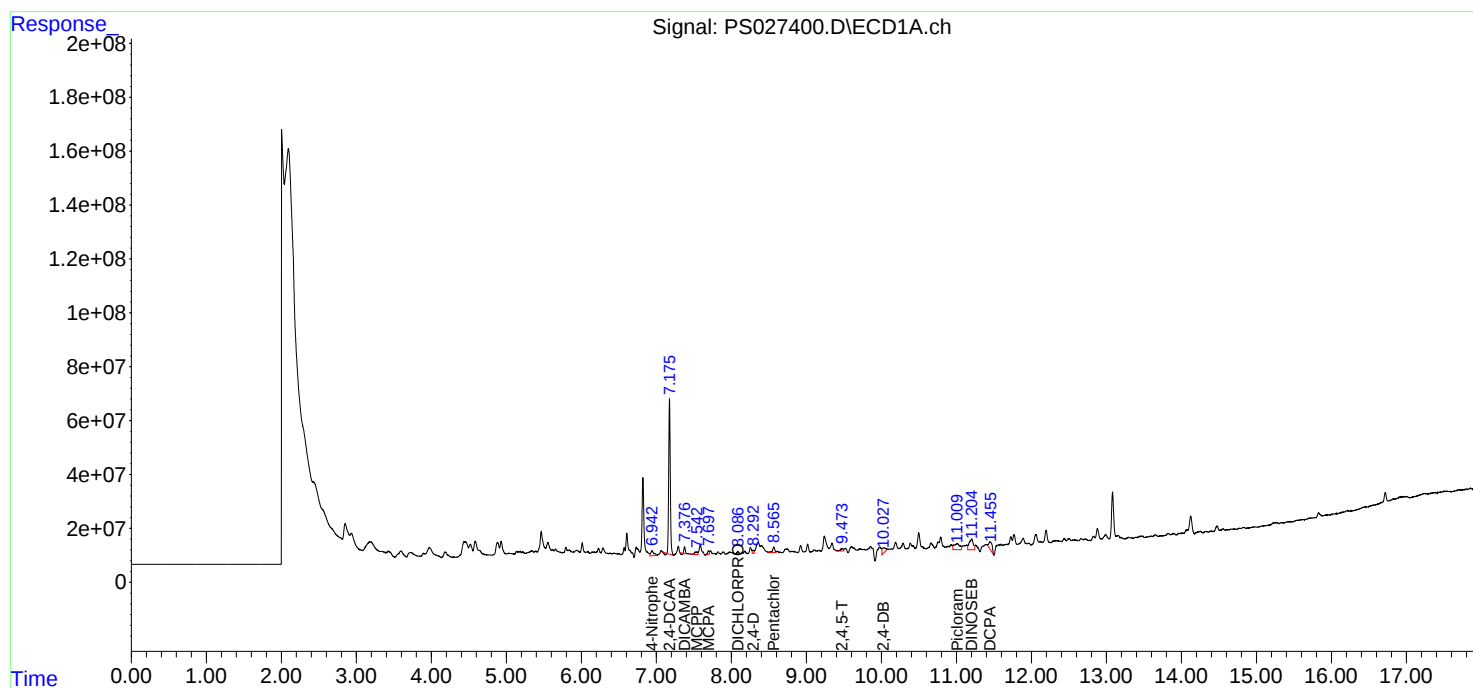

The printer must be in Portrait mode.

Instrument :
ECD_S
ClientSampleId :
BBR200036