

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081224\
 Data File : PS027401.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2024 10:52
 Operator : AR\AJ
 Sample : P3548-06
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 343

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 03:14:50 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080524.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 06 08:10:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.175	7.741	503.3E6	355.8E6	200.123	191.310
Target Compounds							
2) T	3,5-DICHL...	6.385	6.705	-545480	1641173	N.D.	<MDL
3) T	4-Nitroph...	6.943f	7.259	65402554	9496822	43.261	7.590 #
5) T	DICAMBA	7.375	7.940	22630365	5823065	2.050	<MDL #
6) T	MCP	7.518f	8.031	31967308	17246143	4.201	3.029 #
7) T	MCPA	7.697	8.266	86974639	5435573	8.977	<MDL #
8) T	DICHLORPROP	8.086	8.650	21865984	3512955	8.264	1.680 #
9) T	2,4-D	8.255f	8.976	68440962	2748736	24.005	1.180 #
10) T	Pentachlo...	8.565	9.540f	21786506	24473041	<MDL	<MDL #
11) T	2,4,5-TP ...	9.166	9.843f	9018308	2222362	<MDL	<MDL #
12) T	2,4,5-T	9.472f	10.292	38430203	103.9E6	2.631	8.243 #
13) T	2,4-DB	10.021	10.897f	39334389	10697290	19.180	6.767 #
14) T	DINOSEB	11.204	11.245	164.1E6	168.9E6	14.728	19.833 #
15) T	Picloram	11.012	12.334	131.5E6	18142913	6.819	1.006 #
16) T	DCPA	0.000	12.334f	0	18142913	N.D.	1.305



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081224\
Data File : PS027401.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2024 10:52
Operator : AR\AJ
Sample : P3548-06
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
343

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 03:14:50 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080524.M
Quant Title : 8080.M
QLast Update : Tue Aug 06 08:10:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

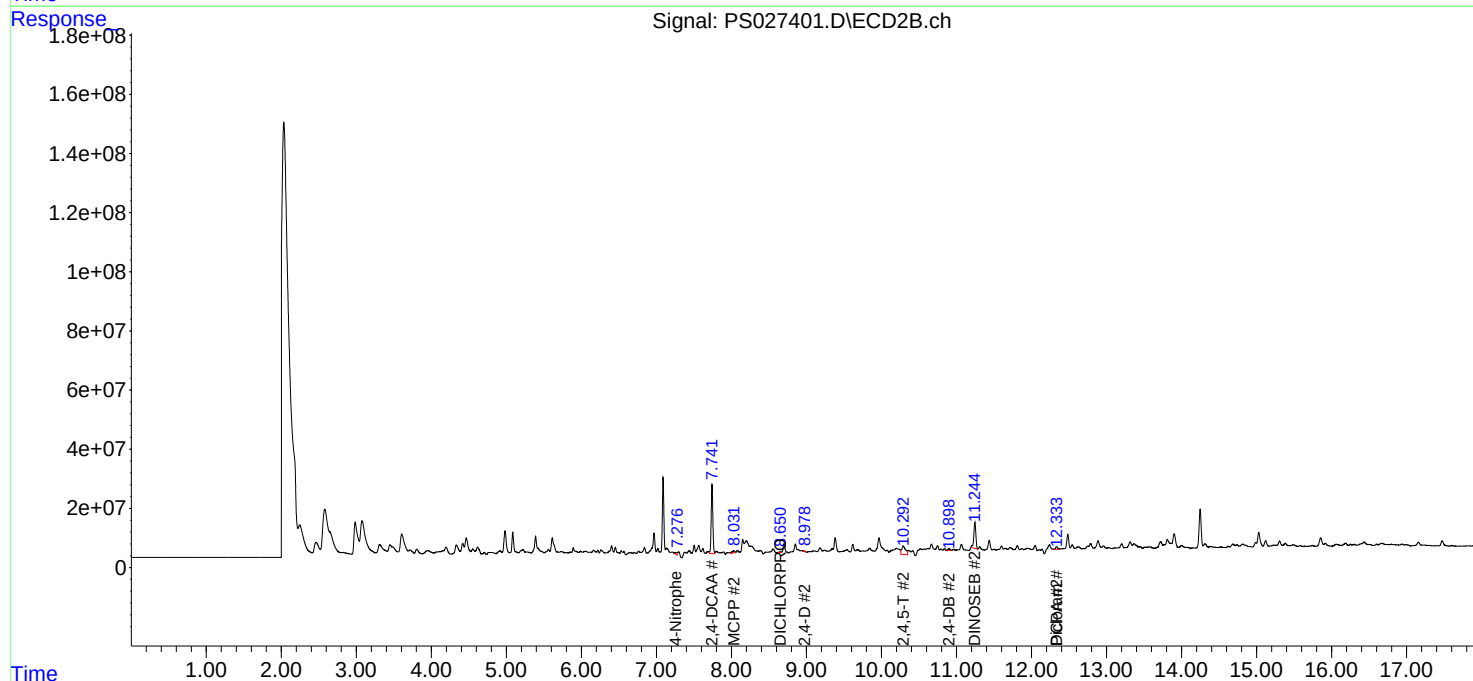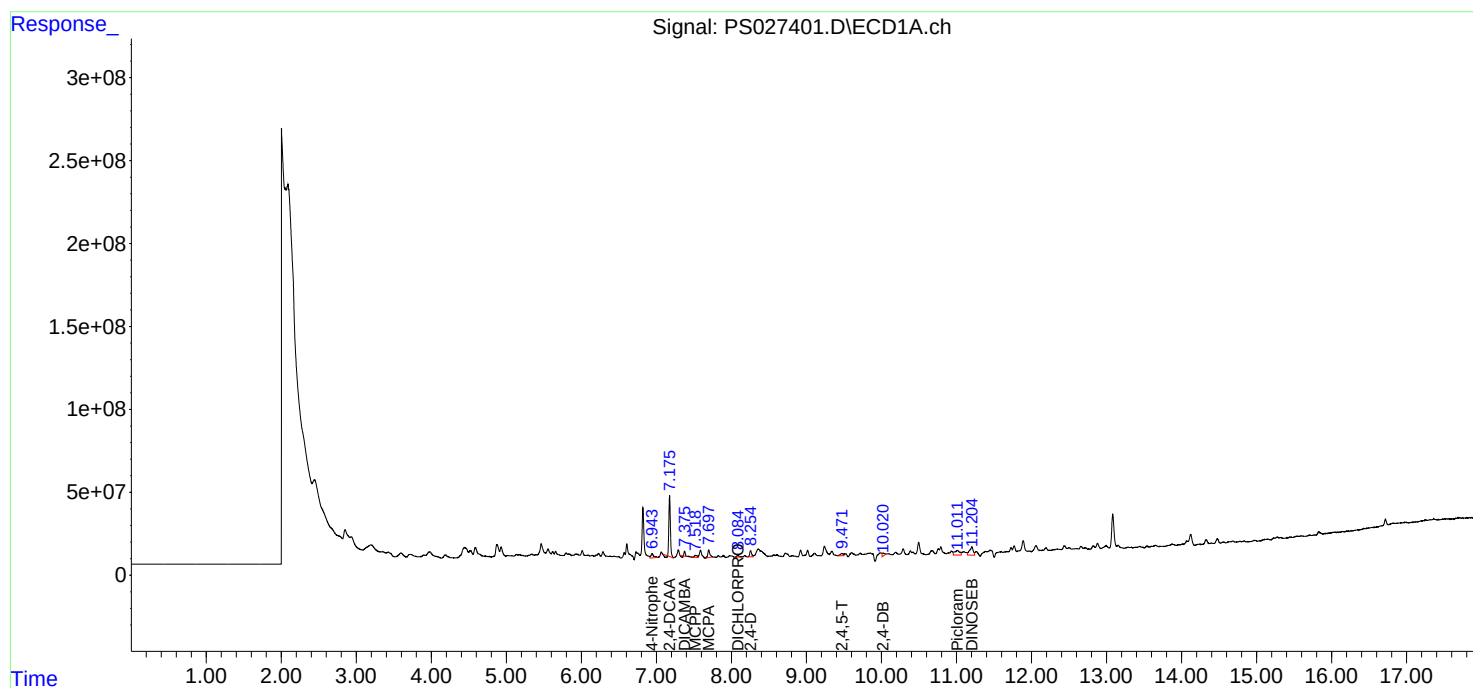

The printer must be in Portrait mode.

Instrument :
ECD_S
ClientSampleId :
343