

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081224\
 Data File : PS027402.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2024 11:16
 Operator : AR\AJ
 Sample : P3548-09
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 289

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 03:15:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080524.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 06 08:10:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.173	7.740	925.2E6	465.4E6	367.860	250.256 #
Target Compounds							
3) T	4-Nitroph...	6.944f	7.254	66944596	6144571	44.281	4.911 #
5) T	DICAMBA	7.375	7.937	-6729790	6855229	N.D.	<MDL
6) T	MCP	7.541	8.032	13400764	19930122	1.761	3.500 #
7) T	MCPA	7.697	8.273	18235177	5628189	1.882	<MDL #
8) T	DICHLORPROP	8.088	8.625f	29626415	9132433	11.197	4.369 #
9) T	2,4-D	8.254f	8.974	76457624	5299713	26.817	2.275 #
10) T	Pentachlo...	8.565	9.510	20534393	9028496	<MDL	<MDL #
11) T	2,4,5-TP ...	9.106f	0.000	47771050	0	3.150	N.D. #
12) T	2,4,5-T	9.471f	10.294	34351743	47108272	2.352	3.736 #
13) T	2,4-DB	10.021	10.896f	42301927	9706904	20.627	6.141 #
14) T	DINOSEB	11.205	11.246	149.2E6	51953345	13.387	6.100 #
15) T	Picloram	11.015	12.332	73679693	19538997	3.821	1.083 #
16) T	DCPA	11.473f	12.332f	54689938	19538997	3.027	1.405 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081224\
Data File : PS027402.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2024 11:16
Operator : AR\AJ
Sample : P3548-09
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
289

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 03:15:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080524.M
Quant Title : 8080.M
QLast Update : Tue Aug 06 08:10:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

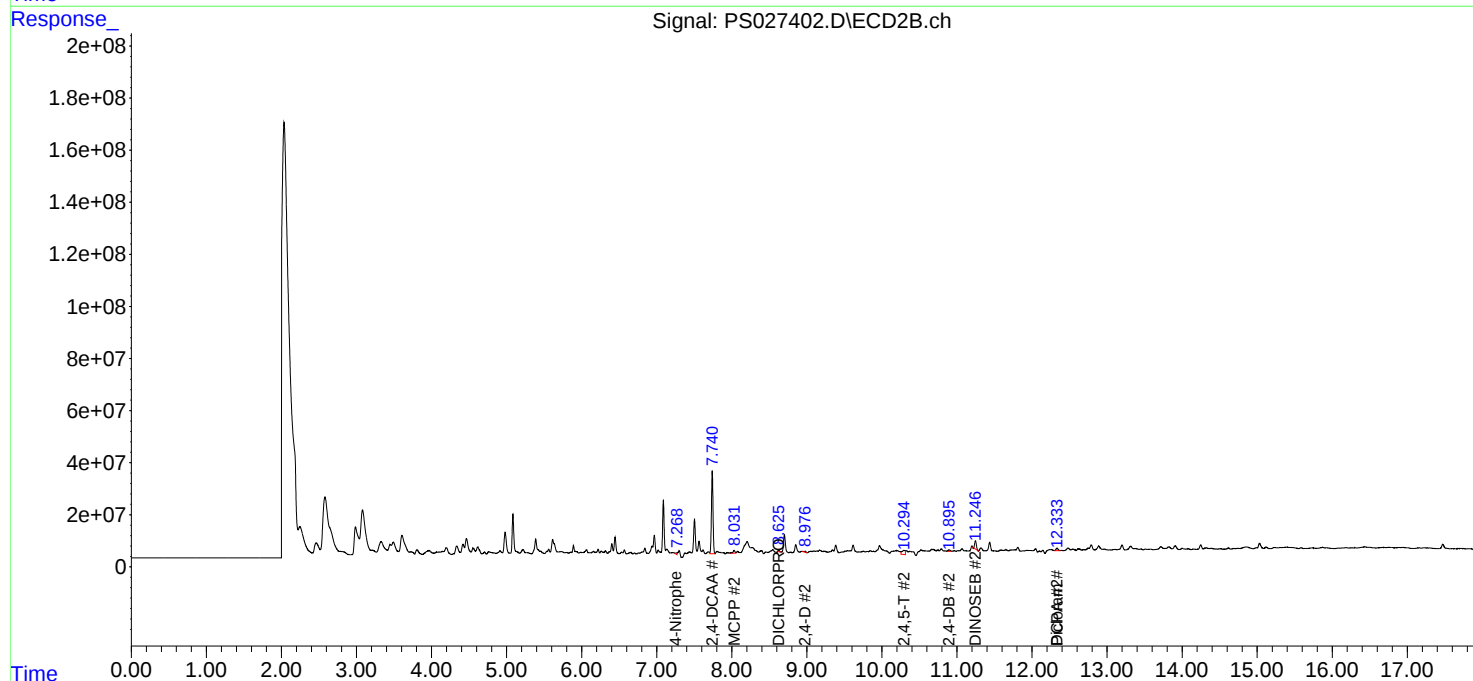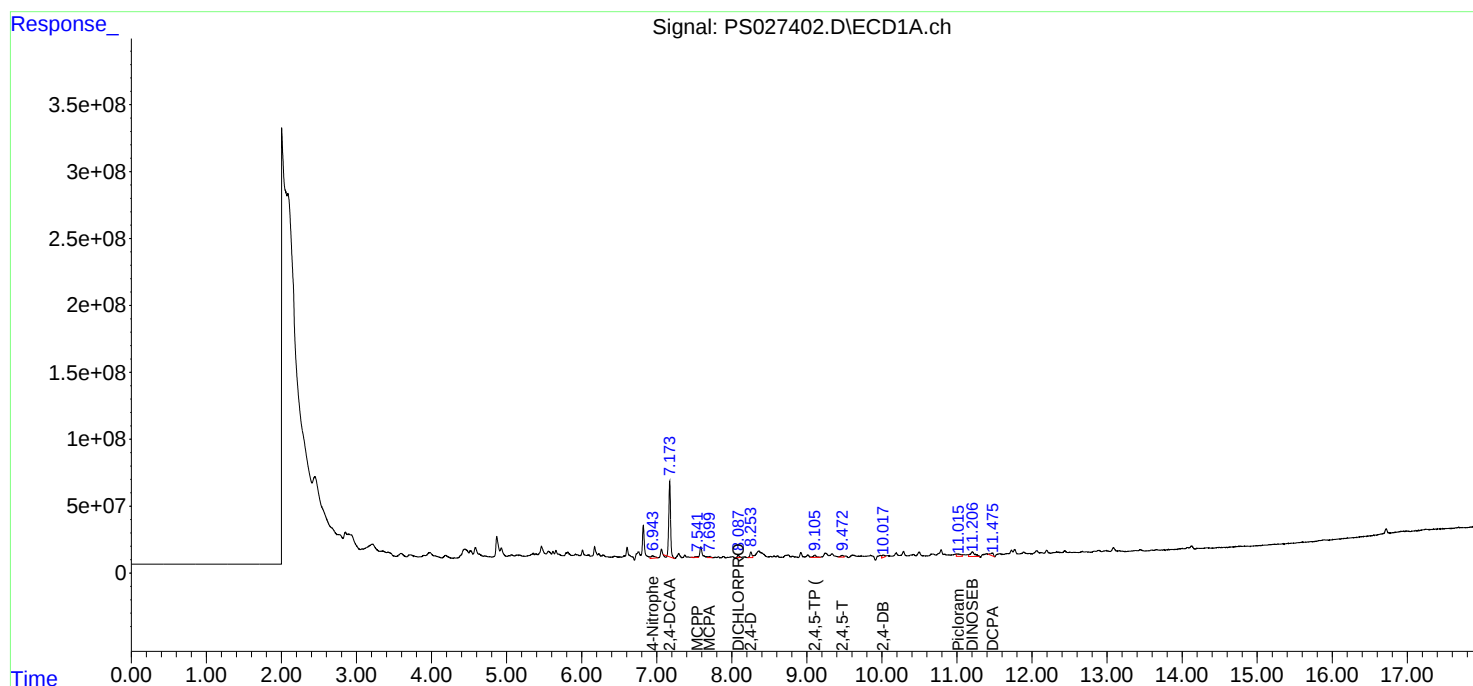

The printer must be in Portrait mode.