

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081224\
 Data File : PS027404.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2024 12:05
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 03:15:26 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080524.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 06 08:10:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.175	7.740	1352.6E6	1002.9E6	537.775	539.286
Target Compounds							
1) T	Dalapon	2.615	2.696	8292974	92943	2.538	<MDL #
2) T	3,5-DICHL...	6.335f	0.000	6113.6E6	0	1535.417	N.D. #
3) T	4-Nitroph...	6.965	0.000	24750243	0	16.371	N.D. #
5) T	DICAMBA	0.000	7.939	0	290046	N.D.	<MDL
6) T	MCP	7.590f	8.042	54571547	3197.3E6	7.171	561.485 #
7) T	MCPA	0.000	8.271	0	4803868	N.D.	<MDL
8) T	DICHLORPROP	8.085	8.652	11616934	286055	4.391	<MDL #
9) T	2,4-D	8.291	8.981	9239.5E6	352016	3240.648	<MDL #
10) T	Pentachlo...	8.576	9.483f	11683027	6804076	<MDL	<MDL #
11) T	2,4,5-TP ...	9.122f	9.901	6071477	5195657	<MDL	<MDL #
12) T	2,4,5-T	0.000	10.299	0	2315706	N.D.	<MDL
13) T	2,4-DB	0.000	10.902f	0	6277881	N.D.	3.971
14) T	DINOSEB	11.228f	0.000	5203720	0	<MDL	N.D. #
15) T	Picloram	10.977f	12.335	535.7E6	82414758	27.784	4.568 #
16) T	DCPA	11.477	12.246f	10921960	47099723	<MDL	3.387 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081224\
Data File : PS027404.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2024 12:05
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 03:15:26 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080524.M
Quant Title : 8080.M
QLast Update : Tue Aug 06 08:10:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

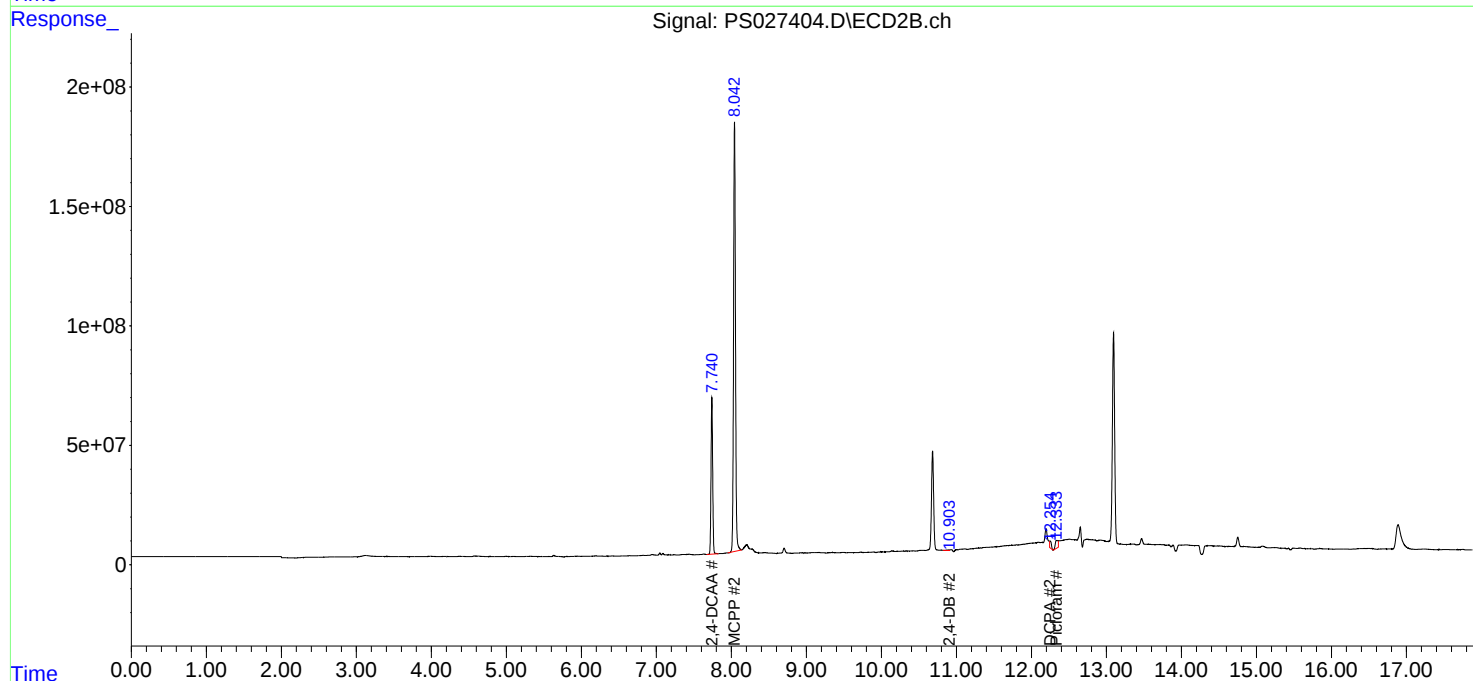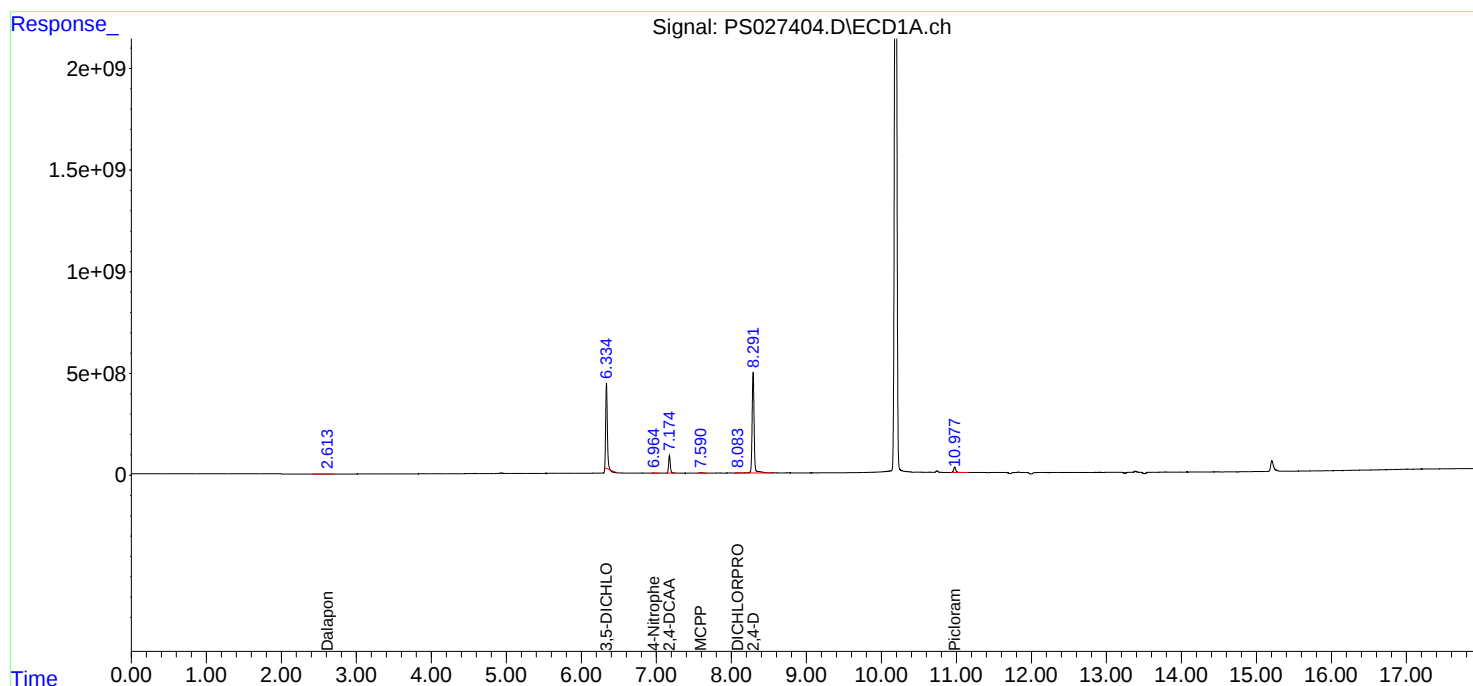

The printer must be in Portrait mode.

Instrument :
ECD_S
ClientSampleId :
I.BLK