

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081318\
 Data File : PS001458.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2018 17:51
 Operator : UA
 Sample : PB111979BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 01:06:26 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.612	11.033	107.6E6	91627544	579.842	503.794
Target Compounds							
1) T	Dalapon	3.002	2.399	270582	4744251	1.141	20.820 #
2) T	3,5-DICHL...	0.000	9.120	0	692566	N.D.	2.719 #
5) T	DICAMBA	0.000	11.277	0	6300028	N.D.	9.192 #
6) T	MCP	12.305	0.000	9854850	0	19.607	N.D. #
7) T	MCPA	12.580	0.000	13419890	0	17.017	N.D. #
8) T	DICHLORPROP	0.000	12.404	0	1591884	N.D.	8.986 #
12) T	2,4,5-T	0.000	14.655	0	13963673	N.D.	15.117 #
14) T	DINOSEB	0.000	15.727	0	5943473	N.D.	8.362 #
15) T	Picloram	0.000	16.973	0	20296144	N.D.	14.723 #
16) T	DCPA	0.000	16.973	0	20296144	N.D.	14.053 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081318\
Data File : PS001458.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2018 17:51
Operator : UA
Sample : PB111979BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 01:06:26 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

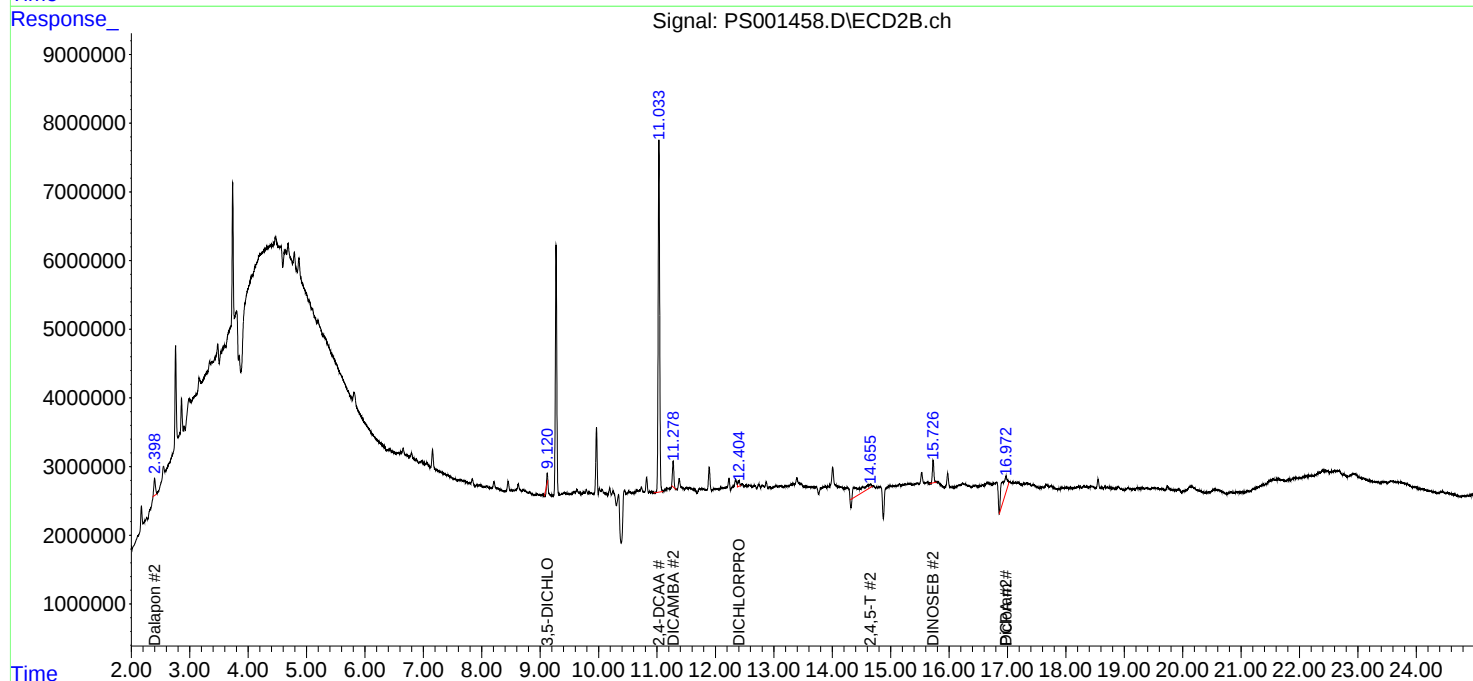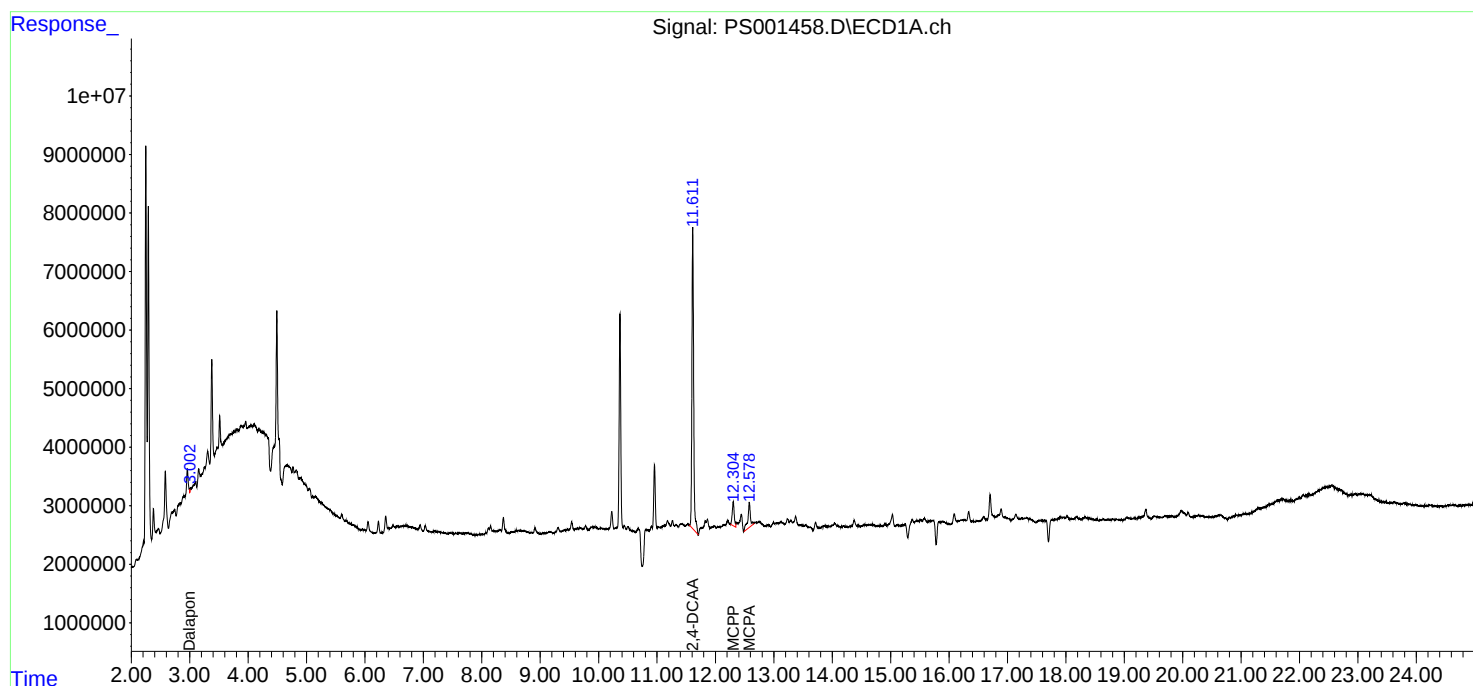


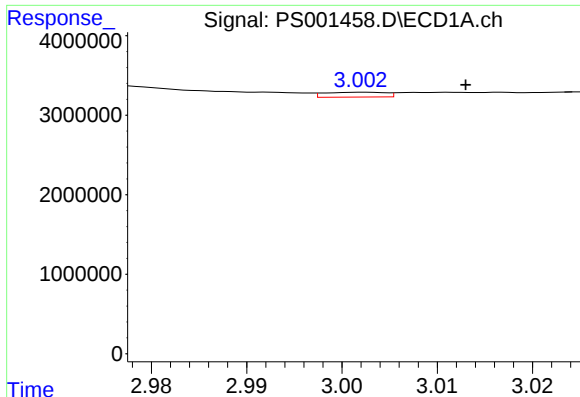

#1 Dalapon


R.T.: 3.002 min
Delta R.T.: -0.011 min
Response: 270582
Conc: 1.14 ng/ml

Instrument :
ECD_S
ClientSampleId :

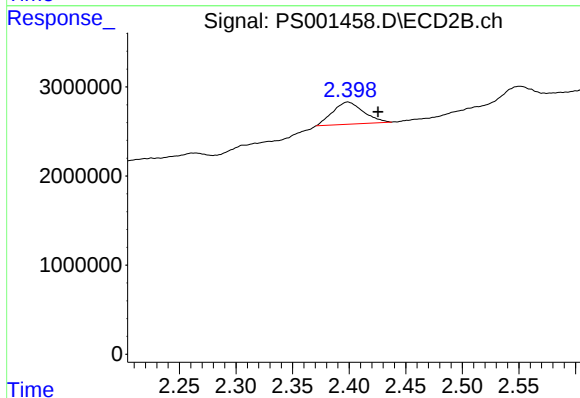


#1 Dalapon

R.T.: 2.399 min
Delta R.T.: -0.027 min
Response: 4744251
Conc: 20.82 ng/ml

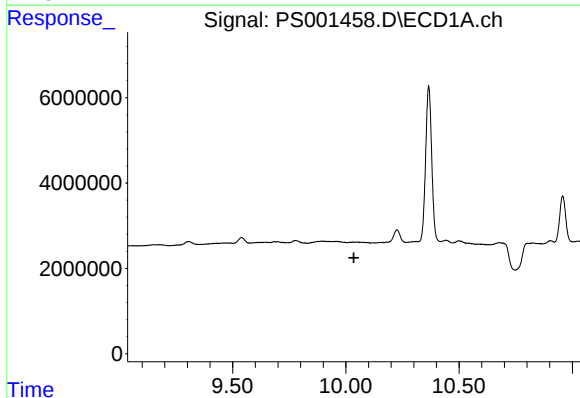


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.035 min
Response: 0
Conc: N.D.

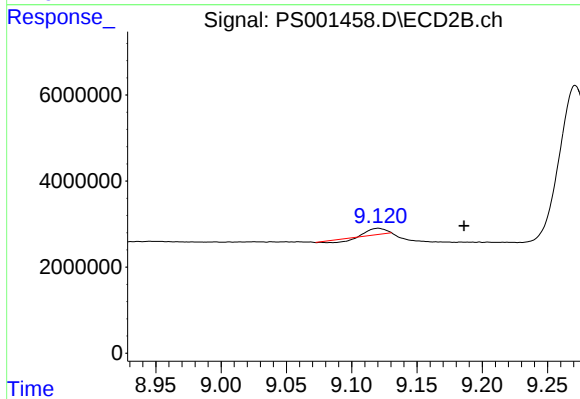

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.120 min
Delta R.T.: -0.066 min
Response: 692566
Conc: 2.72 ng/ml

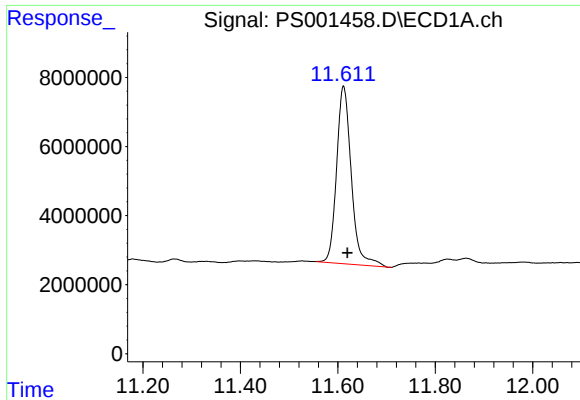

#4 2,4-DCAA


R.T.: 11.612 min
Delta R.T.: -0.008 min
Response: 107589672
Conc: 579.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

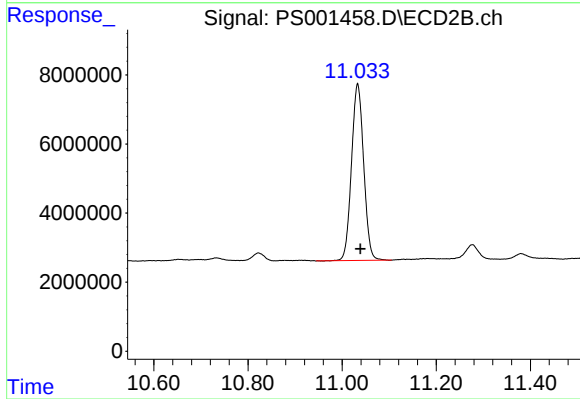


#4 2,4-DCAA

R.T.: 11.033 min
Delta R.T.: -0.006 min
Response: 91627544
Conc: 503.79 ng/ml

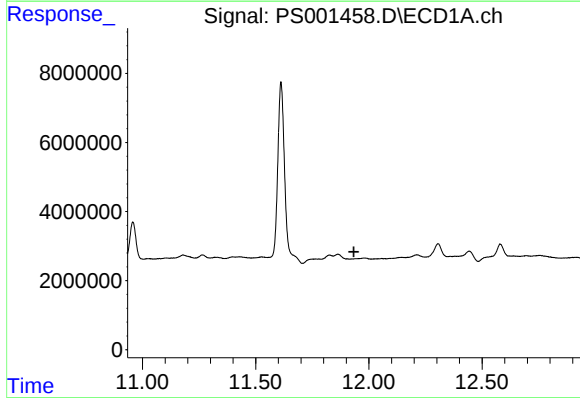


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.934 min
Response: 0
Conc: N.D.

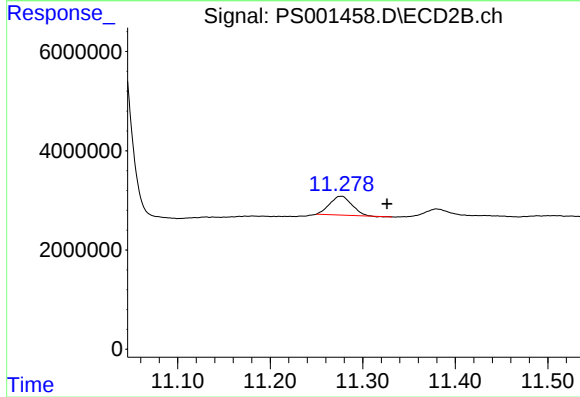

#5 DICAMBA


R.T.: 11.277 min
Delta R.T.: -0.050 min
Response: 6300028
Conc: 9.19 ng/ml

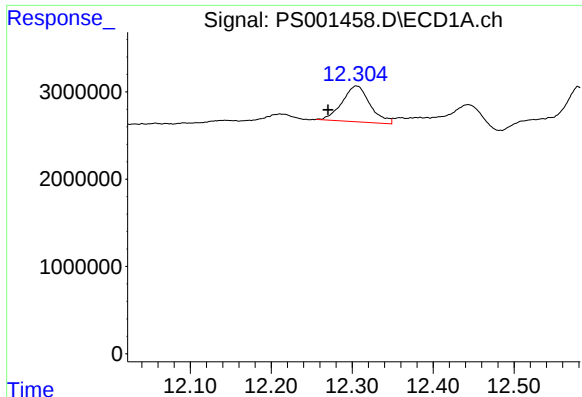

#6 MCPP


R.T.: 12.305 min
Delta R.T.: 0.035 min
Response: 9854850
Conc: 19.61 ug/ml

Instrument :
ECD_S
ClientSampleId :

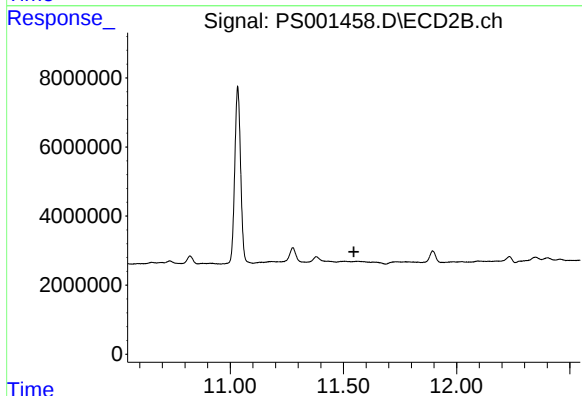


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.546 min
Response: 0
Conc: N.D.

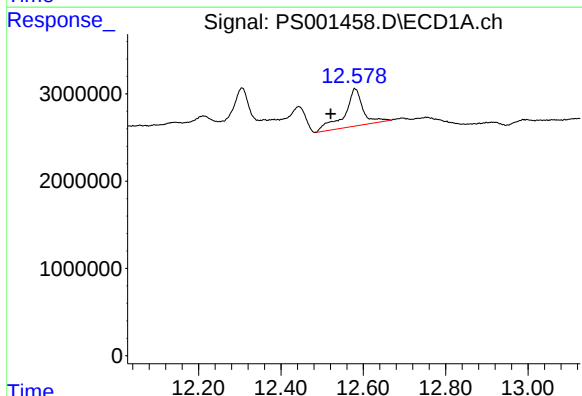


#7 MCPA

R.T.: 12.580 min
Delta R.T.: 0.059 min
Response: 13419890
Conc: 17.02 ug/ml

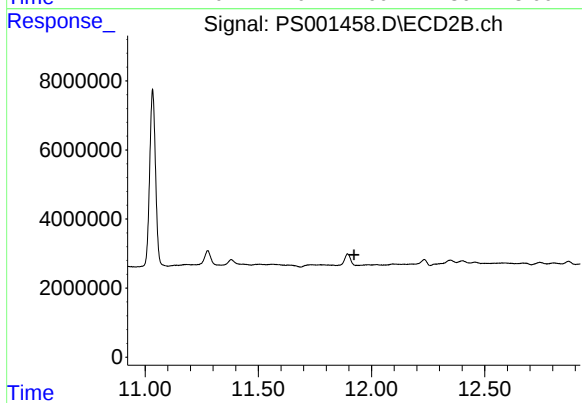

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 11.922 min
Response: 0
Conc: N.D.

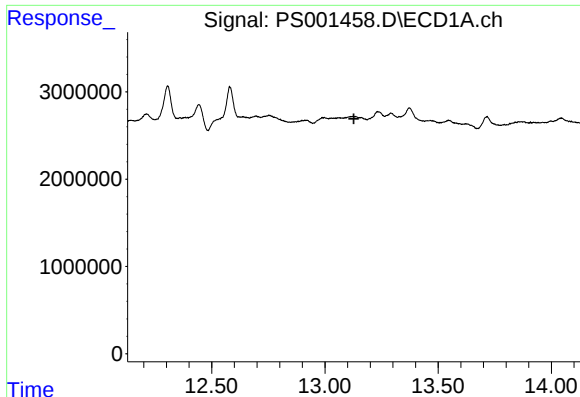

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 13.128 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

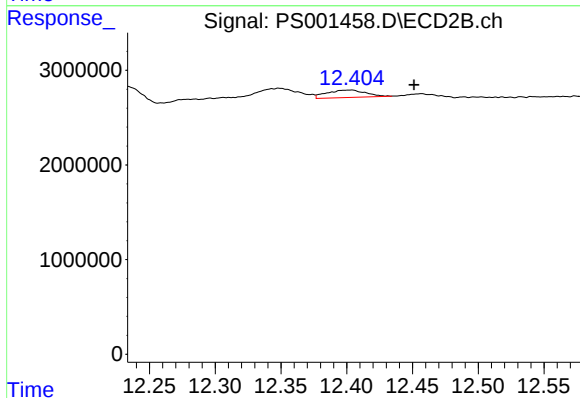


#8 DICHLORPROP

R.T.: 12.404 min
Delta R.T.: -0.048 min
Response: 1591884
Conc: 8.99 ng/ml

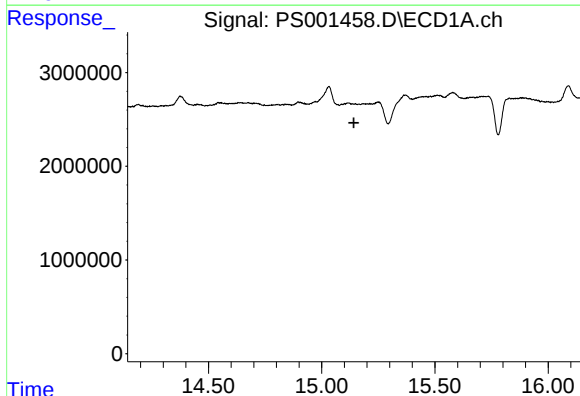


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 15.142 min
Response: 0
Conc: N.D.

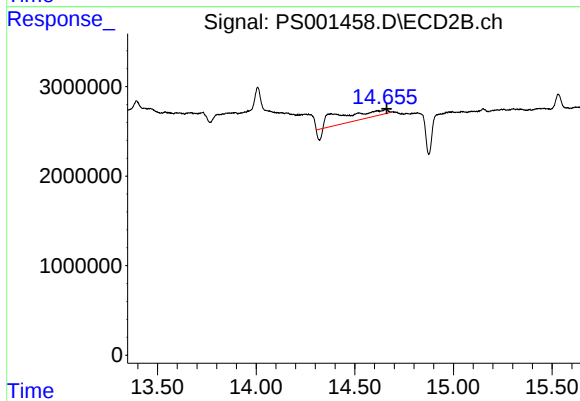

#12 2,4,5-T


R.T.: 14.655 min
Delta R.T.: -0.007 min
Response: 13963673
Conc: 15.12 ng/ml

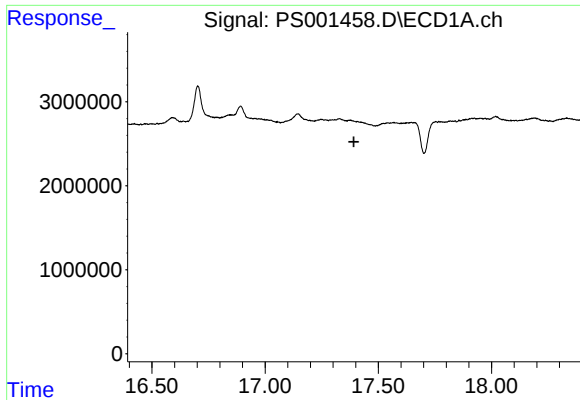

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 17.392 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

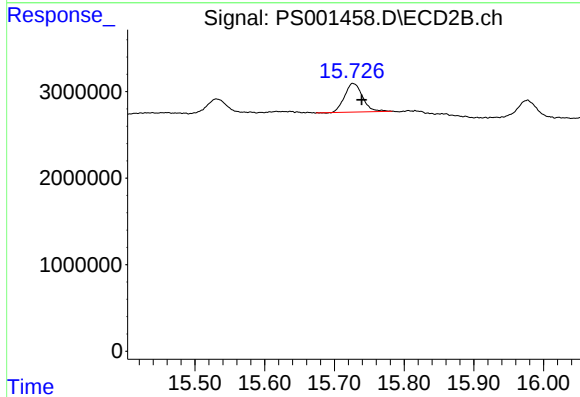


#14 DINOSEB

R.T.: 15.727 min
Delta R.T.: -0.013 min
Response: 5943473
Conc: 8.36 ng/ml

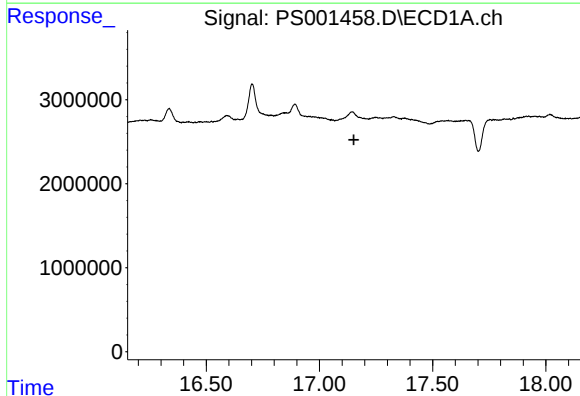


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 17.152 min
Response: 0
Conc: N.D.

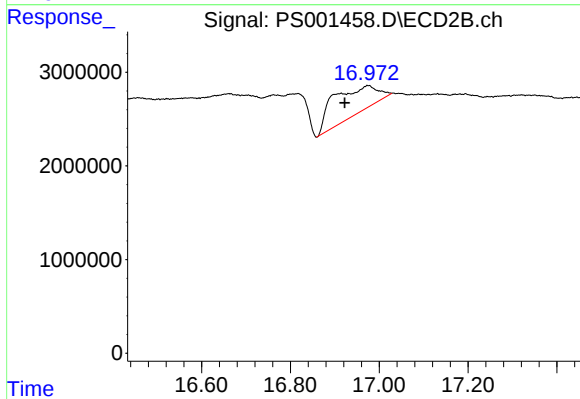

#15 Picloram


R.T.: 16.973 min
Delta R.T.: 0.051 min
Response: 20296144
Conc: 14.72 ng/ml

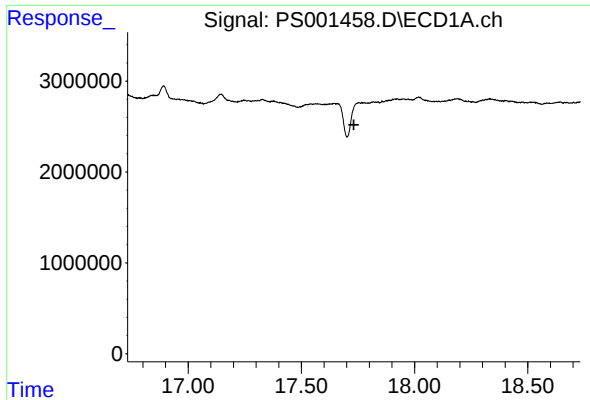

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.732 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

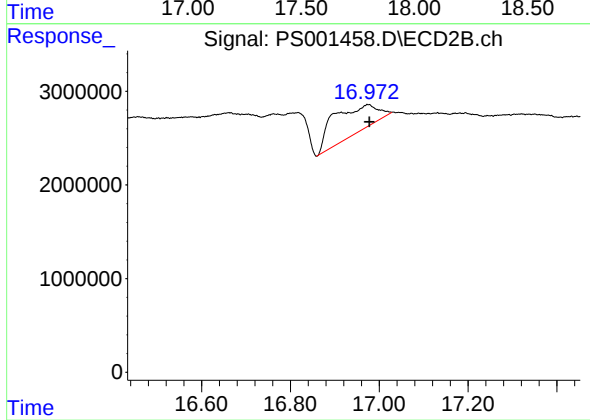

#16 DCPA

R.T.: 16.973 min
Delta R.T.: -0.005 min
Response: 20296144
Conc: 14.05 ng/ml