

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081318\
 Data File : PS001468.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2018 23:02
 Operator : UA
 Sample : J4442-20
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 01:10:05 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.611	11.031	95679538	87357774	515.654	480.318
Target Compounds							
1) T	Dalapon	2.958	2.399	3599037	2245232	15.178	9.853 #
2) T	3,5-DICHL...	0.000	9.118	0	2059503	N.D.	8.084 #
5) T	DICAMBA	11.988	11.274	3720738	5874085	5.175	8.571 #
6) T	MCP	12.303	0.000	9706637	0	19.313	N.D. #
9) T	2,4-D	0.000	12.867	0	3042001	N.D.	12.820 #
15) T	Picloram	0.000	16.969	0	1415375	N.D.	1.027 #
16) T	DCPA	0.000	16.969	0	1415375	N.D.	0.980 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081318\
Data File : PS001468.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2018 23:02
Operator : UA
Sample : J4442-20
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 01:10:05 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

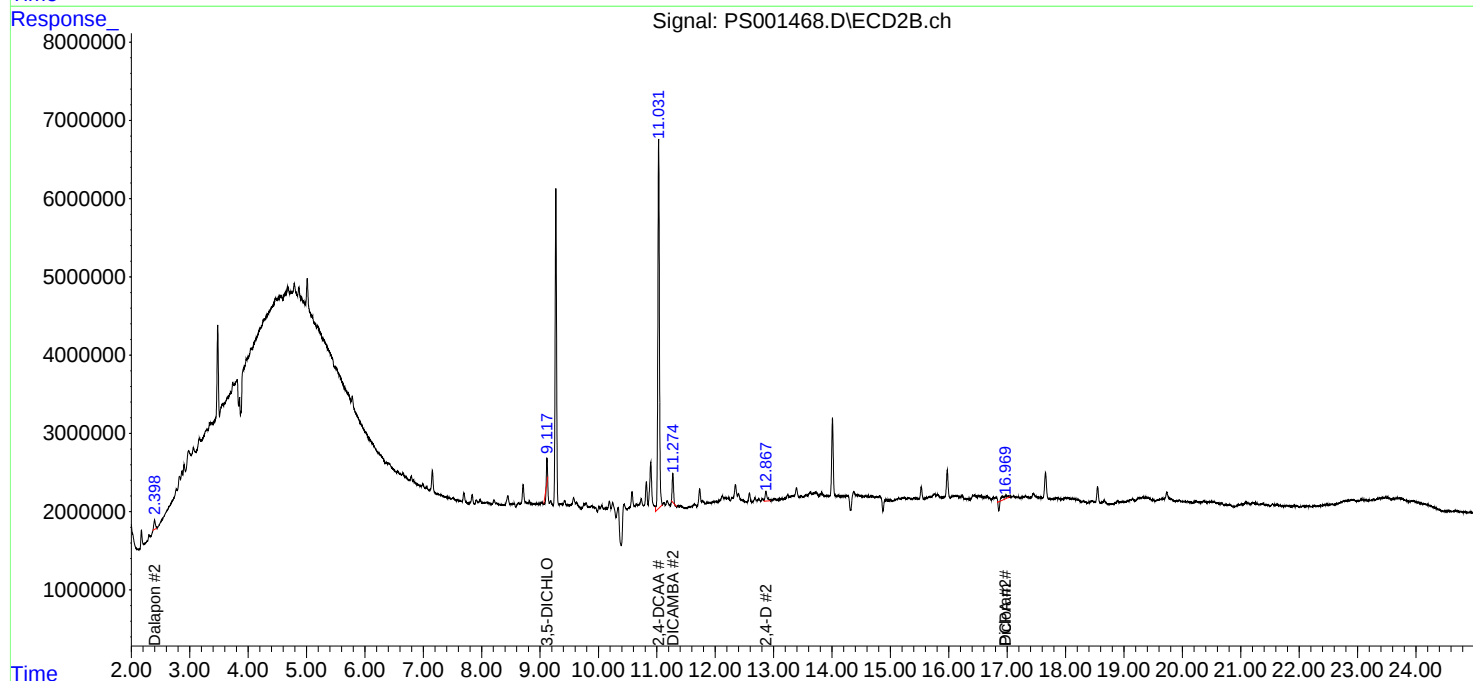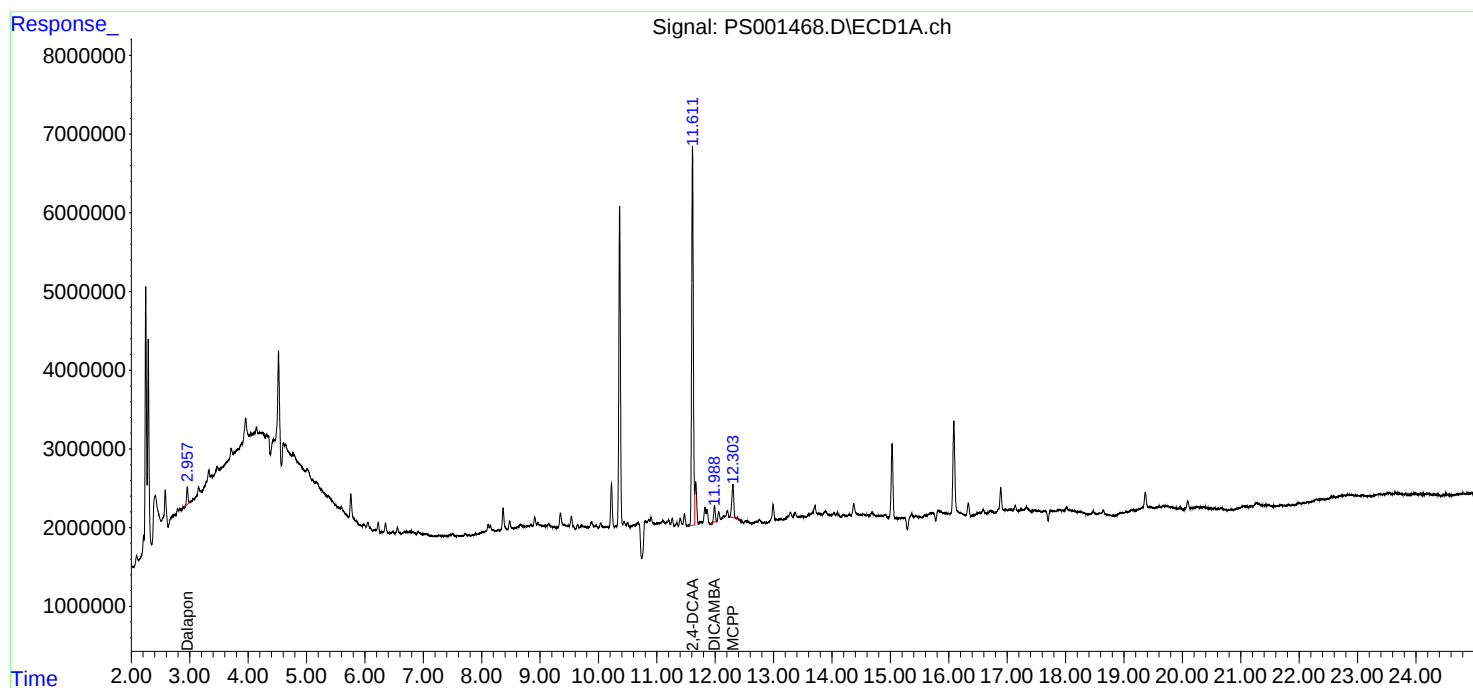


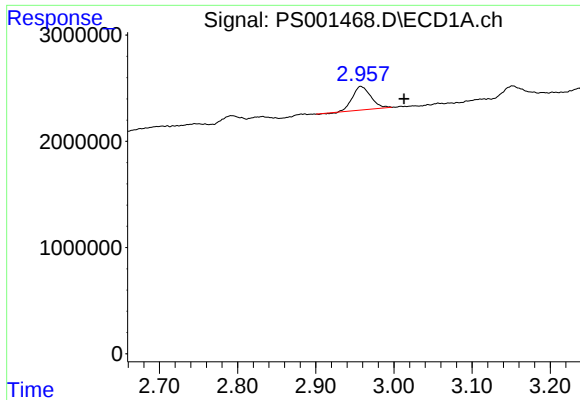

#1 Dalapon


R.T.: 2.958 min
Delta R.T.: -0.055 min
Response: 3599037
Conc: 15.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

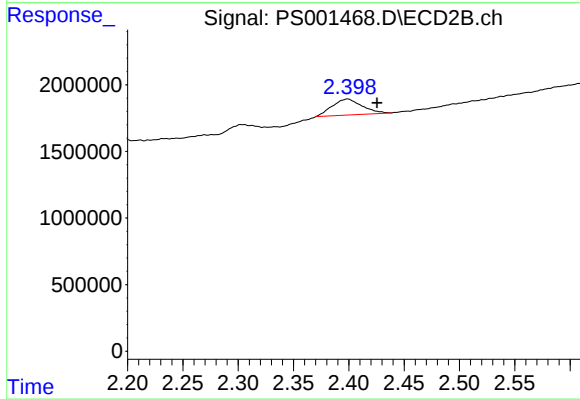


#1 Dalapon

R.T.: 2.399 min
Delta R.T.: -0.027 min
Response: 2245232
Conc: 9.85 ng/ml

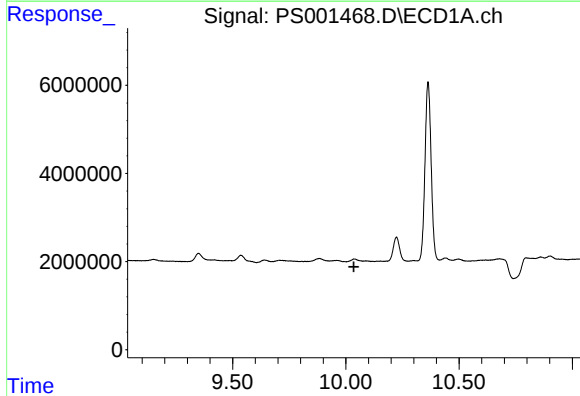


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.035 min
Response: 0
Conc: N.D.

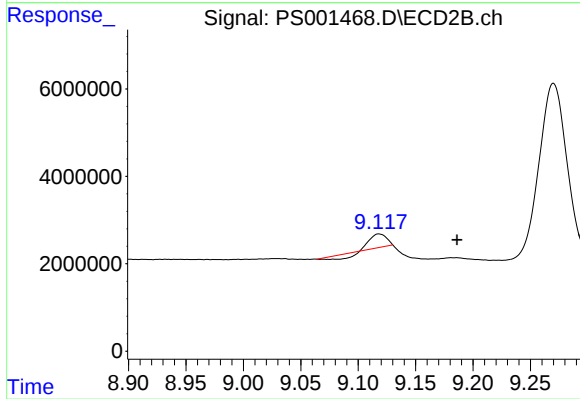

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.118 min
Delta R.T.: -0.068 min
Response: 2059503
Conc: 8.08 ng/ml

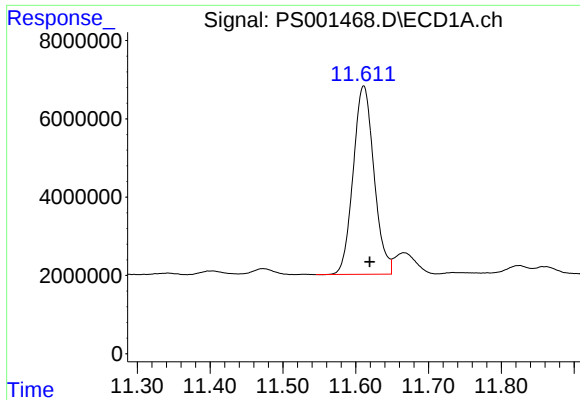

#4 2,4-DCAA


R.T.: 11.611 min
Delta R.T.: -0.008 min
Response: 95679538
Conc: 515.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

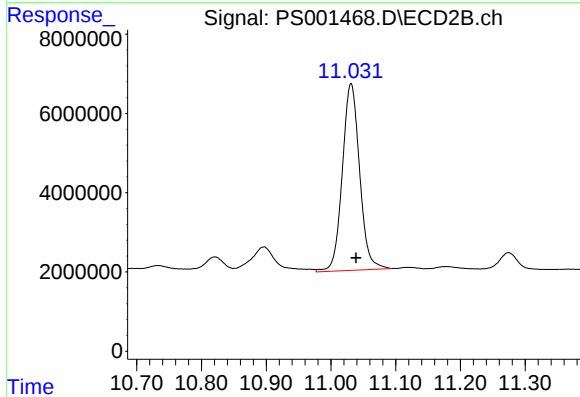


#4 2,4-DCAA

R.T.: 11.031 min
Delta R.T.: -0.008 min
Response: 87357774
Conc: 480.32 ng/ml

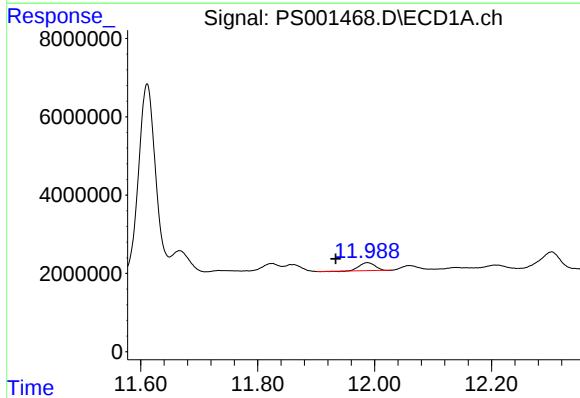


#5 DICAMBA

R.T.: 11.988 min
Delta R.T.: 0.054 min
Response: 3720738
Conc: 5.18 ng/ml

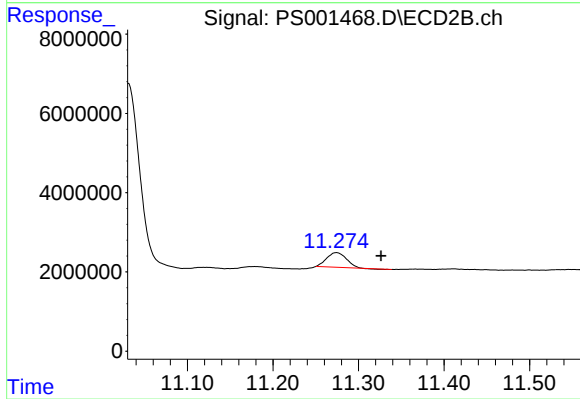

#5 DICAMBA


R.T.: 11.274 min
Delta R.T.: -0.052 min
Response: 5874085
Conc: 8.57 ng/ml

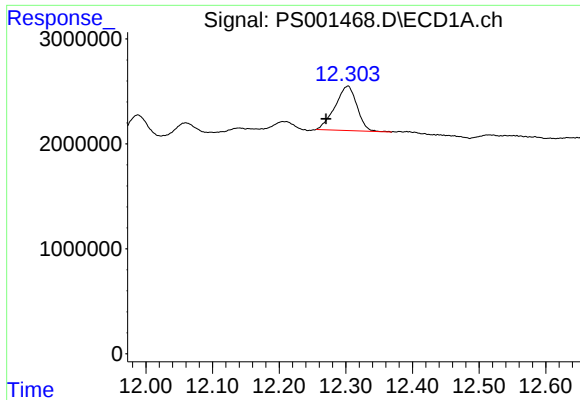

#6 MCP


R.T.: 12.303 min
Delta R.T.: 0.033 min
Response: 9706637
Conc: 19.31 ug/ml

Instrument :
ECD_S
ClientSampleId :

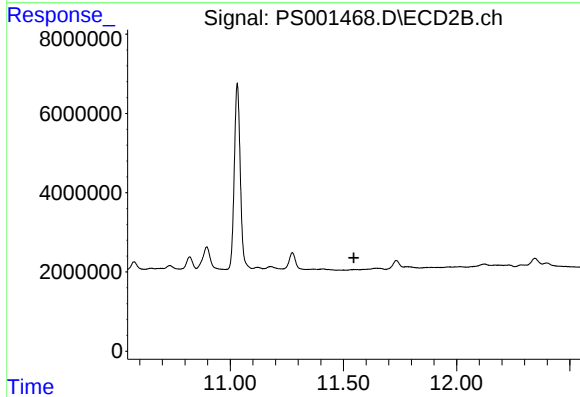


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.546 min
Response: 0
Conc: N.D.

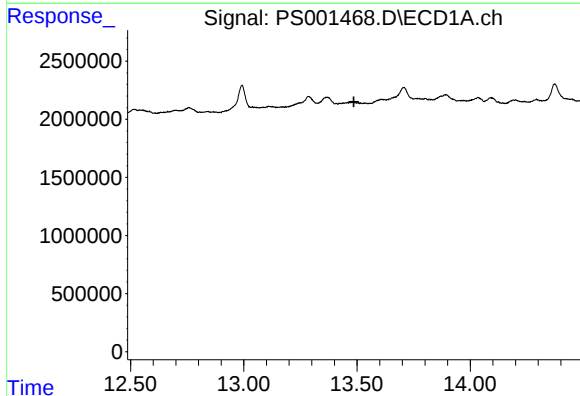


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.486 min
Response: 0
Conc: N.D.

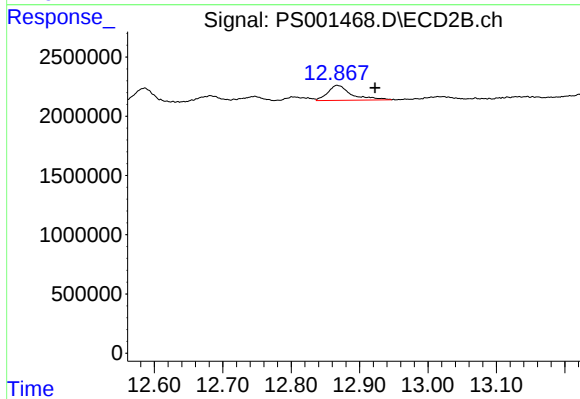

#9 2,4-D


R.T.: 12.867 min
Delta R.T.: -0.056 min
Response: 3042001
Conc: 12.82 ng/ml

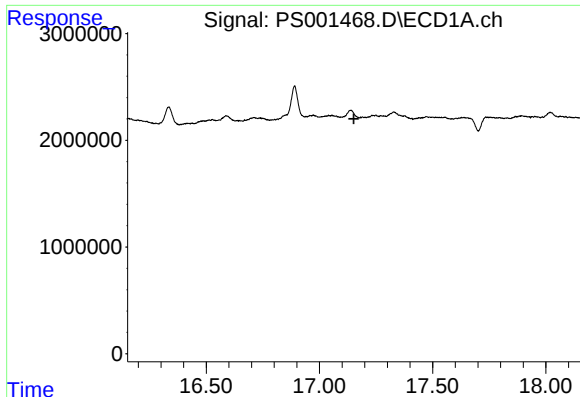

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 17.152 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

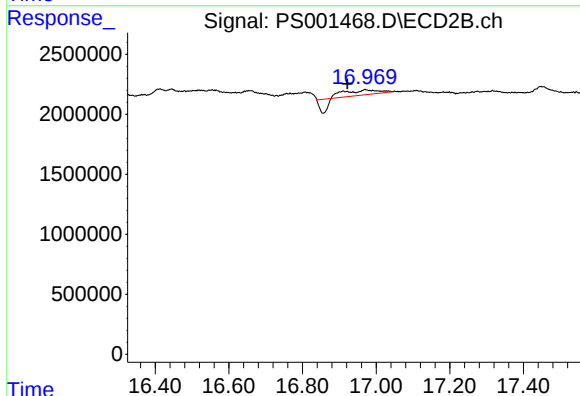


#15 Picloram

R.T.: 16.969 min
Delta R.T.: 0.047 min
Response: 1415375
Conc: 1.03 ng/ml

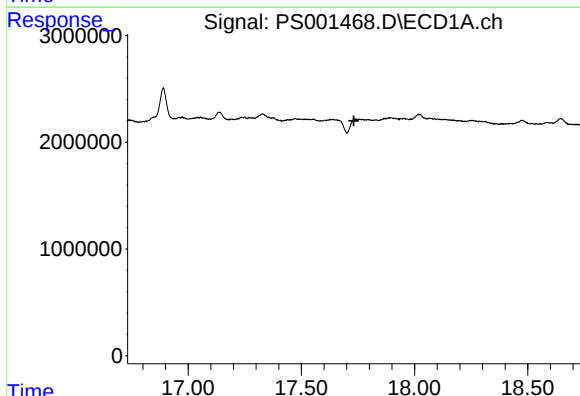

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.732 min
Response: 0
Conc: N.D.

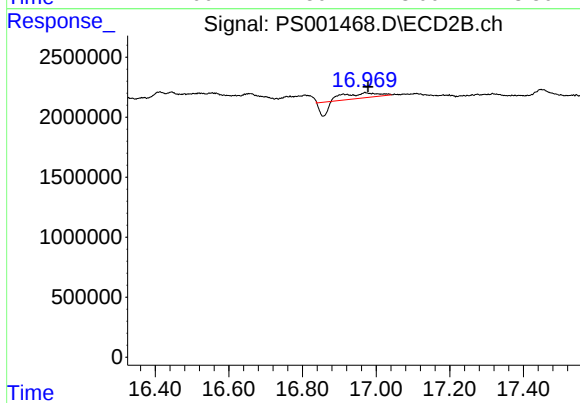

#16 DCPA

R.T.: 16.969 min
Delta R.T.: -0.008 min
Response: 1415375
Conc: 0.98 ng/ml