

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081318\
 Data File : PS001470.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2018 00:04
 Operator : UA
 Sample : J4442-40
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 01:10:46 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.646	11.068	92954031	83421147	500.965	458.673
Target Compounds							
1) T	Dalapon	2.994	2.434	4131514	3056634	17.423	13.414
2) T	3,5-DICHL...	0.000	9.156	0	9190886	N.D.	36.078 #
5) T	DICAMBA	0.000	11.312	0	8180777	N.D.	11.936 #
6) T	MCP	12.340	0.000	7741896	0	15.403	N.D. #
8) T	DICHLORPROP	0.000	12.433	0	2001820	N.D.	11.300 #
9) T	2,4-D	0.000	12.905	0	2168930	N.D.	9.140 #
10) T	Pentachlo...	13.902	13.428	1891597	-137558	0.672	N.D. #
11) T	2,4,5-TP ...	0.000	14.045	0	517696	N.D.	0.473 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081318\
Data File : PS001470.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2018 00:04
Operator : UA
Sample : J4442-40
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 01:10:46 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

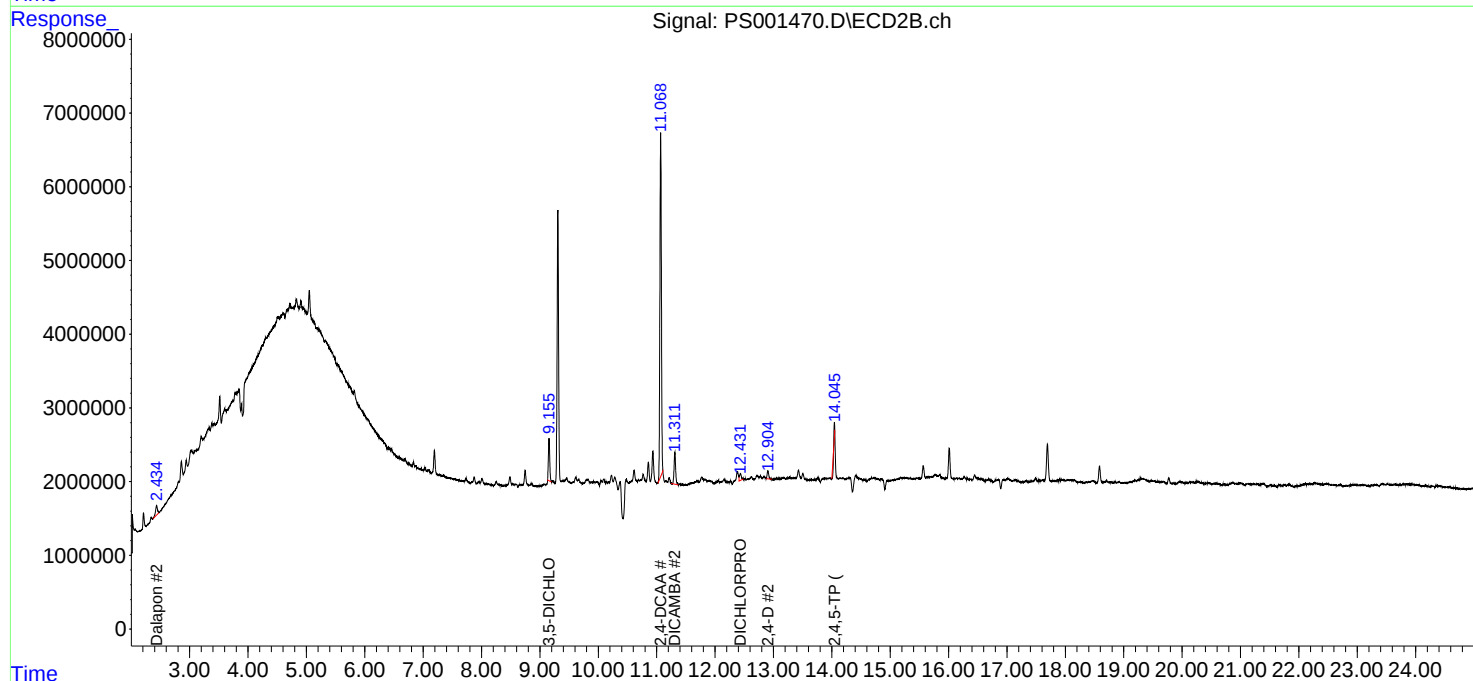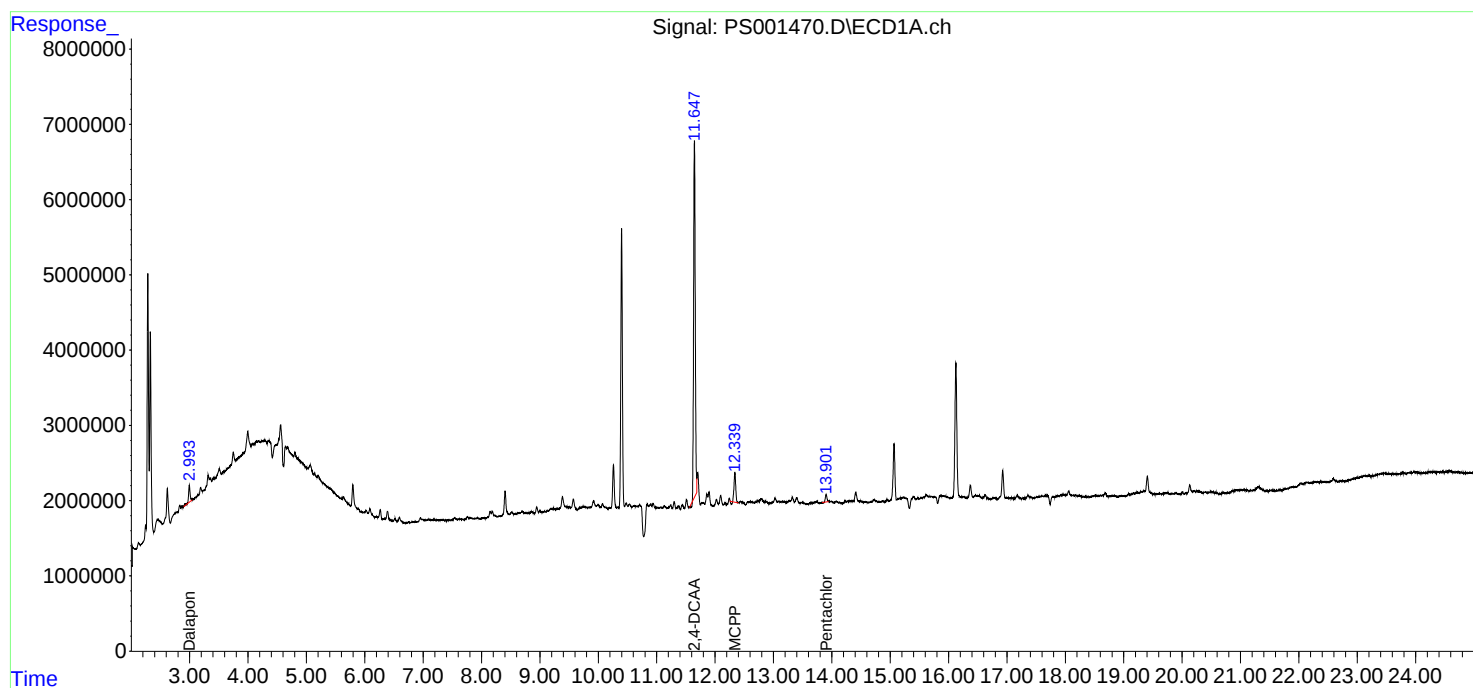


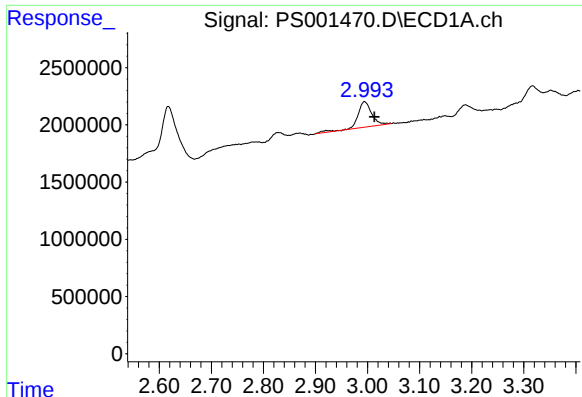

#1 Dalapon


R.T.: 2.994 min
Delta R.T.: -0.019 min
Response: 4131514
Conc: 17.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

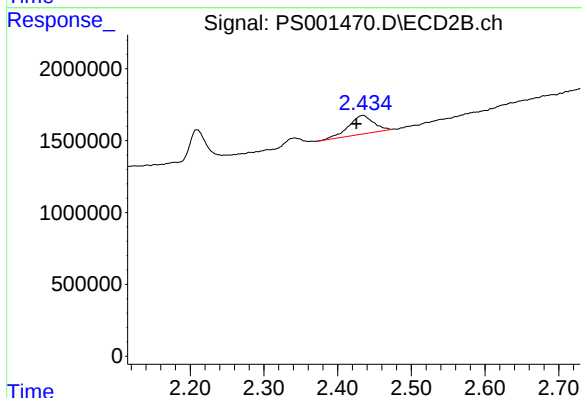


#1 Dalapon

R.T.: 2.434 min
Delta R.T.: 0.009 min
Response: 3056634
Conc: 13.41 ng/ml

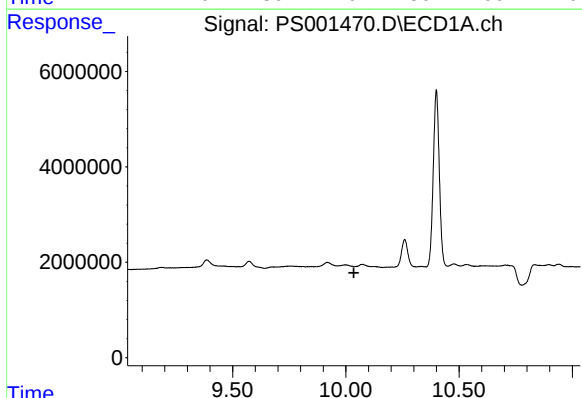


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.035 min
Response: 0
Conc: N.D.

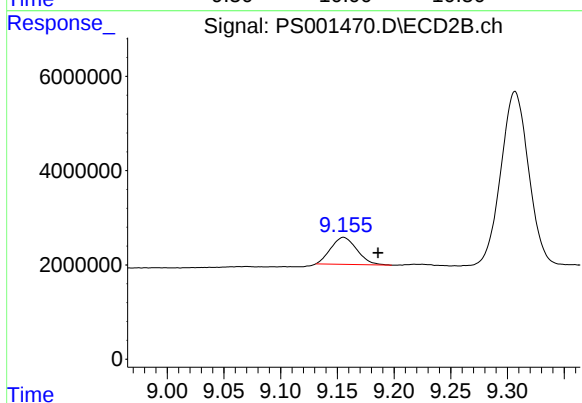

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.156 min
Delta R.T.: -0.030 min
Response: 9190886
Conc: 36.08 ng/ml

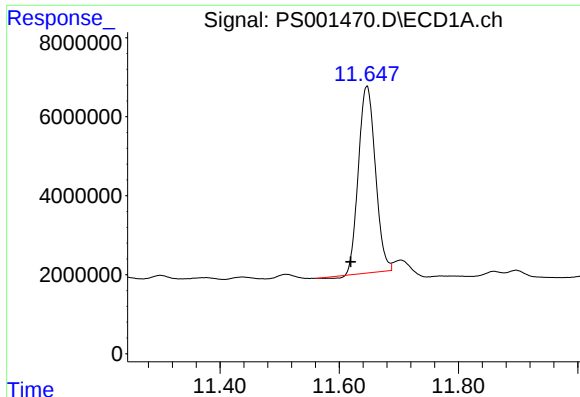

#4 2,4-DCAA


R.T.: 11.646 min
Delta R.T.: 0.027 min
Response: 92954031
Conc: 500.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

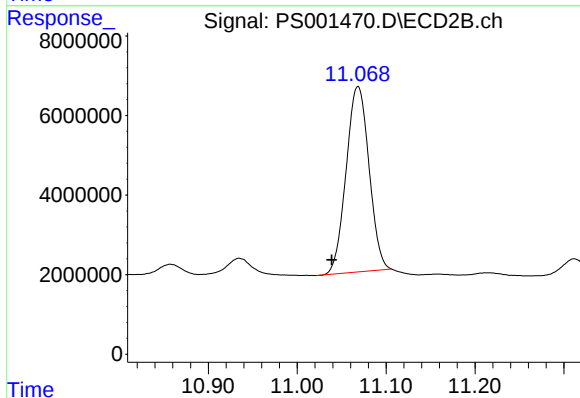


#4 2,4-DCAA

R.T.: 11.068 min
Delta R.T.: 0.030 min
Response: 83421147
Conc: 458.67 ng/ml

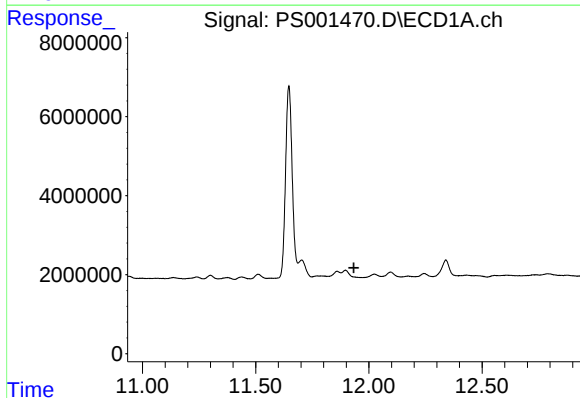


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.934 min
Response: 0
Conc: N.D.

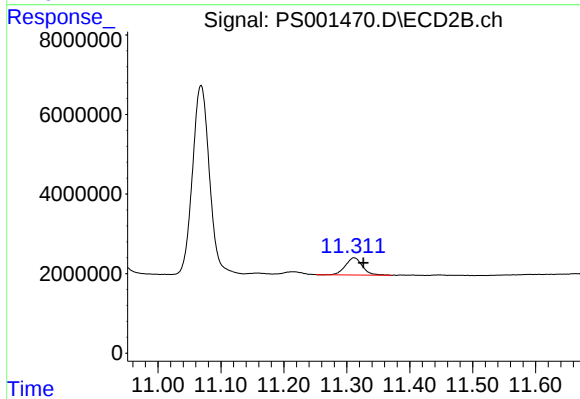

#5 DICAMBA


R.T.: 11.312 min
Delta R.T.: -0.015 min
Response: 8180777
Conc: 11.94 ng/ml

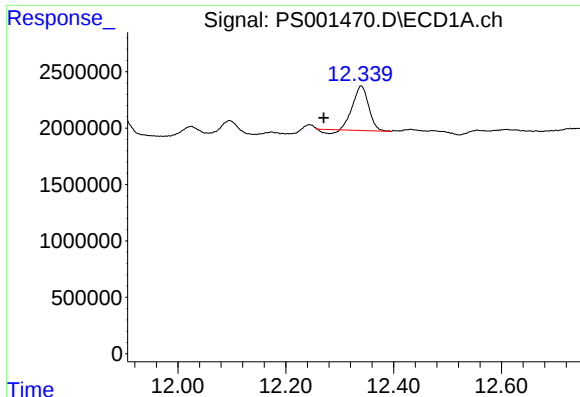

#6 MCP


R.T.: 12.340 min
Delta R.T.: 0.069 min
Response: 7741896
Conc: 15.40 ug/ml

Instrument :
ECD_S
ClientSampleId :

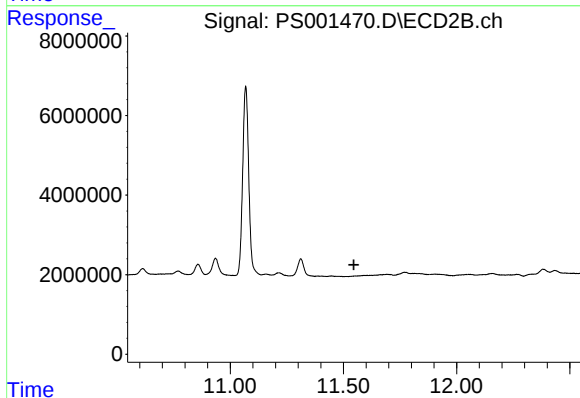


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.546 min
Response: 0
Conc: N.D.

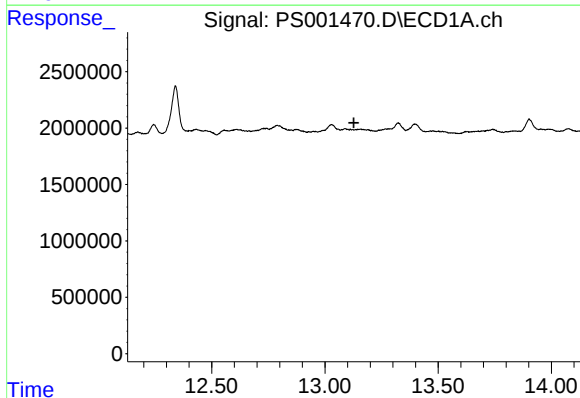


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.128 min
Response: 0
Conc: N.D.

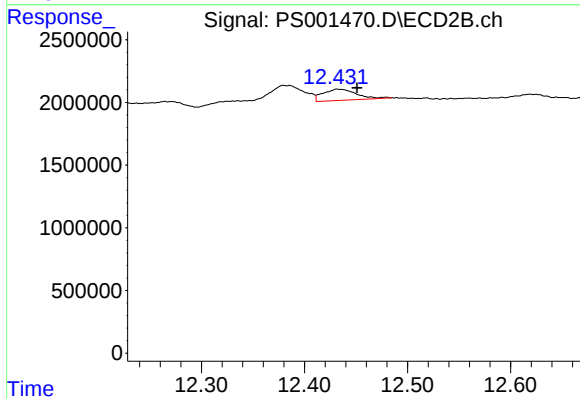

#8 DICHLORPROP


R.T.: 12.433 min
Delta R.T.: -0.018 min
Response: 2001820
Conc: 11.30 ng/ml

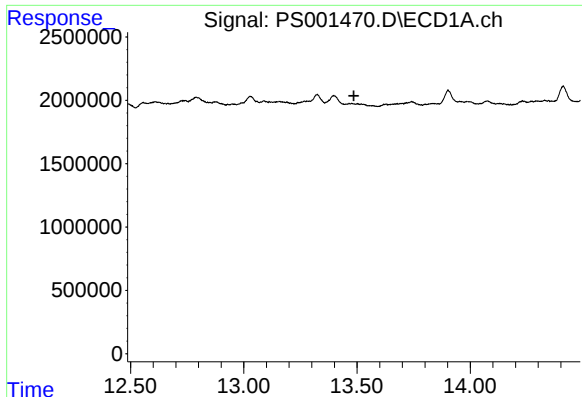

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.486 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

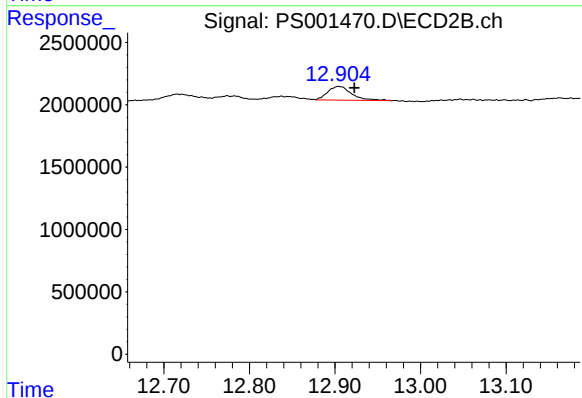


#9 2,4-D

R.T.: 12.905 min
Delta R.T.: -0.018 min
Response: 2168930
Conc: 9.14 ng/ml

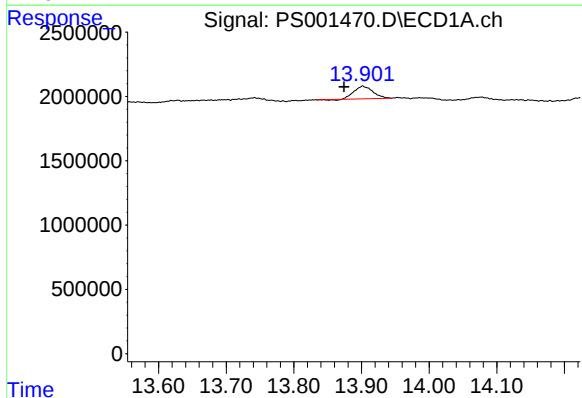


#10 Pentachlorophenol

R.T.: 13.902 min
Delta R.T.: 0.028 min
Response: 1891597
Conc: 0.67 ng/ml

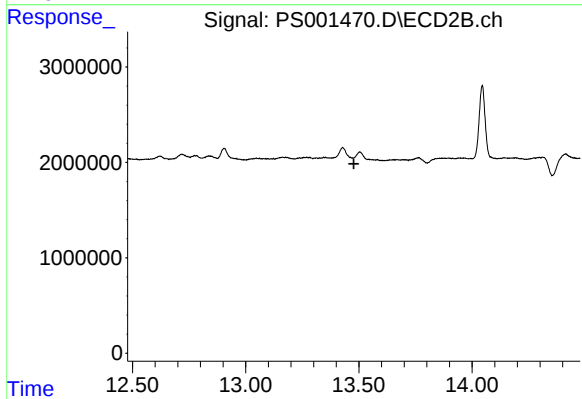

#10 Pentachlorophenol


R.T.: 13.428 min
Delta R.T.: -0.050 min
Response: -137558
Conc: N.D.

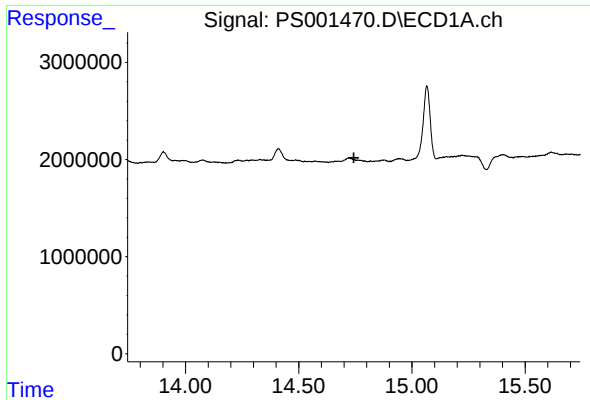

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.743 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

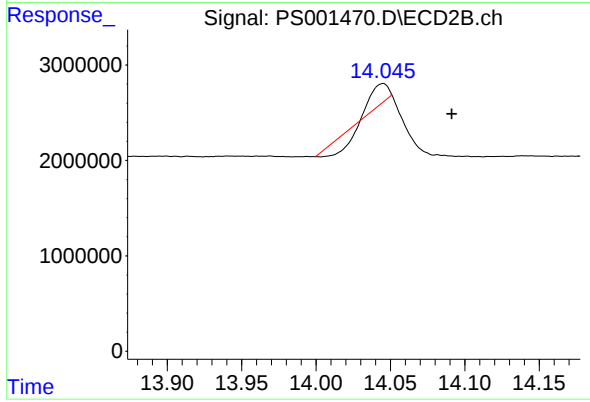

#11 2,4,5-TP (SILVEX)

R.T.: 14.045 min
Delta R.T.: -0.047 min
Response: 517696
Conc: 0.47 ng/ml