

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081318\
 Data File : PS001476.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2018 03:10
 Operator : UA
 Sample : J4447-15
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 05:11:23 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.627	11.046	106.6E6	87879193	574.367	483.185
Target Compounds							
1) T	Dalapon	2.974	2.412	4354964	3368937	18.366	14.784
5) T	DICAMBA	0.000	11.290	0	5207220	N.D.	7.598 #
6) T	MCPD	12.319	0.000	6424040	0	12.781	N.D. #
11) T	2,4,5-TP ...	0.000	14.024	0	13617917	N.D.	12.454 #
15) T	Picloram	0.000	16.985	0	12845530	N.D.	9.318 #
16) T	DCPA	0.000	16.985	0	12845530	N.D.	8.894 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081318\
Data File : PS001476.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2018 03:10
Operator : UA
Sample : J4447-15
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 05:11:23 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

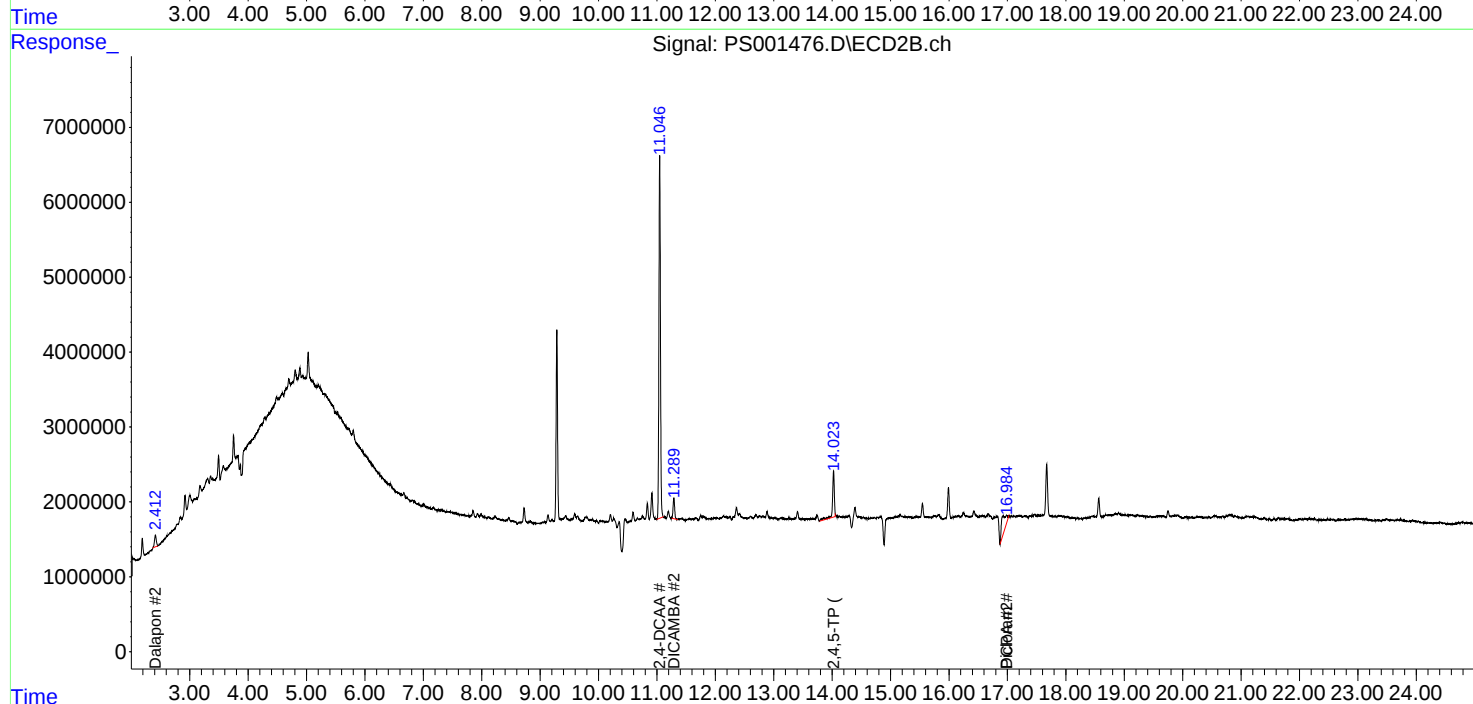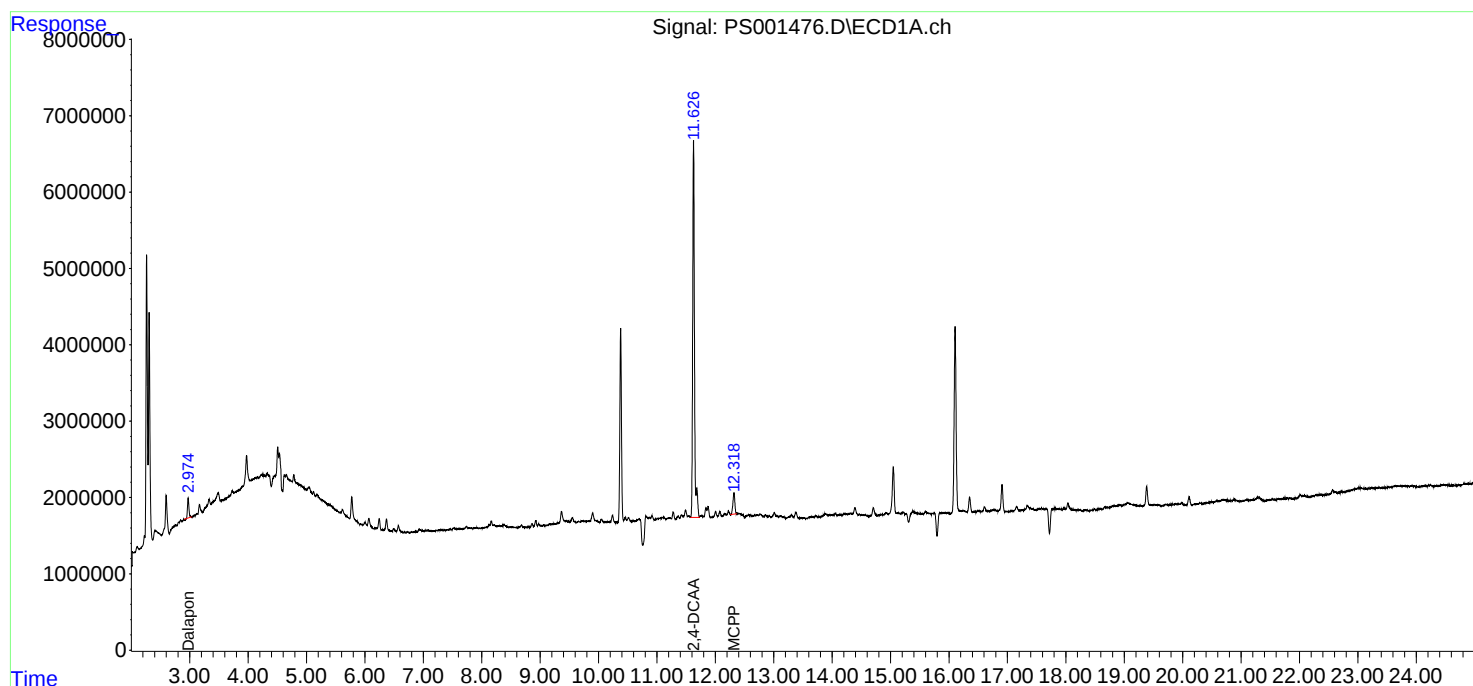


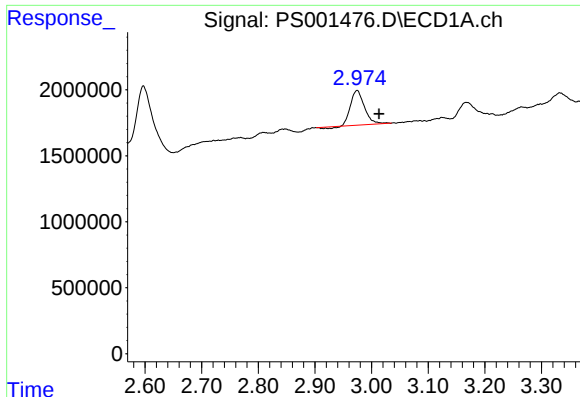

#1 Dalapon


R.T.: 2.974 min
Delta R.T.: -0.039 min
Response: 4354964
Conc: 18.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

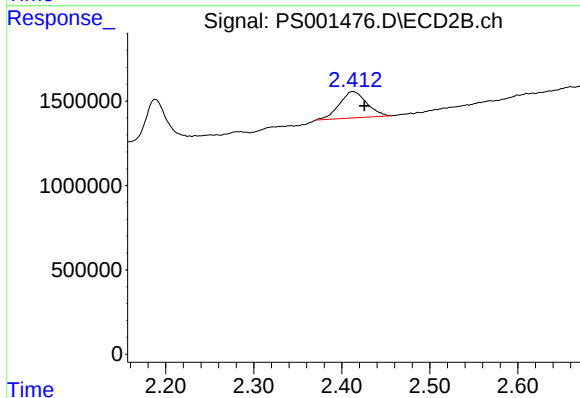


#1 Dalapon

R.T.: 2.412 min
Delta R.T.: -0.013 min
Response: 3368937
Conc: 14.78 ng/ml

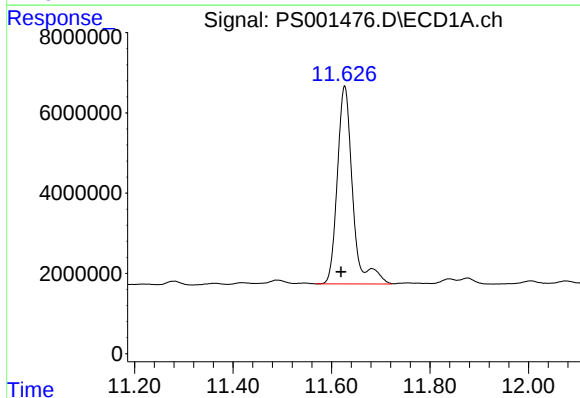


#4 2,4-DCAA

R.T.: 11.627 min
Delta R.T.: 0.007 min
Response: 106573691
Conc: 574.37 ng/ml

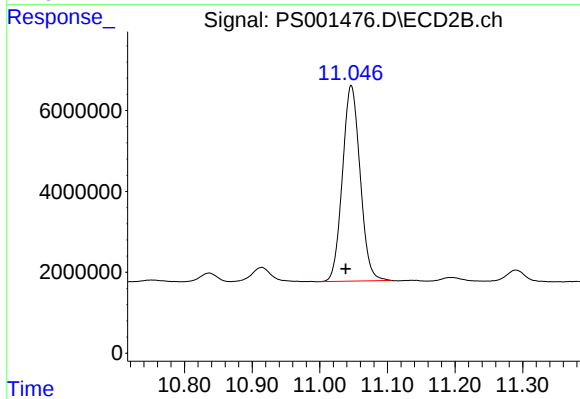

#4 2,4-DCAA


R.T.: 11.046 min
Delta R.T.: 0.008 min
Response: 87879193
Conc: 483.18 ng/ml

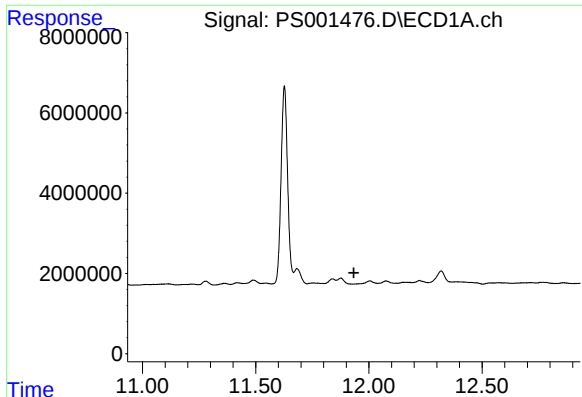

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.934 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

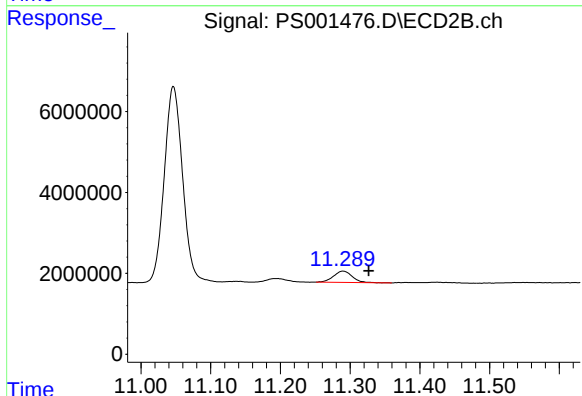


#5 DICAMBA

R.T.: 11.290 min
Delta R.T.: -0.037 min
Response: 5207220
Conc: 7.60 ng/ml

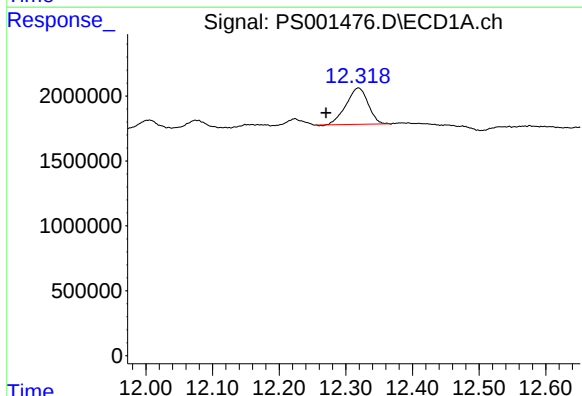


#6 MCP

R.T.: 12.319 min
Delta R.T.: 0.048 min
Response: 6424040
Conc: 12.78 ug/ml

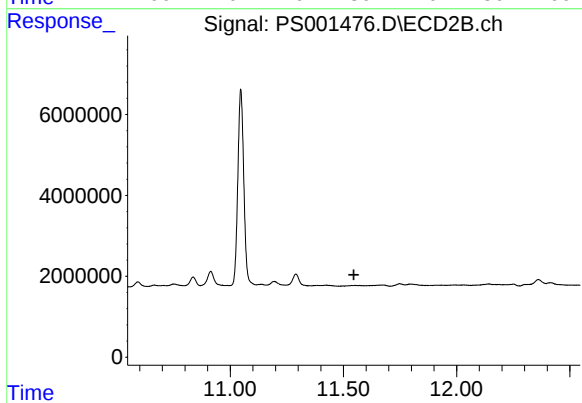

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.546 min
Response: 0
Conc: N.D.

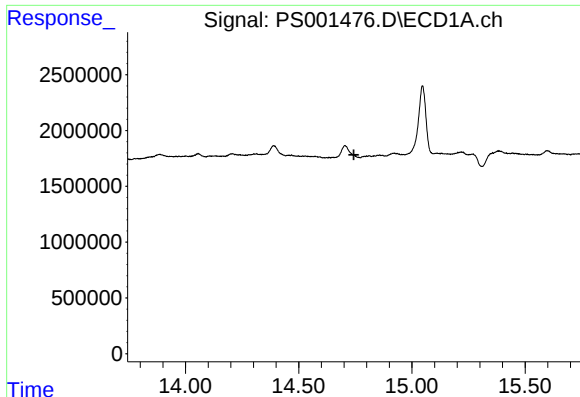

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.743 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

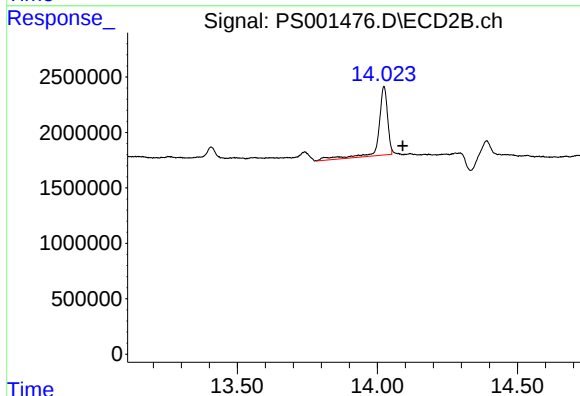


#11 2,4,5-TP (SILVEX)

R.T.: 14.024 min
Delta R.T.: -0.068 min
Response: 13617917
Conc: 12.45 ng/ml

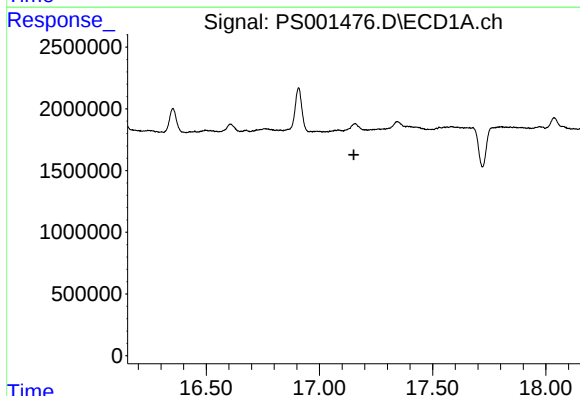


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 17.152 min
Response: 0
Conc: N.D.

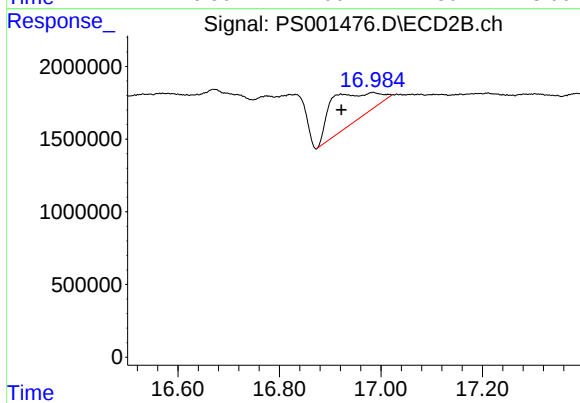

#15 Picloram


R.T.: 16.985 min
Delta R.T.: 0.063 min
Response: 12845530
Conc: 9.32 ng/ml

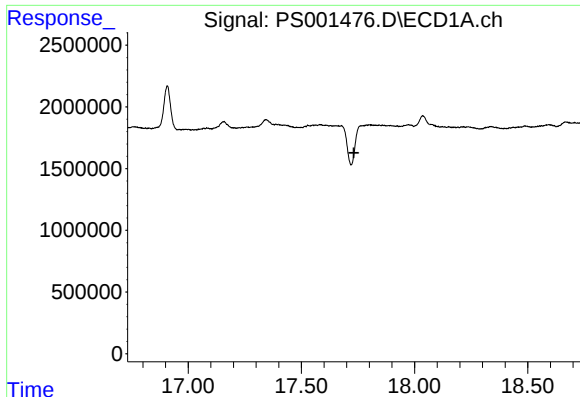

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.732 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

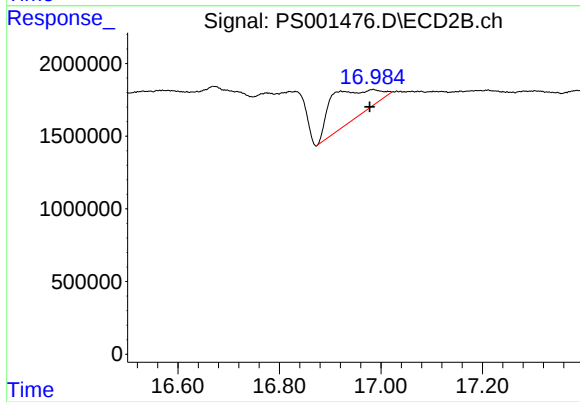

#16 DCPA

R.T.: 16.985 min
Delta R.T.: 0.007 min
Response: 12845530
Conc: 8.89 ng/ml