

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081320\
 Data File : PS011764.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2020 22:25
 Operator : DD\AJ
 Sample : L3508-16
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 02:31:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.915	315.1E6	182.9E6	288.833	342.035
Target Compounds							
1) T	Dalapon	2.993	2.586	38461739	55087996	30.877	72.882 #
2) T	3,5-DICHL...	0.000	6.096	0	57183208	N.D.	69.514
3) T	4-Nitroph...	6.991	0.000	1682409	0	2.856	N.D. #
5) T	DICAMBA	7.397	7.049	7542268	11682006	1.841	5.407 #
6) T	MCPD	7.571	0.000	13103920	0	4.101	N.D. #
7) T	MCPA	7.684	7.396	308.2E6	9491671	67.769	3.464 #
8) T	DICHLORPROP	0.000	7.737	0	14222913	N.D.	25.190
9) T	2,4-D	8.400	7.977	114.0E6	9329851	100.980	12.699 #
10) T	Pentachlo...	8.641	8.429	8525618	10898162	<MDL	1.604 #
11) T	2,4,5-TP ...	0.000	8.788	0	16210620	N.D.	5.545
12) T	2,4,5-T	9.413	0.000	23357006	0	3.942	N.D. #
15) T	Picloram	10.994	0.000	13176116	0	1.686	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081320\
Data File : PS011764.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2020 22:25
Operator : DD\AJ
Sample : L3508-16
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 02:31:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

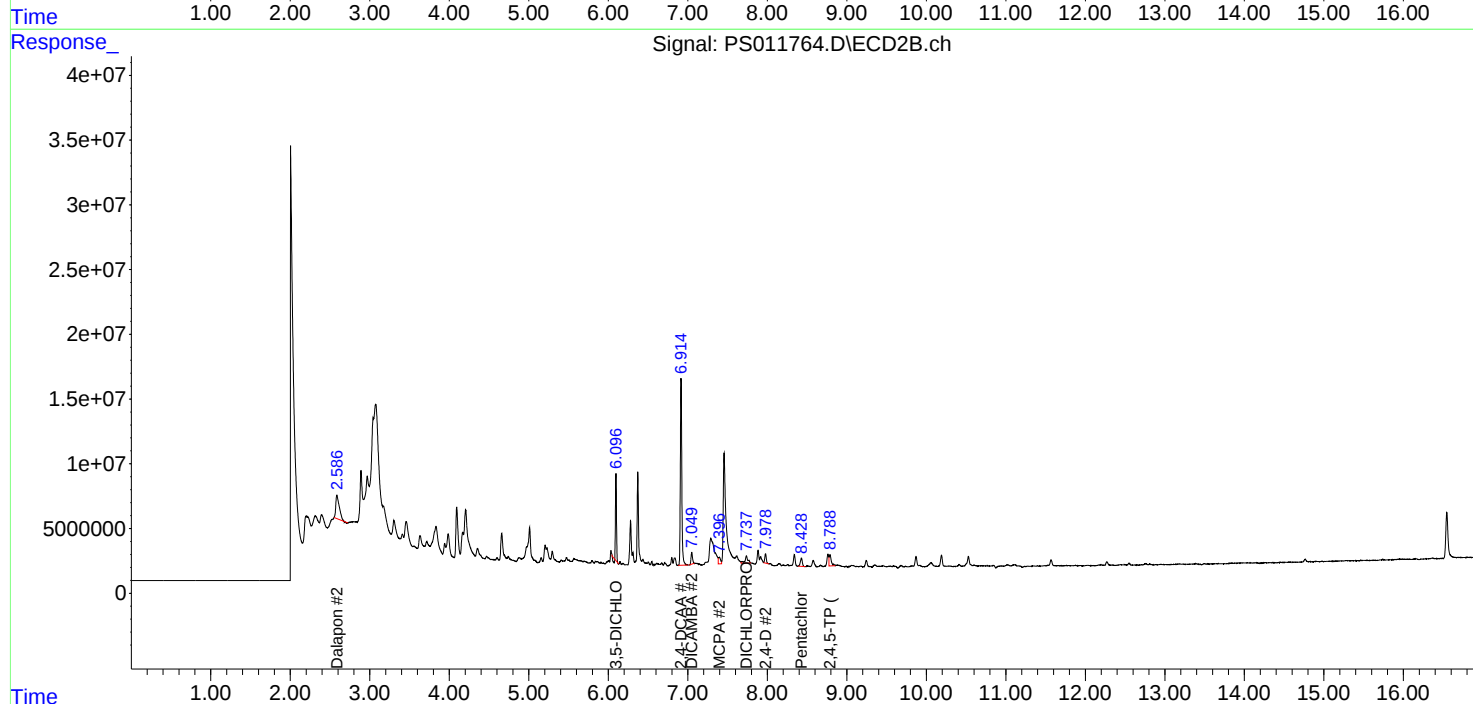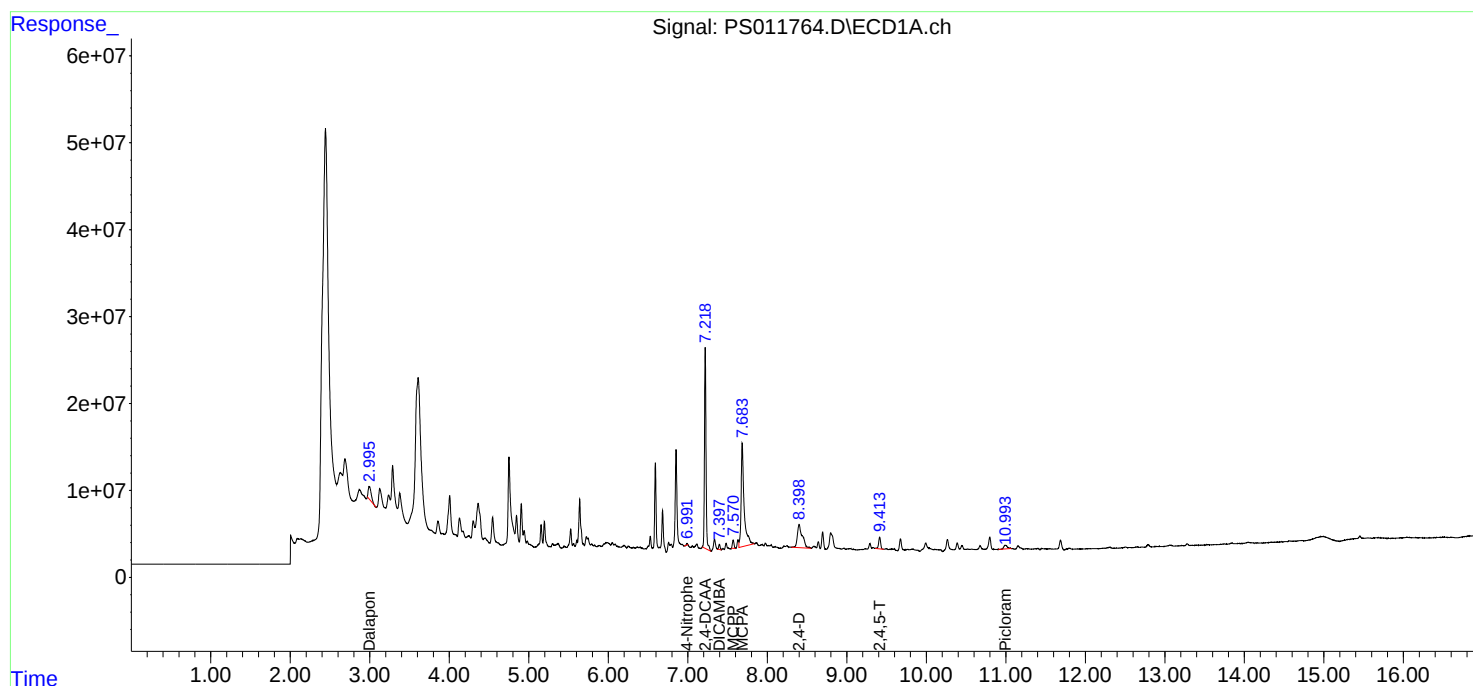


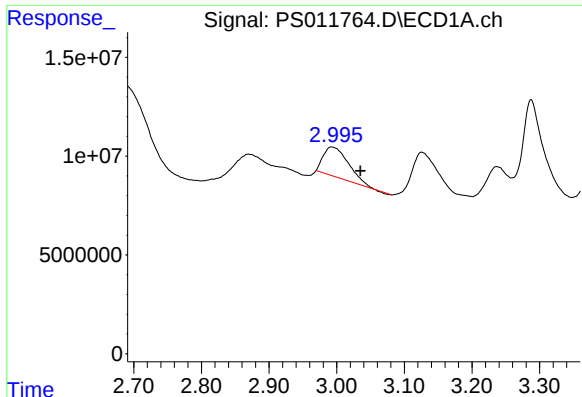

#1 Dalapon


R.T.: 2.993 min
Delta R.T.: -0.042 min
Response: 38461739
Conc: 30.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

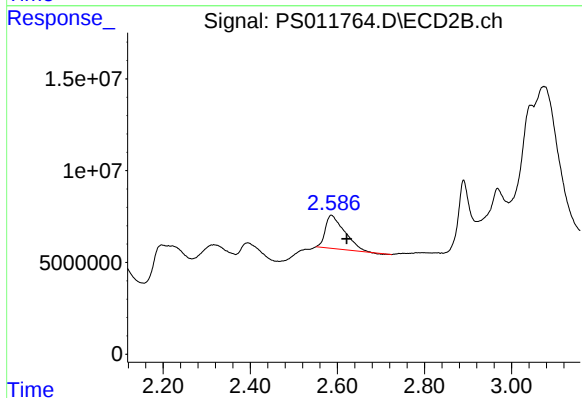


#1 Dalapon

R.T.: 2.586 min
Delta R.T.: -0.035 min
Response: 55087996
Conc: 72.88 ng/ml

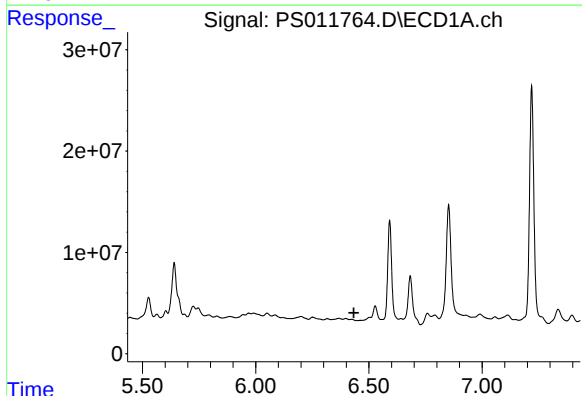


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.434 min
Response: 0
Conc: N.D.

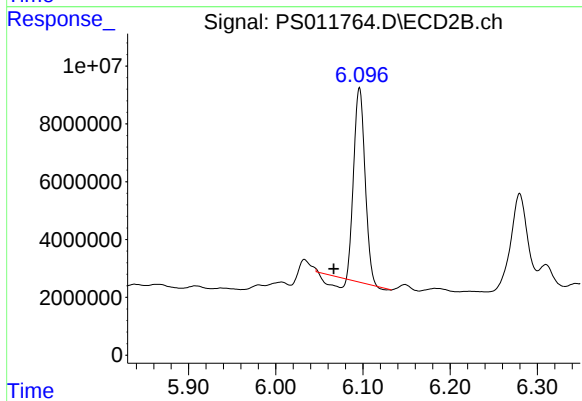

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.096 min
Delta R.T.: 0.029 min
Response: 57183208
Conc: 69.51 ng/ml

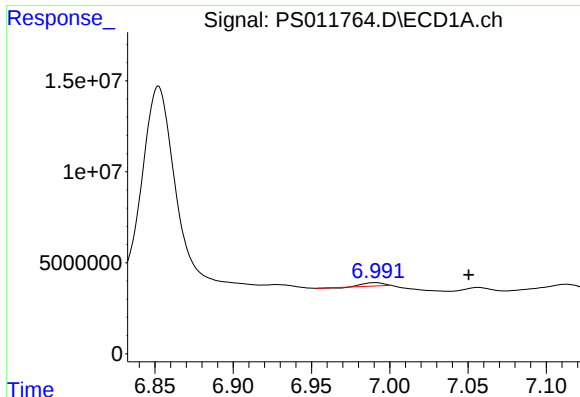

#3 4-Nitrophenol


R.T.: 6.991 min
Delta R.T.: -0.060 min
Response: 1682409
Conc: 2.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

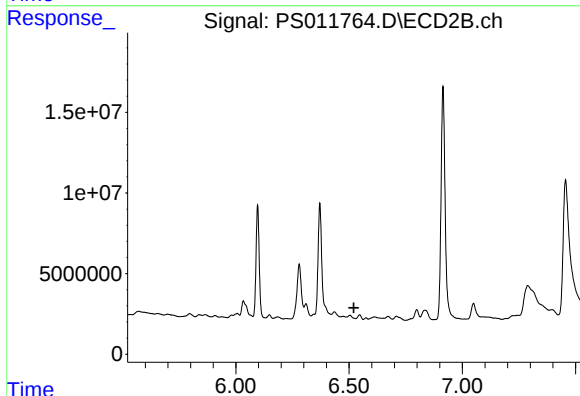


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.521 min
Response: 0
Conc: N.D.

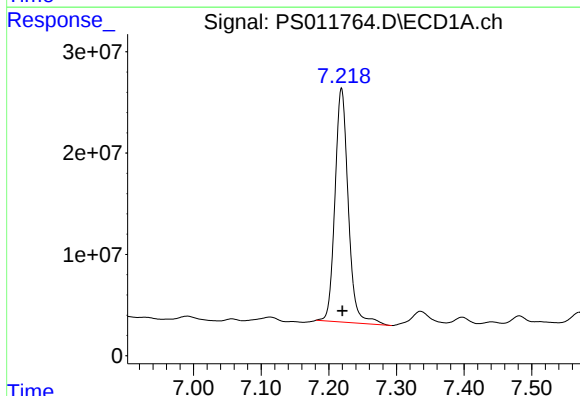


#4 2,4-DCAA

R.T.: 7.219 min
Delta R.T.: -0.001 min
Response: 315050236
Conc: 288.83 ng/ml

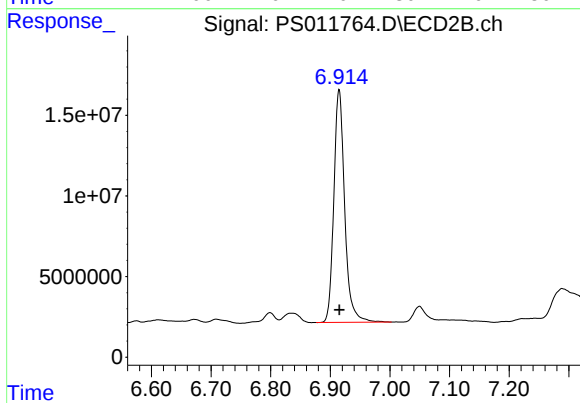

#4 2,4-DCAA


R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 182915692
Conc: 342.03 ng/ml

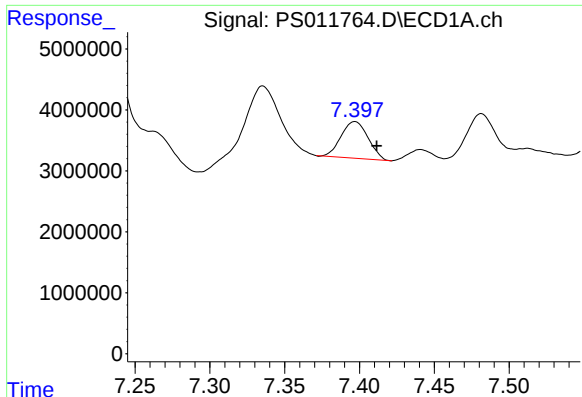

#5 DICAMBA


R.T.: 7.397 min
Delta R.T.: -0.015 min
Response: 7542268
Conc: 1.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

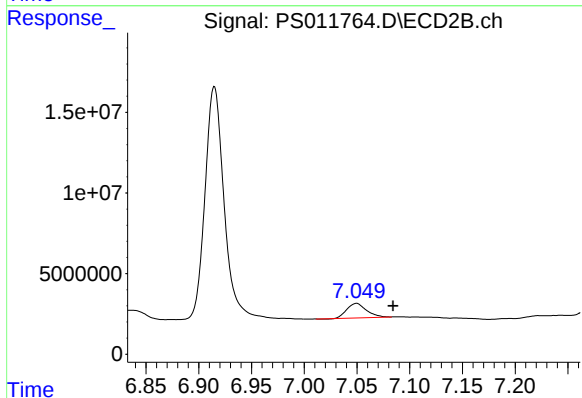


#5 DICAMBA

R.T.: 7.049 min
Delta R.T.: -0.035 min
Response: 11682006
Conc: 5.41 ng/ml

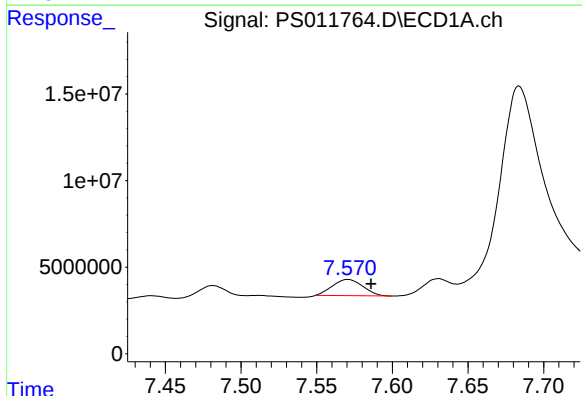


#6 MCP

R.T.: 7.571 min
Delta R.T.: -0.015 min
Response: 13103920
Conc: 4.10 ug/ml

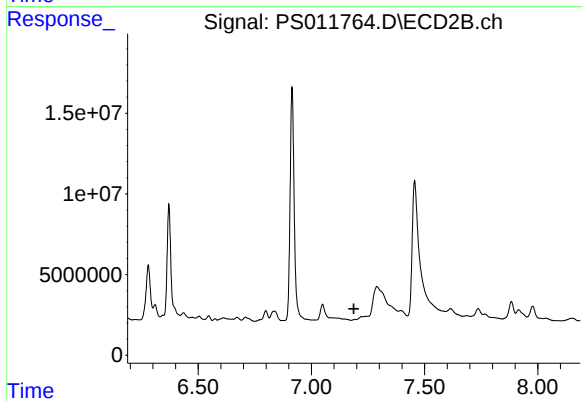

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.188 min
Response: 0
Conc: N.D.

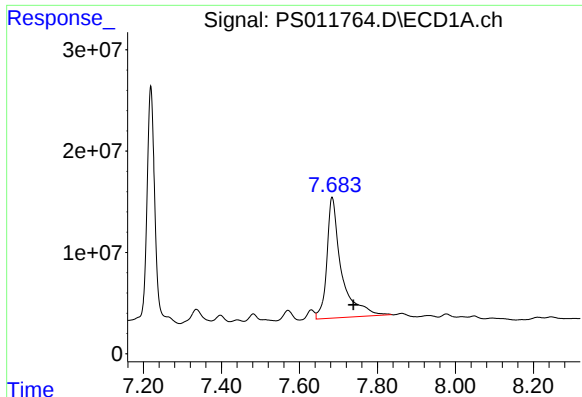

#7 MCPA


R.T.: 7.684 min
Delta R.T.: -0.054 min
Response: 308245911
Conc: 67.77 ug/ml

Instrument :
ECD_S
ClientSampleId :

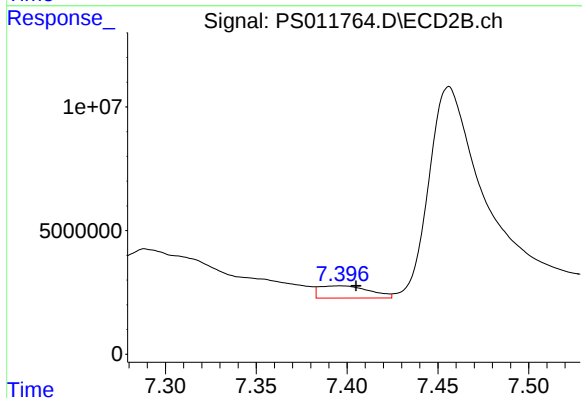


#7 MCPA

R.T.: 7.396 min
Delta R.T.: -0.009 min
Response: 9491671
Conc: 3.46 ug/ml

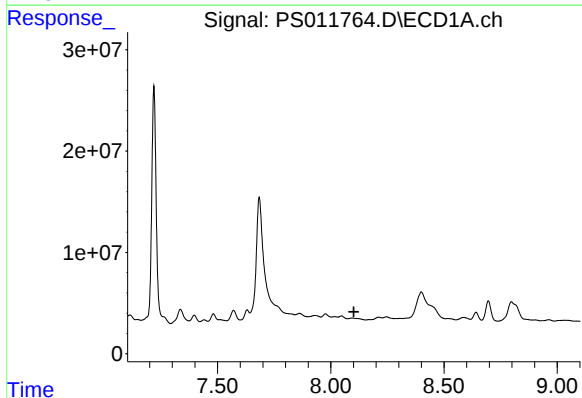


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.102 min
Response: 0
Conc: N.D.

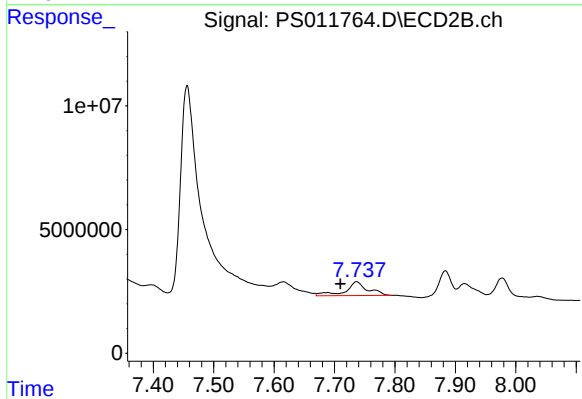

#8 DICHLORPROP


R.T.: 7.737 min
Delta R.T.: 0.027 min
Response: 14222913
Conc: 25.19 ng/ml

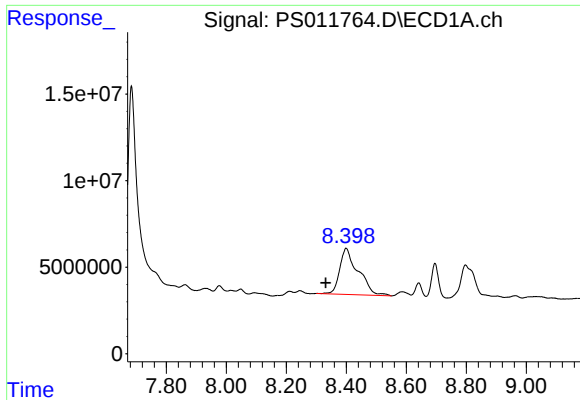

#9 2,4-D


R.T.: 8.400 min
Delta R.T.: 0.068 min
Response: 114015370
Conc: 100.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

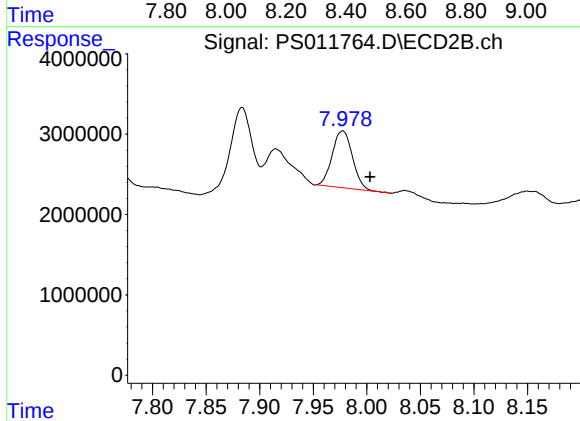


#9 2,4-D

R.T.: 7.977 min
Delta R.T.: -0.026 min
Response: 9329851
Conc: 12.70 ng/ml

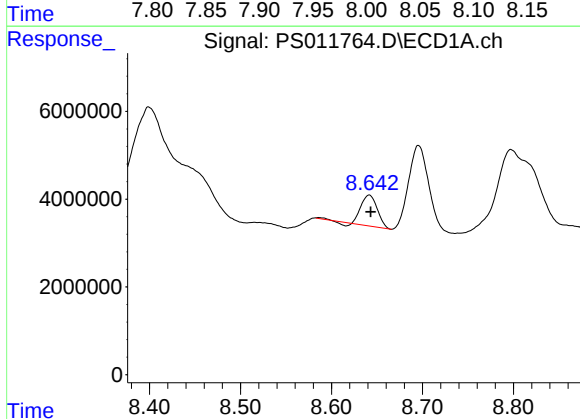


#10 Pentachlorophenol

R.T.: 8.641 min
Delta R.T.: -0.002 min
Response: 8525618
Conc: N.D.

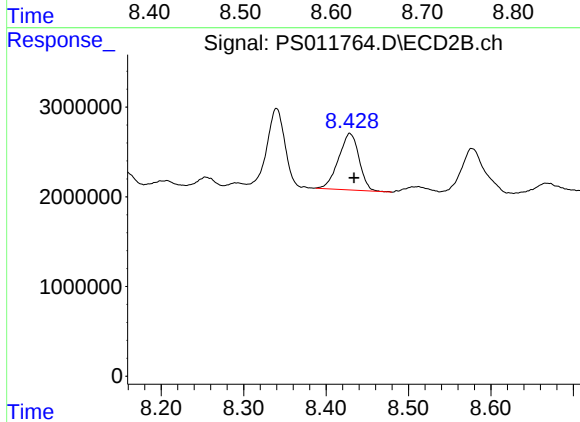

#10 Pentachlorophenol


R.T.: 8.429 min
Delta R.T.: -0.005 min
Response: 10898162
Conc: 1.60 ng/ml

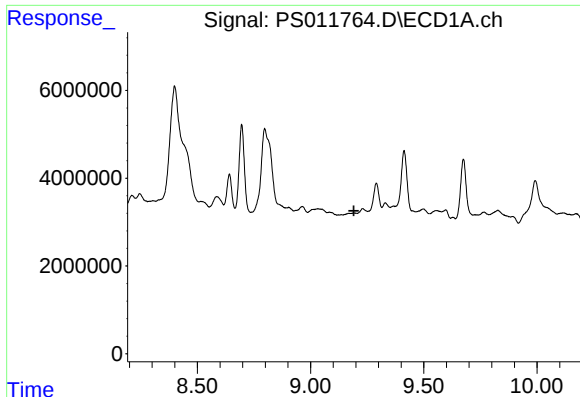

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

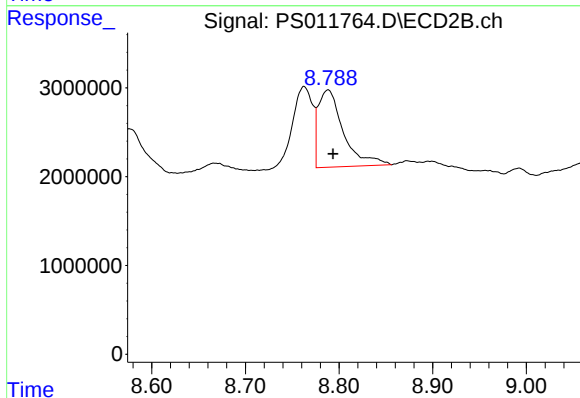


#11 2,4,5-TP (SILVEX)

R.T.: 8.788 min
Delta R.T.: -0.005 min
Response: 16210620
Conc: 5.54 ng/ml

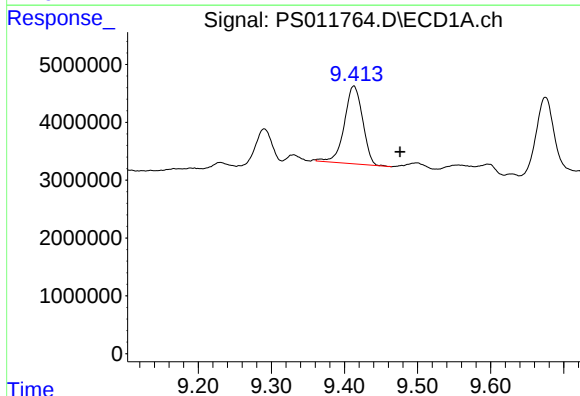


#12 2,4,5-T

R.T.: 9.413 min
Delta R.T.: -0.063 min
Response: 23357006
Conc: 3.94 ng/ml

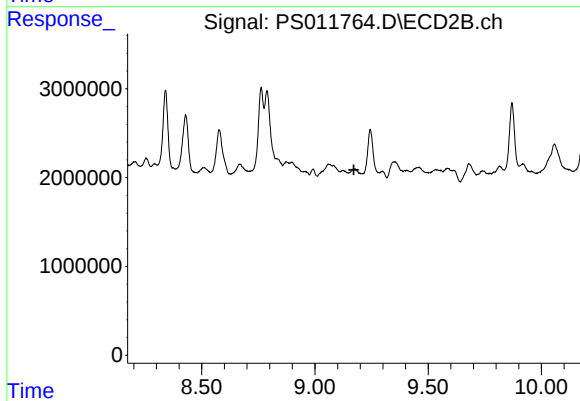

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.172 min
Response: 0
Conc: N.D.

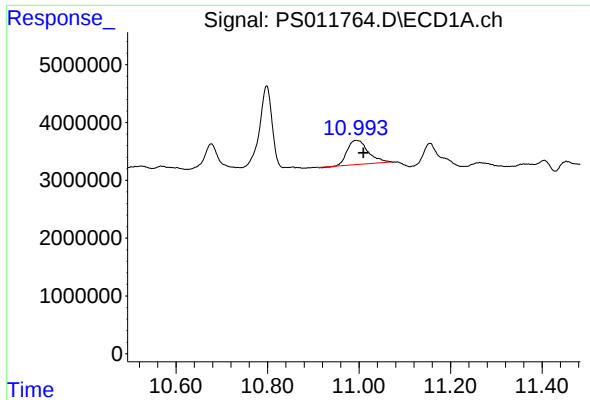

#15 Picloram

R.T.: 10.994 min
Delta R.T.: -0.015 min
Response: 13176116
Conc: 1.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

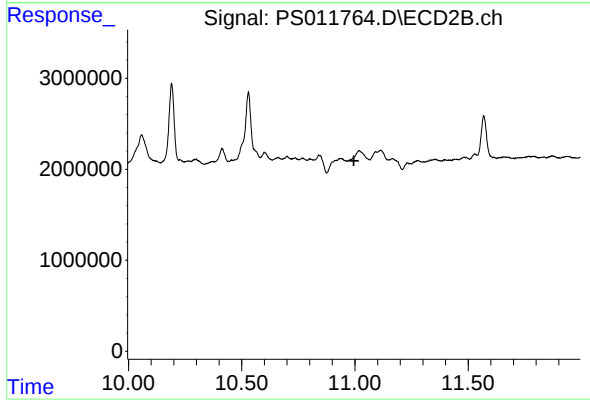

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.995 min
Response: 0
Conc: N.D.