

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081320\
 Data File : PS011766.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2020 23:11
 Operator : DD\AJ
 Sample : L3659-05
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 02:32:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.915	258.5E6	151.0E6	236.969	282.418
Target Compounds							
1) T	Dalapon	2.996	2.586	31509493	35396728	25.295	46.830 #
2) T	3,5-DICHL...	0.000	6.096	0	42930845	N.D.	52.188
5) T	DICAMBA	7.397	7.049	6108802	12233902	1.491	5.663 #
6) T	MCP	7.571	0.000	11605941	0	3.632	N.D. #
7) T	MCPA	7.686	7.458	357.5E6	257.5E6	78.607	93.964
8) T	DICHLORPROP	0.000	7.738	0	9627641	N.D.	17.051
9) T	2,4-D	8.399	7.977	109.7E6	7342704	97.146	9.995 #
10) T	Pentachlo...	8.696	0.000	24910590	0	1.732	N.D. #
11) T	2,4,5-TP ...	0.000	8.764	0	12381270	N.D.	4.235
12) T	2,4,5-T	9.414	0.000	34627777	0	5.844	N.D. #
15) T	Picloram	11.005	0.000	10572701	0	1.353	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081320\
Data File : PS011766.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2020 23:11
Operator : DD\AJ
Sample : L3659-05
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 02:32:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

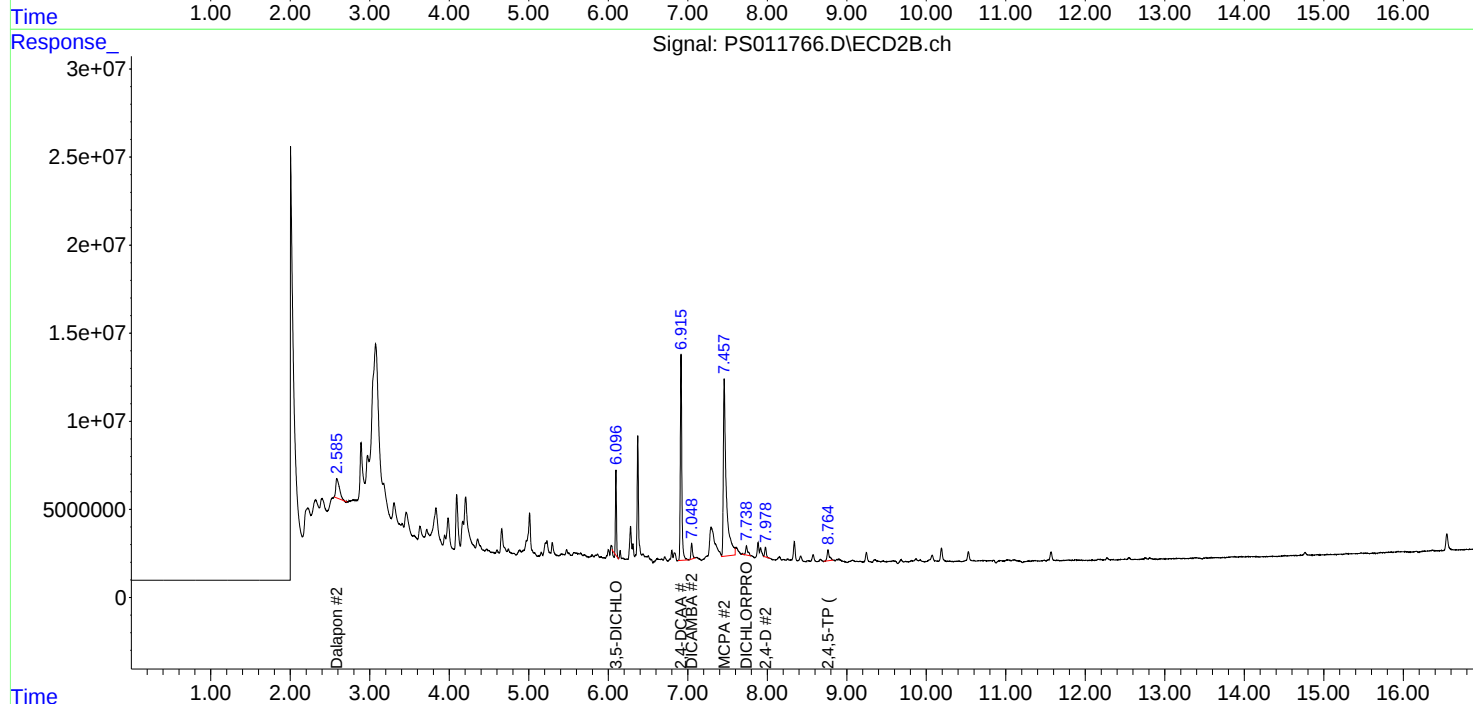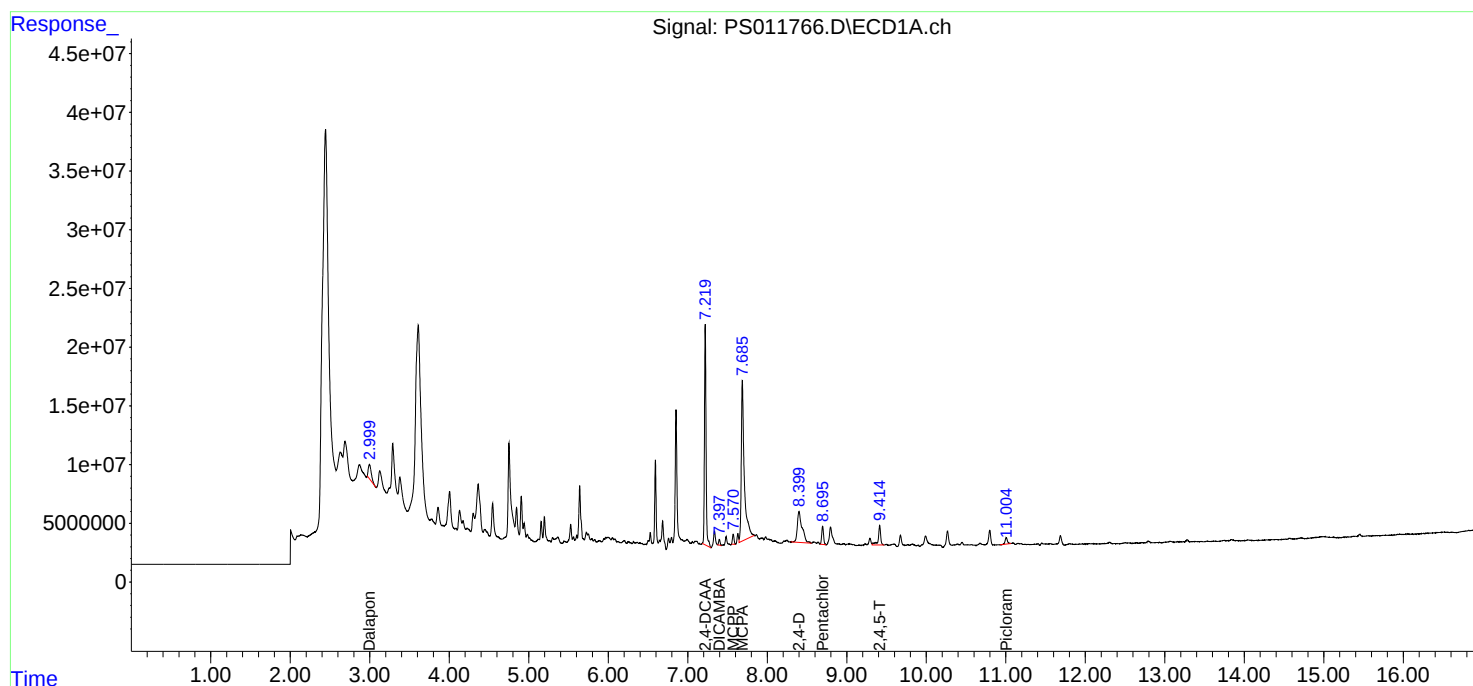


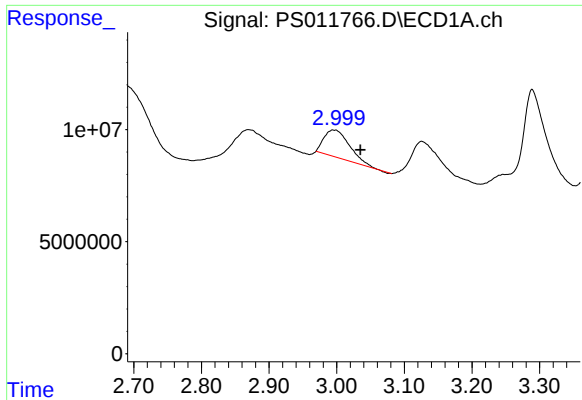

#1 Dalapon


R.T.: 2.996 min
Delta R.T.: -0.039 min
Response: 31509493
Conc: 25.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

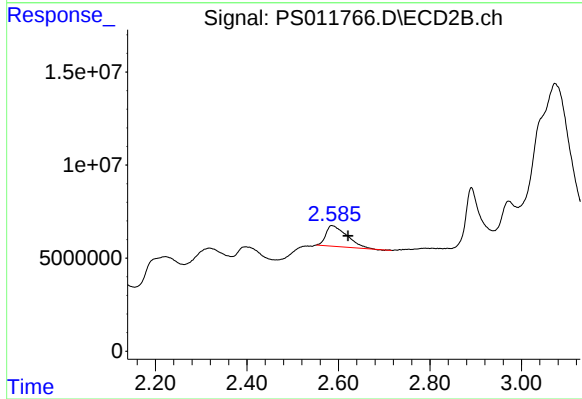


#1 Dalapon

R.T.: 2.586 min
Delta R.T.: -0.035 min
Response: 35396728
Conc: 46.83 ng/ml

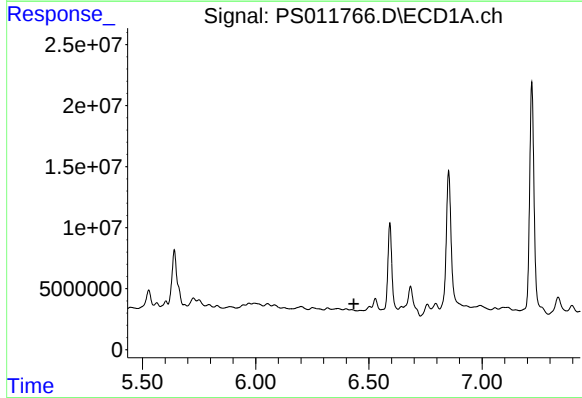


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.434 min
Response: 0
Conc: N.D.

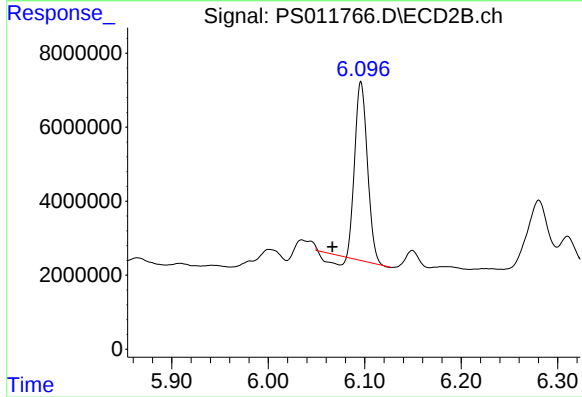

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.096 min
Delta R.T.: 0.030 min
Response: 42930845
Conc: 52.19 ng/ml

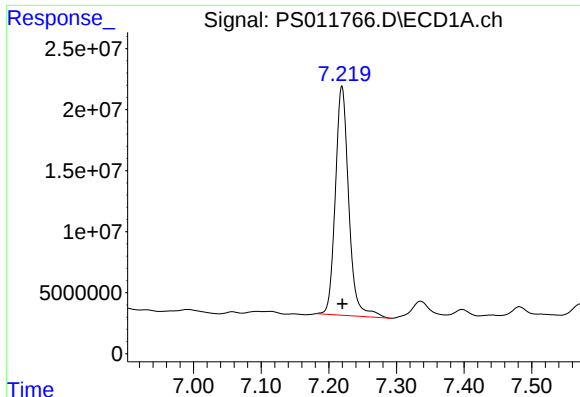

#4 2,4-DCAA


R.T.: 7.219 min
Delta R.T.: 0.000 min
Response: 258478230
Conc: 236.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

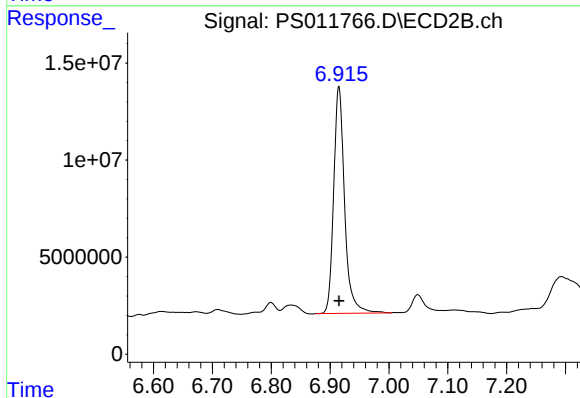


#4 2,4-DCAA

R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 151033373
Conc: 282.42 ng/ml

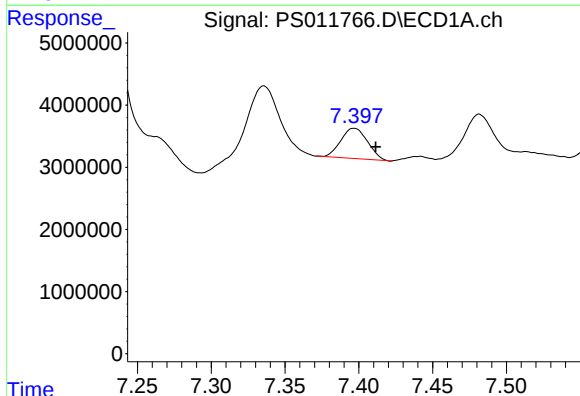


#5 DICAMBA

R.T.: 7.397 min
Delta R.T.: -0.015 min
Response: 6108802
Conc: 1.49 ng/ml

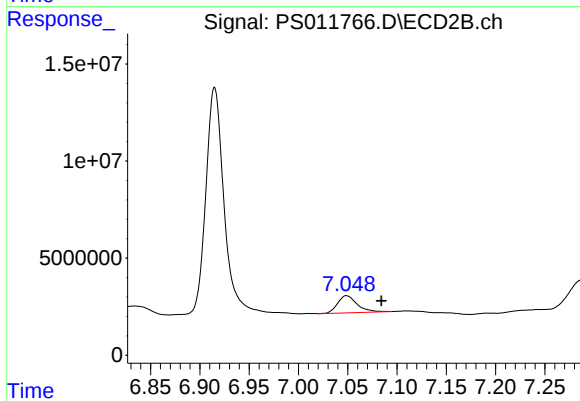

#5 DICAMBA


R.T.: 7.049 min
Delta R.T.: -0.035 min
Response: 12233902
Conc: 5.66 ng/ml

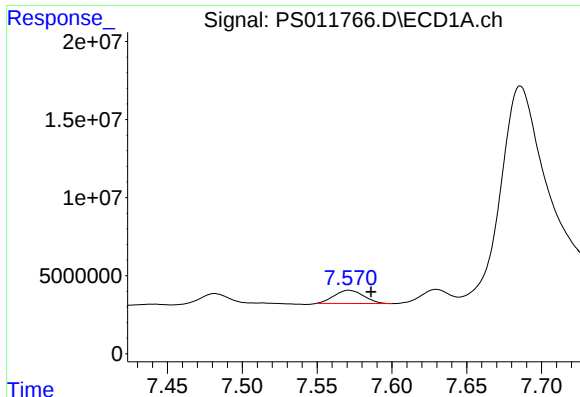

#6 MCPP


R.T.: 7.571 min
Delta R.T.: -0.015 min
Response: 11605941
Conc: 3.63 ug/ml

Instrument :
ECD_S
ClientSampleId :

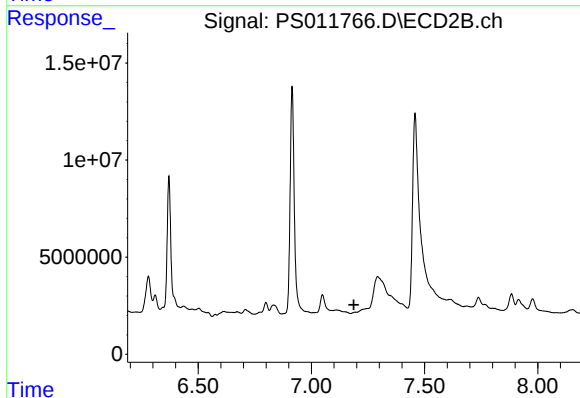


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

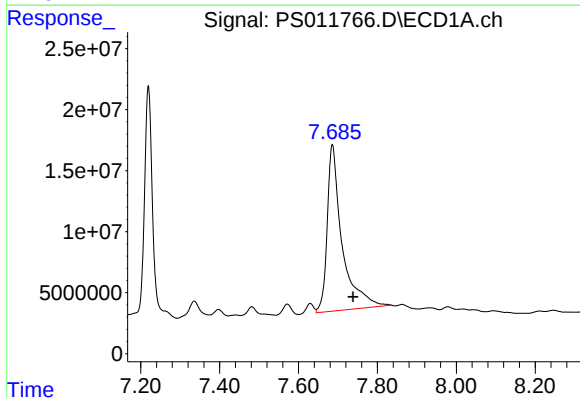


#7 MCPA

R.T.: 7.686 min
Delta R.T.: -0.052 min
Response: 357542196
Conc: 78.61 ug/ml

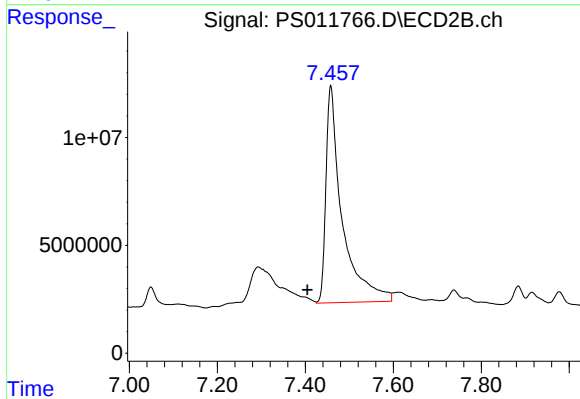

#7 MCPA


R.T.: 7.458 min
Delta R.T.: 0.053 min
Response: 257473838
Conc: 93.96 ug/ml

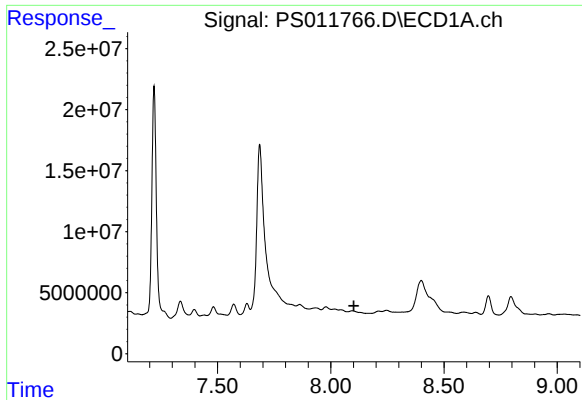

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

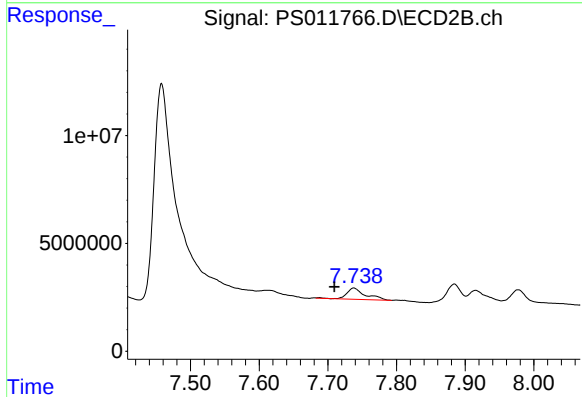


#8 DICHLORPROP

R.T.: 7.738 min
Delta R.T.: 0.028 min
Response: 9627641
Conc: 17.05 ng/ml

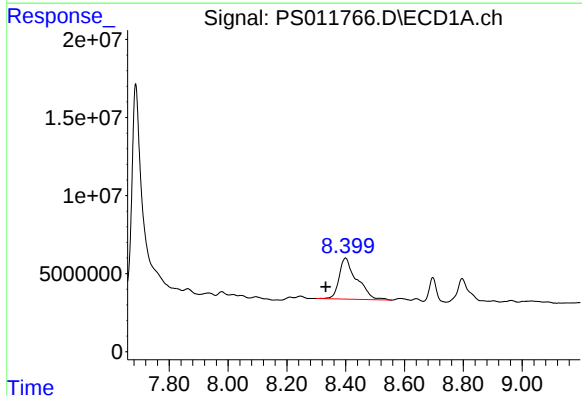


#9 2,4-D

R.T.: 8.399 min
Delta R.T.: 0.067 min
Response: 109687030
Conc: 97.15 ng/ml

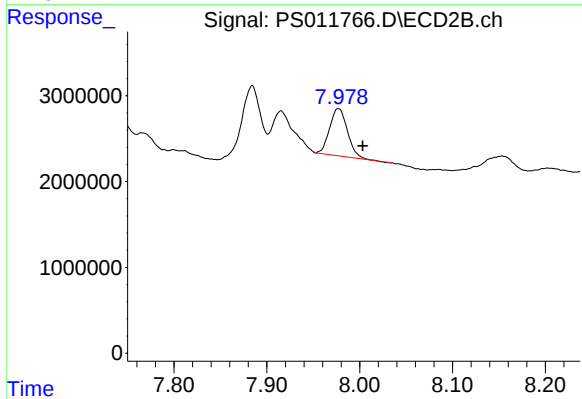

#9 2,4-D


R.T.: 7.977 min
Delta R.T.: -0.026 min
Response: 7342704
Conc: 9.99 ng/ml

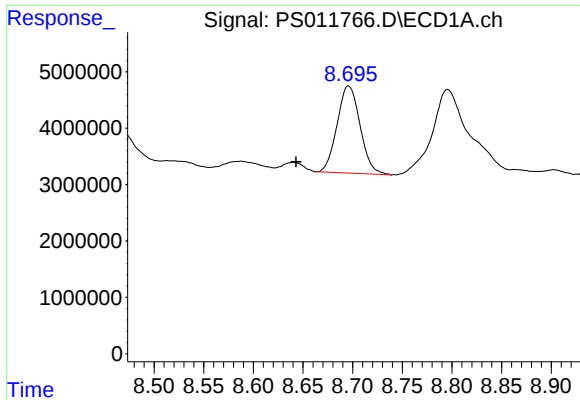

#10 Pentachlorophenol


R.T.: 8.696 min
Delta R.T.: 0.053 min
Response: 24910590
Conc: 1.73 ng/ml

Instrument :
ECD_S
ClientSampleId :

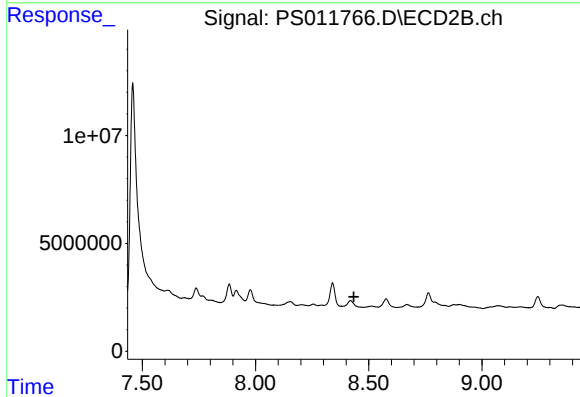


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 8.434 min
Response: 0
Conc: N.D.

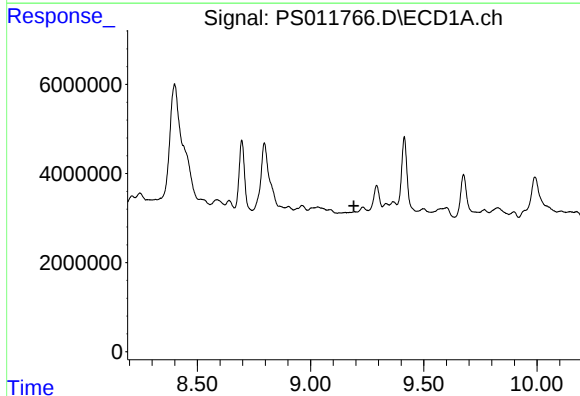


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.191 min
Response: 0
Conc: N.D.

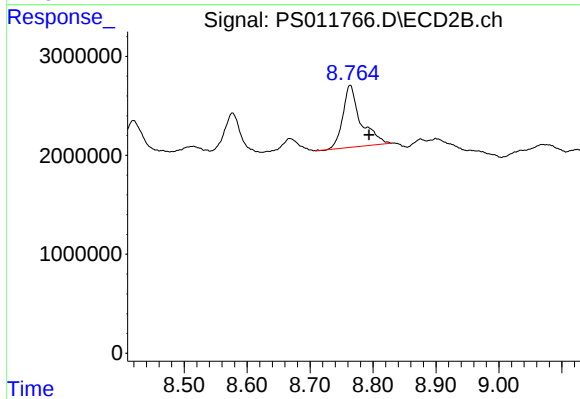

#11 2,4,5-TP (SILVEX)


R.T.: 8.764 min
Delta R.T.: -0.030 min
Response: 12381270
Conc: 4.23 ng/ml

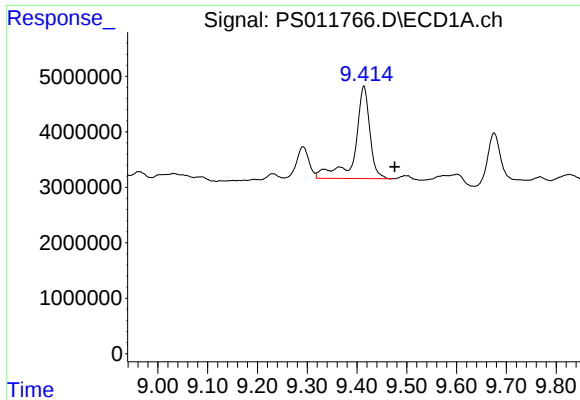

#12 2,4,5-T


R.T.: 9.414 min
Delta R.T.: -0.062 min
Response: 34627777
Conc: 5.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

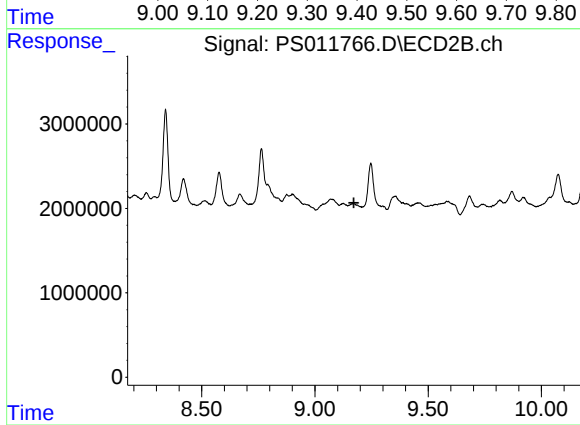


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.

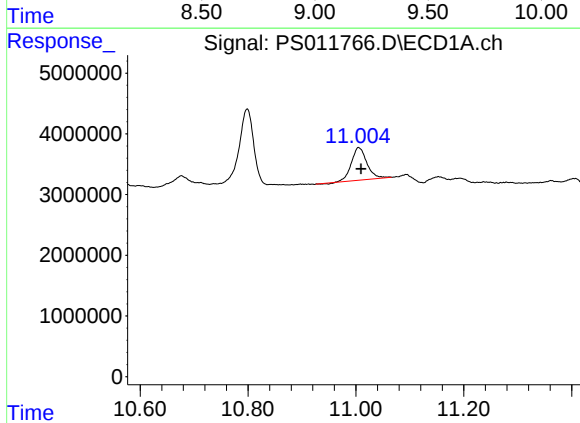

#15 Picloram

R.T.: 11.005 min
Delta R.T.: -0.004 min
Response: 10572701
Conc: 1.35 ng/ml

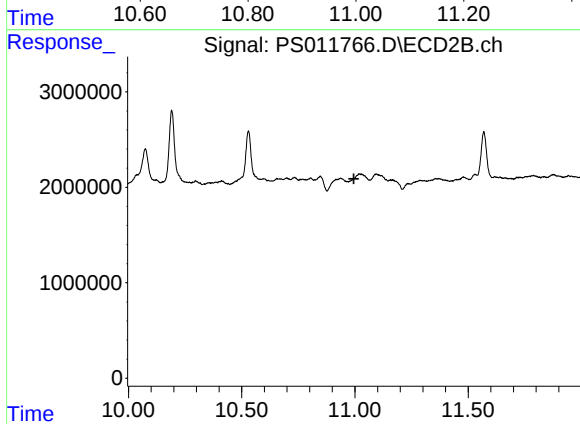

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.995 min
Response: 0
Conc: N.D.