

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081324\
 Data File : PS027409-1.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Aug 2024 17:54
 Operator : AR\AJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 03:54:45 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080524.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 06 08:10:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.176	7.737	1814.7E6	1355.3E6	721.501	728.743
Target Compounds							
1) T	Dalapon	2.600	2.687	2126.2E6	2168.9E6	650.593	650.020
2) T	3,5-DICHL...	6.356	6.691	2673.4E6	1826.1E6	671.420	666.333
3) T	4-Nitroph...	6.974	7.265	982.7E6	799.4E6	650.034	638.926
5) T	DICAMBA	7.359	7.936	7499.3E6	6116.9E6	679.497	710.145
6) T	MCPD	7.538	8.038	520.8E6	397.4E6	68.442	69.791
7) T	MCPA	7.684	8.281	655.4E6	514.5E6	67.648	68.112
8) T	DICHLORPROP	8.052	8.648	1951.0E6	1410.9E6	737.355	674.901
9) T	2,4-D	8.279	8.978	1994.4E6	1584.9E6	699.513	680.303
10) T	Pentachlo...	8.569	9.504	28129.3E6	22222.0E6	711.608	698.209
11) T	2,4,5-TP ...	9.141	9.879	10657.5E6	8774.8E6	702.692	687.087
12) T	2,4,5-T	9.430	10.297	10332.6E6	8681.7E6	707.436	688.521
13) T	2,4-DB	9.998	10.861	1449.2E6	1073.0E6	706.619	678.824
14) T	DINOSEB	11.187	11.240	7758.5E6	5713.0E6	696.129	670.765
15) T	Picloram	11.003	12.332	13393.4E6	12350.9E6	694.667	684.596
16) T	DCPA	11.485	12.281	13018.0E6	9651.9E6	720.632	694.066



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081324\
Data File : PS027409-1.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Aug 2024 17:54
Operator : AR\AJ
Sample : HSTDCCC750
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 03:54:45 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080524.M
Quant Title : 8080.M
QLast Update : Tue Aug 06 08:10:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

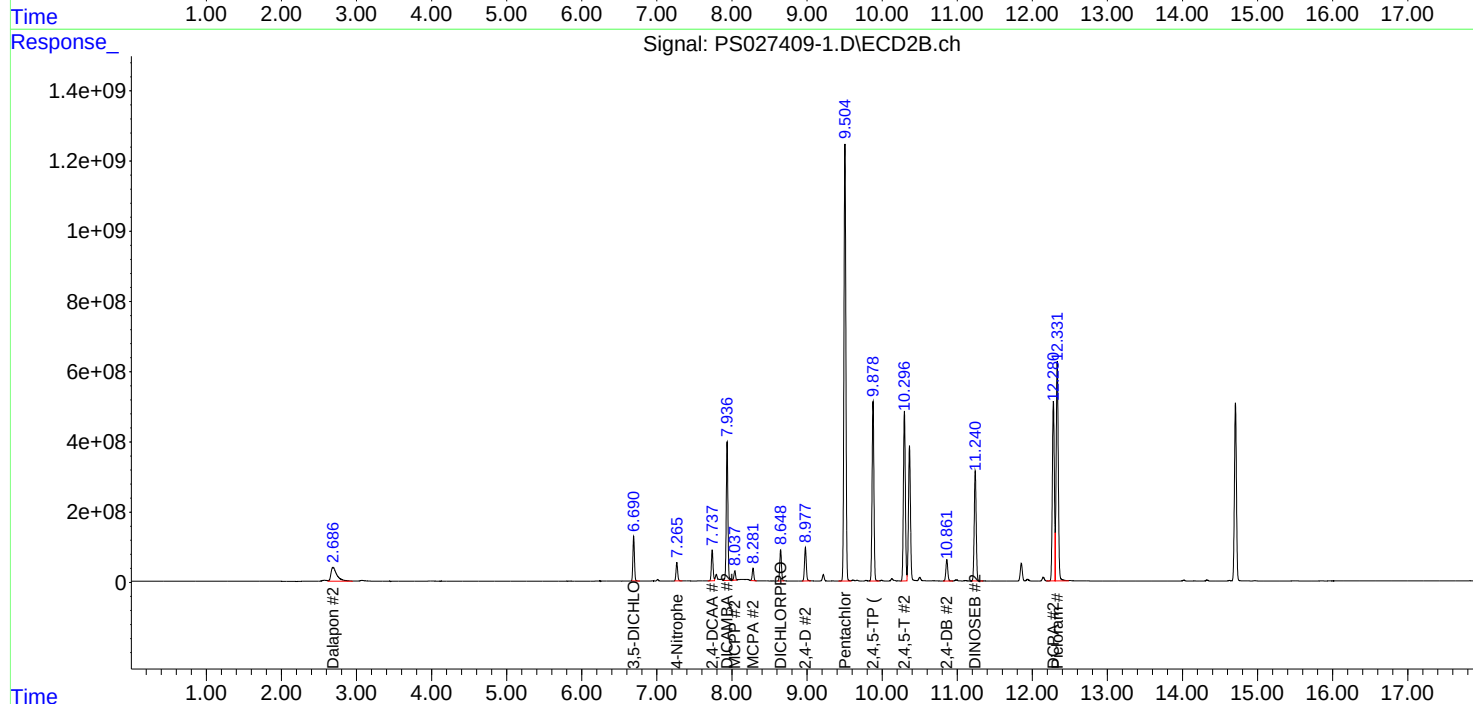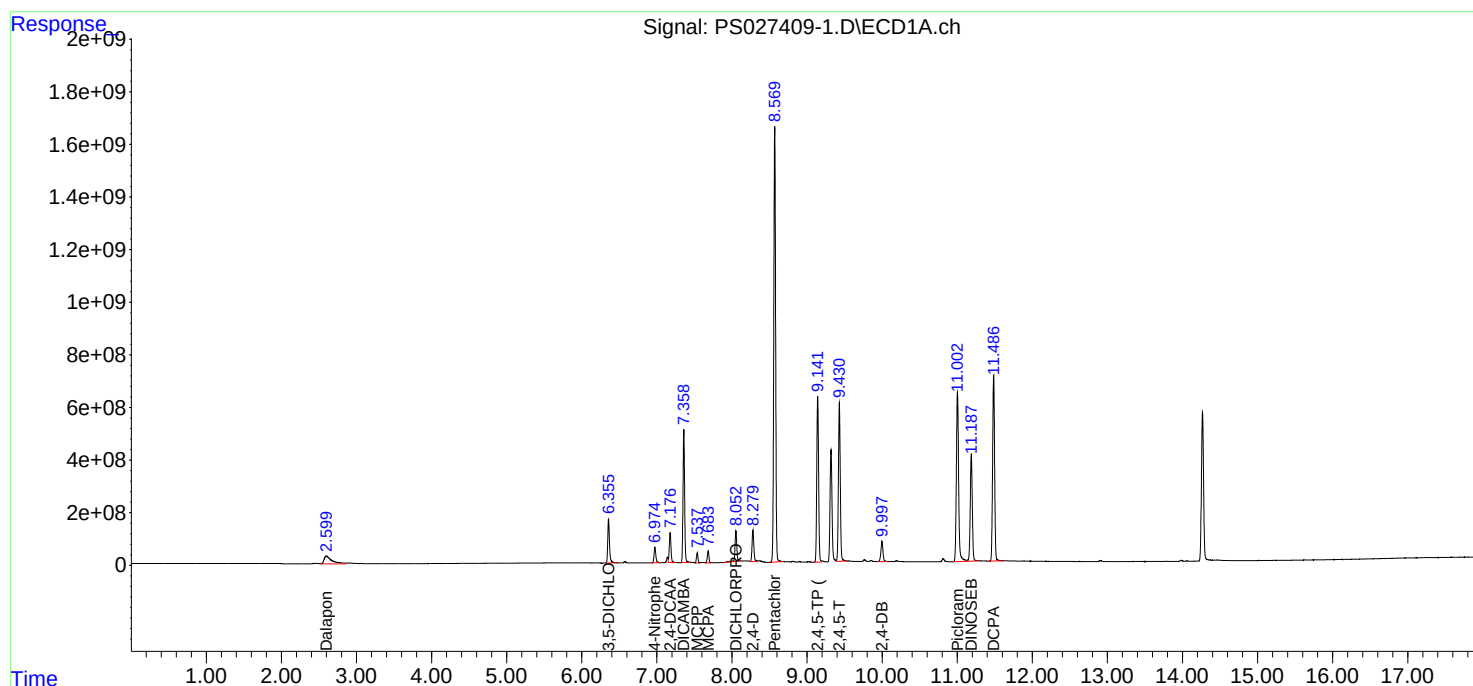

The printer must be in Portrait mode.

Instrument :
ECD_S
ClientSampleId :