

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081324\
 Data File : PS027432CC-1.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2024 04:01
 Operator : AR\AJ
 Sample : HSTDCCC750
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 05:13:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080524.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 06 08:10:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.172	7.740	1867.2E6	1356.8E6	742.374	729.560
Target Compounds							
1) T	Dalapon	2.600	2.694	2165.5E6	2241.3E6	662.621	671.713
2) T	3,5-DICHL...	6.354	6.695	2742.0E6	1859.4E6	688.640	678.478
3) T	4-Nitroph...	6.971	7.269	1030.2E6	834.6E6	681.428	667.058
5) T	DICAMBA	7.355	7.938	7712.5E6	6008.1E6	698.811	697.516
6) T	MCPD	7.534	8.040	543.9E6	403.3E6	71.469	70.823
7) T	MCPA	7.680	8.284	691.5E6	536.3E6	71.373	70.989
8) T	DICHLORPROP	8.047	8.650	1848.0E6	1440.2E6	698.458	688.926
9) T	2,4-D	8.273	8.979	2007.2E6	1616.1E6	704.012	693.683
10) T	Pentachlo...	8.564	9.506	28849.6E6	22589.5E6	729.830	709.754
11) T	2,4,5-TP ...	9.136	9.880	10984.9E6	8937.8E6	724.278	699.849
12) T	2,4,5-T	9.424	10.299	10763.6E6	8865.3E6	736.945	703.084
13) T	2,4-DB	9.991	10.863	1528.0E6	1102.6E6	745.062	697.530
14) T	DINOSEB	11.180	11.241	8109.4E6	5937.1E6	727.606	697.080
15) T	Picloram	10.995	12.333	14435.0E6	13199.6E6	748.688	731.641
16) T	DCPA	11.477	12.281	13394.0E6	9873.1E6	741.442	709.969



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081324\
Data File : PS027432CC-1.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2024 04:01
Operator : AR\AJ
Sample : HSTDCCC750
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 05:13:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080524.M
Quant Title : 8080.M
QLast Update : Tue Aug 06 08:10:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

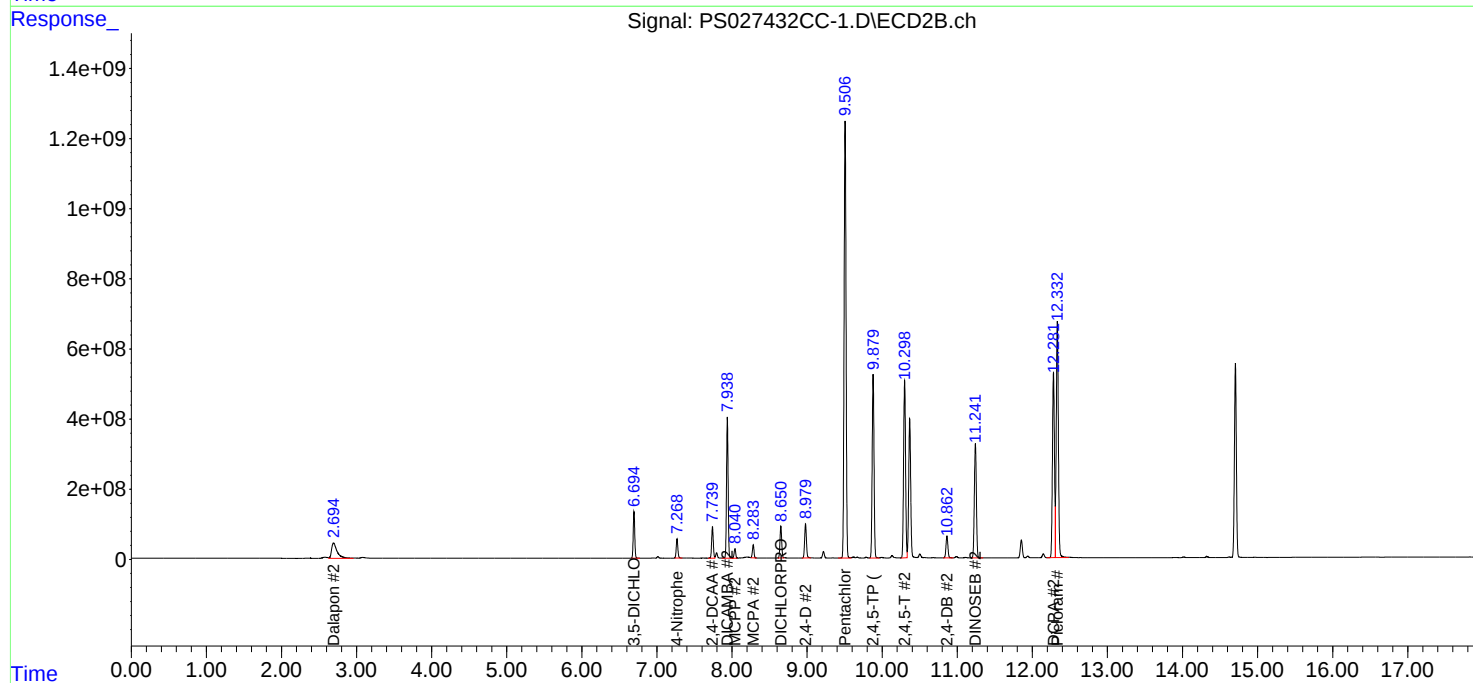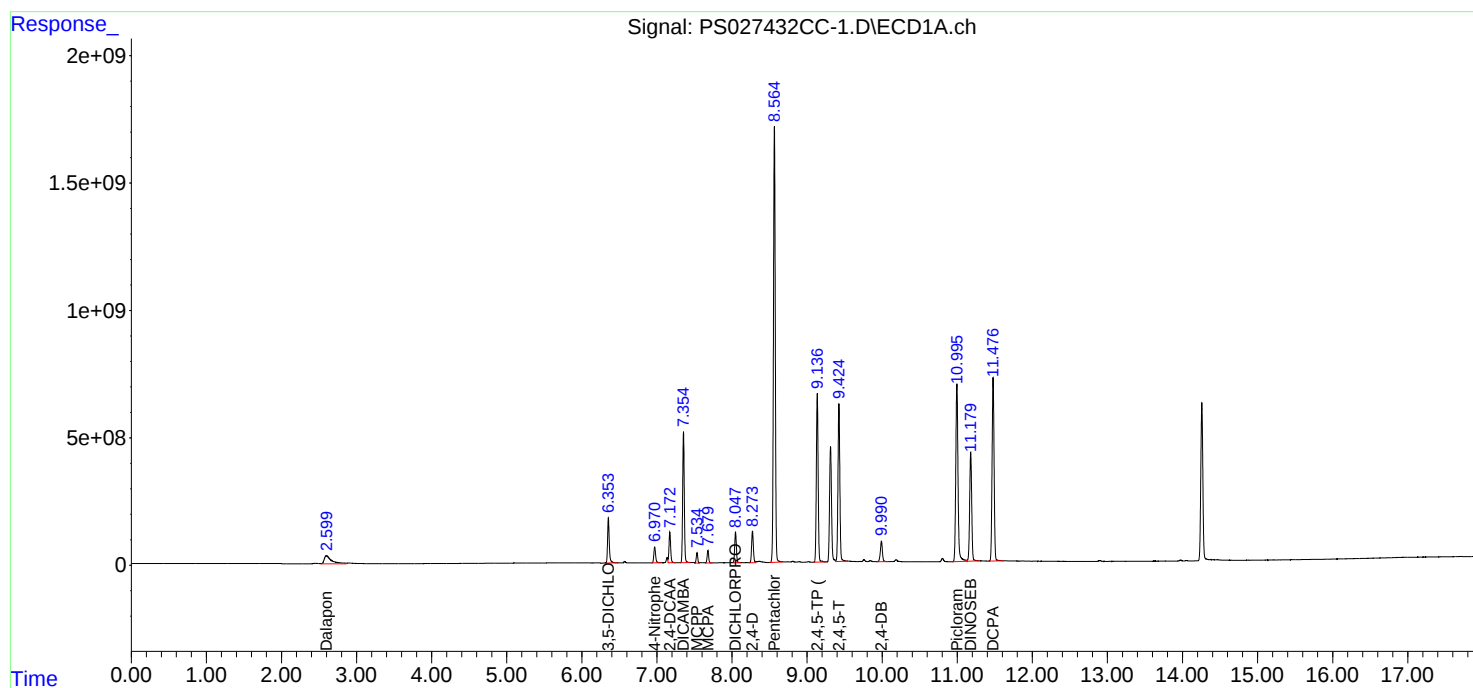

The printer must be in Portrait mode.

Instrument :
ECD_S
ClientSampleId :