

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081419\
 Data File : PS006047.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2019 12:01
 Operator : SM\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 15:11:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
3) T	4-Nitroph...	0.000	4.905	0	3962072	N.D. 15.994
7) T	MCPA	5.913	0.000	181.5E6	0	57.481 N.D. #
12) T	2,4,5-T	0.000	7.296	0	45537781	N.D. 18.317
15) T	Picloram	9.040	8.993	233.4E6	154.1E6	31.365 34.173
16) T	DCPA	0.000	8.993	0	154.1E6	N.D. 44.205



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081419\
Data File : PS006047.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2019 12:01
Operator : SM\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 15:11:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

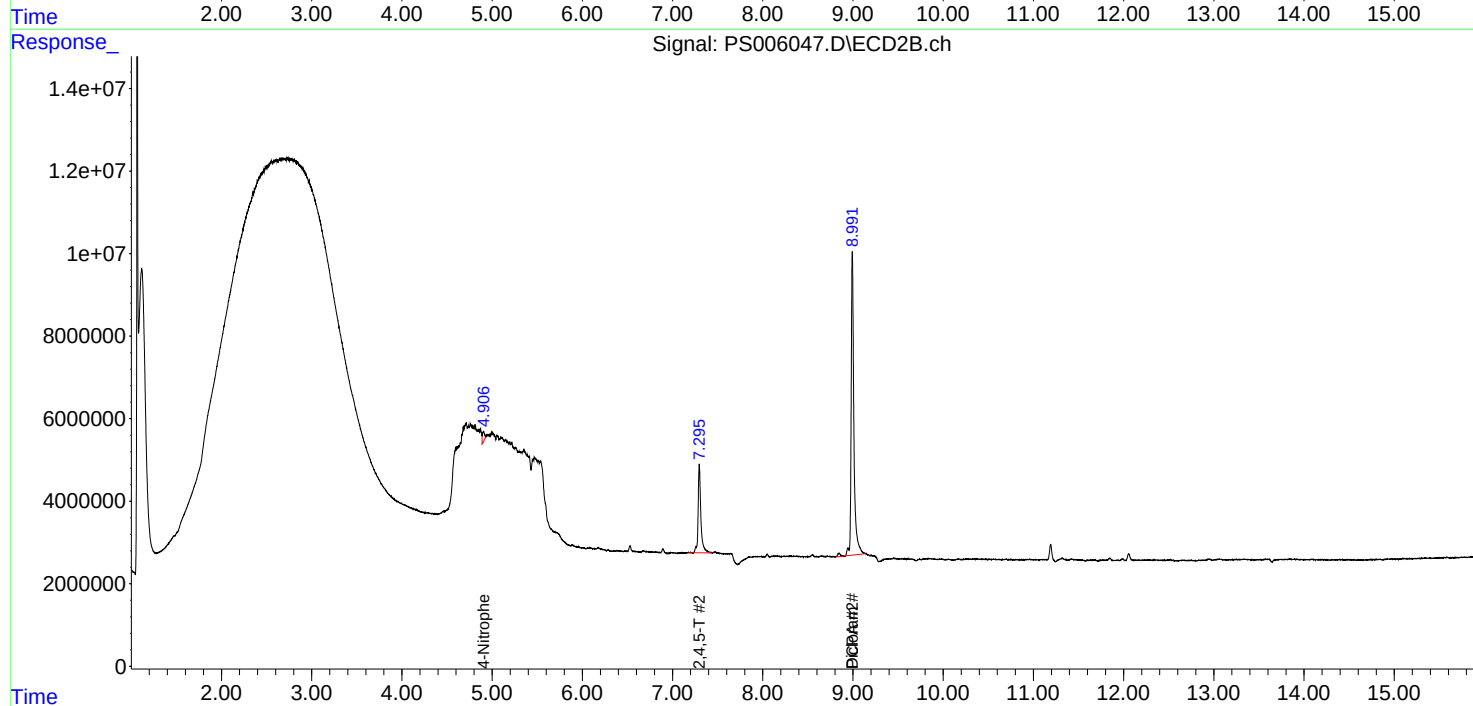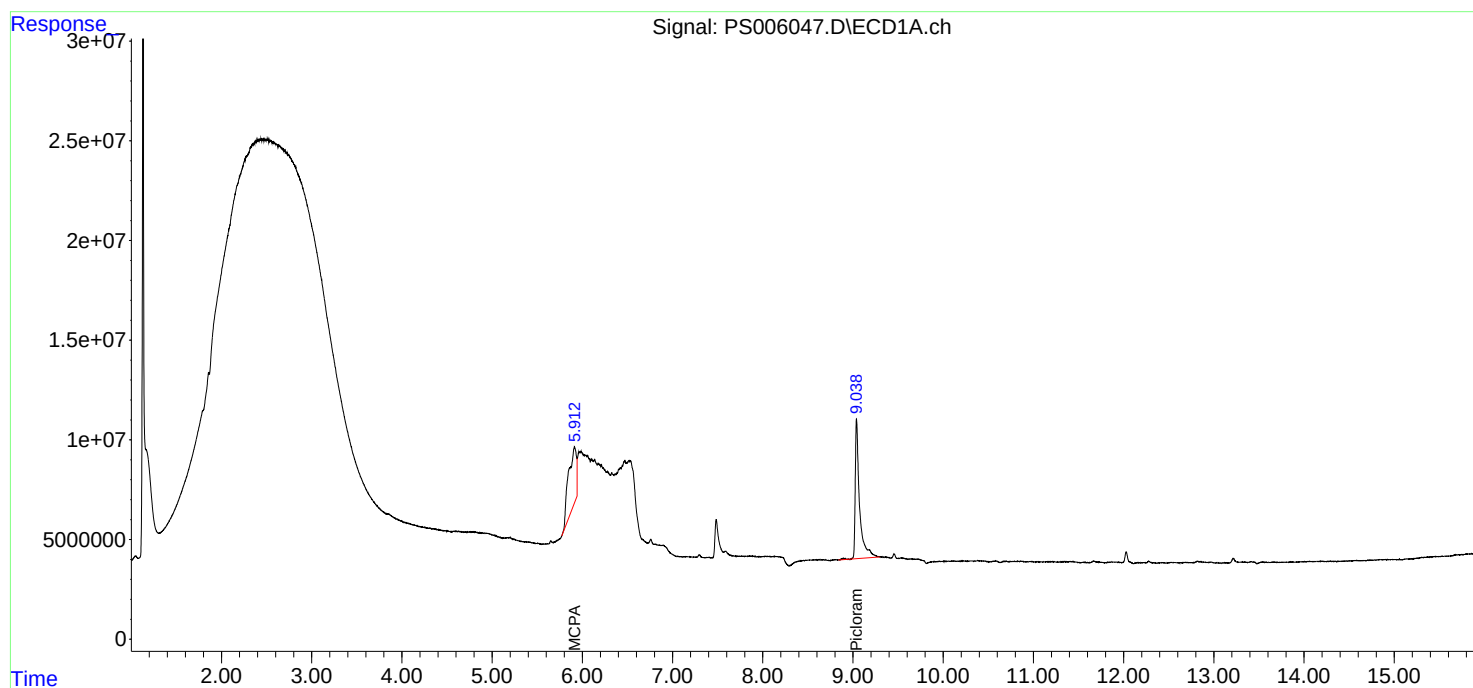


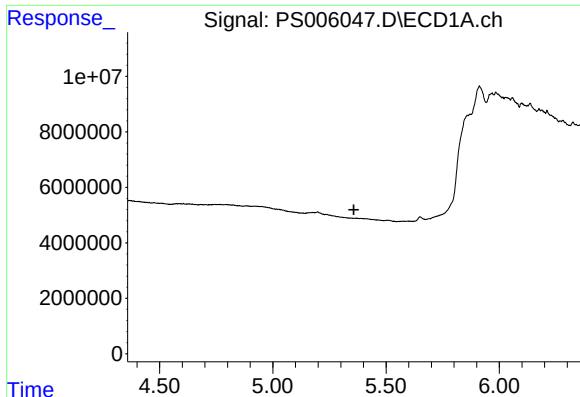

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 5.358 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

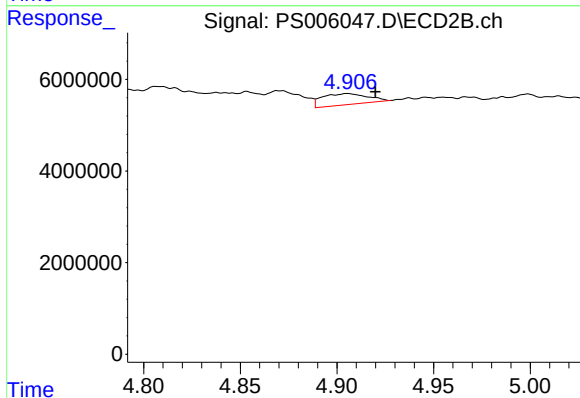


#3 4-Nitrophenol

R.T.: 4.905 min
Delta R.T.: -0.014 min
Response: 3962072
Conc: 15.99 ng/ml

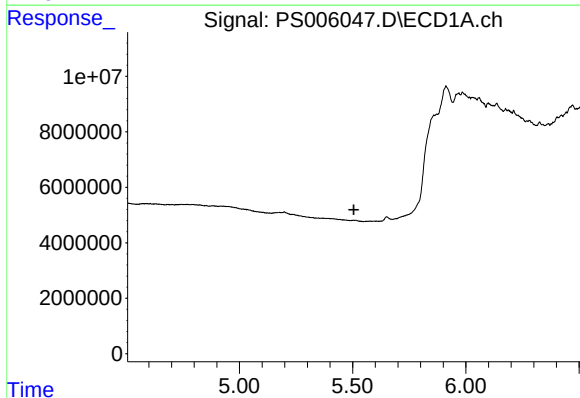


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 5.505 min
Response: 0
Conc: N.D.

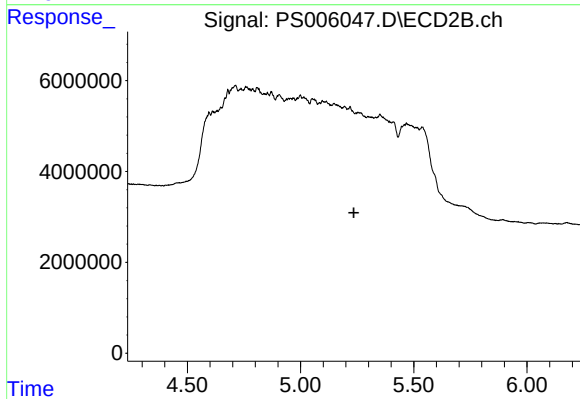

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 5.236 min
Response: 0
Conc: N.D.

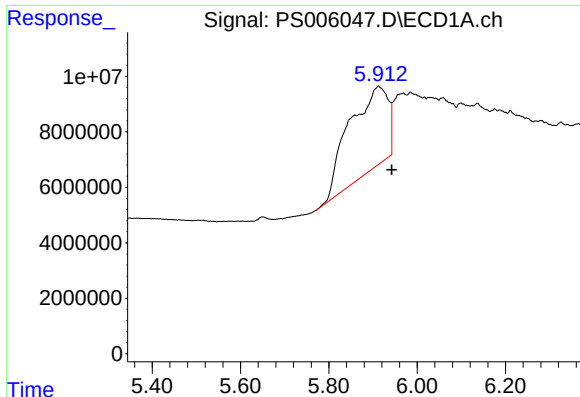

#7 MCPA


R.T.: 5.913 min
Delta R.T.: -0.030 min
Response: 181471950
Conc: 57.48 ug/ml

Instrument :
ECD_S
ClientSampleId :

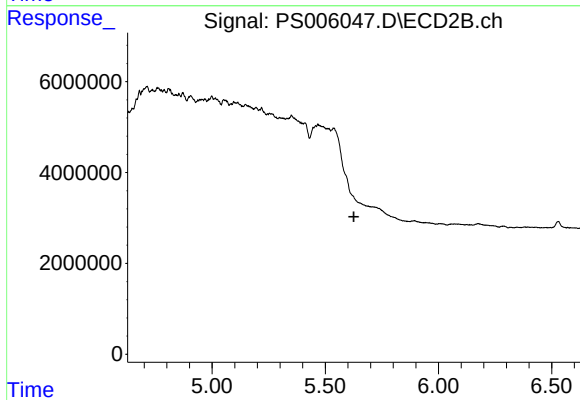


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 5.626 min
Response: 0
Conc: N.D.

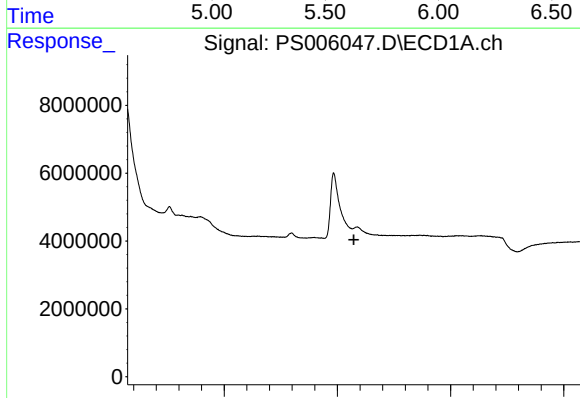


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.573 min
Response: 0
Conc: N.D.

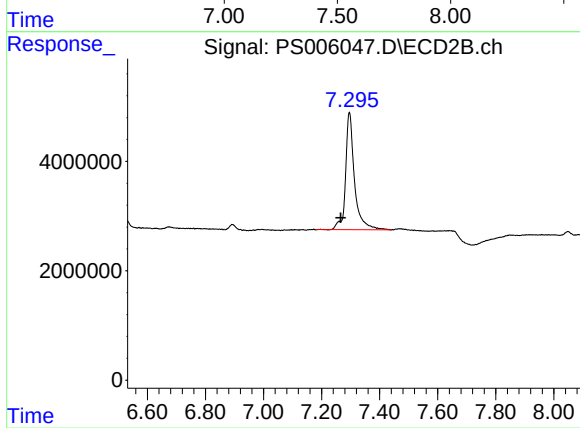

#12 2,4,5-T


R.T.: 7.296 min
Delta R.T.: 0.030 min
Response: 45537781
Conc: 18.32 ng/ml

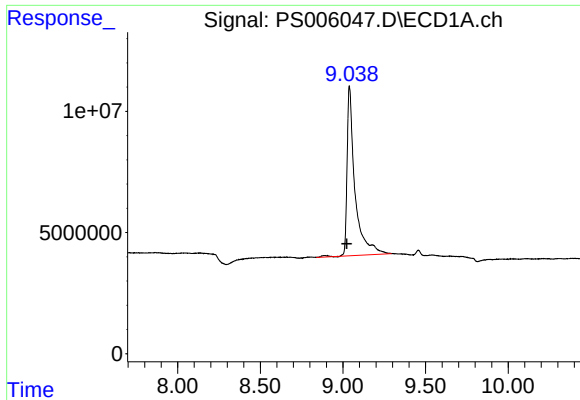

#15 Picloram


R.T.: 9.040 min
Delta R.T.: 0.016 min
Response: 233375012
Conc: 31.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

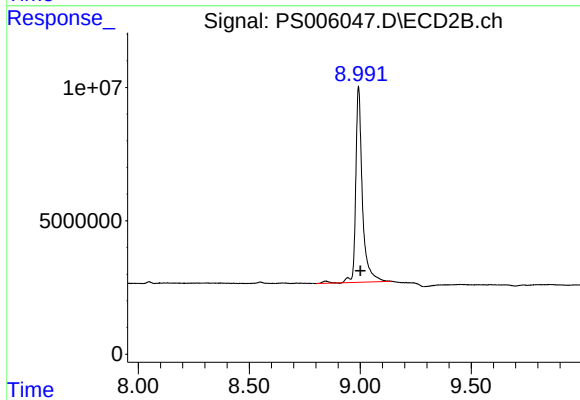


#15 Picloram

R.T.: 8.993 min
Delta R.T.: -0.008 min
Response: 154148893
Conc: 34.17 ng/ml

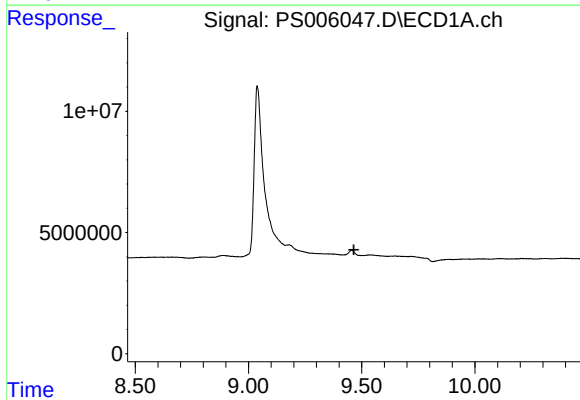

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.465 min
Response: 0
Conc: N.D.

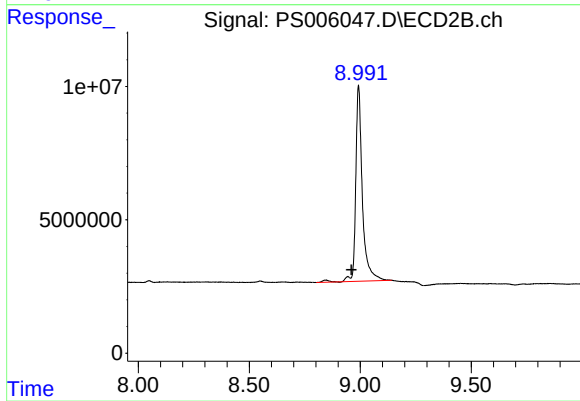

#16 DCPA

R.T.: 8.993 min
Delta R.T.: 0.033 min
Response: 154148893
Conc: 44.20 ng/ml