

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081419\
 Data File : PS006048.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2019 12:23
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 15:12:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.489	5.216	318.1E6	185.3E6	368.458	376.750
Target Compounds							
9) T	2,4-D	6.551	0.000	147.4E6	0	180.934	N.D. #
12) T	2,4,5-T	7.503	7.304	24955567	28743645	5.047	11.562 #
15) T	Picloram	9.044	8.995	178.5E6	123.6E6	23.986	27.406
16) T	DCPA	0.000	8.995	0	123.6E6	N.D.	35.452



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081419\
Data File : PS006048.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2019 12:23
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 15:12:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

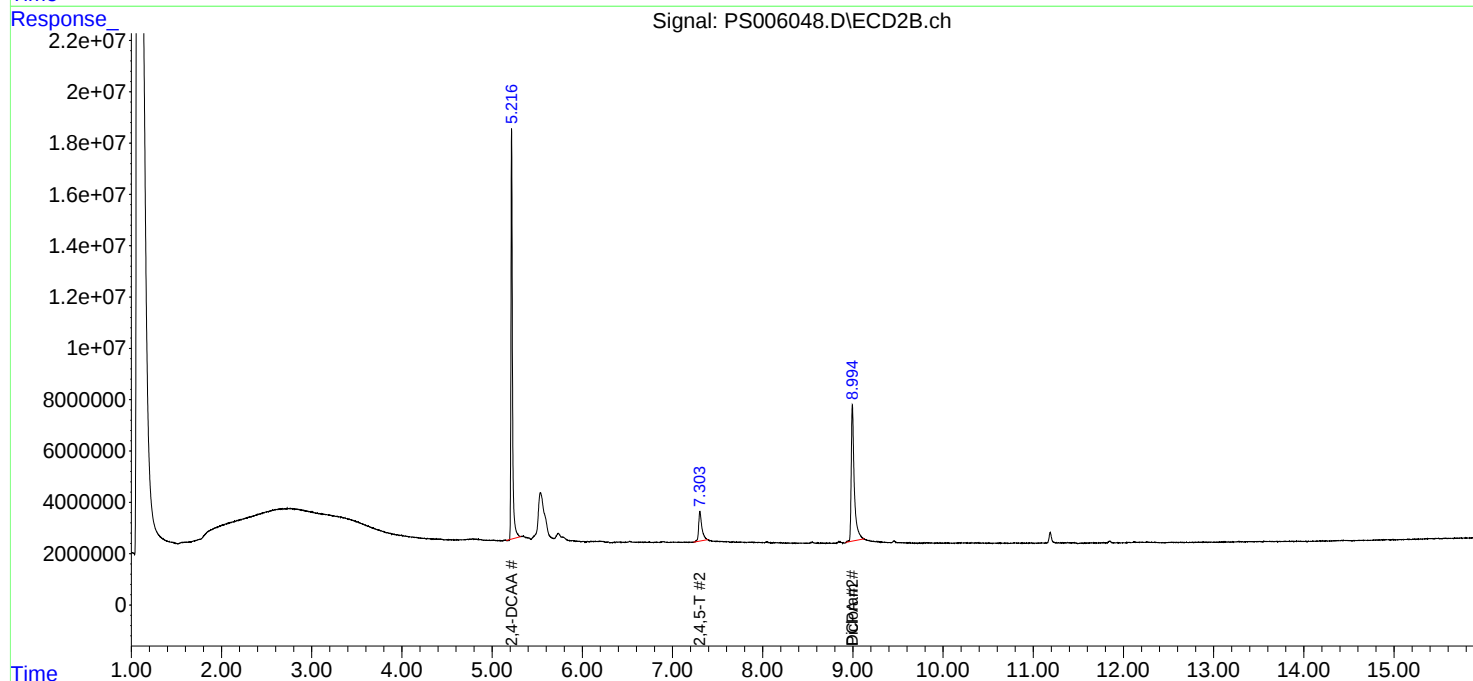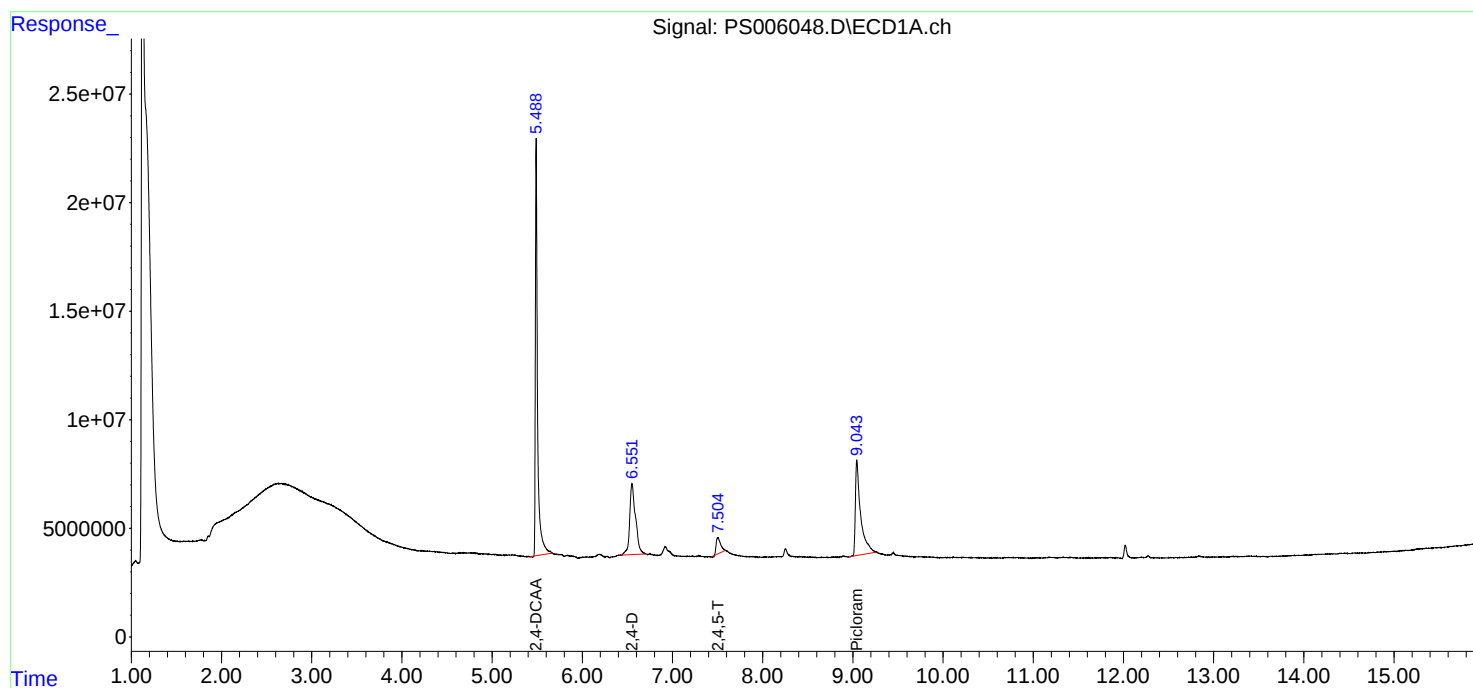


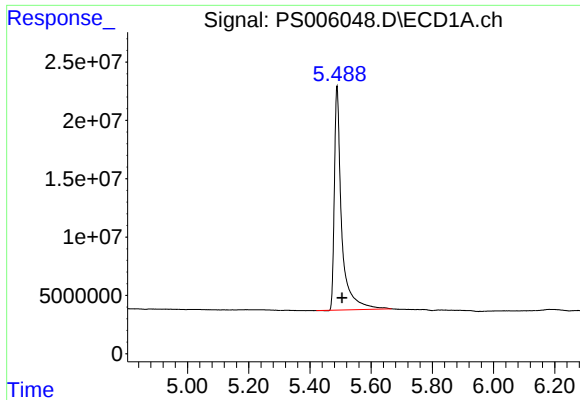

#4 2,4-DCAA


R.T.: 5.489 min
Delta R.T.: -0.016 min
Response: 318053465
Conc: 368.46 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

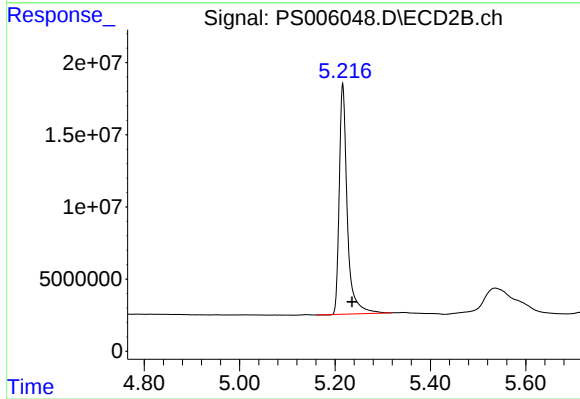


#4 2,4-DCAA

R.T.: 5.216 min
Delta R.T.: -0.019 min
Response: 185305080
Conc: 376.75 ng/ml

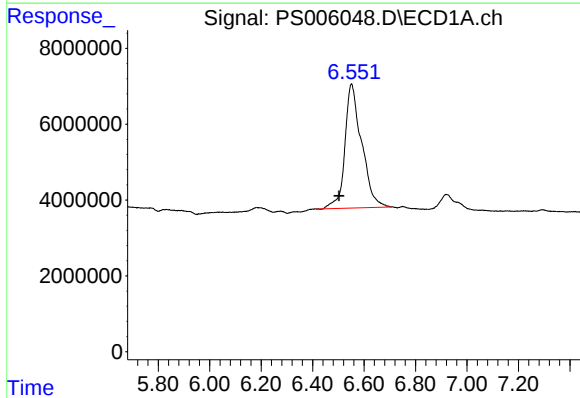


#9 2,4-D

R.T.: 6.551 min
Delta R.T.: 0.048 min
Response: 147422026
Conc: 180.93 ng/ml

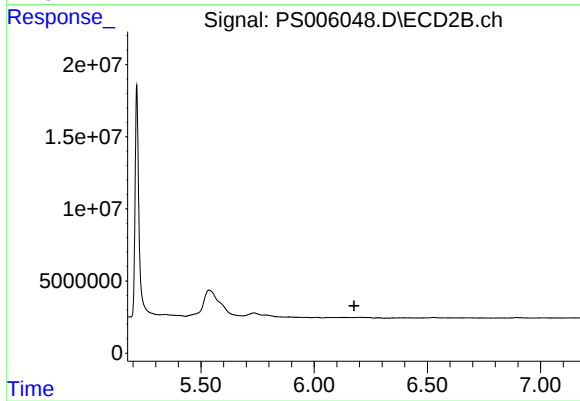

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.176 min
Response: 0
Conc: N.D.

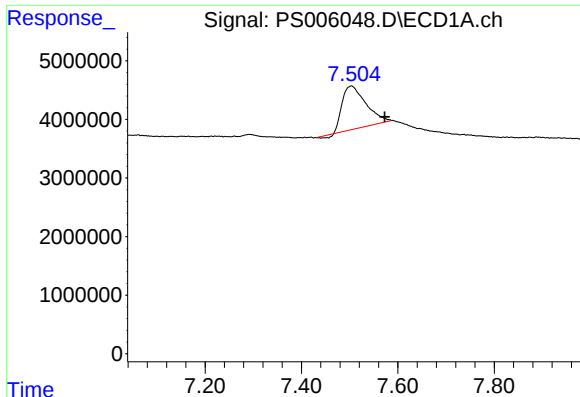

#12 2,4,5-T


R.T.: 7.503 min
Delta R.T.: -0.069 min
Response: 24955567
Conc: 5.05 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

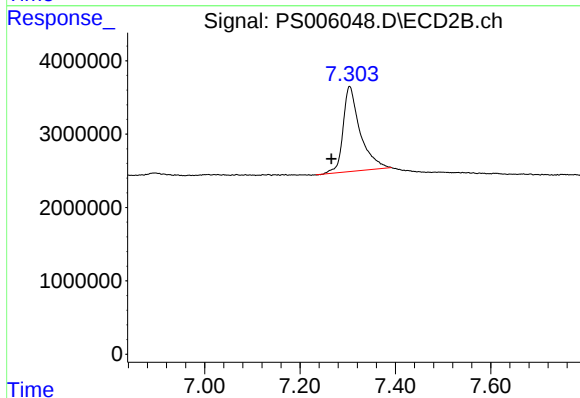


#12 2,4,5-T

R.T.: 7.304 min
Delta R.T.: 0.038 min
Response: 28743645
Conc: 11.56 ng/ml

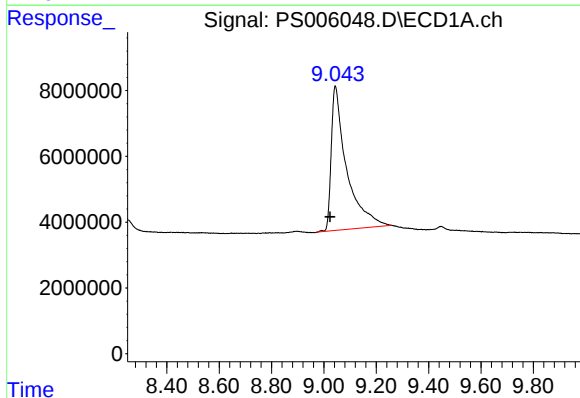


#15 Picloram

R.T.: 9.044 min
Delta R.T.: 0.020 min
Response: 178473325
Conc: 23.99 ng/ml

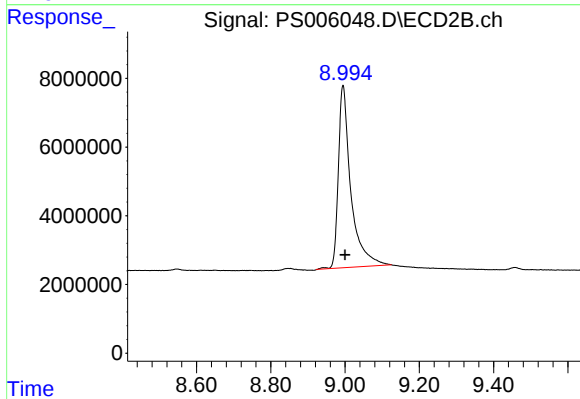

#15 Picloram


R.T.: 8.995 min
Delta R.T.: -0.006 min
Response: 123626719
Conc: 27.41 ng/ml

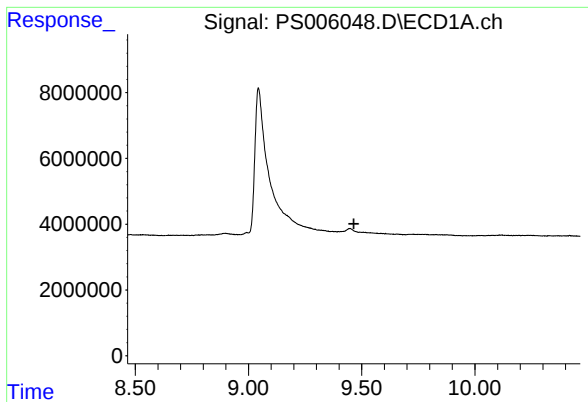

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

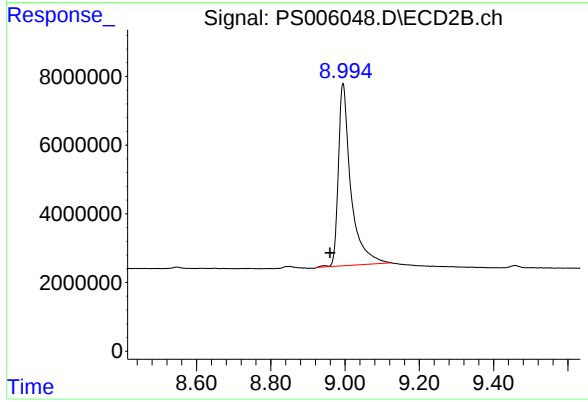

#16 DCPA

R.T.: 8.995 min
Delta R.T.: 0.035 min
Response: 123626719
Conc: 35.45 ng/ml