

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081419\
 Data File : PS006056.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2019 14:58
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 08:21:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.472	5.201	311.4E6	189.0E6	360.699	384.271
Target Compounds							
9) T	2,4-D	6.534	0.000	220.2E6	0	270.204	N.D. #
12) T	2,4,5-T	0.000	7.286	0	51265838	N.D.	20.621
15) T	Picloram	9.028	8.980	202.3E6	147.5E6	27.186	32.690
16) T	DCPA	0.000	8.980	0	147.5E6	N.D.	42.287



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081419\
Data File : PS006056.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2019 14:58
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 08:21:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

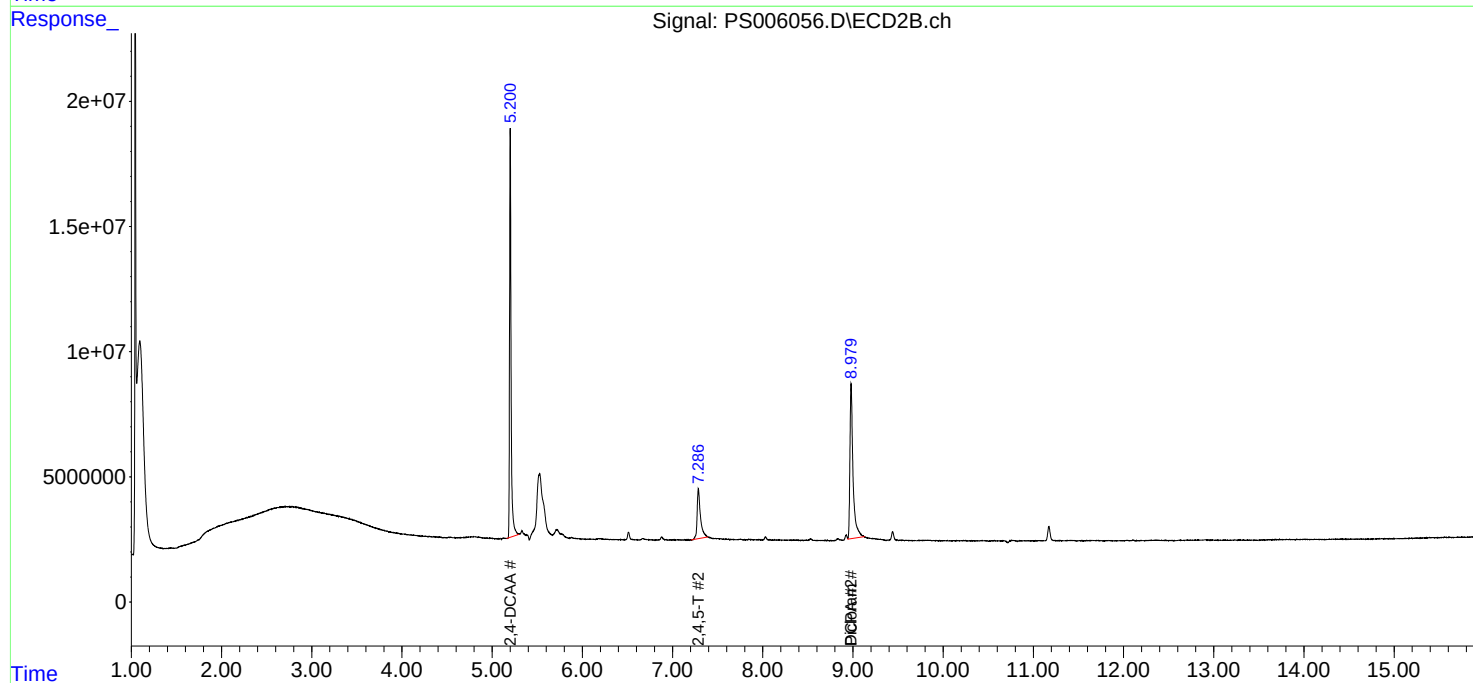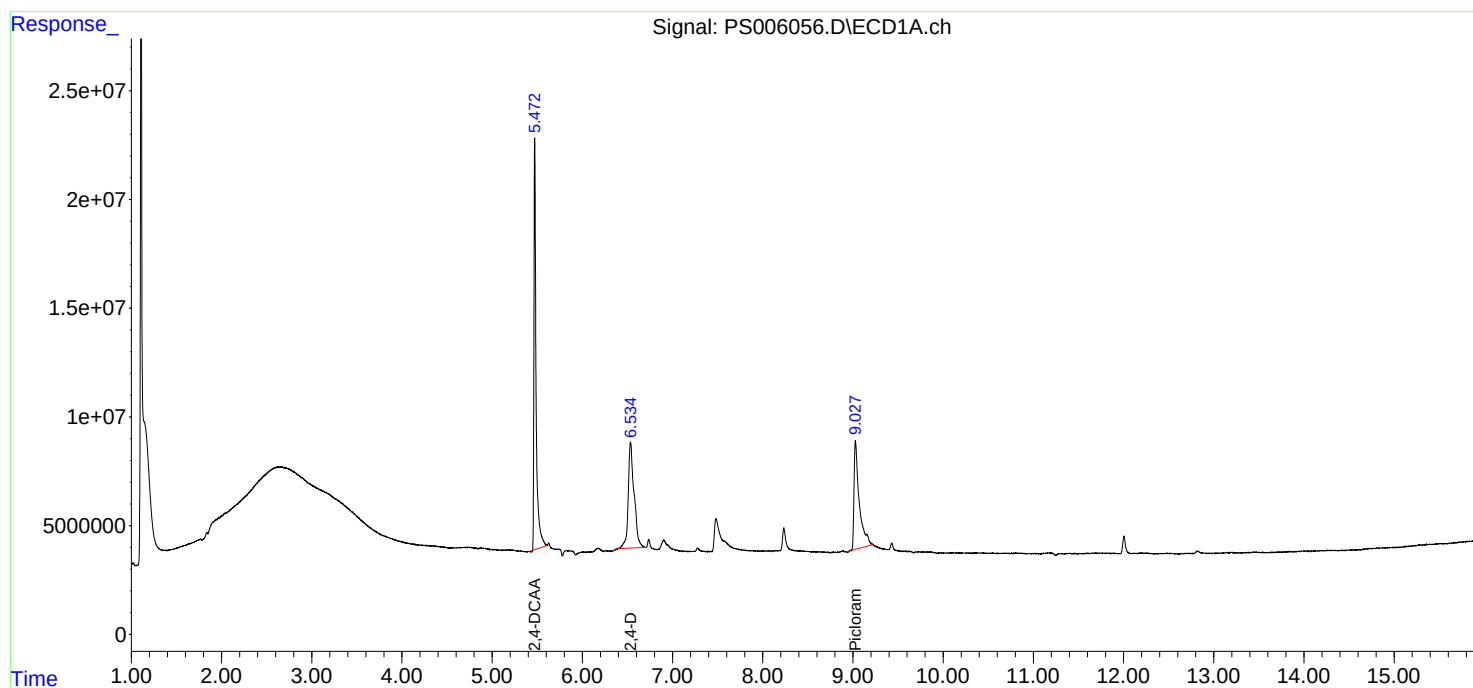


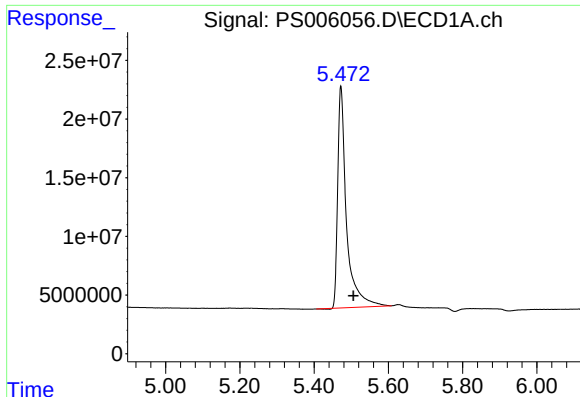

#4 2,4-DCAA


R.T.: 5.472 min
Delta R.T.: -0.033 min
Response: 311355698
Conc: 360.70 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

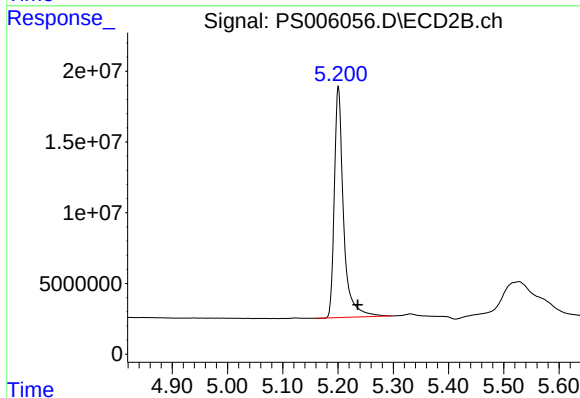


#4 2,4-DCAA

R.T.: 5.201 min
Delta R.T.: -0.035 min
Response: 189004384
Conc: 384.27 ng/ml

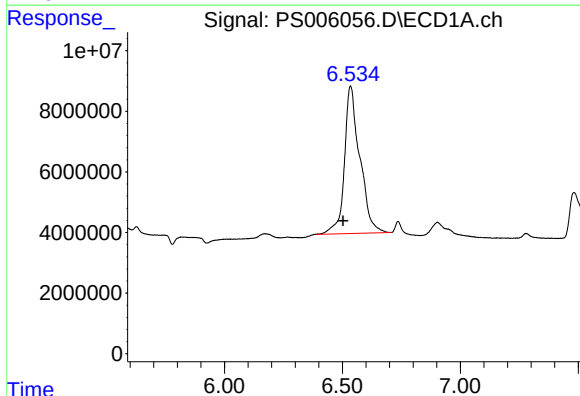


#9 2,4-D

R.T.: 6.534 min
Delta R.T.: 0.031 min
Response: 220157924
Conc: 270.20 ng/ml

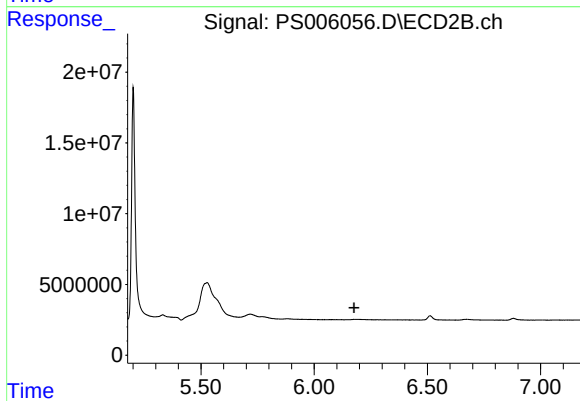

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.176 min
Response: 0
Conc: N.D.

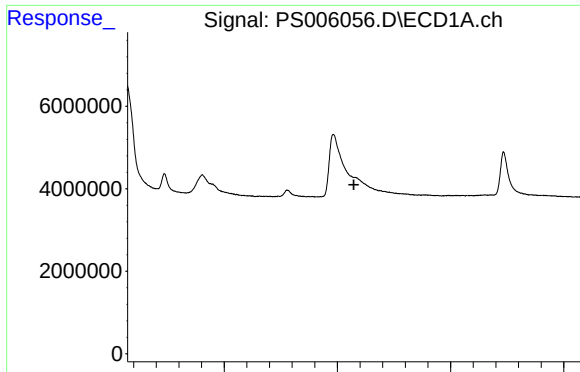

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.573 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

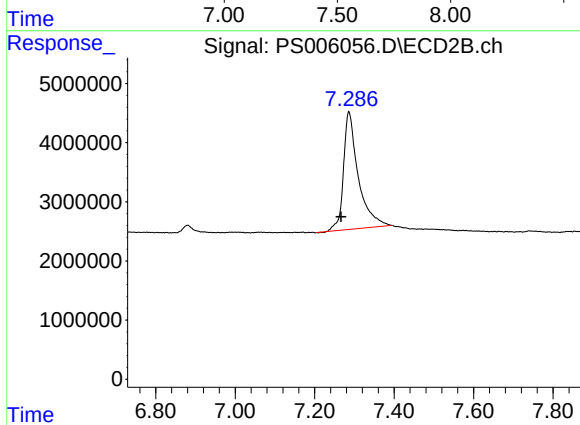


#12 2,4,5-T

R.T.: 7.286 min
Delta R.T.: 0.020 min
Response: 51265838
Conc: 20.62 ng/ml

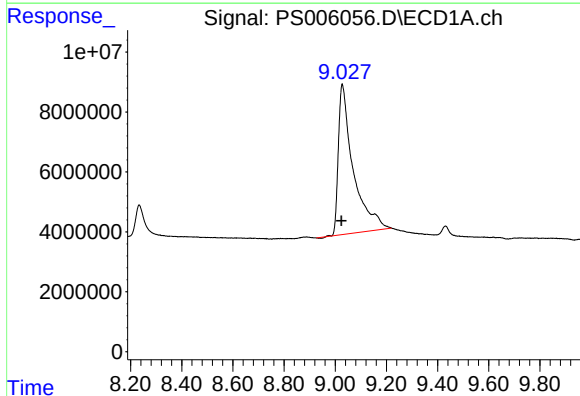


#15 Picloram

R.T.: 9.028 min
Delta R.T.: 0.004 min
Response: 202283283
Conc: 27.19 ng/ml

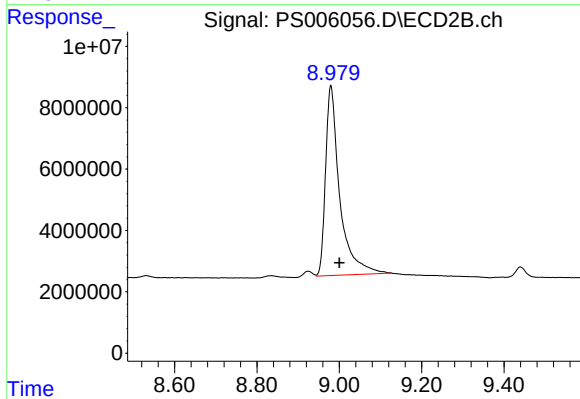

#15 Picloram


R.T.: 8.980 min
Delta R.T.: -0.021 min
Response: 147460020
Conc: 32.69 ng/ml

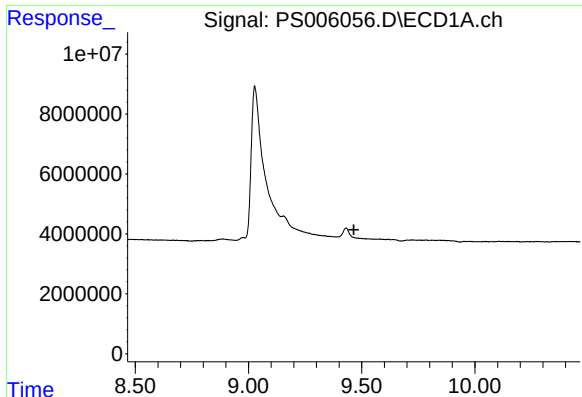

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

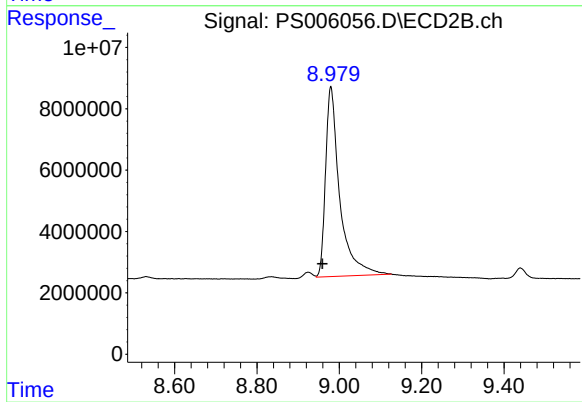

#16 DCPA

R.T.: 8.980 min
Delta R.T.: 0.020 min
Response: 147460020
Conc: 42.29 ng/ml