

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081419\
 Data File : PS006058.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2019 15:42
 Operator : SM\AJ
 Sample : IDOC BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 IDOC BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 08:22:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.494	5.222	311.4E6	188.8E6	360.730	383.905
Target Compounds							
9) T	2,4-D	6.556	0.000	222.7E6	0	273.309	N.D. #
12) T	2,4,5-T	7.511	7.311	31144763	40709923	6.299	16.375 #
15) T	Picloram	9.055	9.003	181.2E6	120.9E6	24.347	26.811
16) T	DCPA	0.000	9.003	0	120.9E6	N.D.	34.682



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081419\
Data File : PS006058.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2019 15:42
Operator : SM\AJ
Sample : IDOC BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
IDOC BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 08:22:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

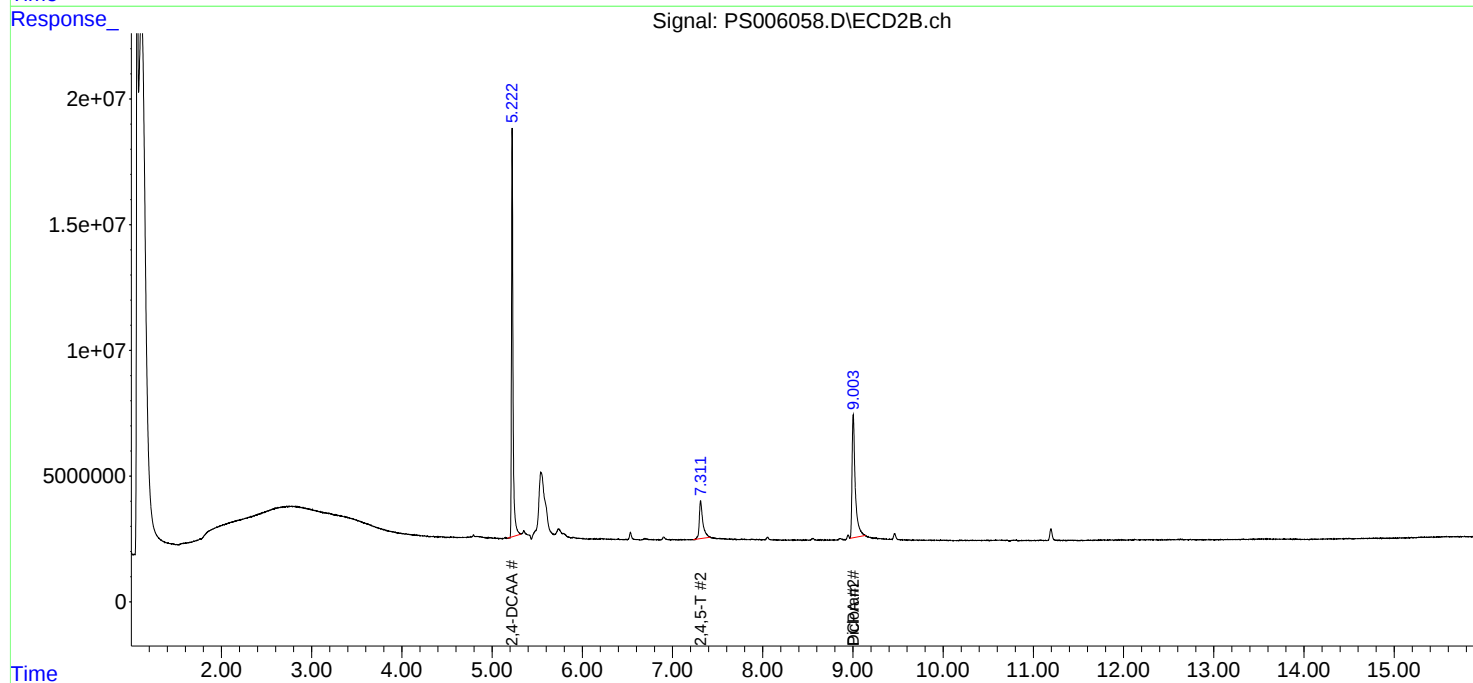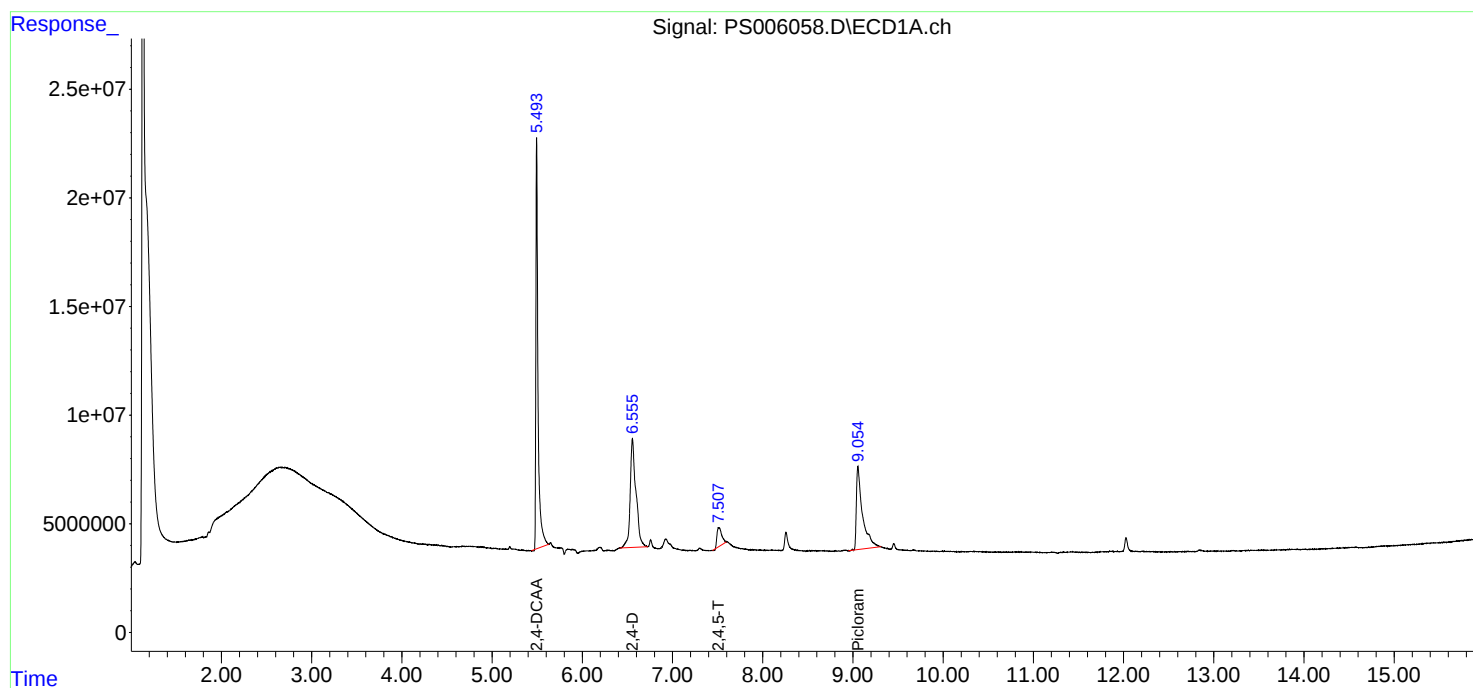


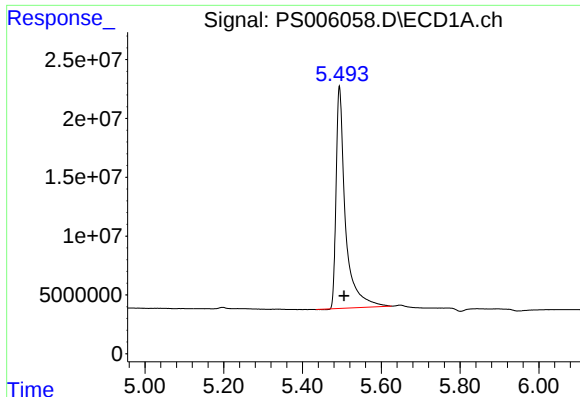

#4 2,4-DCAA


R.T.: 5.494 min
Delta R.T.: -0.011 min
Response: 311382391
Conc: 360.73 ng/ml

Instrument :
ECD_S
ClientSampleId :
IDOC BL

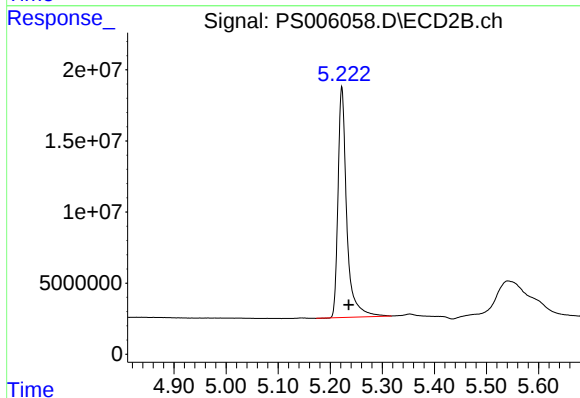


#4 2,4-DCAA

R.T.: 5.222 min
Delta R.T.: -0.013 min
Response: 188824369
Conc: 383.90 ng/ml

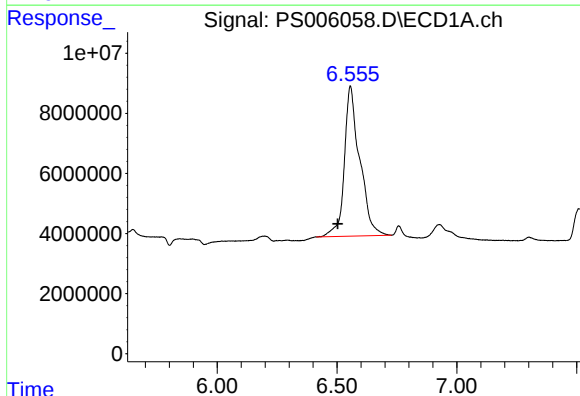


#9 2,4-D

R.T.: 6.556 min
Delta R.T.: 0.053 min
Response: 222687806
Conc: 273.31 ng/ml

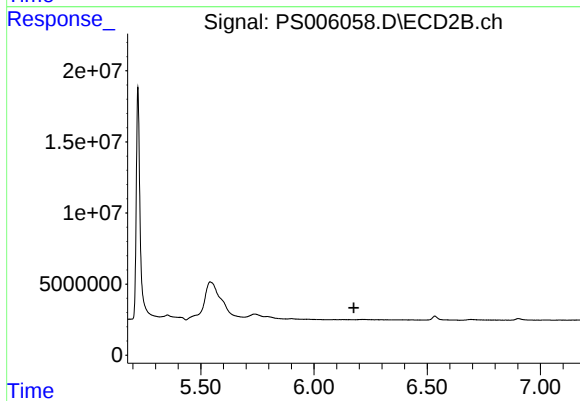

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.176 min
Response: 0
Conc: N.D.

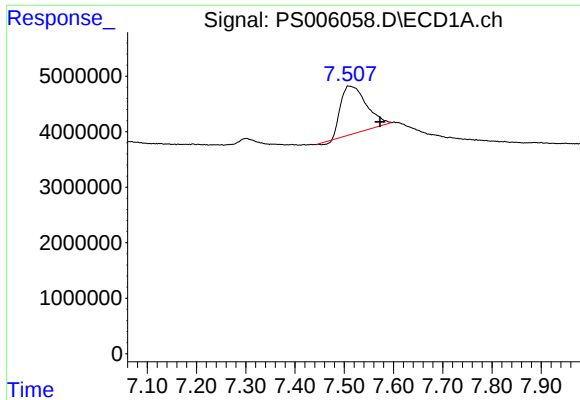

#12 2,4,5-T


R.T.: 7.511 min
Delta R.T.: -0.062 min
Response: 31144763
Conc: 6.30 ng/ml

Instrument :
ECD_S
ClientSampleId :
IDOC BL

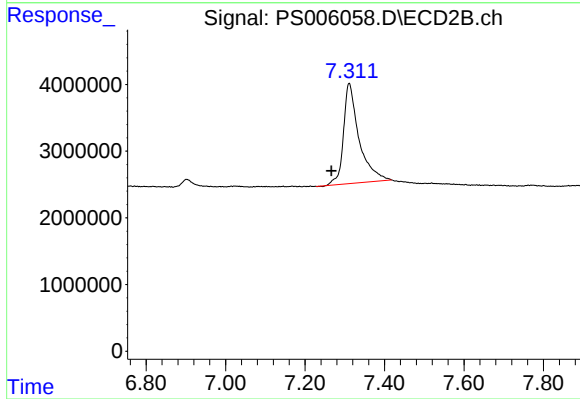


#12 2,4,5-T

R.T.: 7.311 min
Delta R.T.: 0.045 min
Response: 40709923
Conc: 16.38 ng/ml

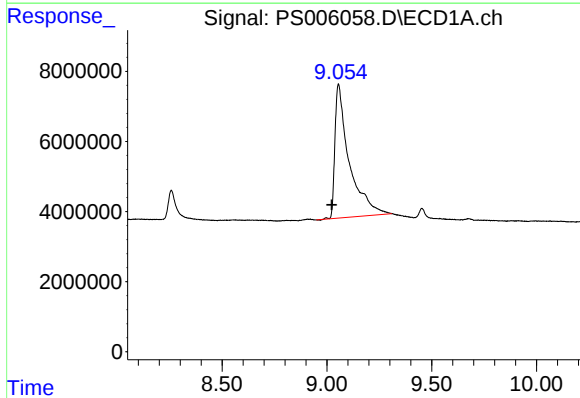


#15 Picloram

R.T.: 9.055 min
Delta R.T.: 0.032 min
Response: 181157865
Conc: 24.35 ng/ml

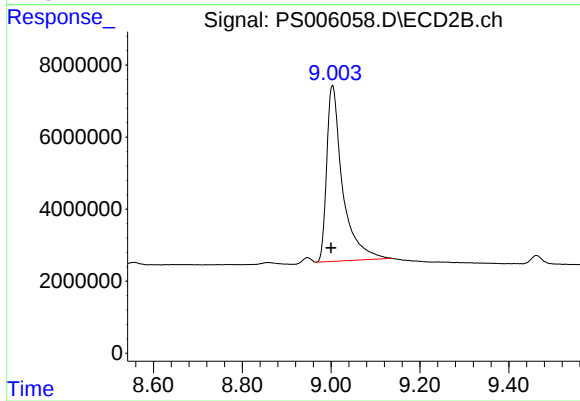

#15 Picloram


R.T.: 9.003 min
Delta R.T.: 0.003 min
Response: 120939765
Conc: 26.81 ng/ml

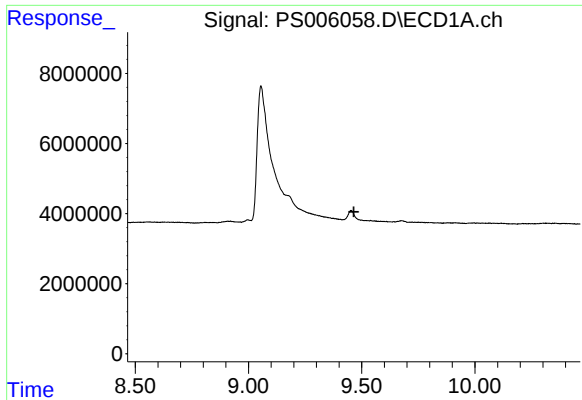

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
IDOC BL

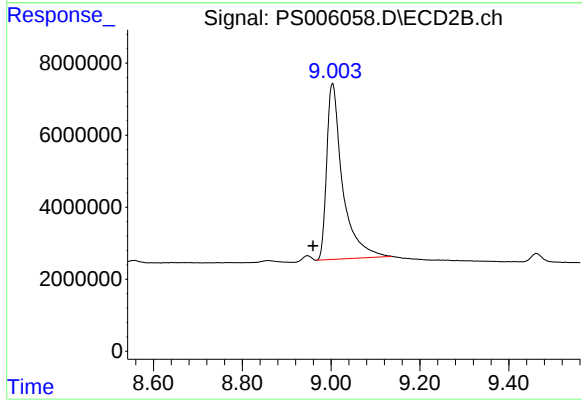

#16 DCPA

R.T.: 9.003 min
Delta R.T.: 0.044 min
Response: 120939765
Conc: 34.68 ng/ml