

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081419\
 Data File : PS006070.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2019 20:08
 Operator : SM\AJ
 Sample : K4245-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMP-25

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 08:26:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.485	5.215	276.7E6	172.2E6	320.605	350.142
Target Compounds							
1) T	Dalapon	2.117	1.742	-21729040	184.7E6	N.D.	294.286
2) T	3,5-DICHL...	0.000	4.543	0	30509776	N.D.	50.371
3) T	4-Nitroph...	5.292	0.000	8442701	0	22.489	N.D. #
7) T	MCPA	5.962	5.592	11765867	35142291	3.727	17.195 #
9) T	2,4-D	6.550	0.000	234.3E6	0	287.525	N.D. #
12) T	2,4,5-T	0.000	7.293	0	49611936	N.D.	19.956
15) T	Picloram	9.022	8.987	301.7E6	224.4E6	40.544	49.754
16) T	DCPA	0.000	8.987	0	224.4E6	N.D.	64.360



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081419\
Data File : PS006070.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2019 20:08
Operator : SM\AJ
Sample : K4245-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
COMP-25

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 08:26:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

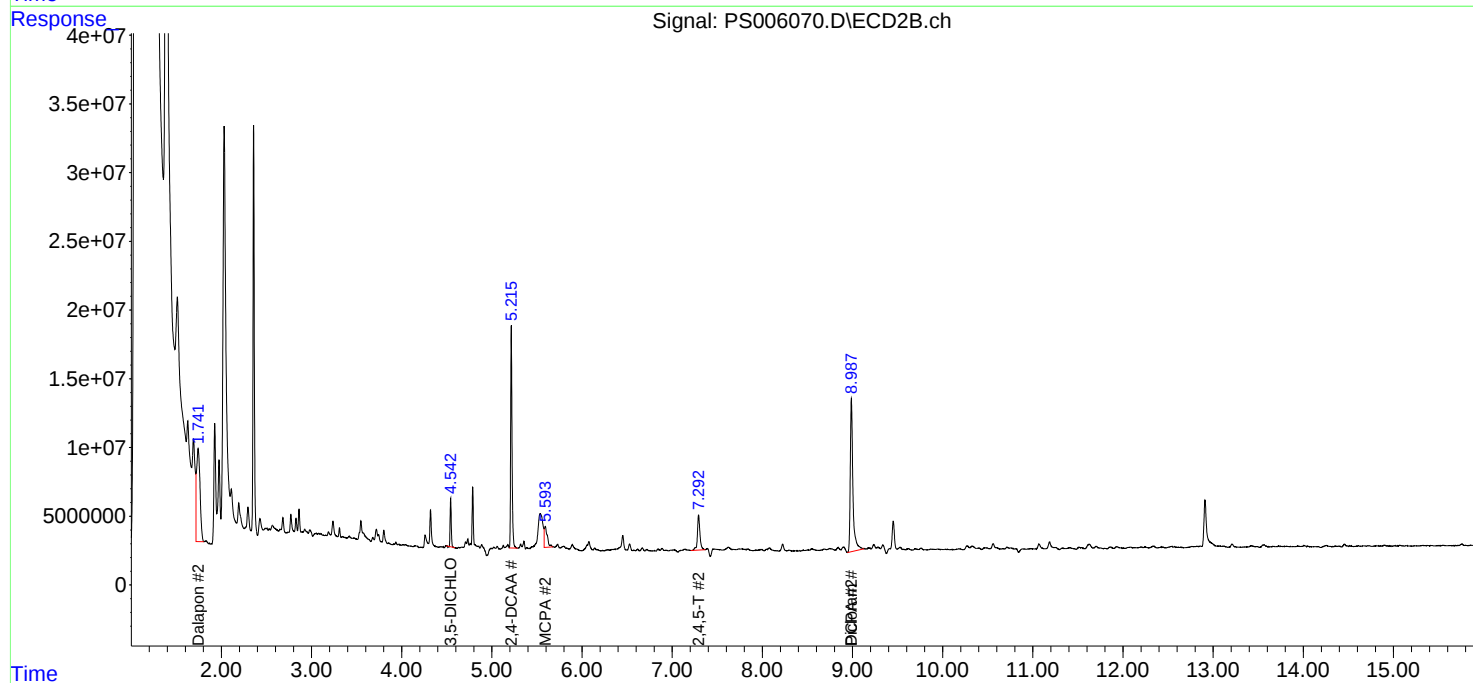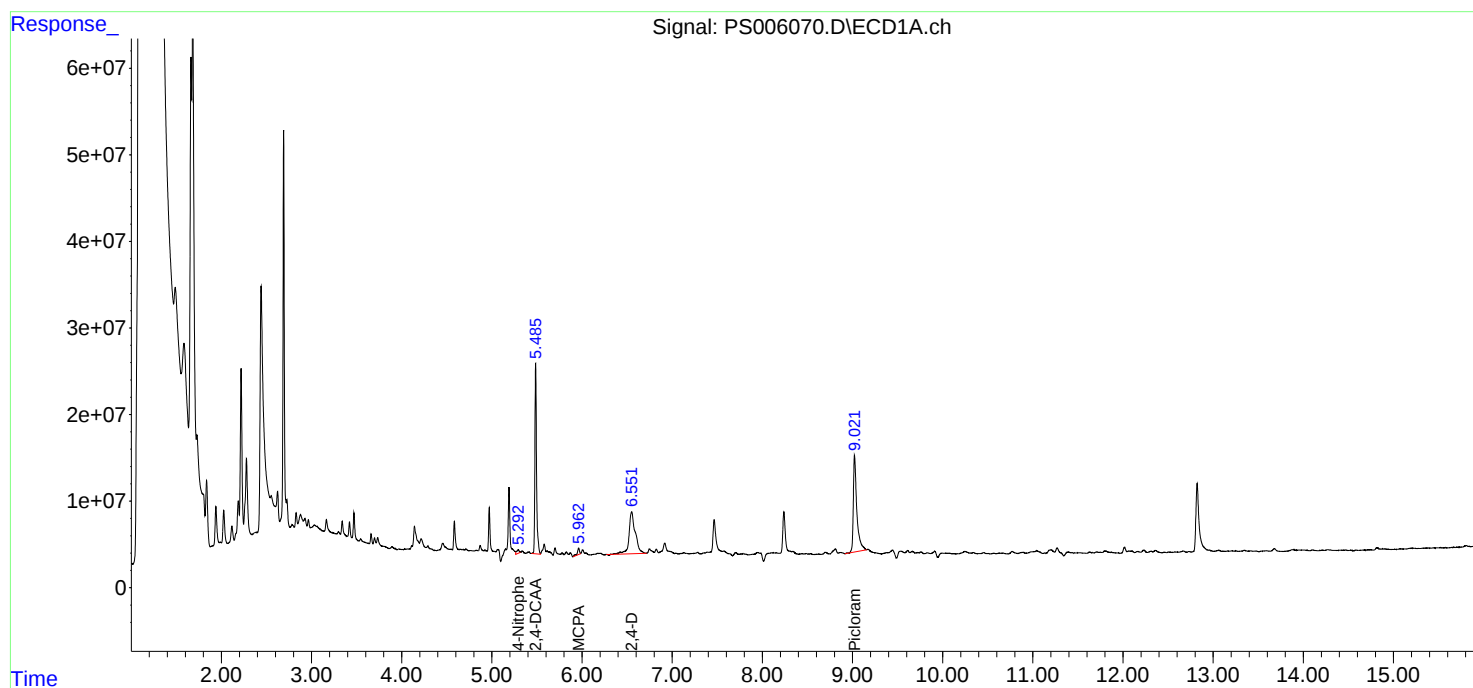


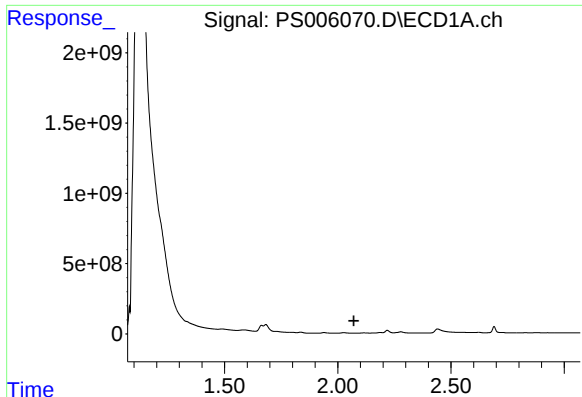

#1 Dalapon


R.T.: 2.117 min
Delta R.T.: 0.046 min
Response: -21729040
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-25

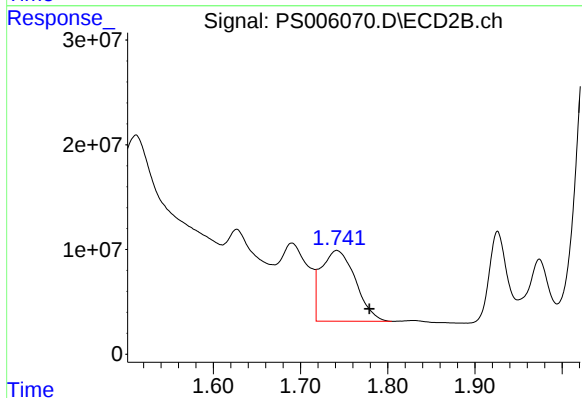


#1 Dalapon

R.T.: 1.742 min
Delta R.T.: -0.037 min
Response: 184662499
Conc: 294.29 ng/ml

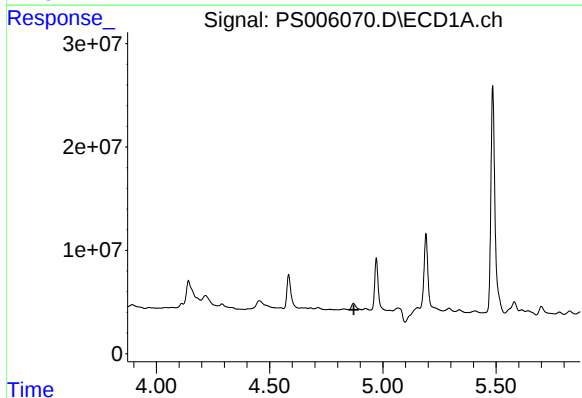


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.872 min
Response: 0
Conc: N.D.

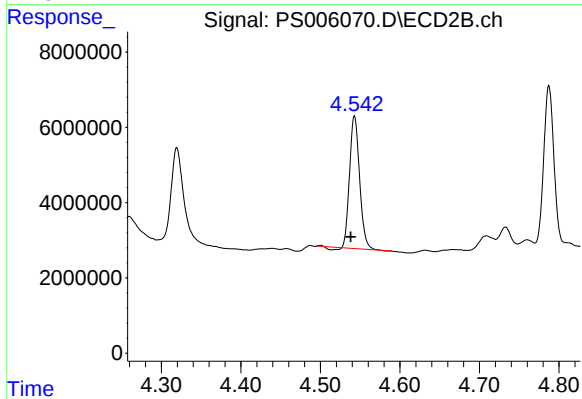

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.543 min
Delta R.T.: 0.005 min
Response: 30509776
Conc: 50.37 ng/ml

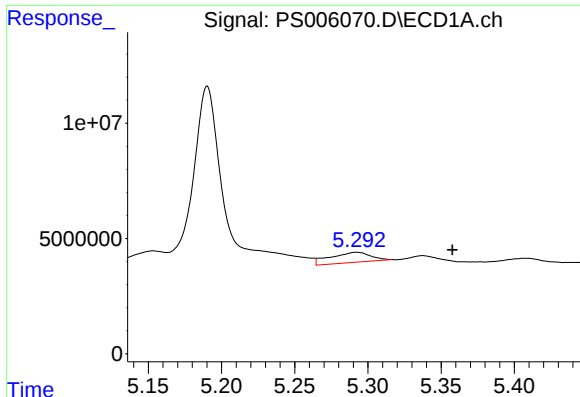

#3 4-Nitrophenol


R.T.: 5.292 min
Delta R.T.: -0.065 min
Response: 8442701
Conc: 22.49 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-25

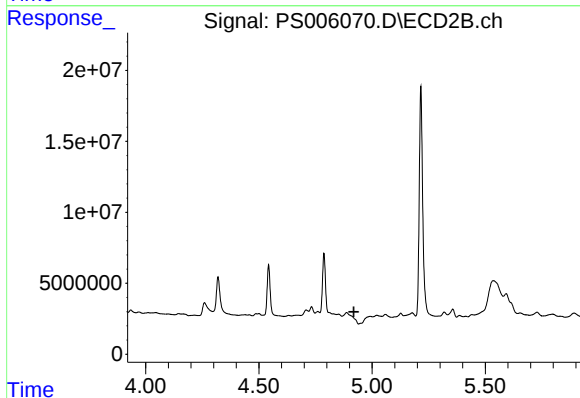


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 4.920 min
Response: 0
Conc: N.D.

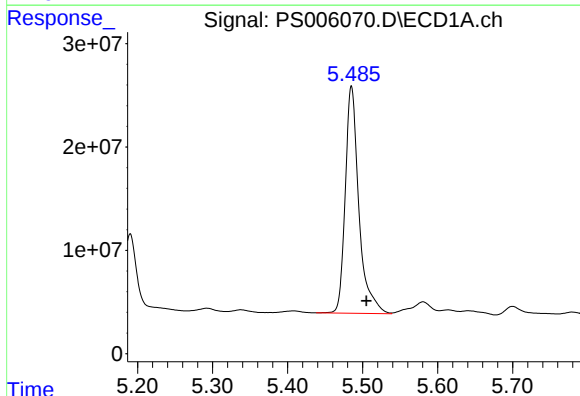


#4 2,4-DCAA

R.T.: 5.485 min
Delta R.T.: -0.020 min
Response: 276746631
Conc: 320.61 ng/ml

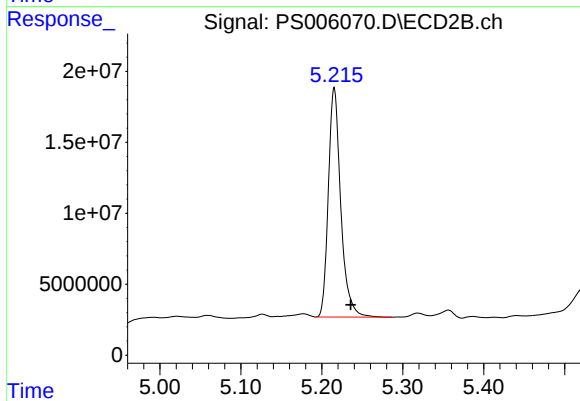

#4 2,4-DCAA


R.T.: 5.215 min
Delta R.T.: -0.020 min
Response: 172218092
Conc: 350.14 ng/ml

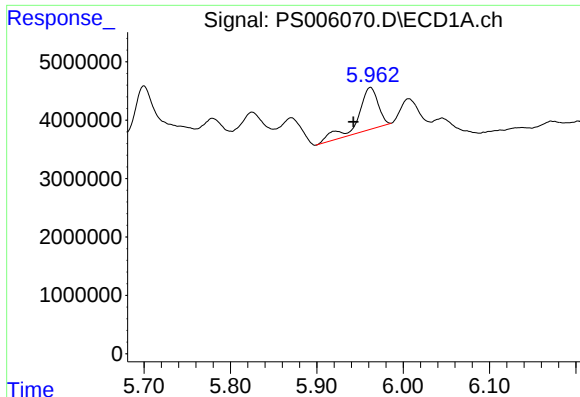

#7 MCPA


R.T.: 5.962 min
Delta R.T.: 0.019 min
Response: 11765867
Conc: 3.73 ug/ml

Instrument :
ECD_S
ClientSampleId :
COMP-25

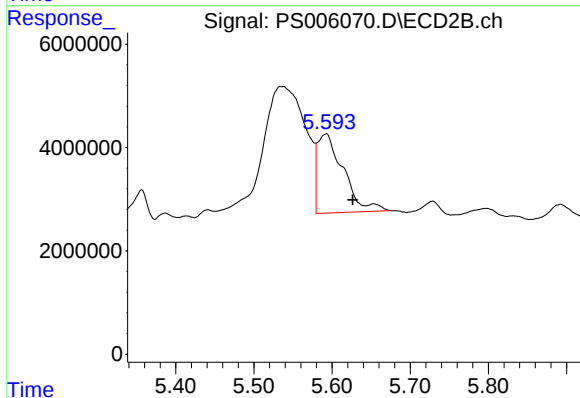


#7 MCPA

R.T.: 5.592 min
Delta R.T.: -0.035 min
Response: 35142291
Conc: 17.20 ug/ml

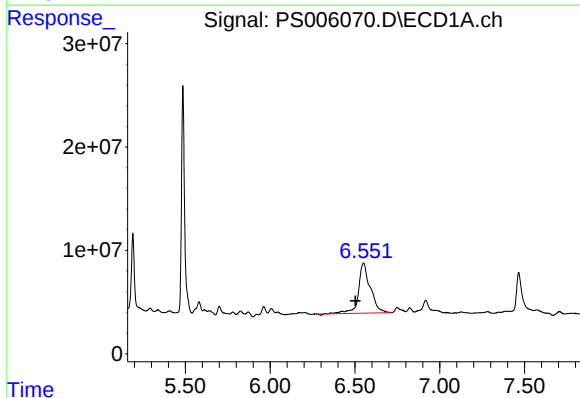


#9 2,4-D

R.T.: 6.550 min
Delta R.T.: 0.048 min
Response: 234270949
Conc: 287.53 ng/ml

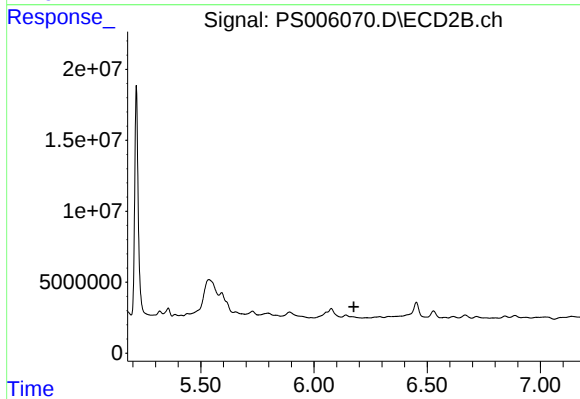

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.176 min
Response: 0
Conc: N.D.

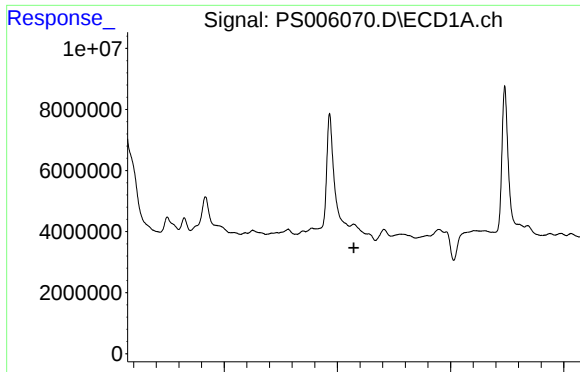

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.573 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-25

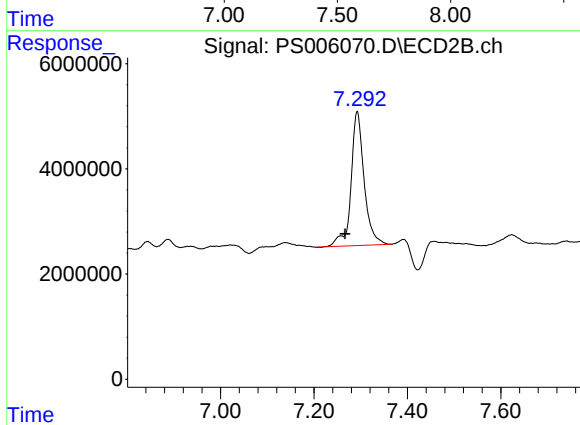


#12 2,4,5-T

R.T.: 7.293 min
Delta R.T.: 0.026 min
Response: 49611936
Conc: 19.96 ng/ml

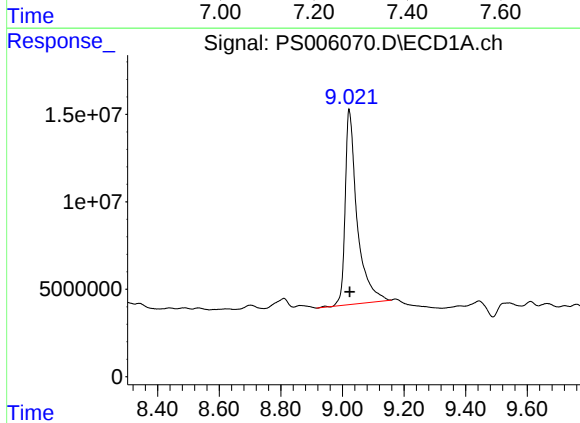


#15 Picloram

R.T.: 9.022 min
Delta R.T.: -0.002 min
Response: 301670573
Conc: 40.54 ng/ml

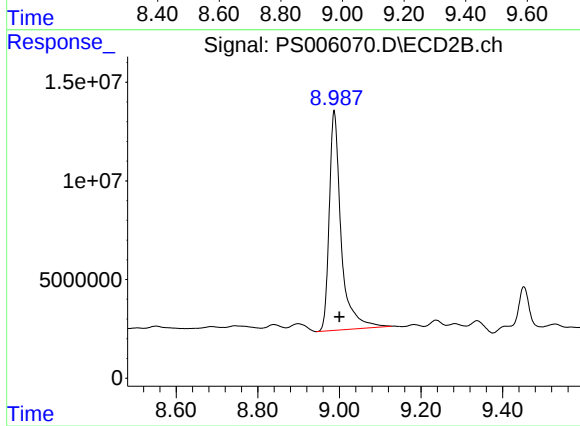

#15 Picloram


R.T.: 8.987 min
Delta R.T.: -0.013 min
Response: 224432737
Conc: 49.75 ng/ml

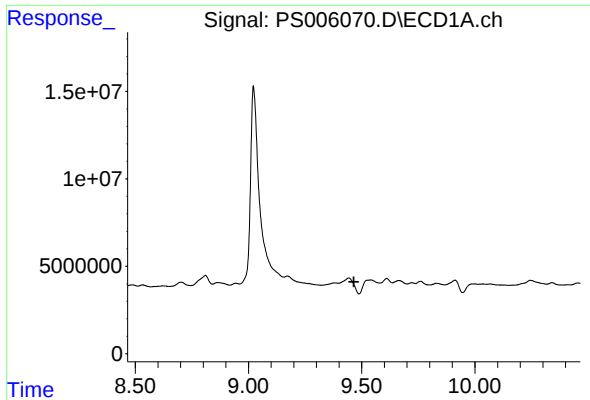

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-25

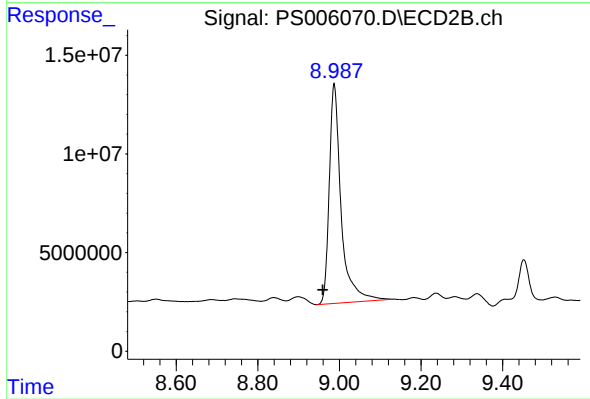

#16 DCPA

R.T.: 8.987 min
Delta R.T.: 0.028 min
Response: 224432737
Conc: 64.36 ng/ml