

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081419\
 Data File : PS006071.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2019 20:30
 Operator : SM\AJ
 Sample : K4245-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMP-26

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 08:26:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.502	5.233	266.5E6	170.6E6	308.790	346.828
Target Compounds							
1) T	Dalapon	2.044	1.758	41431159	153.8E6	38.023	245.062 #
2) T	3,5-DICHL...	0.000	4.561	0	15338420	N.D.	25.323
5) T	DICAMBA	5.597	0.000	17757676	0	5.529	N.D. #
7) T	MCPA	0.000	5.609	0	32074139	N.D.	15.694
9) T	2,4-D	6.567	0.000	216.6E6	0	265.778	N.D. #
15) T	Picloram	0.000	9.013	0	29360326	N.D.	6.509
16) T	DCPA	0.000	9.013	0	29360326	N.D.	8.420



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081419\
Data File : PS006071.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2019 20:30
Operator : SM\AJ
Sample : K4245-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
COMP-26

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 08:26:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

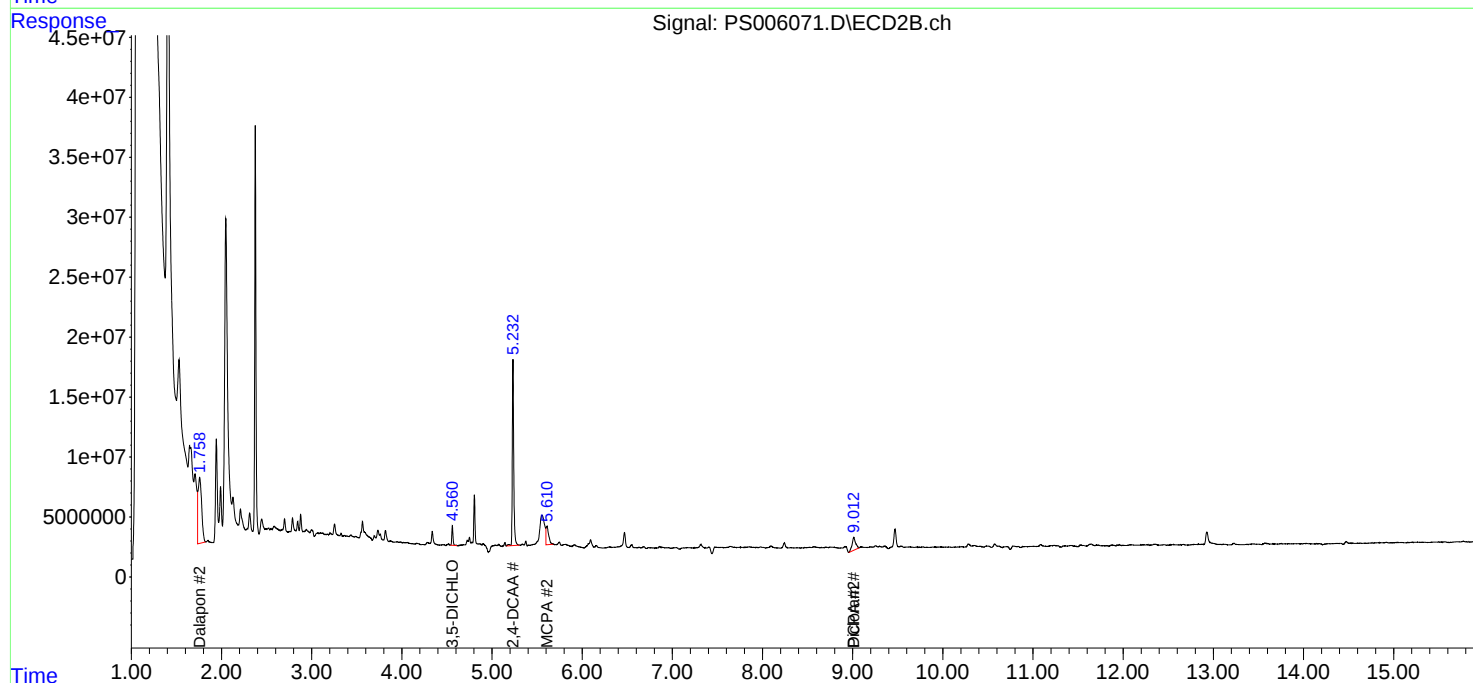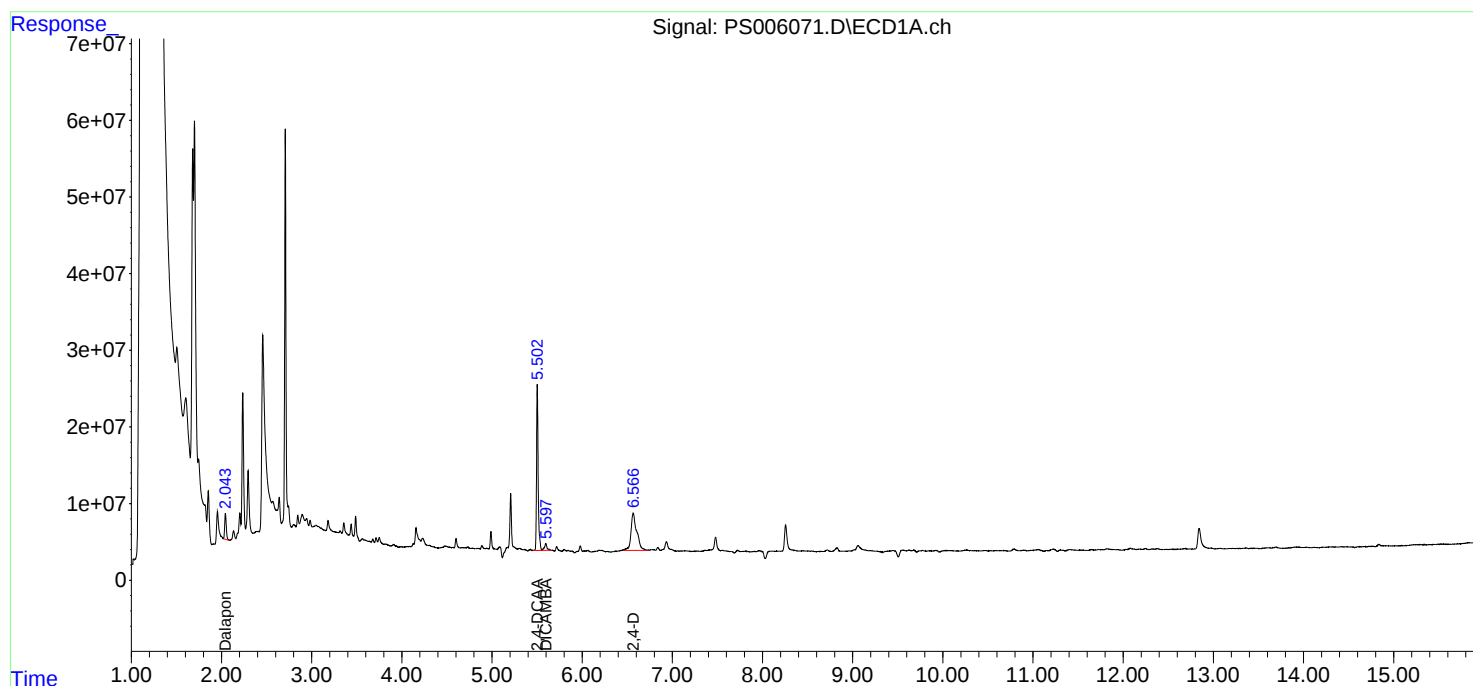


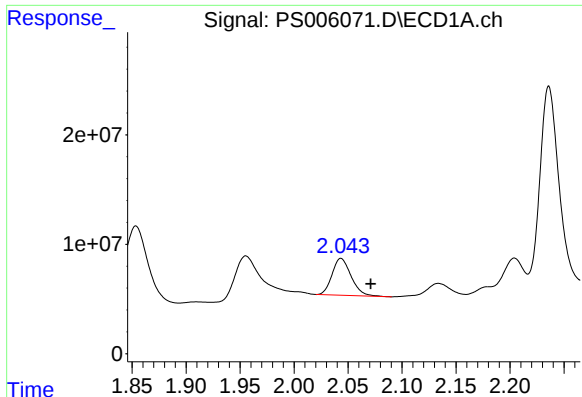

#1 Dalapon


R.T.: 2.044 min
Delta R.T.: -0.027 min
Response: 41431159
Conc: 38.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-26

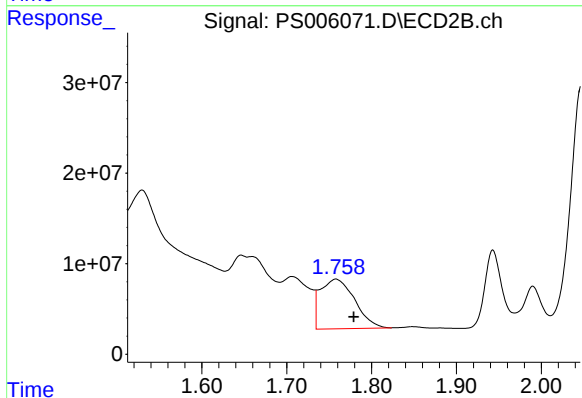


#1 Dalapon

R.T.: 1.758 min
Delta R.T.: -0.021 min
Response: 153774553
Conc: 245.06 ng/ml

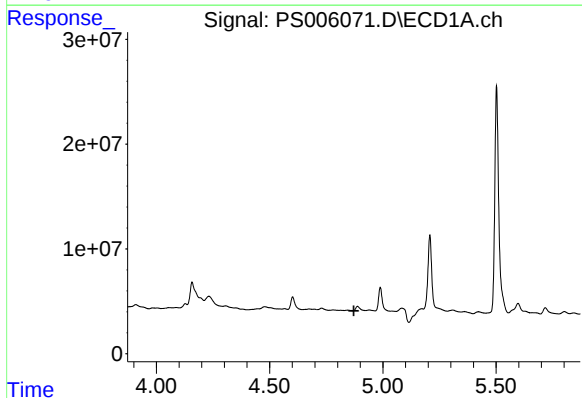


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.872 min
Response: 0
Conc: N.D.

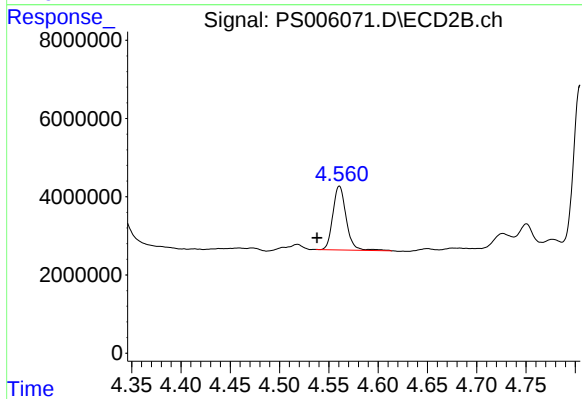

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.561 min
Delta R.T.: 0.023 min
Response: 15338420
Conc: 25.32 ng/ml

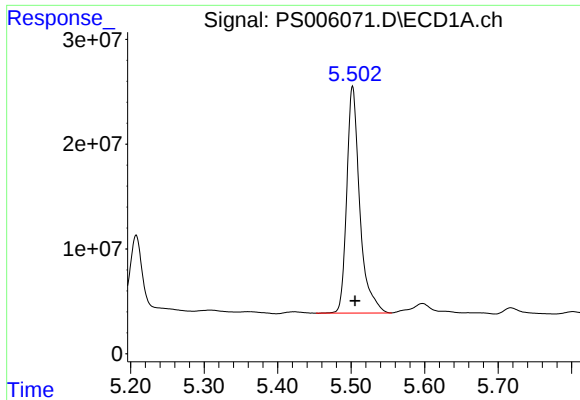

#4 2,4-DCAA


R.T.: 5.502 min
Delta R.T.: -0.003 min
Response: 266547781
Conc: 308.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-26

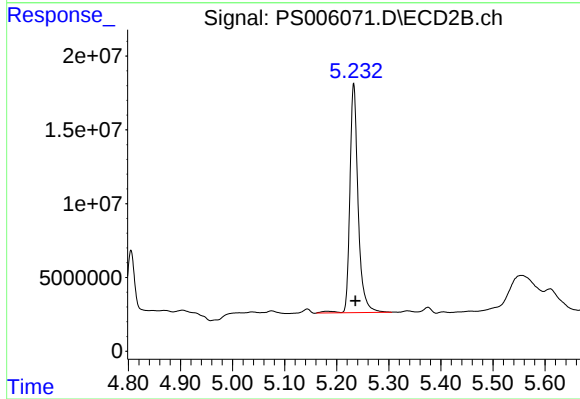


#4 2,4-DCAA

R.T.: 5.233 min
Delta R.T.: -0.003 min
Response: 170588166
Conc: 346.83 ng/ml

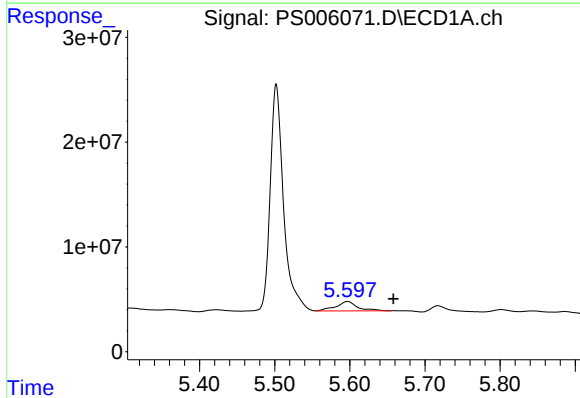


#5 DICAMBA

R.T.: 5.597 min
Delta R.T.: -0.061 min
Response: 17757676
Conc: 5.53 ng/ml

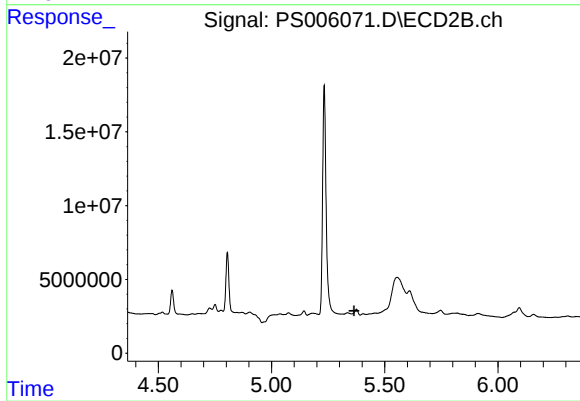

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.364 min
Response: 0
Conc: N.D.

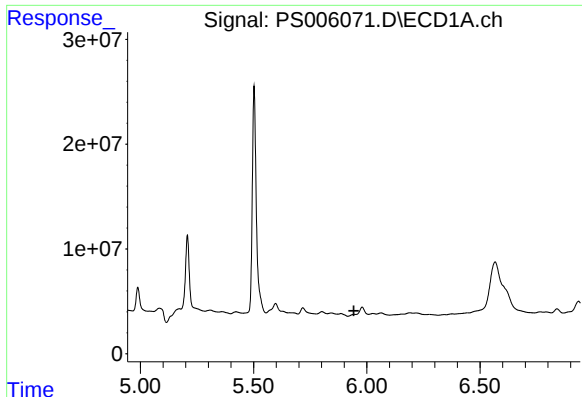

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.943 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-26

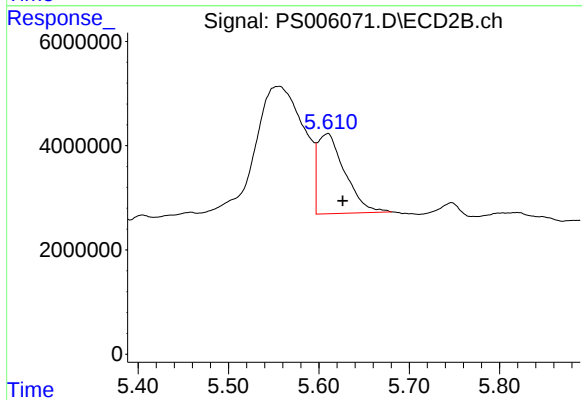


#7 MCPA

R.T.: 5.609 min
Delta R.T.: -0.017 min
Response: 32074139
Conc: 15.69 ug/ml

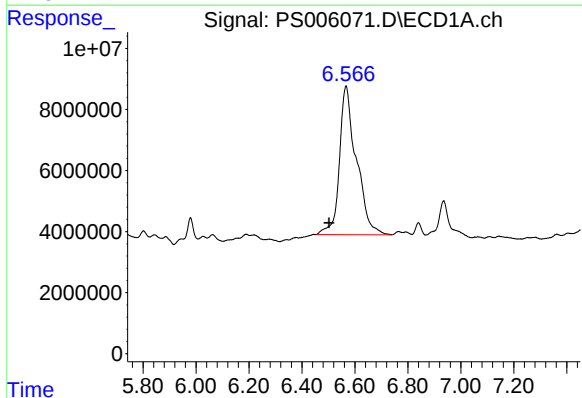


#9 2,4-D

R.T.: 6.567 min
Delta R.T.: 0.064 min
Response: 216551871
Conc: 265.78 ng/ml

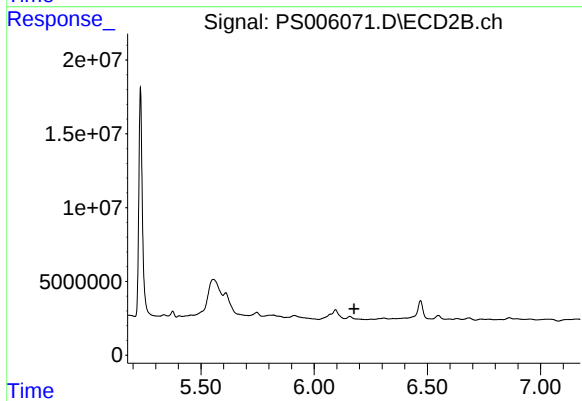

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.176 min
Response: 0
Conc: N.D.

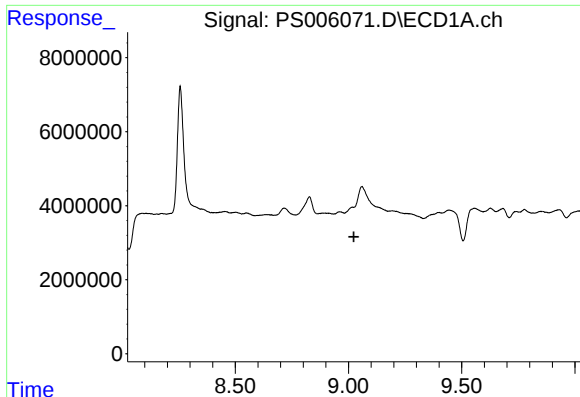

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 9.024 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-26

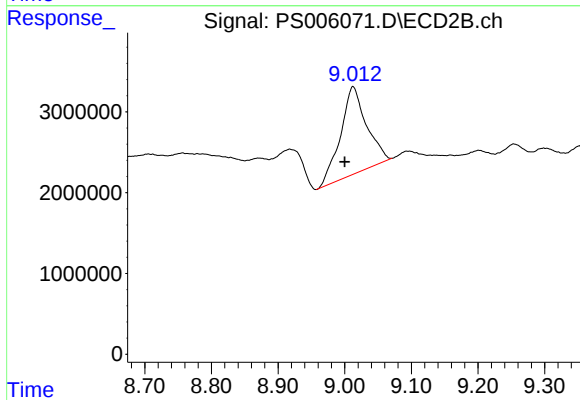


#15 Picloram

R.T.: 9.013 min
Delta R.T.: 0.013 min
Response: 29360326
Conc: 6.51 ng/ml

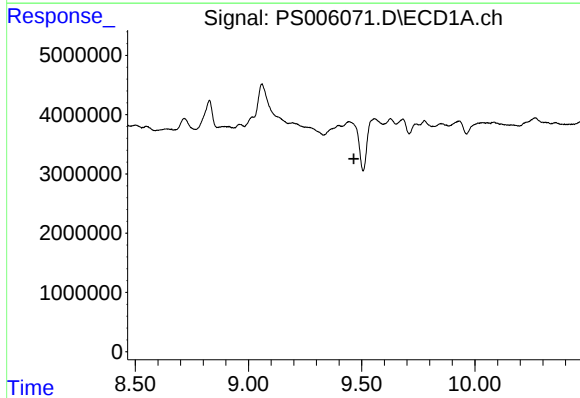

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.465 min
Response: 0
Conc: N.D.

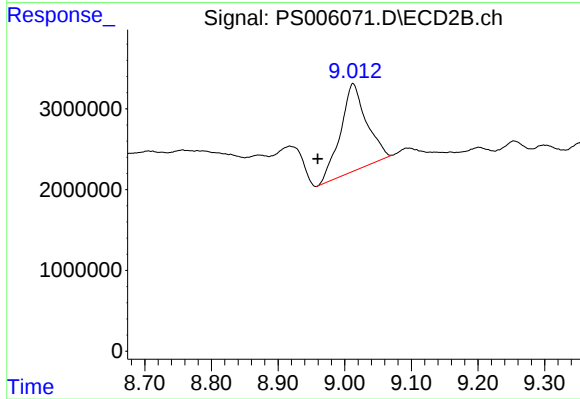

#16 DCPA

R.T.: 9.013 min
Delta R.T.: 0.053 min
Response: 29360326
Conc: 8.42 ng/ml