

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081419\
 Data File : PS006072.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2019 20:52
 Operator : SM\AJ
 Sample : K4245-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 COMP-27

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 08:27:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.485	5.216	280.5E6	168.9E6	324.984	343.442
Target Compounds							
1) T	Dalapon	2.118	1.743	6246081	184.0E6	5.732	293.196 #
2) T	3,5-DICHL...	4.866	4.545	135.8E6	13379161	125.915	22.089 #
5) T	DICAMBA	0.000	5.358	0	77184482	N.D.	41.846
7) T	MCPA	5.963	5.593	15294826	33122413	4.845	16.207 #
8) T	DICHLORPROP	0.000	5.891	0	17437930	N.D.	39.221
9) T	2,4-D	6.550	0.000	256.6E6	0	314.933	N.D. #
15) T	Picloram	8.987	8.993	93714643	36091935	12.595	8.001 #
16) T	DCPA	0.000	8.993	0	36091935	N.D.	10.350



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081419\
Data File : PS006072.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2019 20:52
Operator : SM\AJ
Sample : K4245-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
COMP-27

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 08:27:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

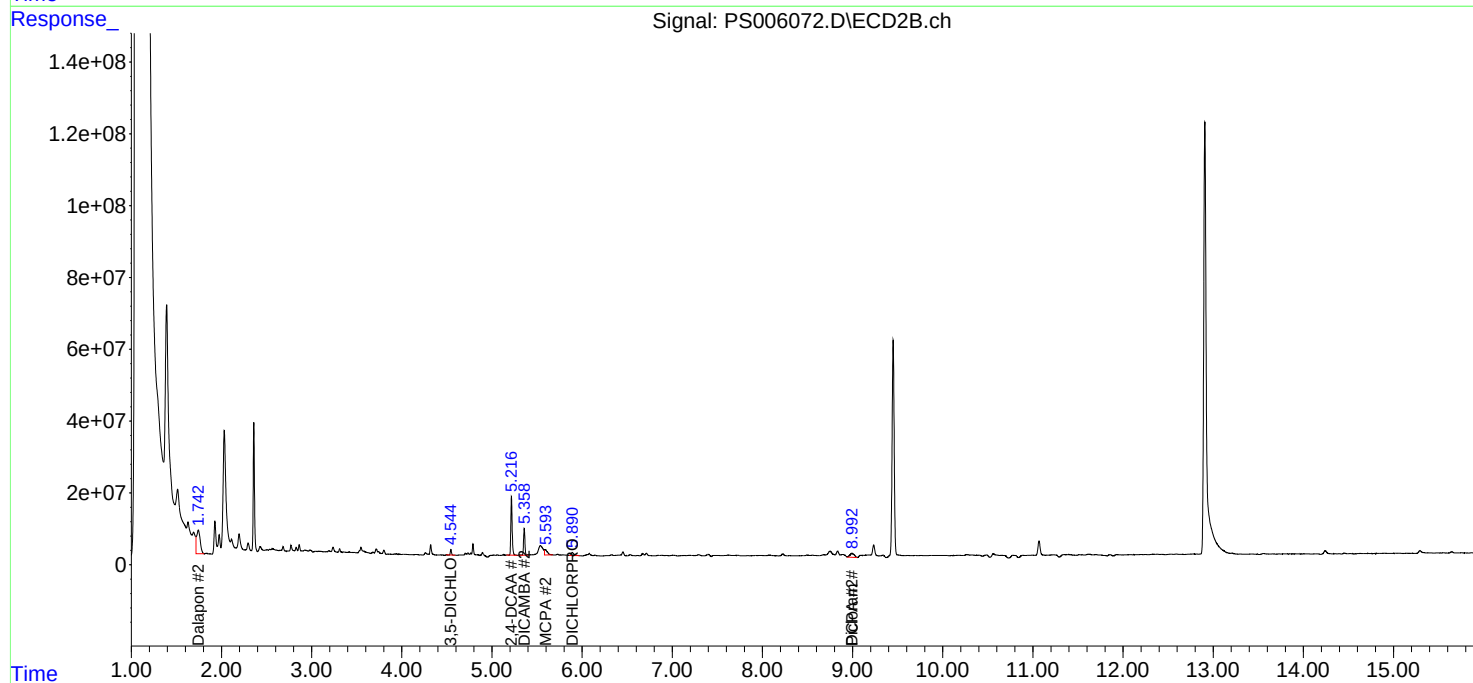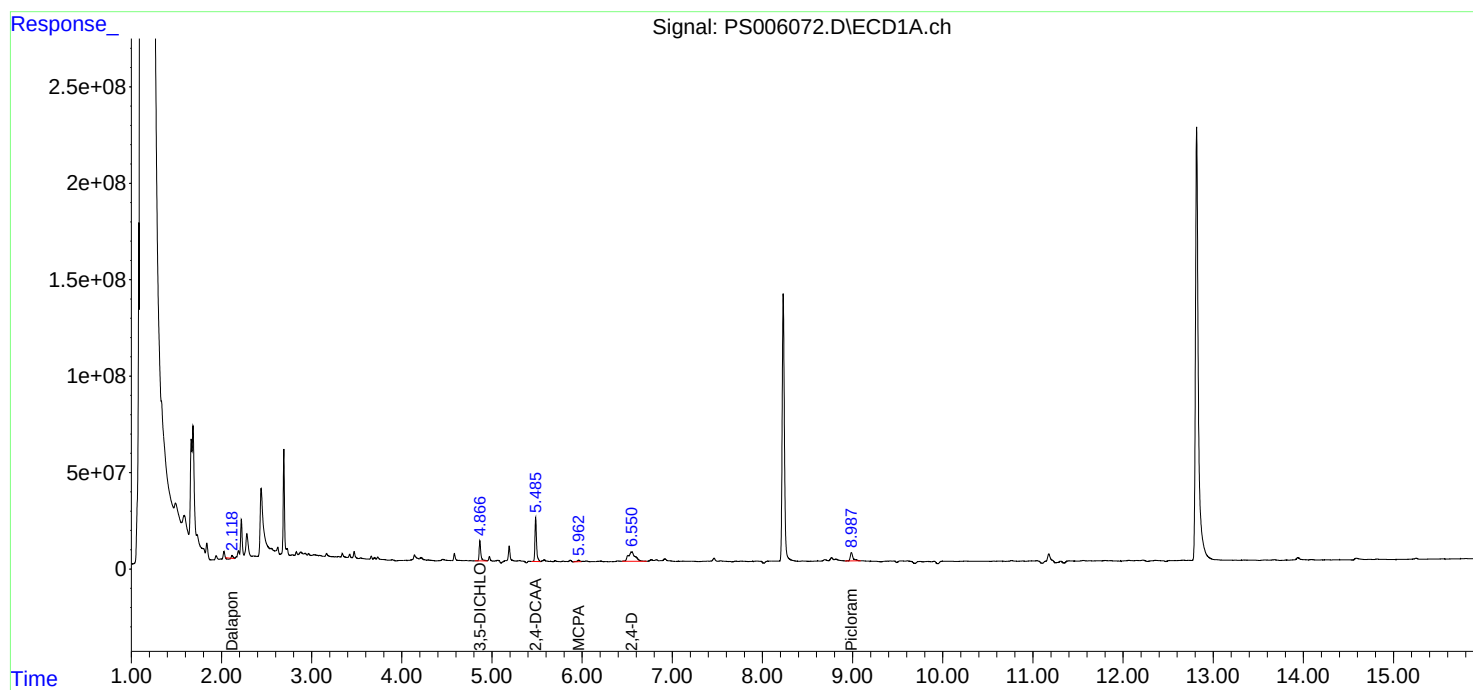


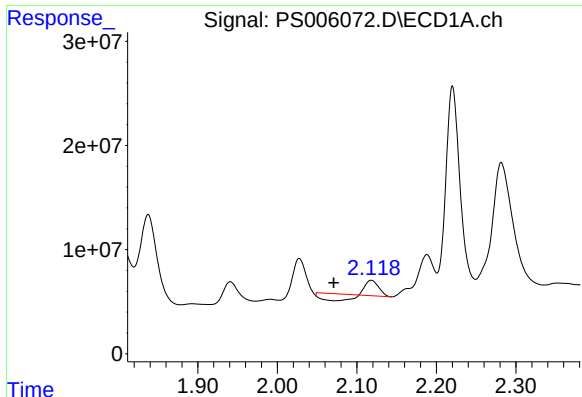

#1 Dalapon


R.T.: 2.118 min
Delta R.T.: 0.047 min
Response: 6246081
Conc: 5.73 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-27

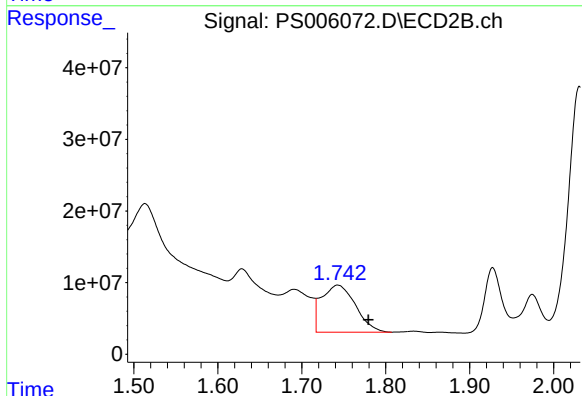


#1 Dalapon

R.T.: 1.743 min
Delta R.T.: -0.036 min
Response: 183978556
Conc: 293.20 ng/ml

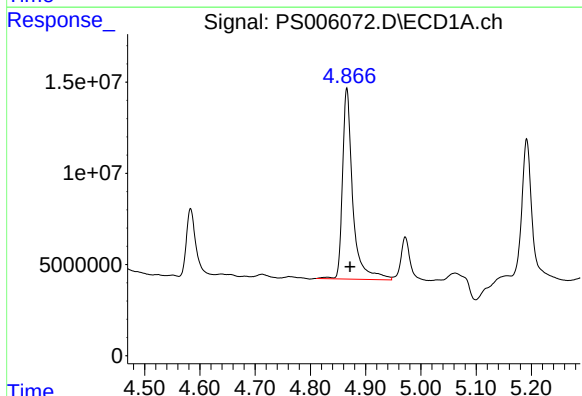


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.866 min
Delta R.T.: -0.006 min
Response: 135753599
Conc: 125.92 ng/ml

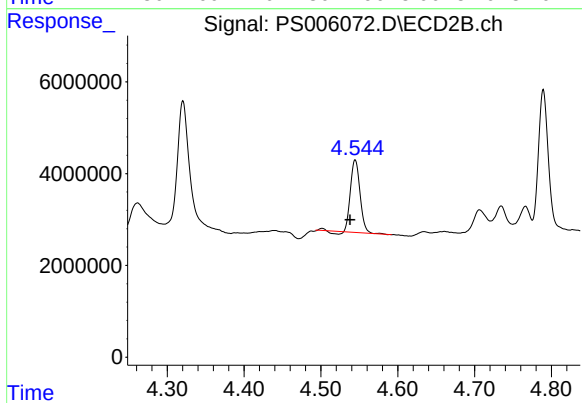

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.545 min
Delta R.T.: 0.007 min
Response: 13379161
Conc: 22.09 ng/ml

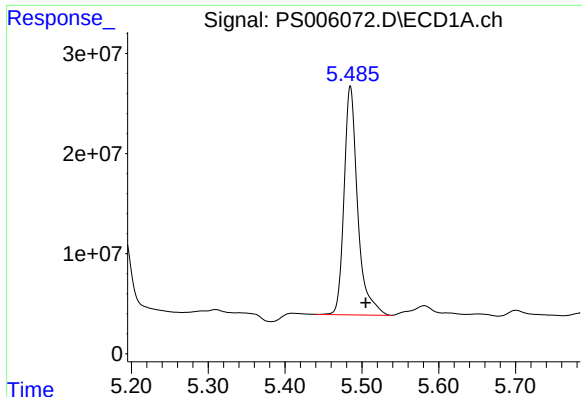

#4 2,4-DCAA


R.T.: 5.485 min
Delta R.T.: -0.020 min
Response: 280526105
Conc: 324.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-27

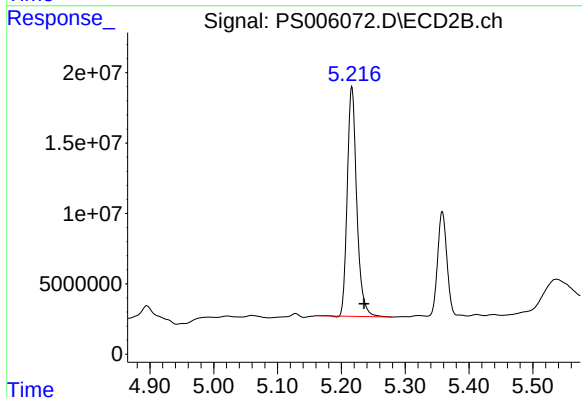


#4 2,4-DCAA

R.T.: 5.216 min
Delta R.T.: -0.019 min
Response: 168922521
Conc: 343.44 ng/ml

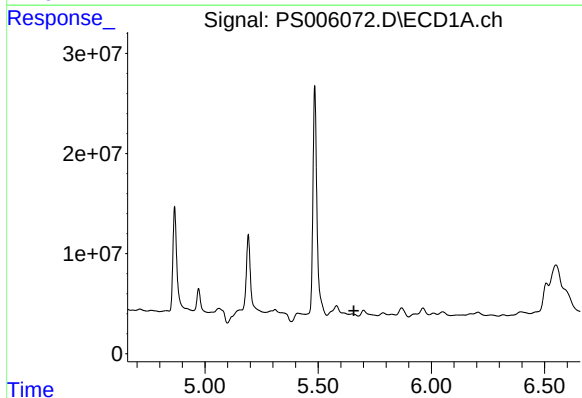


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.658 min
Response: 0
Conc: N.D.

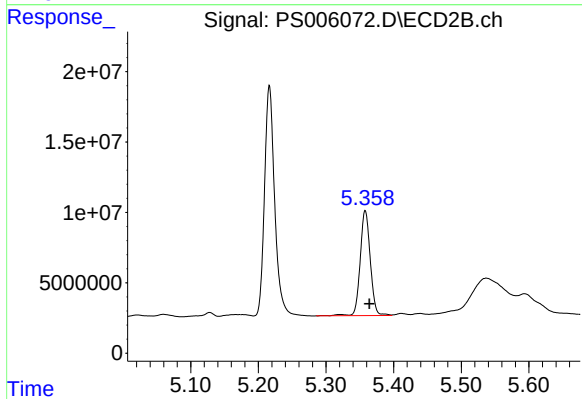

#5 DICAMBA


R.T.: 5.358 min
Delta R.T.: -0.006 min
Response: 77184482
Conc: 41.85 ng/ml

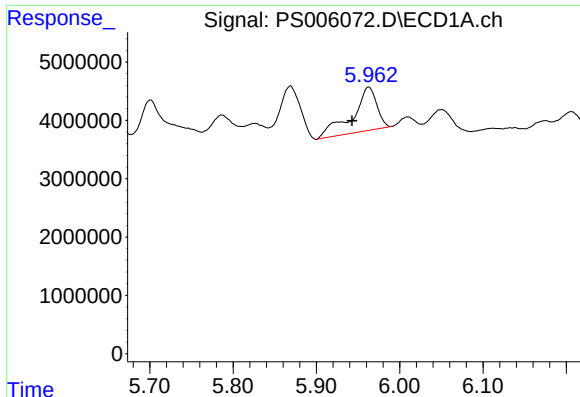

#7 MCPA


R.T.: 5.963 min
Delta R.T.: 0.020 min
Response: 15294826
Conc: 4.84 ug/ml

Instrument :
ECD_S
ClientSampleId :
COMP-27

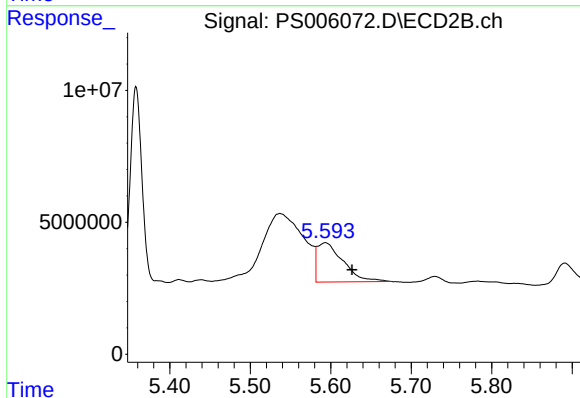


#7 MCPA

R.T.: 5.593 min
Delta R.T.: -0.033 min
Response: 33122413
Conc: 16.21 ug/ml

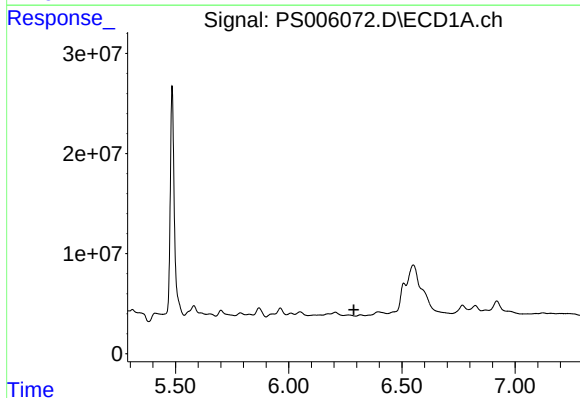


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.288 min
Response: 0
Conc: N.D.

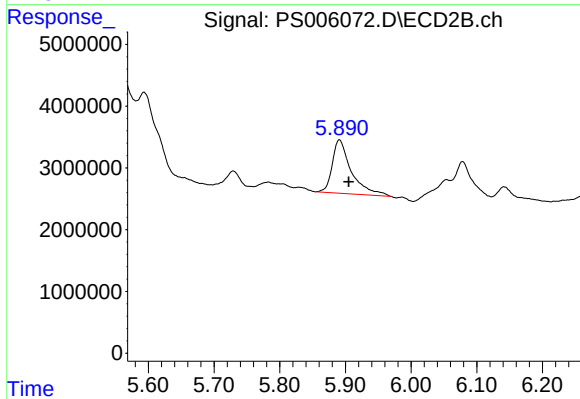

#8 DICHLORPROP


R.T.: 5.891 min
Delta R.T.: -0.014 min
Response: 17437930
Conc: 39.22 ng/ml

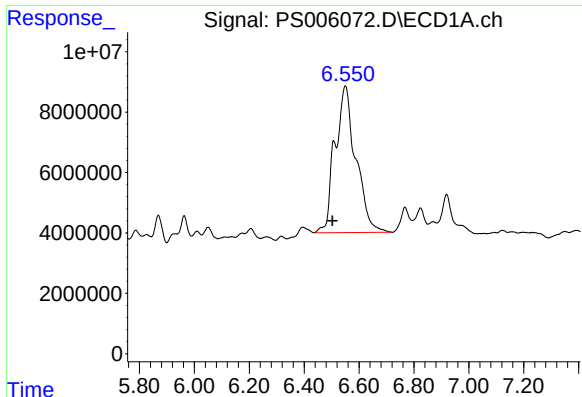

#9 2,4-D


R.T.: 6.550 min
Delta R.T.: 0.047 min
Response: 256602786
Conc: 314.93 ng/ml

Instrument :
ECD_S
ClientSampleId :
COMP-27

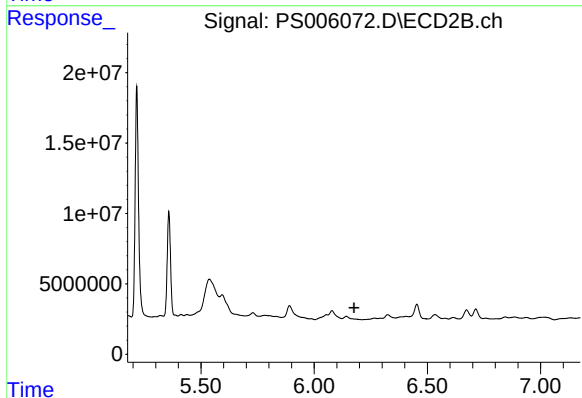


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.176 min
Response: 0
Conc: N.D.

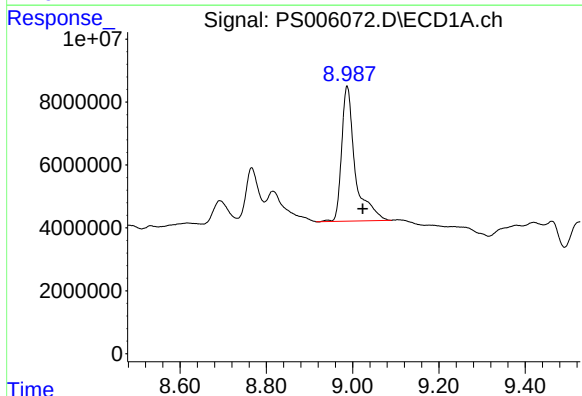


#15 Picloram

R.T.: 8.987 min
Delta R.T.: -0.036 min
Response: 93714643
Conc: 12.60 ng/ml

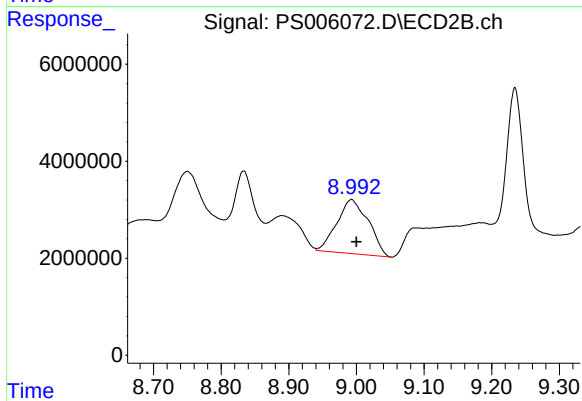

#15 Picloram


R.T.: 8.993 min
Delta R.T.: -0.008 min
Response: 36091935
Conc: 8.00 ng/ml

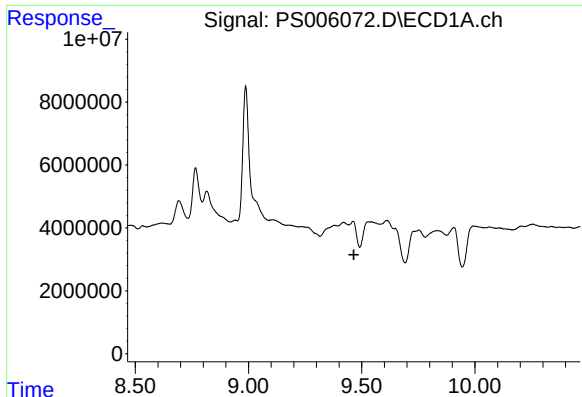

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
COMP-27

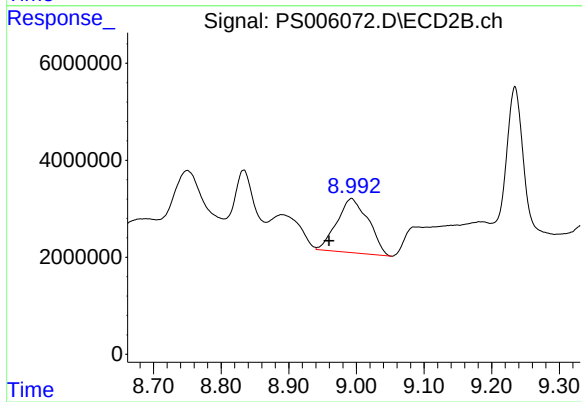

#16 DCPA

R.T.: 8.993 min
Delta R.T.: 0.033 min
Response: 36091935
Conc: 10.35 ng/ml