

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081419\
 Data File : PS006082.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2019 00:33
 Operator : SM\AJ
 Sample : PB122279TB
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB122279TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 08:30:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.492	5.221	126.8E6	88438760	146.877	179.808
Target Compounds							
1) T	Dalapon	2.120	1.744	989745	76587339	<MDL	122.053 #
9) T	2,4-D	6.550	0.000	193.6E6	0	237.588	N.D. #
12) T	2,4,5-T	0.000	7.301	0	26426512	N.D.	10.630
15) T	Picloram	9.032	8.994	163.5E6	105.3E6	21.971	23.354
16) T	DCPA	0.000	8.994	0	105.3E6	N.D.	30.210



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081419\
Data File : PS006082.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2019 00:33
Operator : SM\AJ
Sample : PB122279TB
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB122279TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 08:30:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

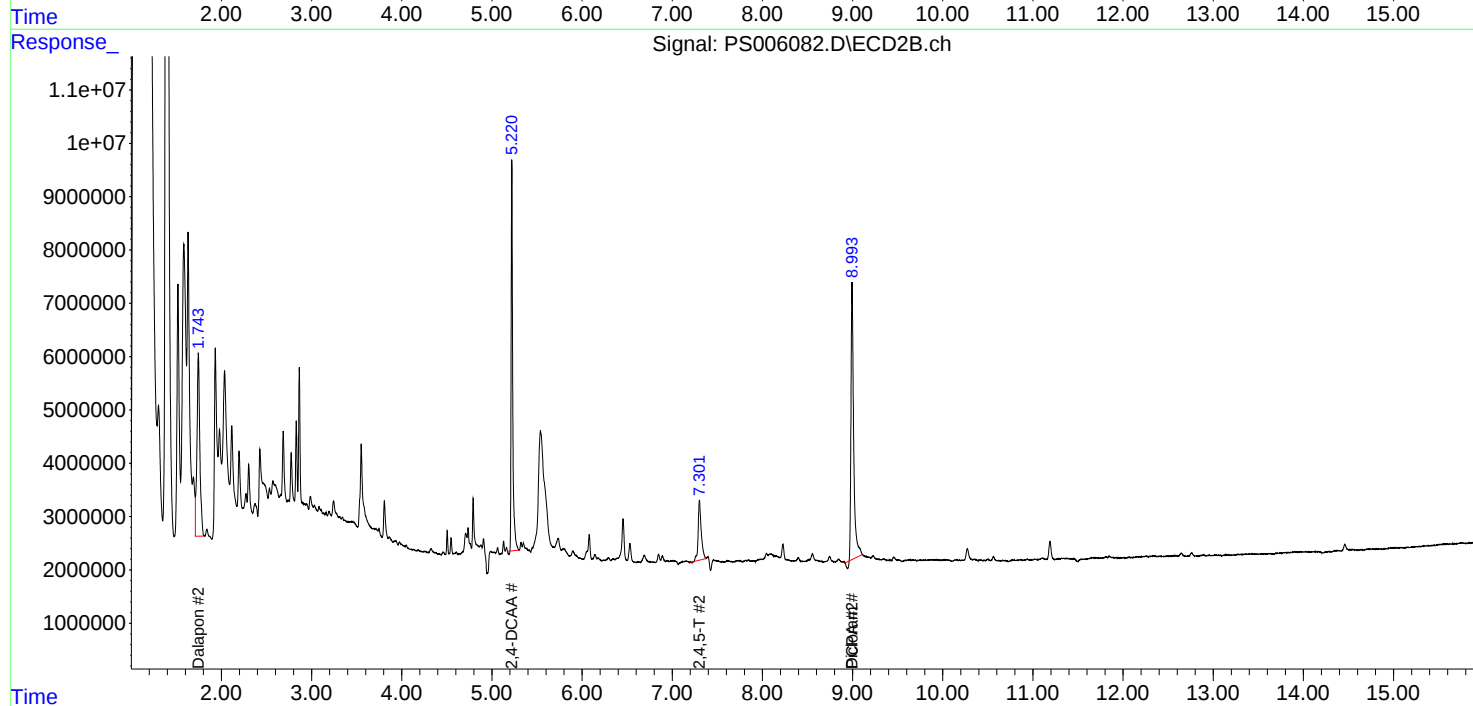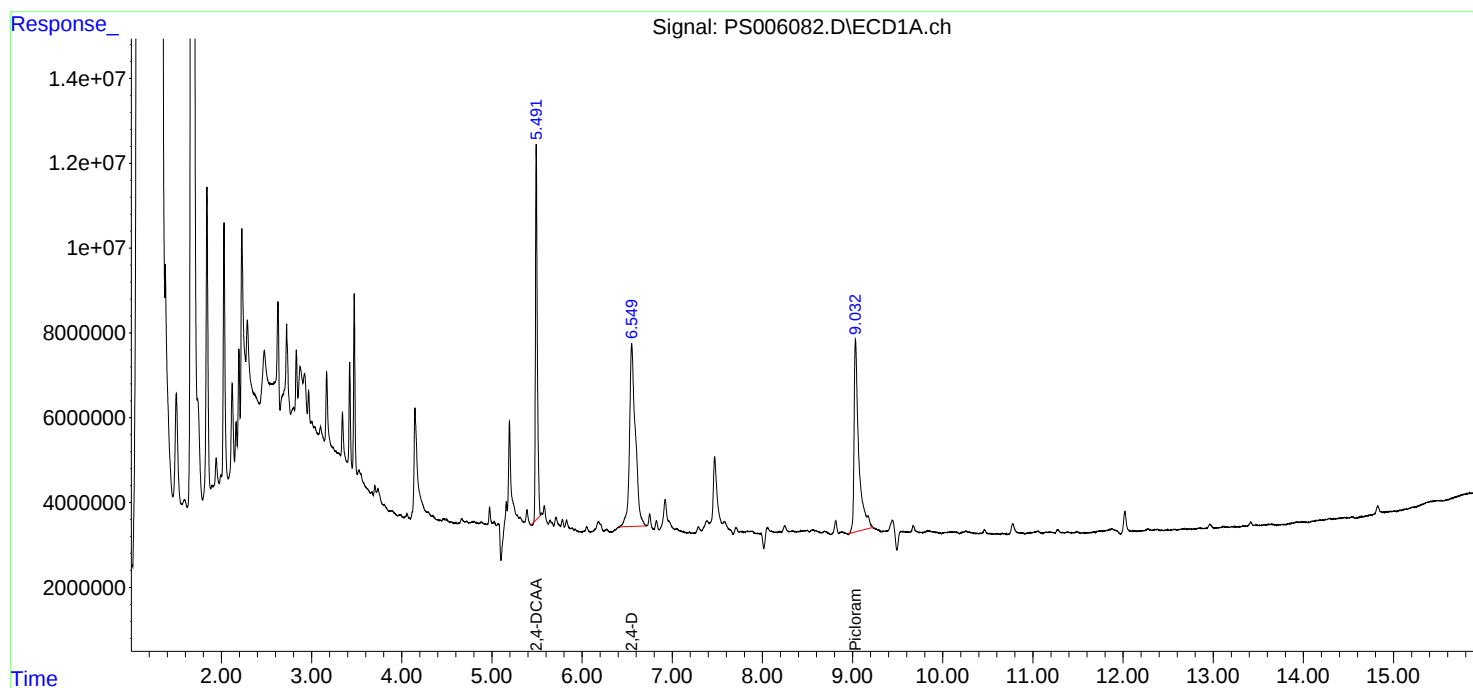


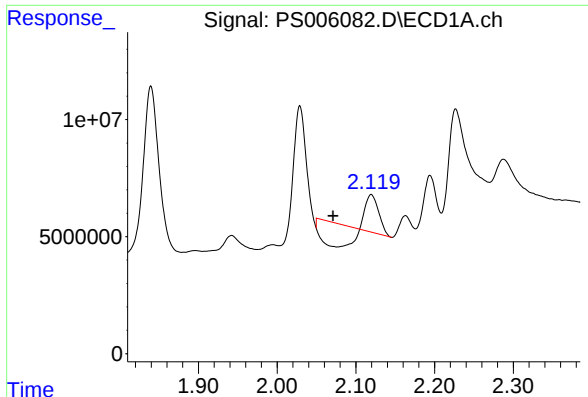

#1 Dalapon


R.T.: 2.120 min
Delta R.T.: 0.049 min
Response: 989745
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB122279TB

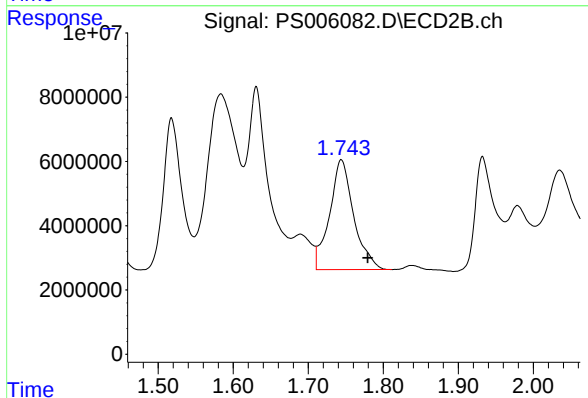


#1 Dalapon

R.T.: 1.744 min
Delta R.T.: -0.035 min
Response: 76587339
Conc: 122.05 ng/ml

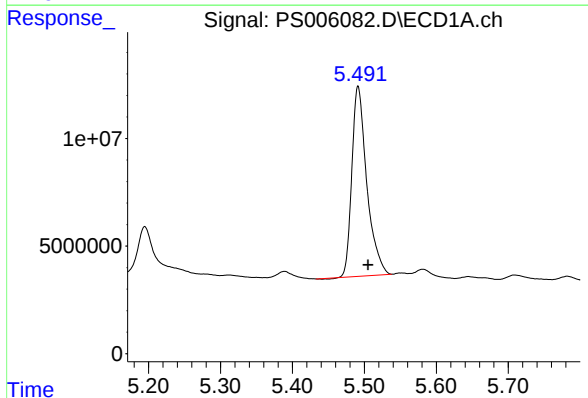


#4 2,4-DCAA

R.T.: 5.492 min
Delta R.T.: -0.014 min
Response: 126784138
Conc: 146.88 ng/ml

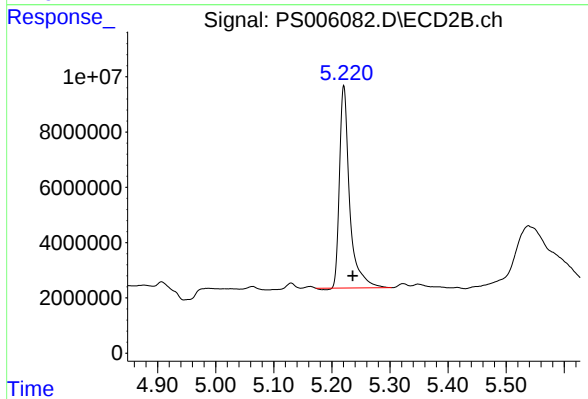

#4 2,4-DCAA


R.T.: 5.221 min
Delta R.T.: -0.015 min
Response: 88438760
Conc: 179.81 ng/ml

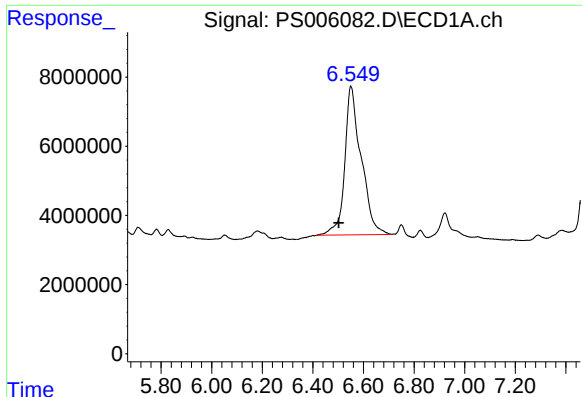

#9 2,4-D


R.T.: 6.550 min
Delta R.T.: 0.047 min
Response: 193583288
Conc: 237.59 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB122279TB

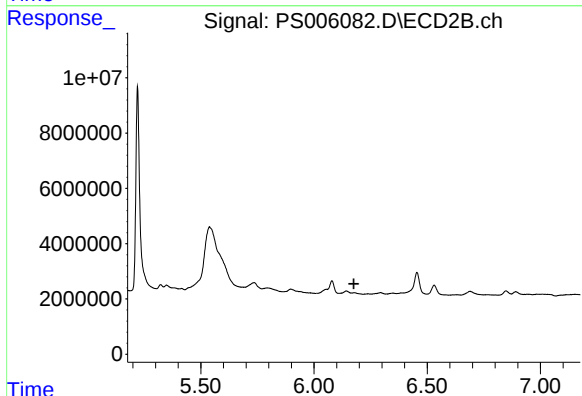


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.

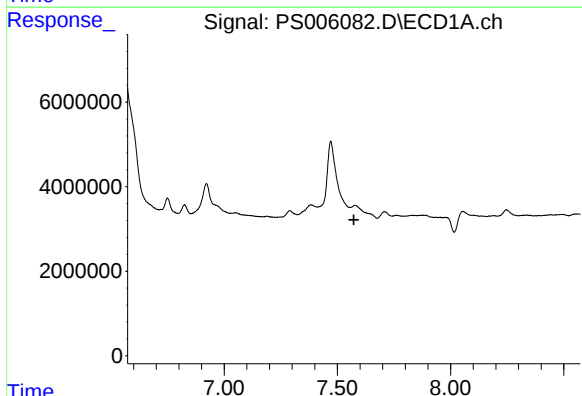


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.573 min
Response: 0
Conc: N.D.

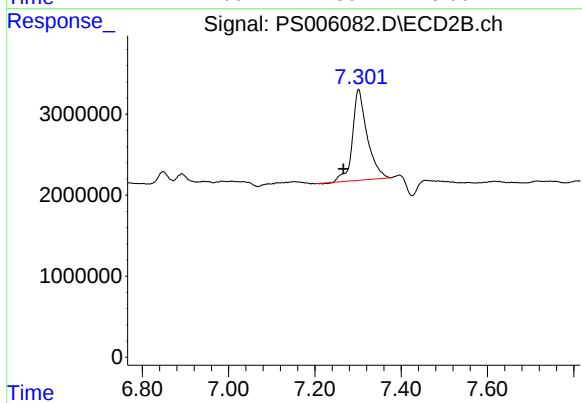

#12 2,4,5-T


R.T.: 7.301 min
Delta R.T.: 0.035 min
Response: 26426512
Conc: 10.63 ng/ml

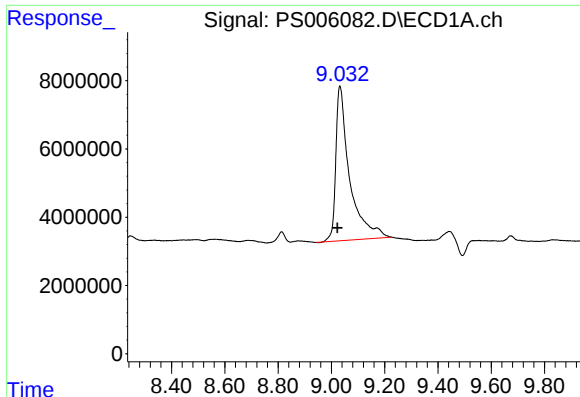

#15 Picloram


R.T.: 9.032 min
Delta R.T.: 0.009 min
Response: 163480140
Conc: 21.97 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB122279TB

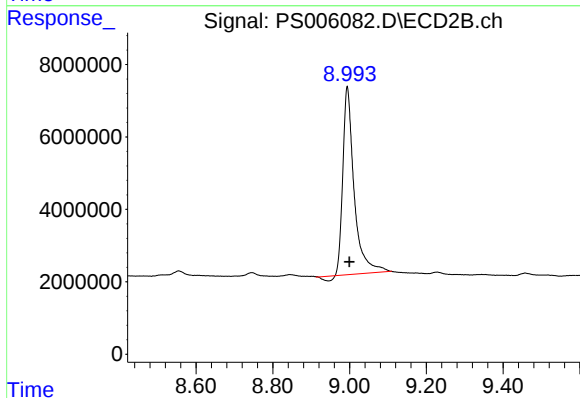


#15 Picloram

R.T.: 8.994 min
Delta R.T.: -0.006 min
Response: 105347458
Conc: 23.35 ng/ml

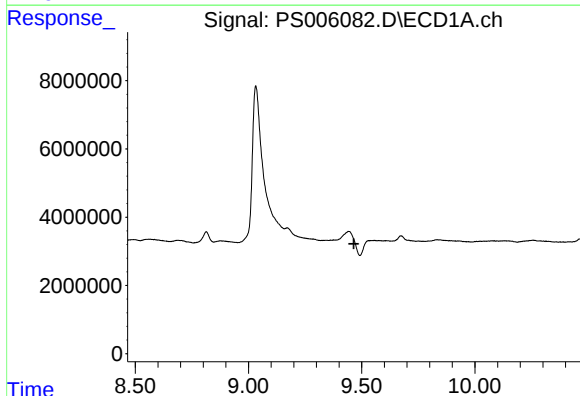

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.465 min
Response: 0
Conc: N.D.

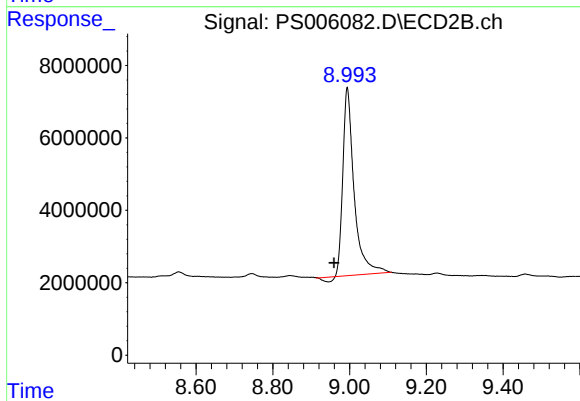

#16 DCPA

R.T.: 8.994 min
Delta R.T.: 0.035 min
Response: 105347458
Conc: 30.21 ng/ml