

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081419\
 Data File : PS006088.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2019 02:46
 Operator : SM\AJ
 Sample : K4324-10
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 T8-F1-(0-4)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 08:32:03 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.505	5.234	170.4E6	113.8E6	197.422	231.427
Target Compounds							
1) T	Dalapon	2.043	1.760	76430257	128.2E6	70.144	204.292 #
2) T	3,5-DICHL...	0.000	4.560	0	52078074	N.D.	85.979
9) T	2,4-D	6.566	0.000	211.1E6	0	259.045	N.D. #
10) T	Pentachlo...	6.764	0.000	15066646	0	1.275	N.D. #
15) T	Picloram	9.055	9.012	71984971	54062613	9.675	11.985
16) T	DCPA	0.000	9.012	0	54062613	N.D.	15.503



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081419\
Data File : PS006088.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2019 02:46
Operator : SM\AJ
Sample : K4324-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
T8-F1-(0-4)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 08:32:03 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

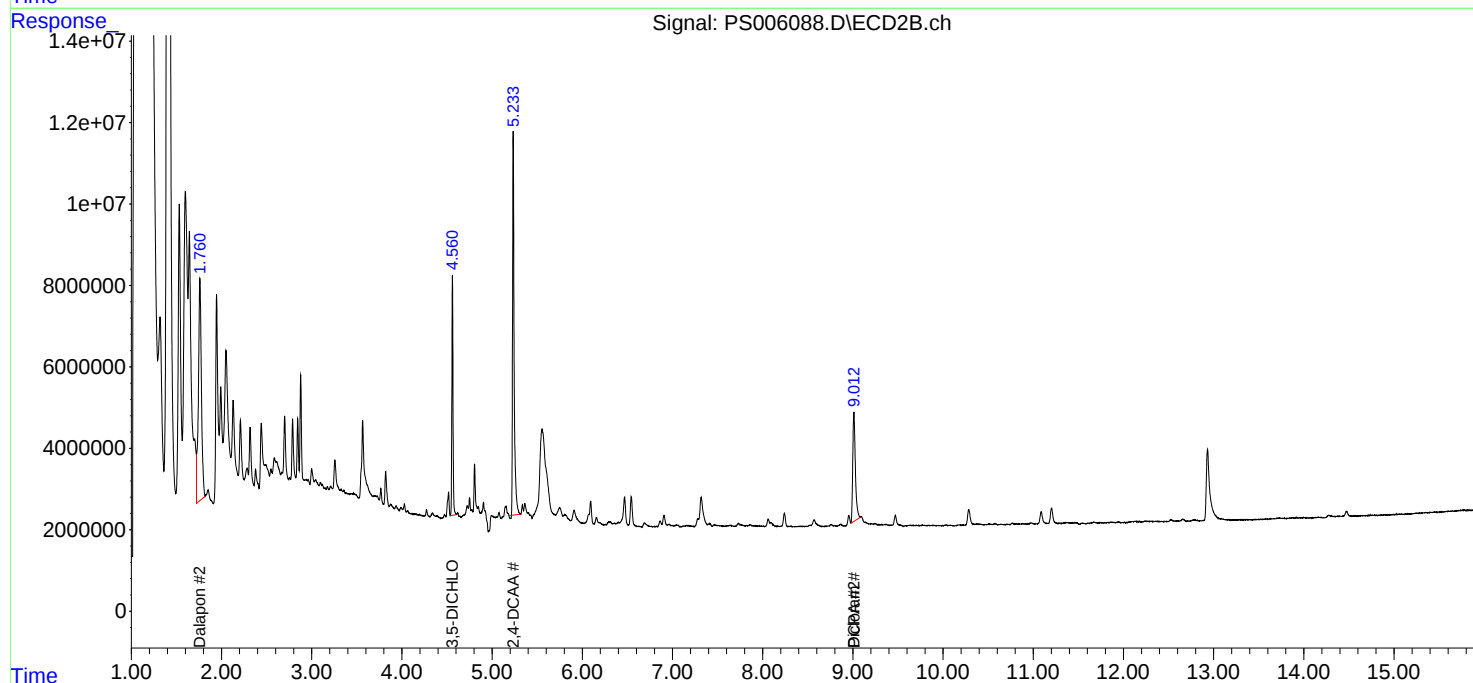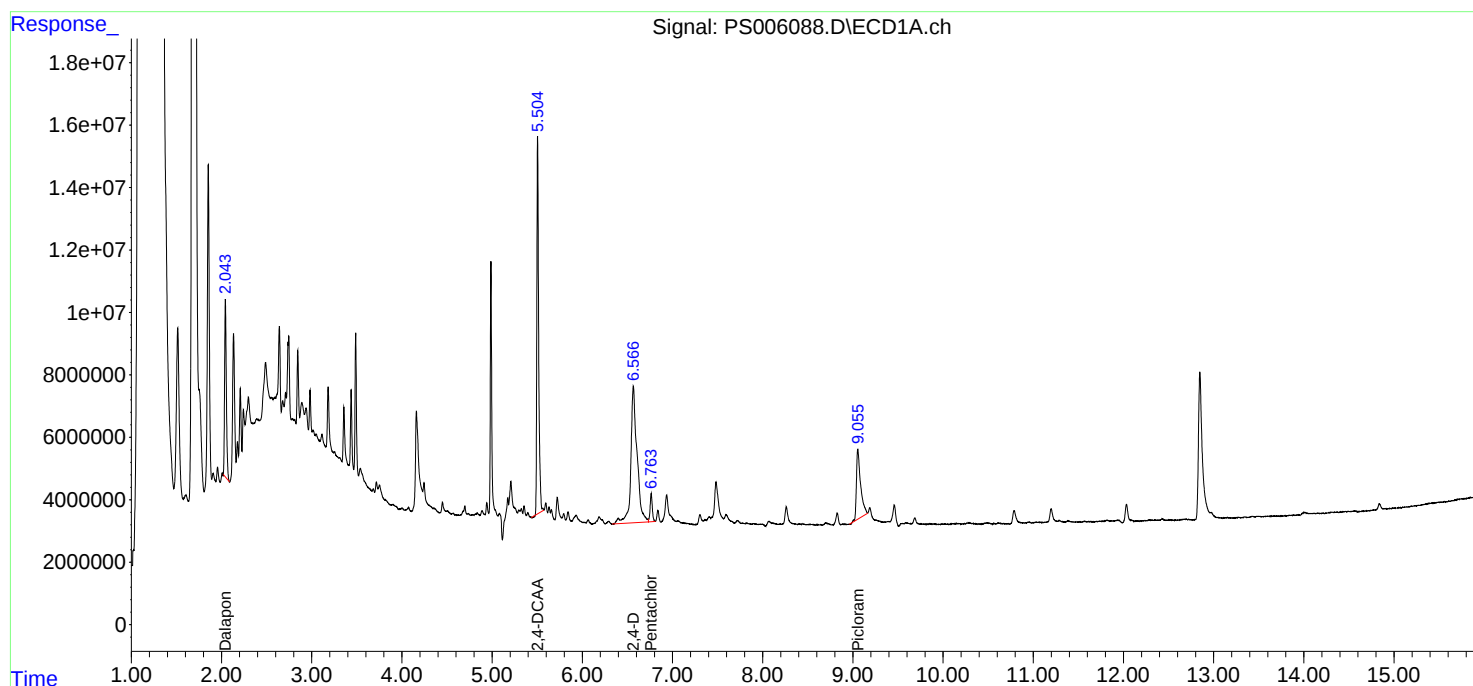


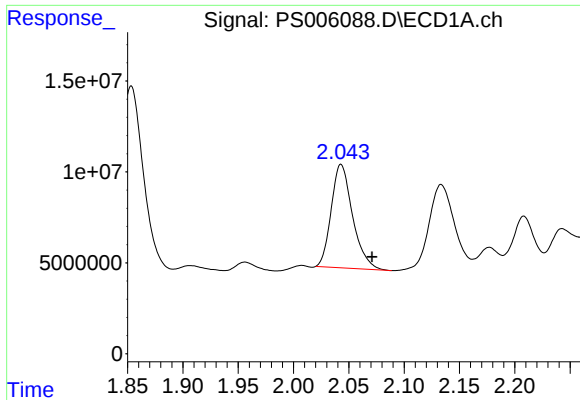

#1 Dalapon


R.T.: 2.043 min
Delta R.T.: -0.028 min
Response: 76430257
Conc: 70.14 ng/ml

Instrument :
ECD_S
ClientSampleId :
T8-F1-(0-4)

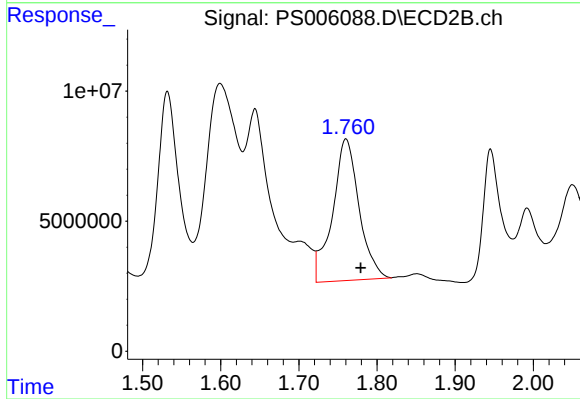


#1 Dalapon

R.T.: 1.760 min
Delta R.T.: -0.019 min
Response: 128191726
Conc: 204.29 ng/ml

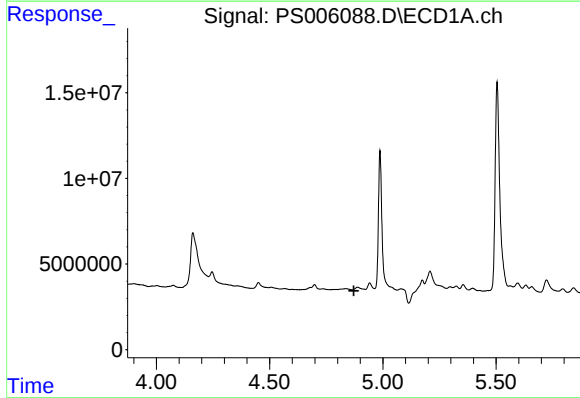


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.872 min
Response: 0
Conc: N.D.

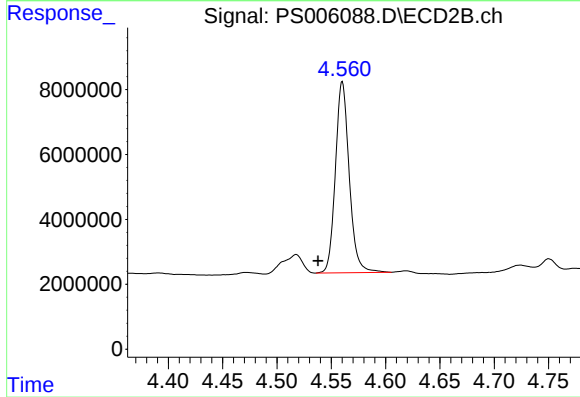

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.560 min
Delta R.T.: 0.022 min
Response: 52078074
Conc: 85.98 ng/ml

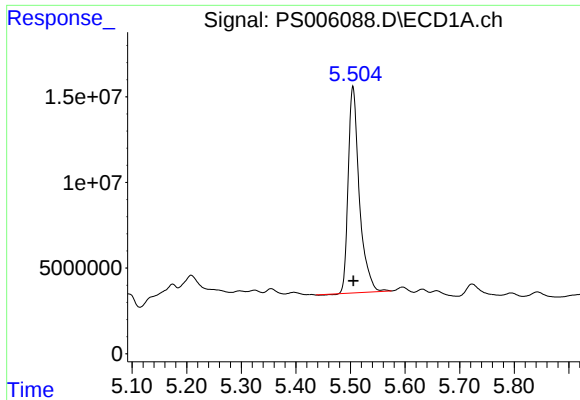

#4 2,4-DCAA


R.T.: 5.505 min
Delta R.T.: 0.000 min
Response: 170414531
Conc: 197.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
T8-F1-(0-4)

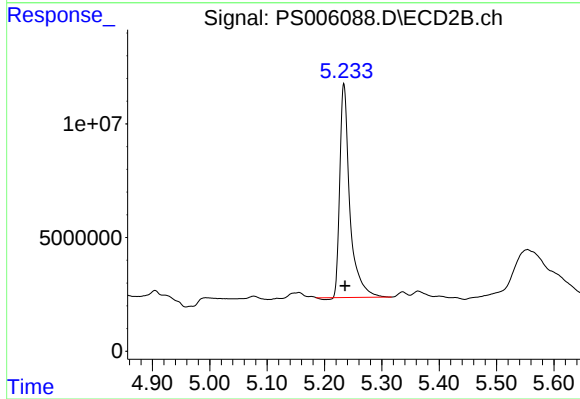


#4 2,4-DCAA

R.T.: 5.234 min
Delta R.T.: -0.002 min
Response: 113827691
Conc: 231.43 ng/ml

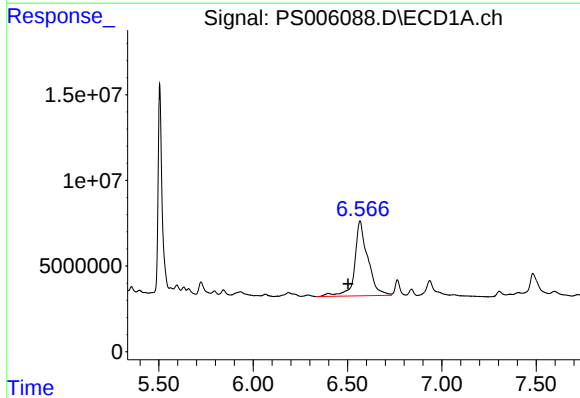


#9 2,4-D

R.T.: 6.566 min
Delta R.T.: 0.063 min
Response: 211065925
Conc: 259.05 ng/ml

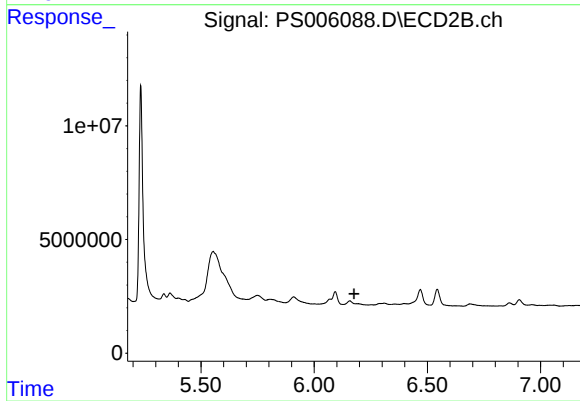

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.176 min
Response: 0
Conc: N.D.

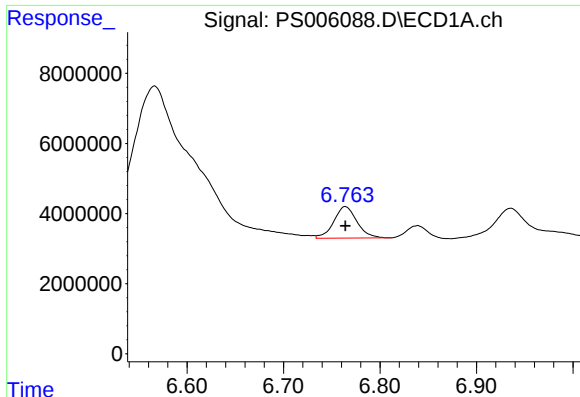

#10 Pentachlorophenol


R.T.: 6.764 min
Delta R.T.: 0.000 min
Response: 15066646
Conc: 1.27 ng/ml

Instrument :
ECD_S
ClientSampleId :
T8-F1-(0-4)

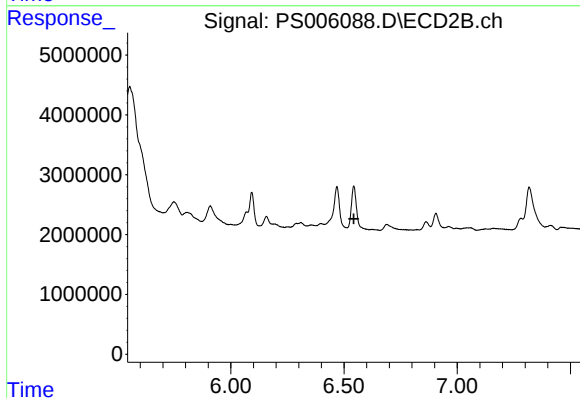


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.544 min
Response: 0
Conc: N.D.

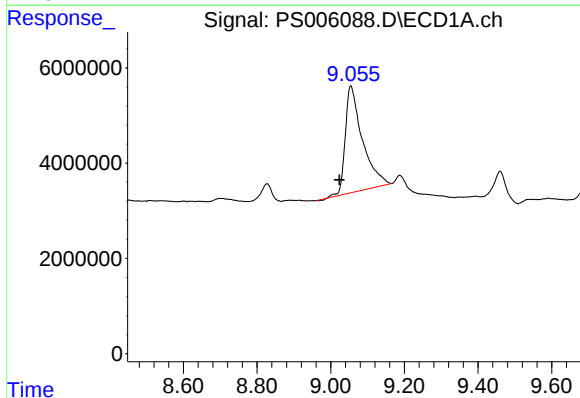


#15 Picloram

R.T.: 9.055 min
Delta R.T.: 0.031 min
Response: 71984971
Conc: 9.67 ng/ml

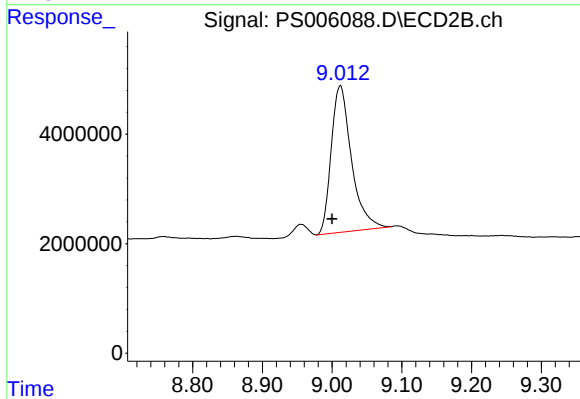

#15 Picloram


R.T.: 9.012 min
Delta R.T.: 0.012 min
Response: 54062613
Conc: 11.99 ng/ml

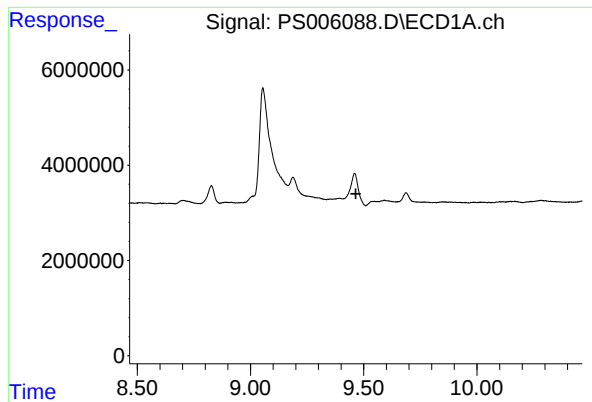

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
T8-F1-(0-4)

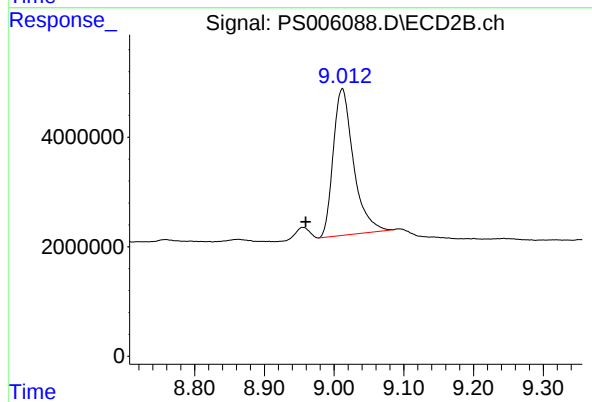

#16 DCPA

R.T.: 9.012 min
Delta R.T.: 0.052 min
Response: 54062613
Conc: 15.50 ng/ml