

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081419\
 Data File : PS006093.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2019 04:36
 Operator : SM\AJ
 Sample : K4329-04
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 WATER-PIT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 08:33:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.490	5.220	306.4E6	197.7E6	354.925	401.958
Target Compounds							
1) T	Dalapon	2.119	1.746	18995654	97612379	17.433	155.559 #
2) T	3,5-DICHL...	0.000	4.548	0	39787716	N.D.	65.688
3) T	4-Nitroph...	5.297	0.000	5460823	0	14.546	N.D. #
7) T	MCPA	0.000	5.596	0	29806918	N.D.	14.585
9) T	2,4-D	6.552	0.000	196.4E6	0	241.003	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081419\
Data File : PS006093.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2019 04:36
Operator : SM\AJ
Sample : K4329-04
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
WATER-PIT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 08:33:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

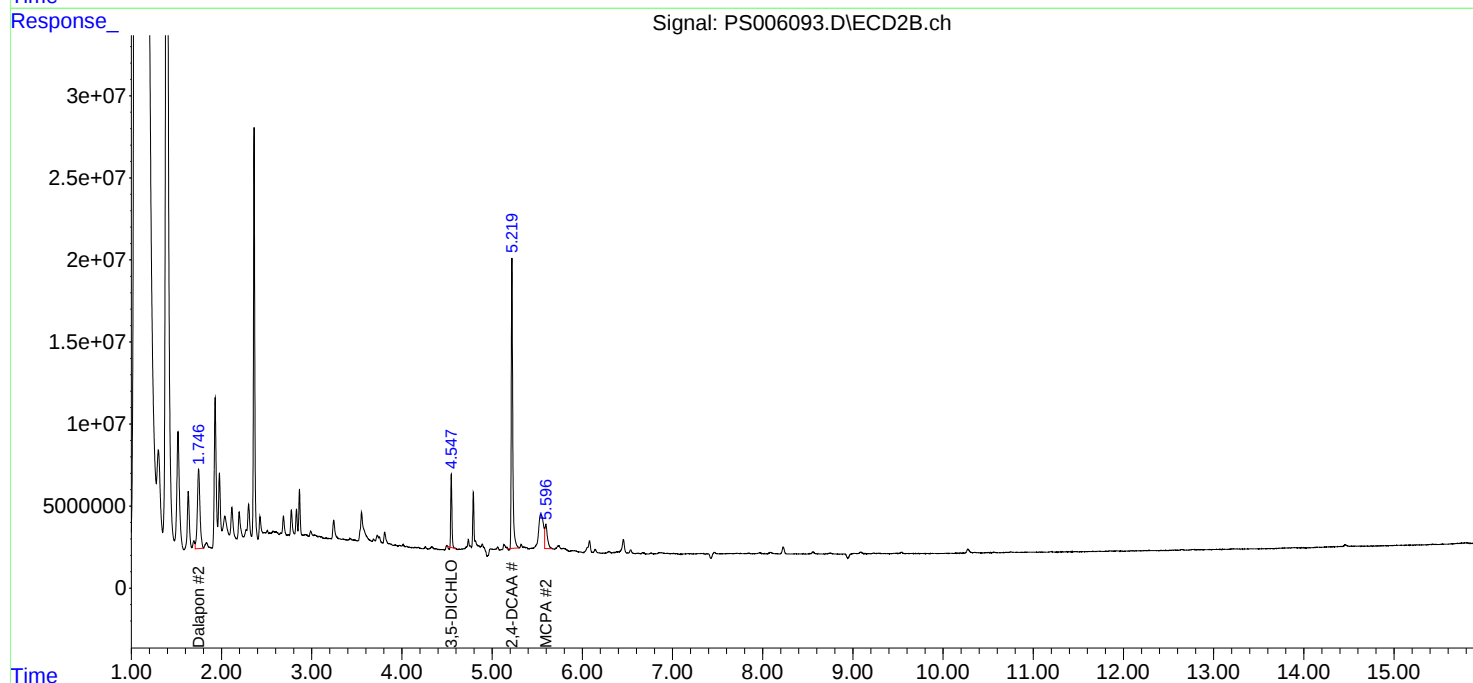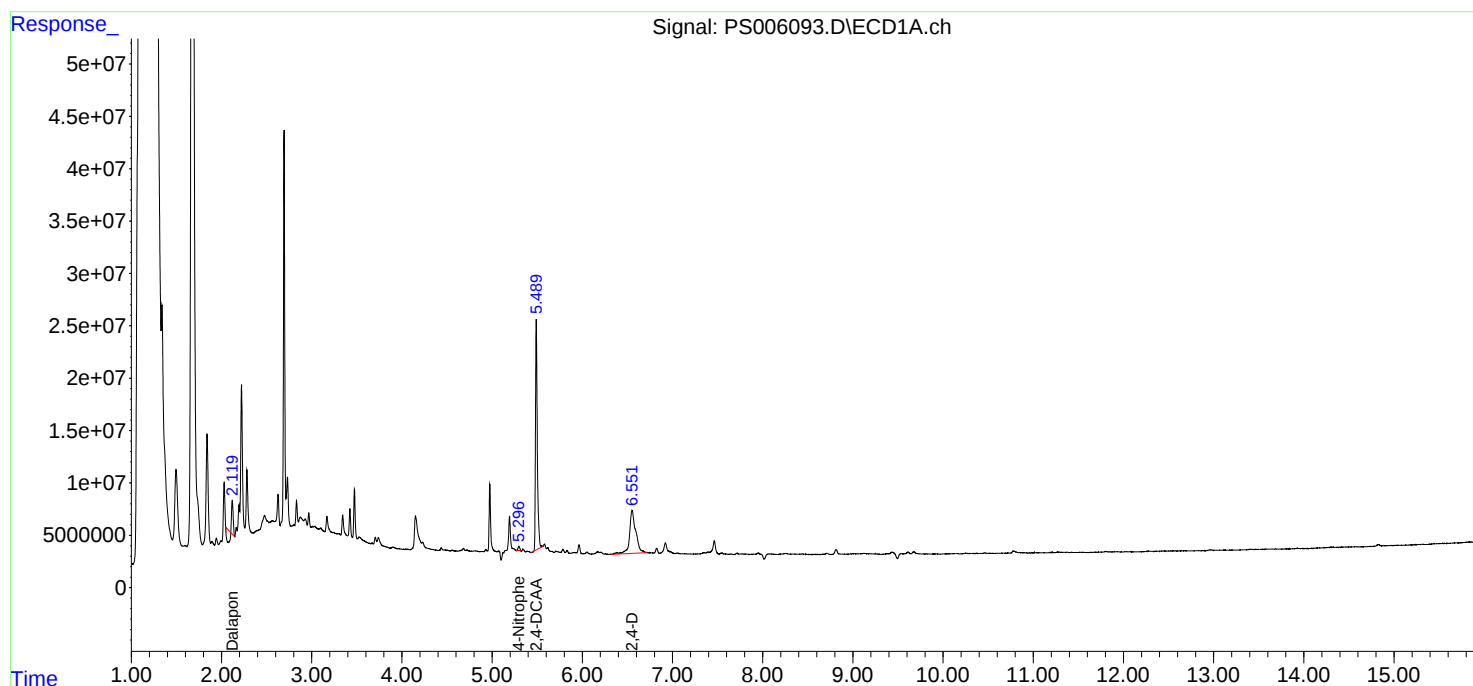


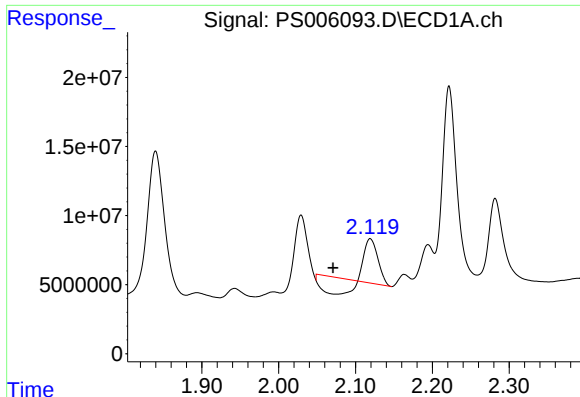

#1 Dalapon


R.T.: 2.119 min
Delta R.T.: 0.048 min
Response: 18995654
Conc: 17.43 ng/ml

Instrument :
ECD_S
ClientSampleId :
WATER-PIT

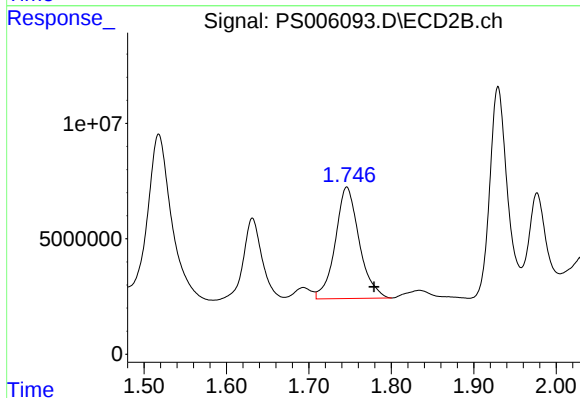


#1 Dalapon

R.T.: 1.746 min
Delta R.T.: -0.033 min
Response: 97612379
Conc: 155.56 ng/ml

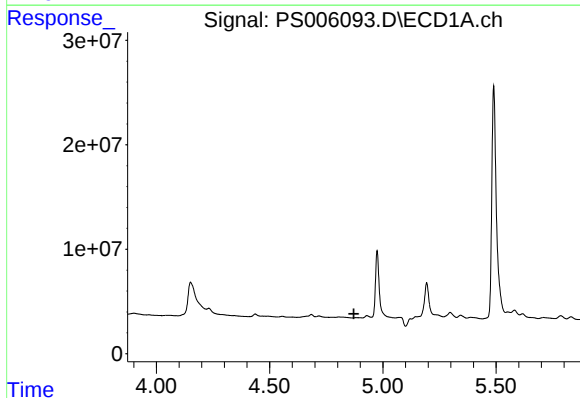


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.872 min
Response: 0
Conc: N.D.

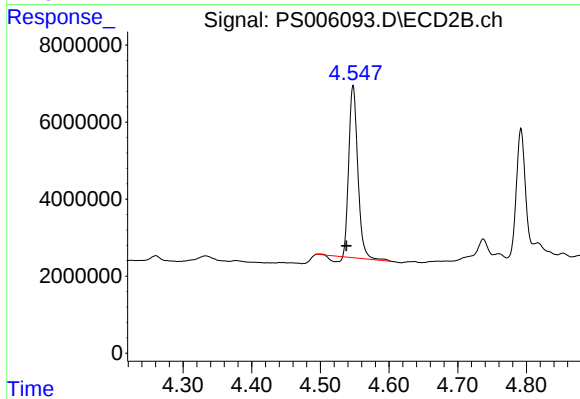

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.548 min
Delta R.T.: 0.010 min
Response: 39787716
Conc: 65.69 ng/ml

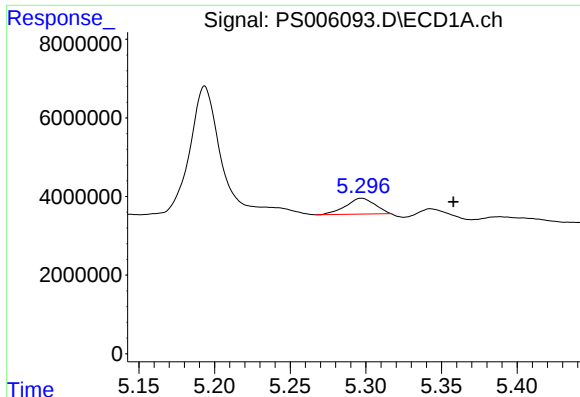

#3 4-Nitrophenol


R.T.: 5.297 min
Delta R.T.: -0.061 min
Response: 5460823
Conc: 14.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
WATER-PIT

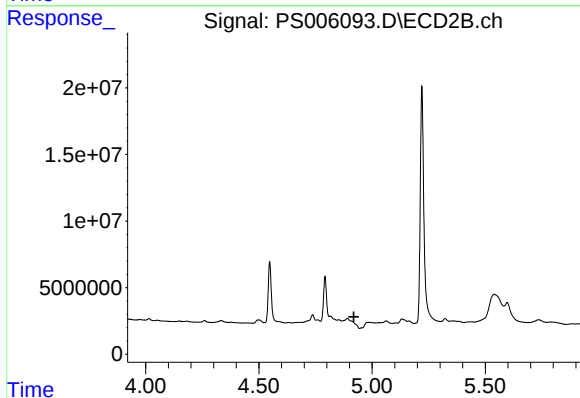


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.920 min
Response: 0
Conc: N.D.

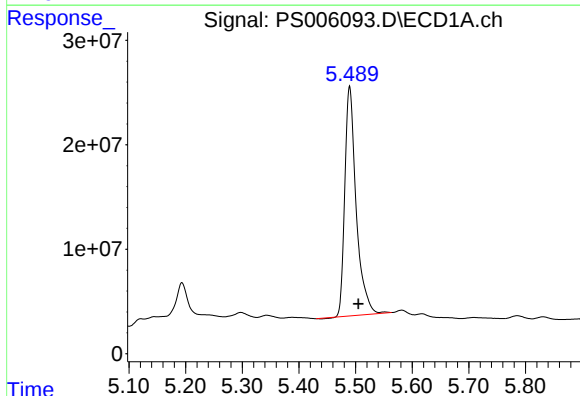


#4 2,4-DCAA

R.T.: 5.490 min
Delta R.T.: -0.015 min
Response: 306371893
Conc: 354.93 ng/ml

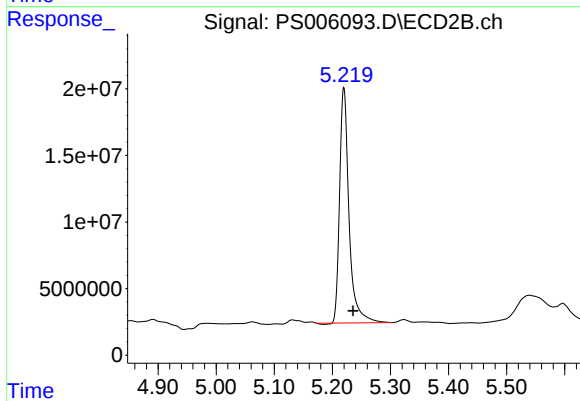

#4 2,4-DCAA


R.T.: 5.220 min
Delta R.T.: -0.016 min
Response: 197703746
Conc: 401.96 ng/ml

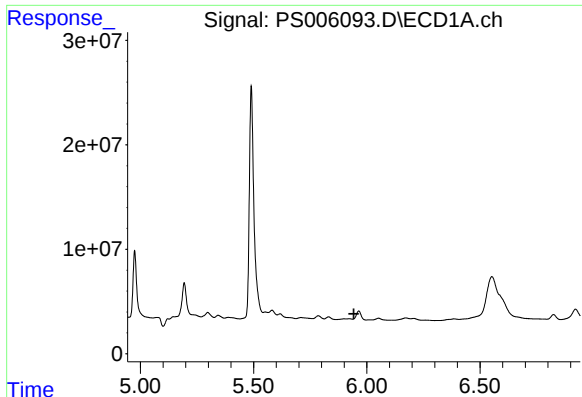

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 5.943 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
WATER-PIT

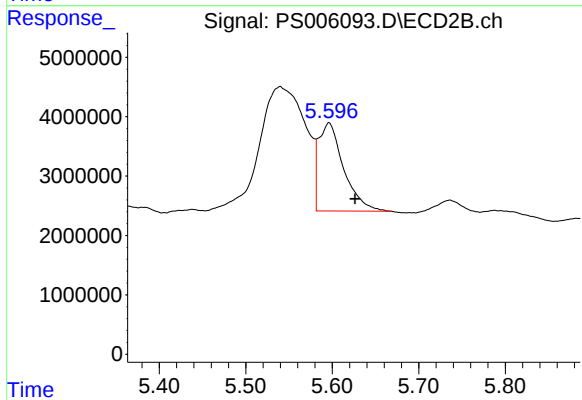


#7 MCPA

R.T.: 5.596 min
Delta R.T.: -0.030 min
Response: 29806918
Conc: 14.58 ug/ml

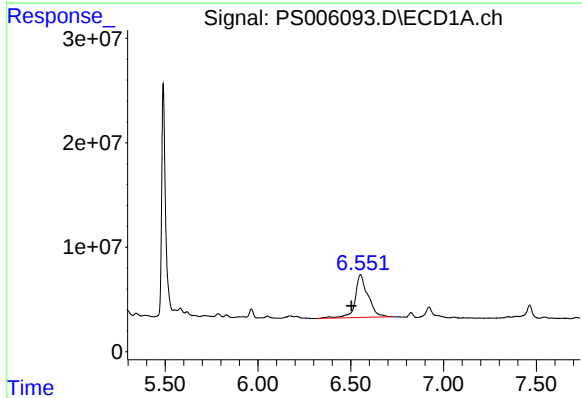

#9 2,4-D

R.T.: 6.552 min
Delta R.T.: 0.049 min
Response: 196365619
Conc: 241.00 ng/ml

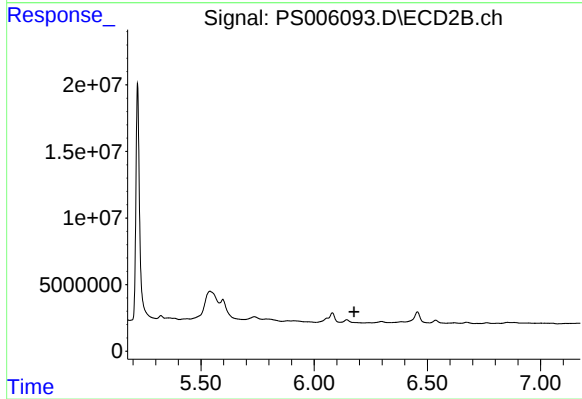

#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.176 min
Response: 0
Conc: N.D.