

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081420\
 Data File : PS011788.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2020 13:27
 Operator : DD\AJ
 Sample : L3508-13
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TR-04-081220

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 13:47:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
1) T	Dalapon	2.992	2.580	21745771	15524889	17.457 20.540
2) T	3,5-DICHL...	0.000	6.096	0	69590107	N.D. 84.596
5) T	DICAMBA	0.000	7.093	0	2739789	N.D. 1.268
6) T	MCP	7.573	0.000	9622637	0	3.012 N.D. #
7) T	MCPA	7.766	7.377	25343558	32773447	5.572 11.960 #
8) T	DICHLORPROP	0.000	7.739	0	12578615	N.D. 22.277
9) T	2,4-D	8.343	7.978	15554311	4706276	13.776 6.406 #
10) T	Pentachlo...	8.697	0.000	26605961	0	1.850 N.D. #
11) T	2,4,5-TP ...	0.000	8.765	0	15320975	N.D. 5.240
12) T	2,4,5-T	9.495	0.000	18549557	0	3.130 N.D. #
15) T	Picloram	0.000	11.022	0	21320016	N.D. 4.704



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081420\
Data File : PS011788.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2020 13:27
Operator : DD\AJ
Sample : L3508-13
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TR-04-081220

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 13:47:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

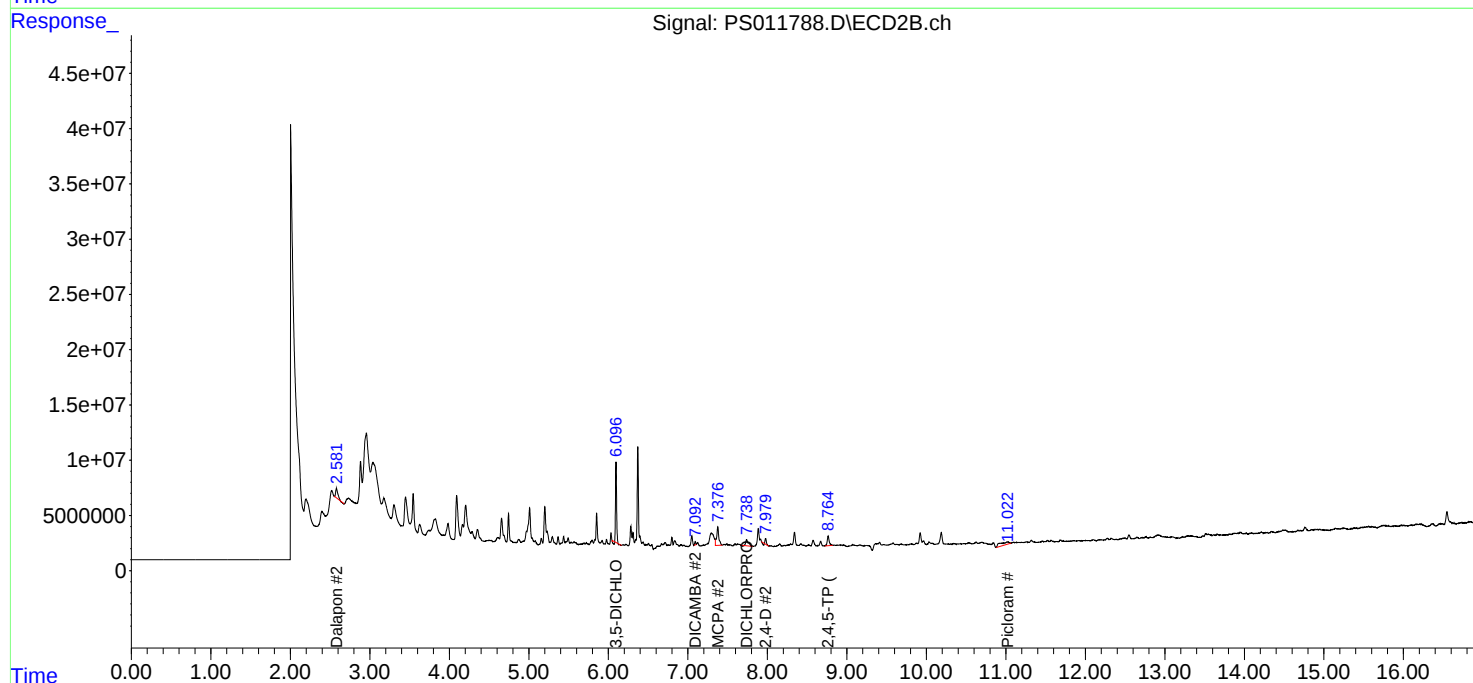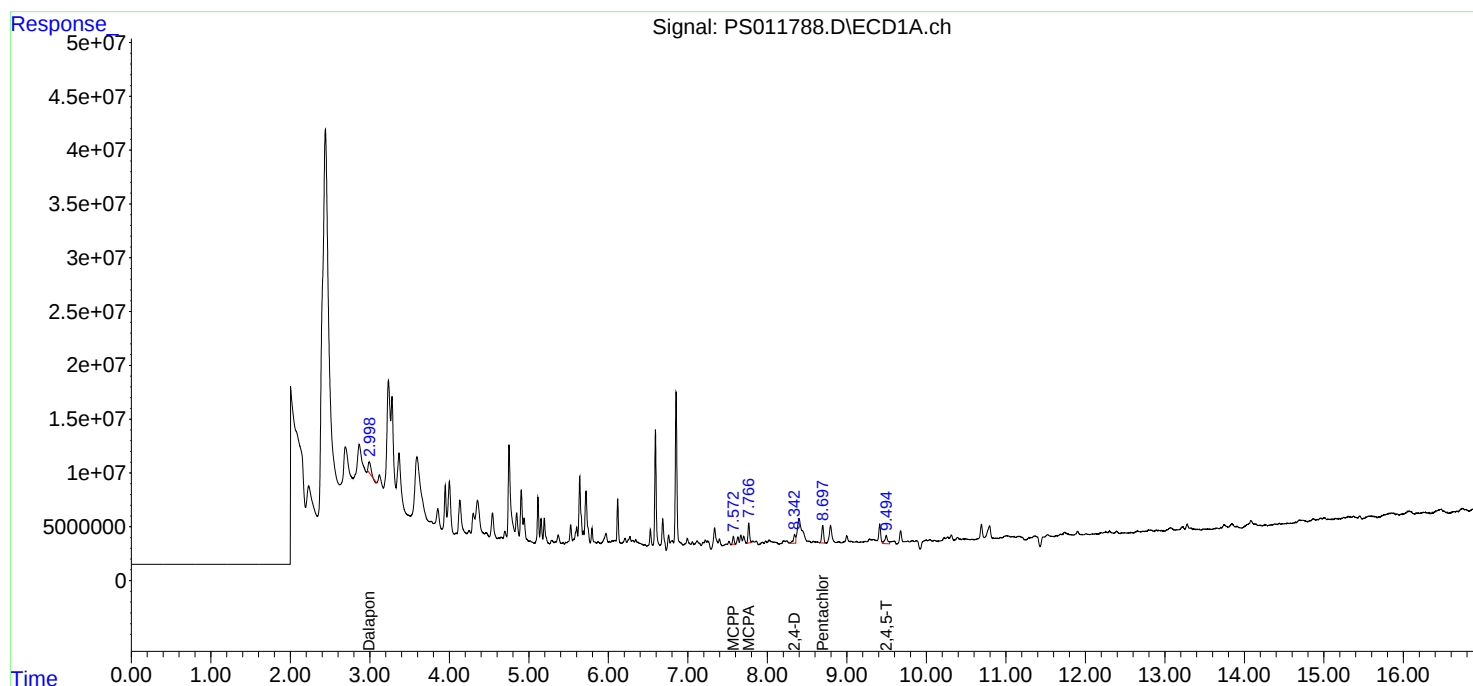


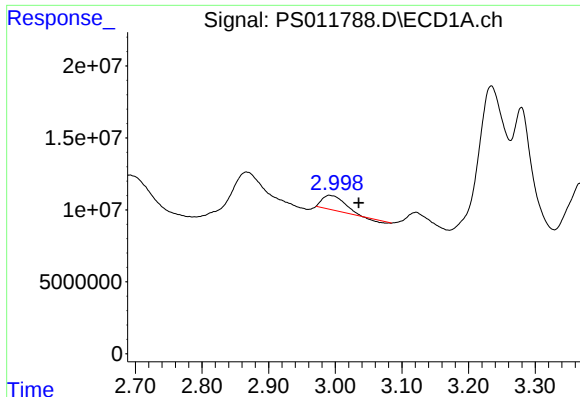

#1 Dalapon


R.T.: 2.992 min
Delta R.T.: -0.043 min
Response: 21745771
Conc: 17.46 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-04-081220

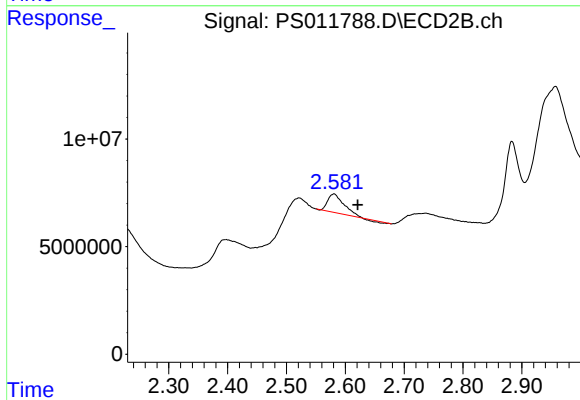


#1 Dalapon

R.T.: 2.580 min
Delta R.T.: -0.041 min
Response: 15524889
Conc: 20.54 ng/ml

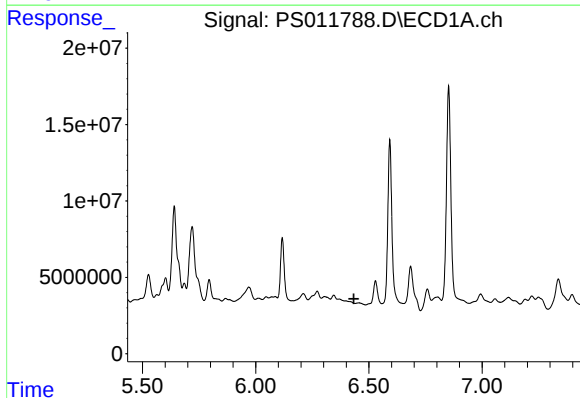


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.434 min
Response: 0
Conc: N.D.

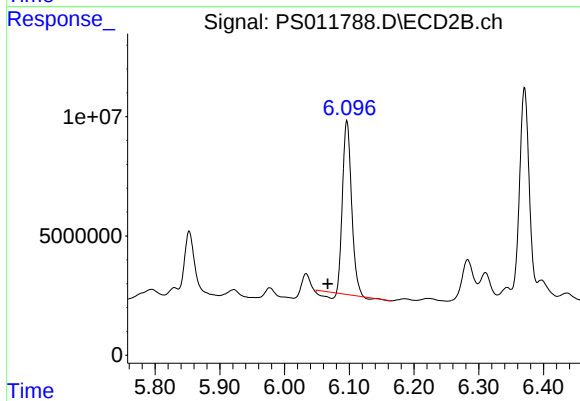

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.096 min
Delta R.T.: 0.030 min
Response: 69590107
Conc: 84.60 ng/ml

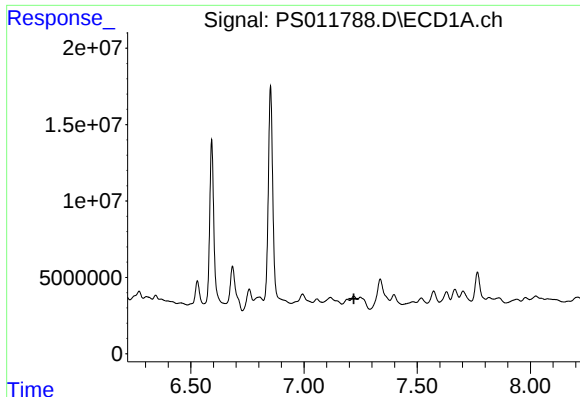

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.220 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TR-04-081220

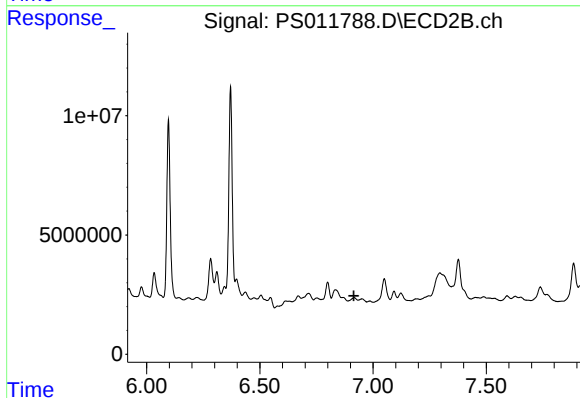


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.915 min
Response: 0
Conc: N.D.

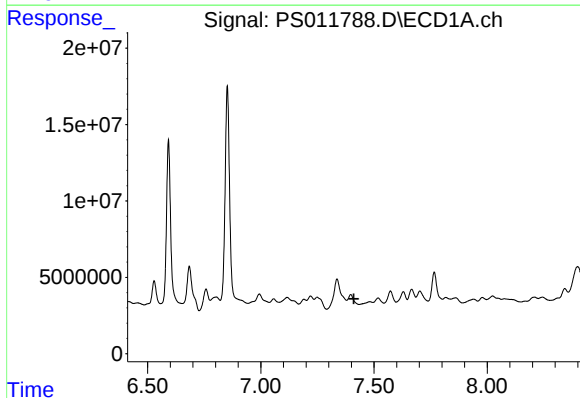


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.412 min
Response: 0
Conc: N.D.

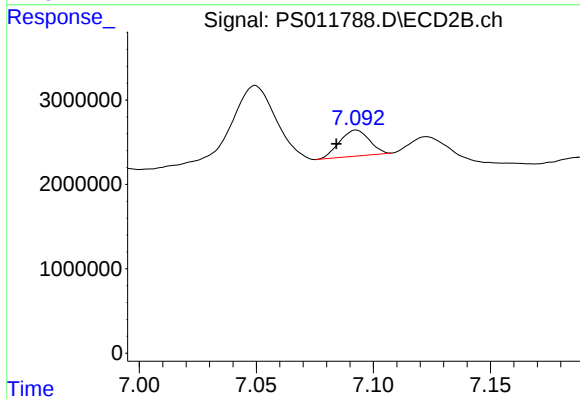

#5 DICAMBA


R.T.: 7.093 min
Delta R.T.: 0.008 min
Response: 2739789
Conc: 1.27 ng/ml

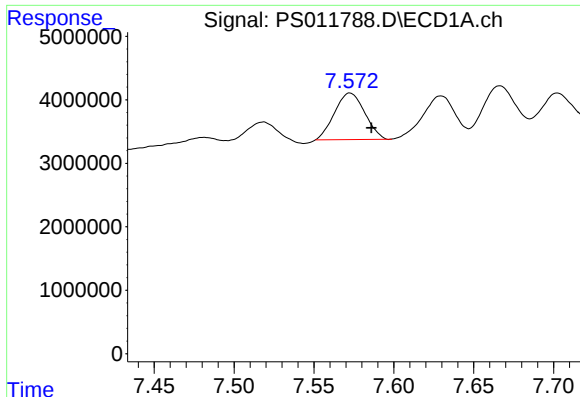

#6 MCPP


R.T.: 7.573 min
Delta R.T.: -0.013 min
Response: 9622637
Conc: 3.01 ug/ml

Instrument :
ECD_S
ClientSampleId :
TR-04-081220

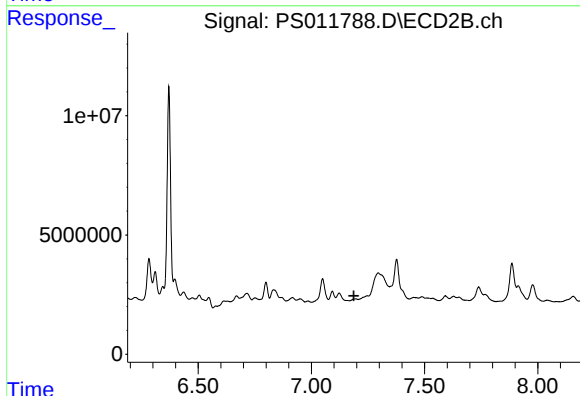


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.188 min
Response: 0
Conc: N.D.

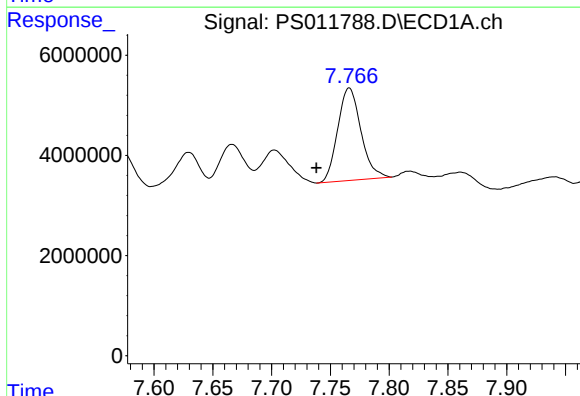


#7 MCPA

R.T.: 7.766 min
Delta R.T.: 0.028 min
Response: 25343558
Conc: 5.57 ug/ml

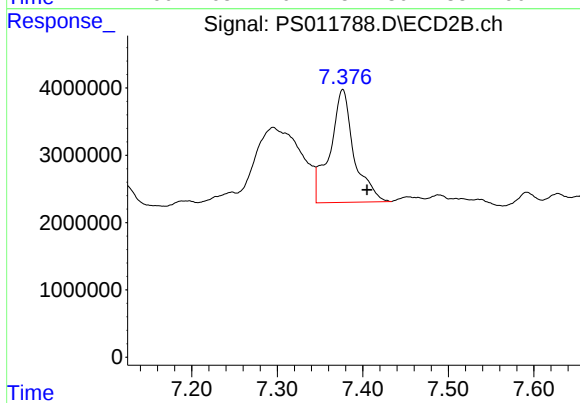

#7 MCPA


R.T.: 7.377 min
Delta R.T.: -0.028 min
Response: 32773447
Conc: 11.96 ug/ml

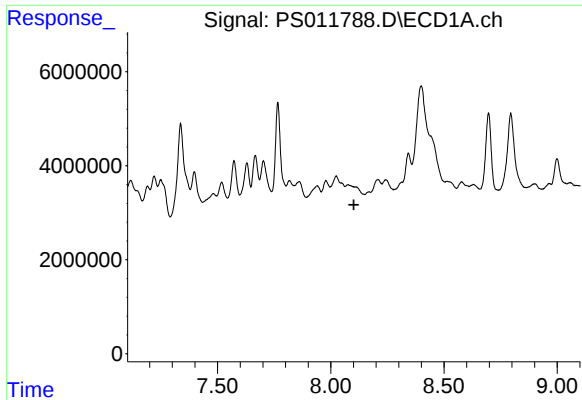

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.102 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TR-04-081220

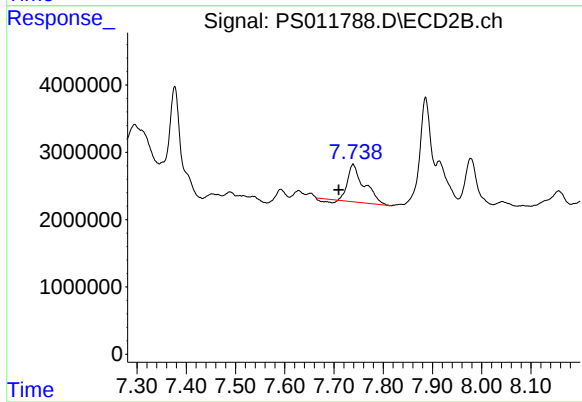


#8 DICHLORPROP

R.T.: 7.739 min
Delta R.T.: 0.029 min
Response: 12578615
Conc: 22.28 ng/ml

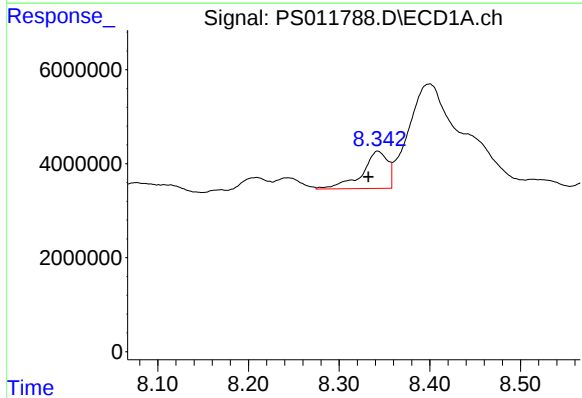


#9 2,4-D

R.T.: 8.343 min
Delta R.T.: 0.011 min
Response: 15554311
Conc: 13.78 ng/ml

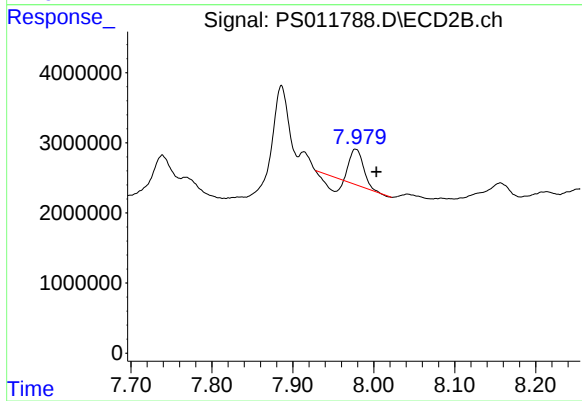

#9 2,4-D


R.T.: 7.978 min
Delta R.T.: -0.025 min
Response: 4706276
Conc: 6.41 ng/ml

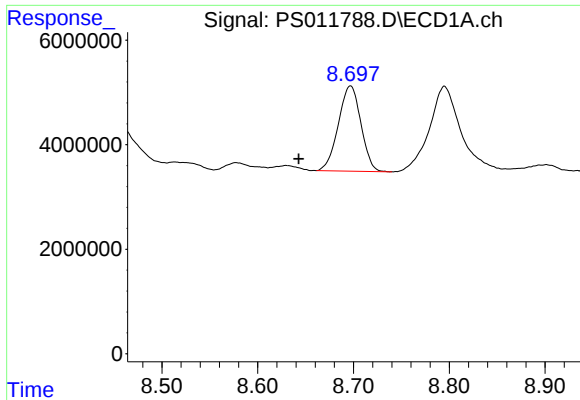

#10 Pentachlorophenol


R.T.: 8.697 min
Delta R.T.: 0.054 min
Response: 26605961
Conc: 1.85 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-04-081220

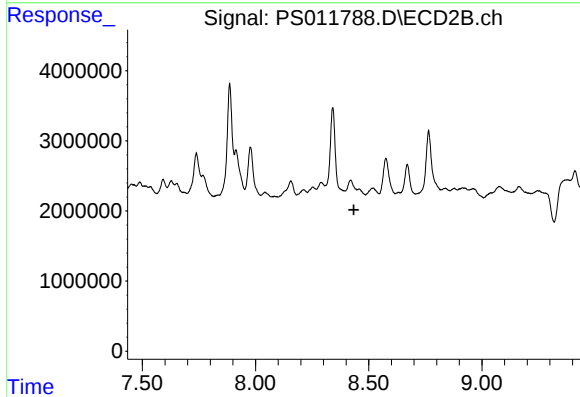


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 8.434 min
Response: 0
Conc: N.D.

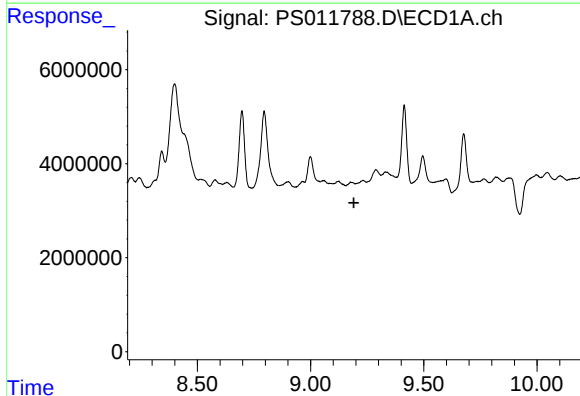


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.191 min
Response: 0
Conc: N.D.

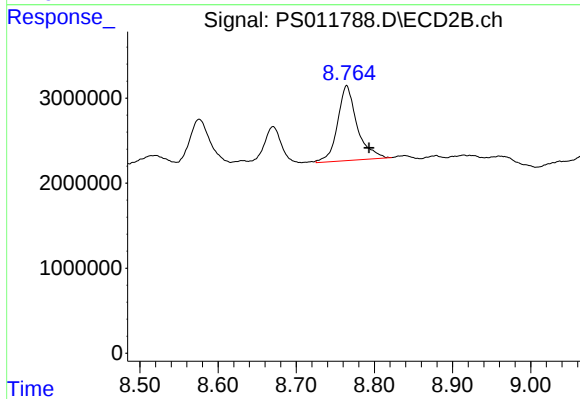

#11 2,4,5-TP (SILVEX)


R.T.: 8.765 min
Delta R.T.: -0.029 min
Response: 15320975
Conc: 5.24 ng/ml

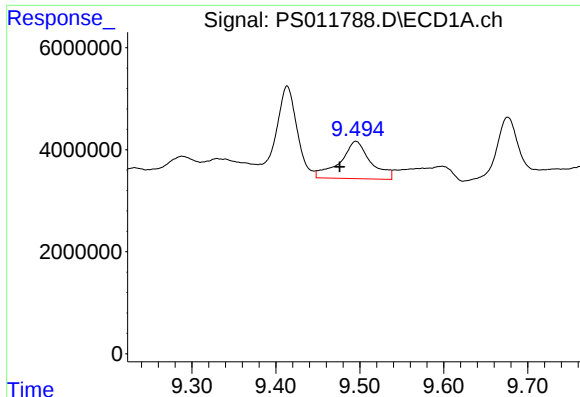

#12 2,4,5-T


R.T.: 9.495 min
Delta R.T.: 0.019 min
Response: 18549557
Conc: 3.13 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-04-081220

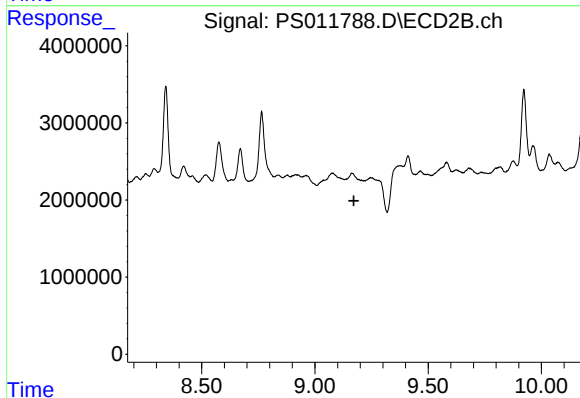


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.

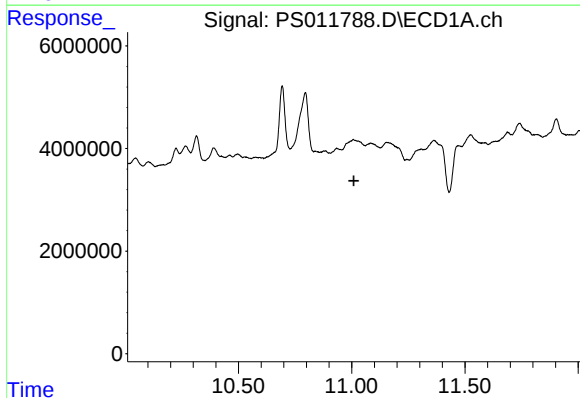

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.009 min
Response: 0
Conc: N.D.

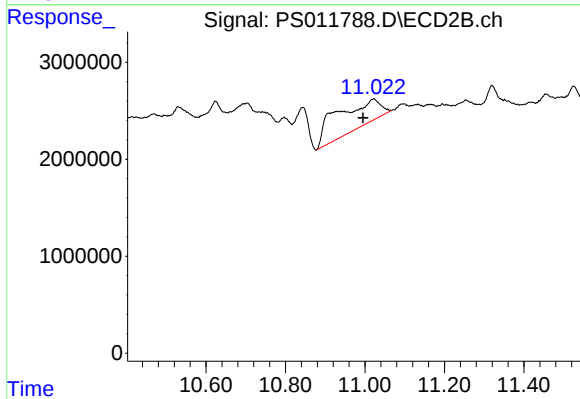

#15 Picloram

R.T.: 11.022 min
Delta R.T.: 0.027 min
Response: 21320016
Conc: 4.70 ng/ml