

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081420\
 Data File : PS011791.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2020 14:36
 Operator : DD\AJ
 Sample : L3508-13RE
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 14:59:32 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.915	284.8E6	164.5E6	261.082	307.657
Target Compounds							
1) T	Dalapon	2.992	2.581	25918858	16233049	20.807	21.477
2) T	3,5-DICHL...	0.000	6.096	0	62149826	N.D.	75.551
3) T	4-Nitroph...	6.993	0.000	1176467	0	1.997	N.D. #
5) T	DICAMBA	0.000	7.049	0	13492229	N.D.	6.245
6) T	MCPD	7.573	0.000	9534985	0	2.984	N.D. #
7) T	MCPA	7.766	7.376	25352406	31965106	5.574	11.665 #
8) T	DICHLORPROP	0.000	7.738	0	16649052	N.D.	29.486
9) T	2,4-D	8.342	7.977	14533049	3012568	12.871	4.101 #
10) T	Pentachlo...	8.696	0.000	24951486	0	1.735	N.D. #
11) T	2,4,5-TP ...	0.000	8.765	0	14977303	N.D.	5.123
12) T	2,4,5-T	9.496	0.000	9548168	0	1.611	N.D. #
15) T	Picloram	0.000	11.022	0	33189396	N.D.	7.323



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081420\
Data File : PS011791.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2020 14:36
Operator : DD\AJ
Sample : L3508-13RE
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 14:59:32 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

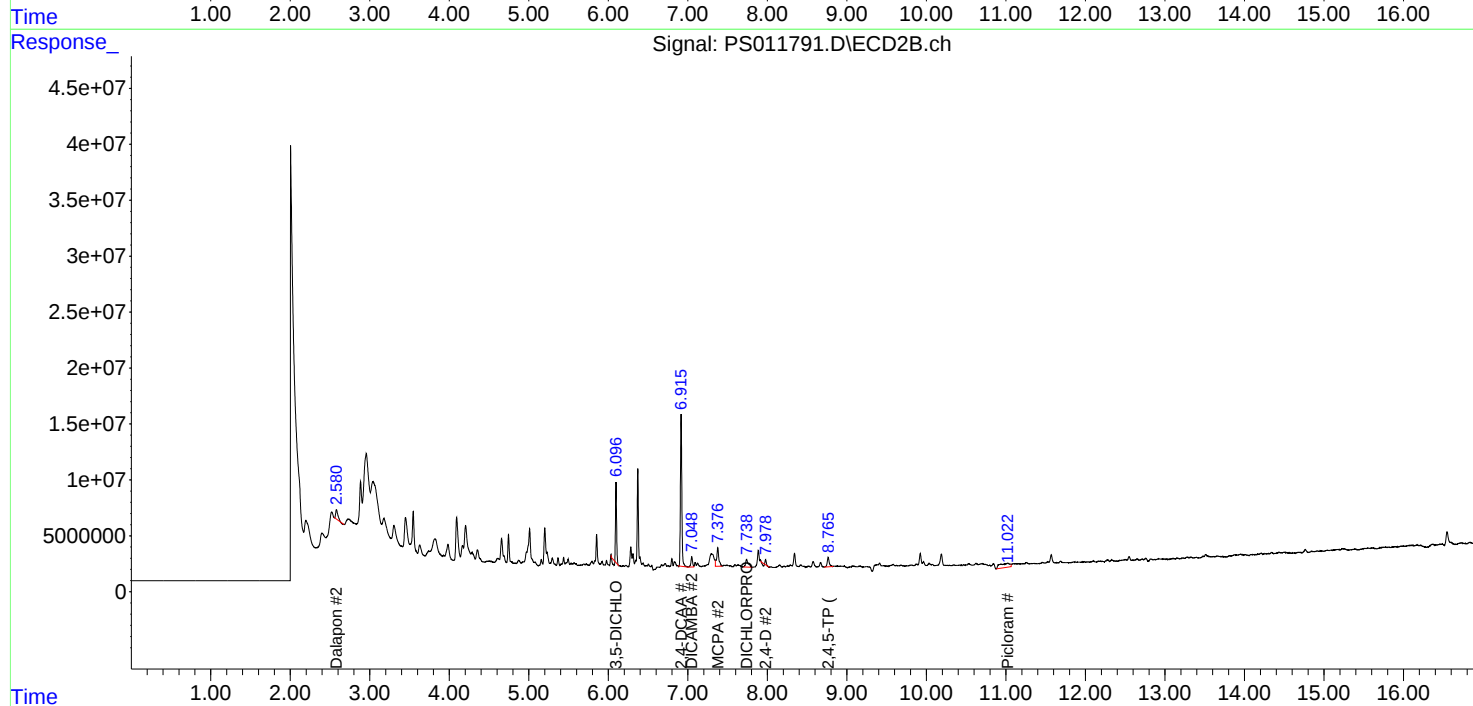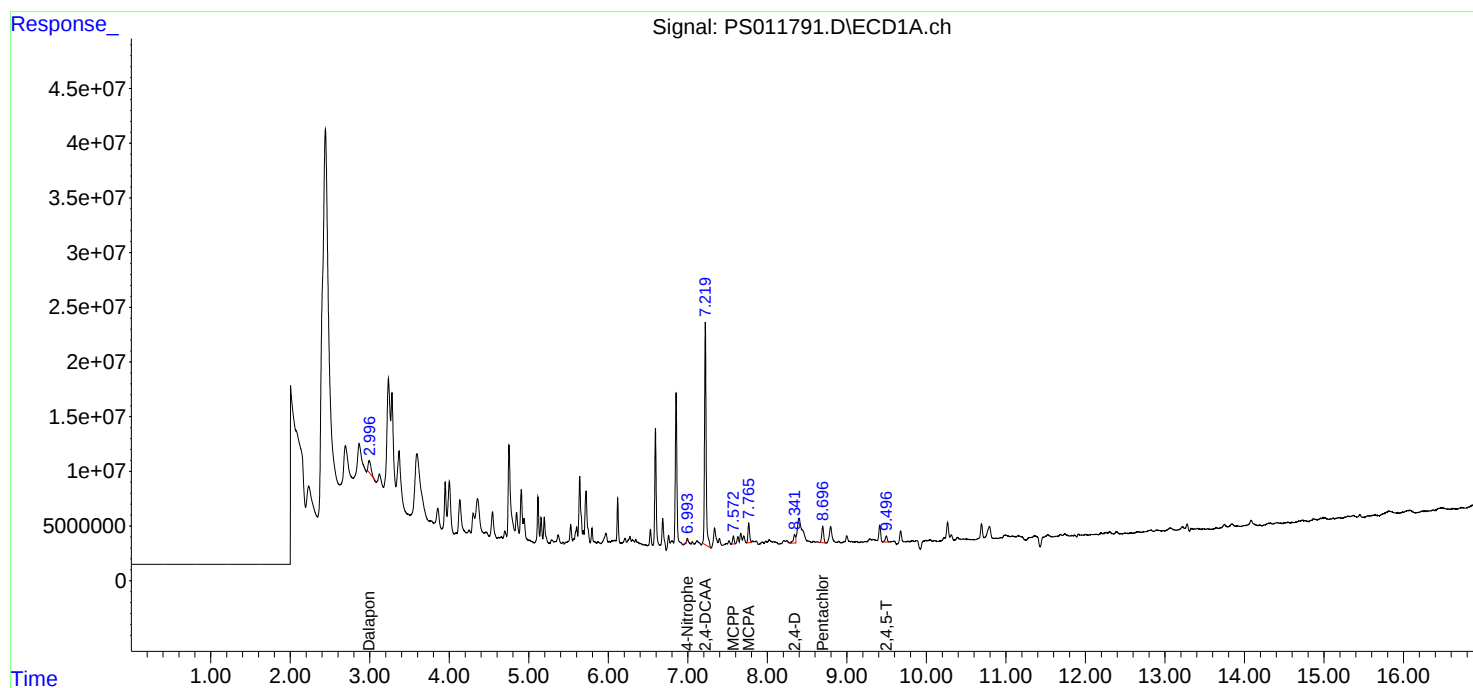


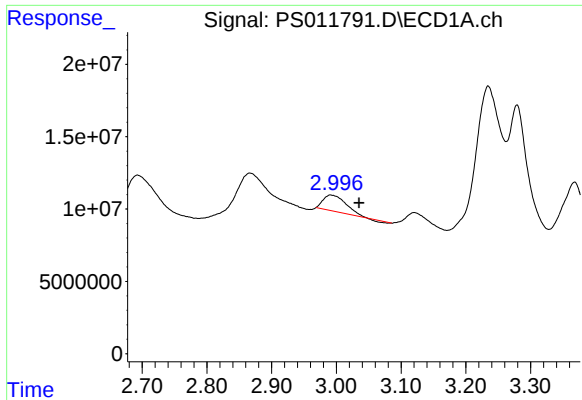

#1 Dalapon


R.T.: 2.992 min
Delta R.T.: -0.043 min
Response: 25918858
Conc: 20.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

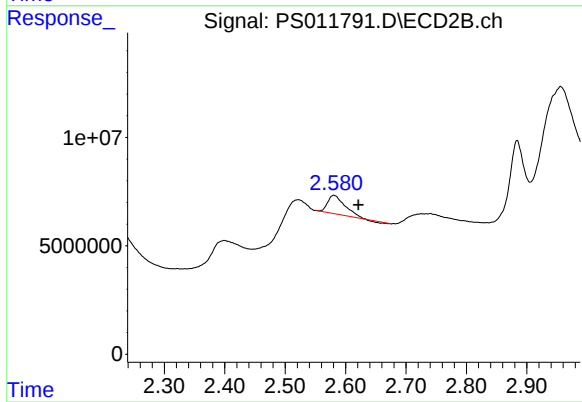


#1 Dalapon

R.T.: 2.581 min
Delta R.T.: -0.040 min
Response: 16233049
Conc: 21.48 ng/ml

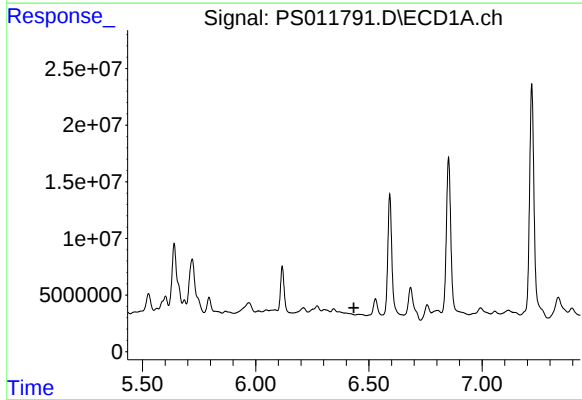


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.434 min
Response: 0
Conc: N.D.

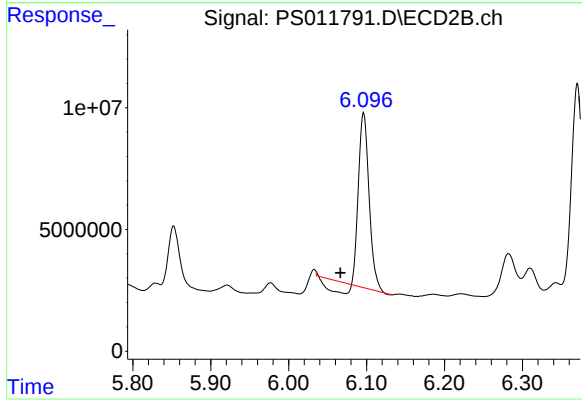

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.096 min
Delta R.T.: 0.030 min
Response: 62149826
Conc: 75.55 ng/ml

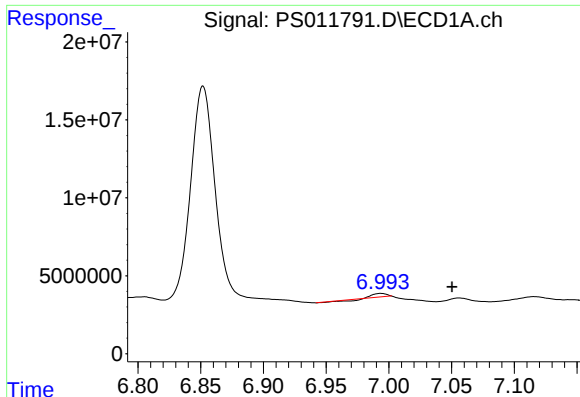

#3 4-Nitrophenol


R.T.: 6.993 min
Delta R.T.: -0.057 min
Response: 1176467
Conc: 2.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

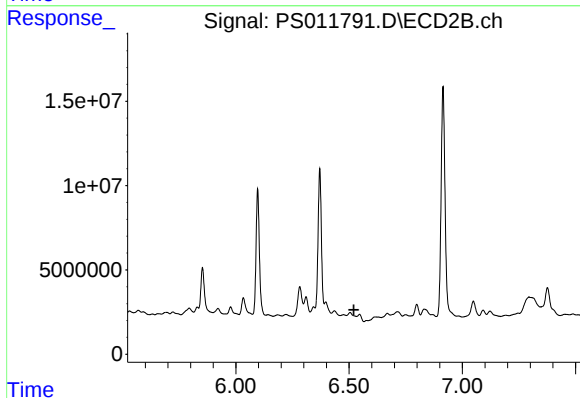


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.521 min
Response: 0
Conc: N.D.

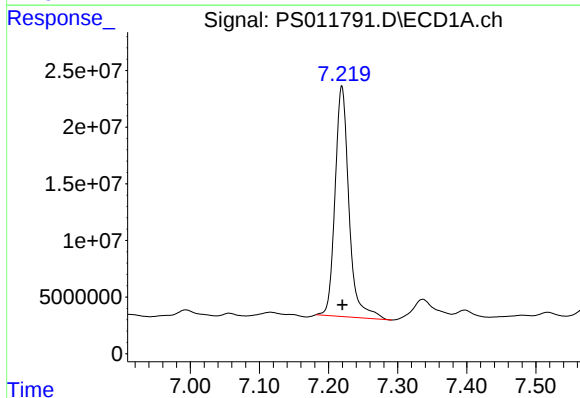


#4 2,4-DCAA

R.T.: 7.219 min
Delta R.T.: 0.000 min
Response: 284780516
Conc: 261.08 ng/ml

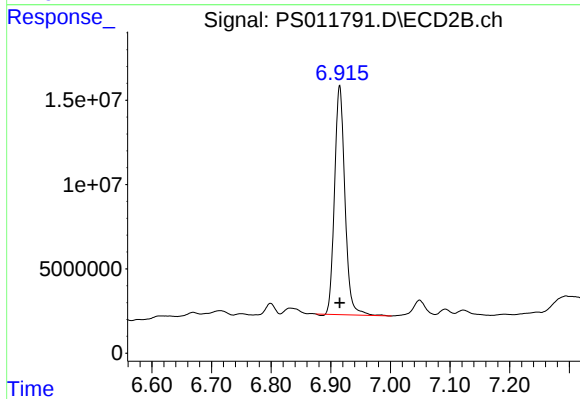

#4 2,4-DCAA


R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 164530787
Conc: 307.66 ng/ml

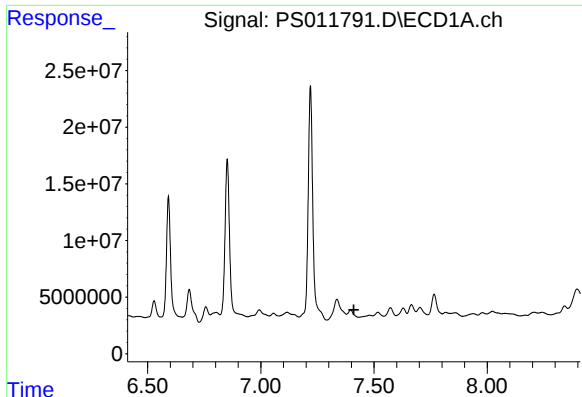

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

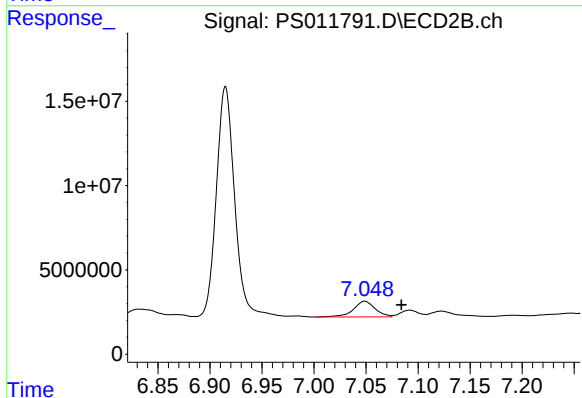


#5 DICAMBA

R.T.: 7.049 min
Delta R.T.: -0.035 min
Response: 13492229
Conc: 6.24 ng/ml

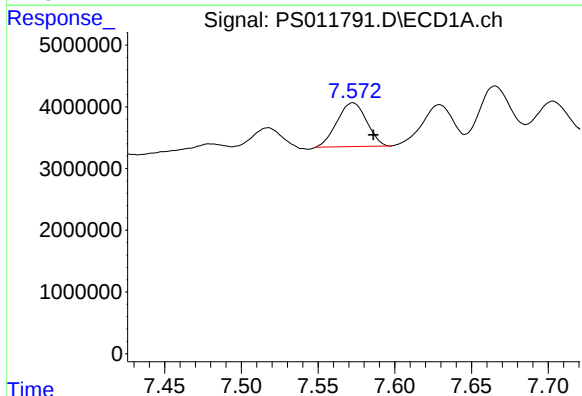


#6 MCP

R.T.: 7.573 min
Delta R.T.: -0.013 min
Response: 9534985
Conc: 2.98 ug/ml

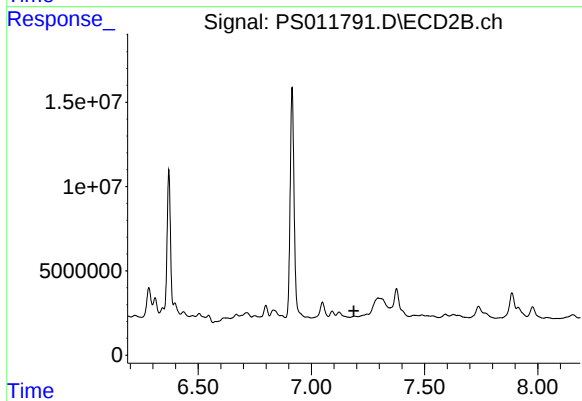

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.188 min
Response: 0
Conc: N.D.

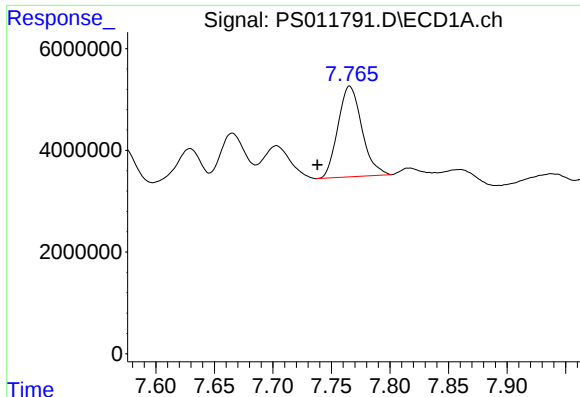

#7 MCPA


R.T.: 7.766 min
Delta R.T.: 0.028 min
Response: 25352406
Conc: 5.57 ug/ml

Instrument :
ECD_S
ClientSampleId :

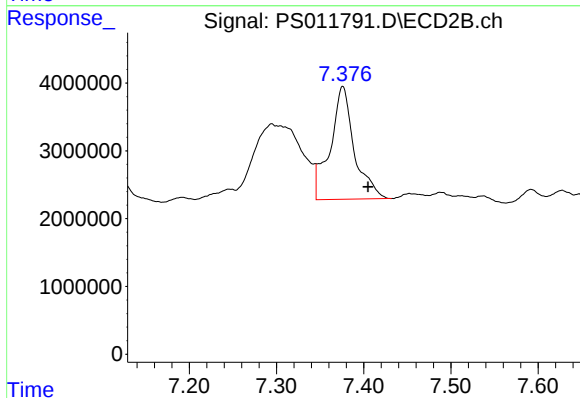


#7 MCPA

R.T.: 7.376 min
Delta R.T.: -0.029 min
Response: 31965106
Conc: 11.67 ug/ml

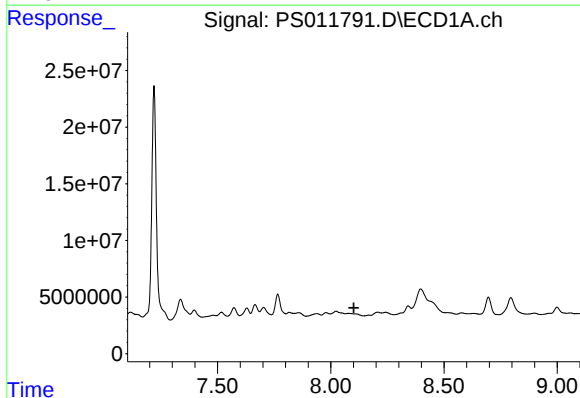


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.102 min
Response: 0
Conc: N.D.

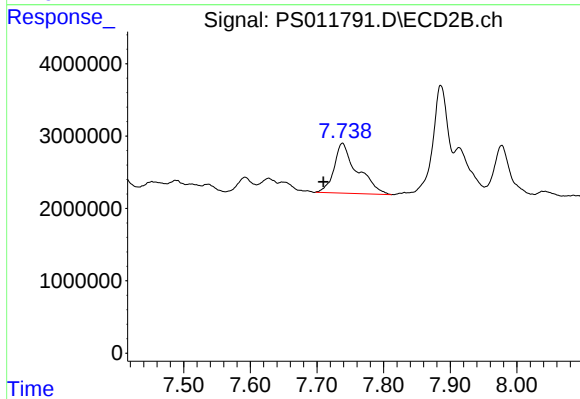

#8 DICHLORPROP


R.T.: 7.738 min
Delta R.T.: 0.029 min
Response: 16649052
Conc: 29.49 ng/ml

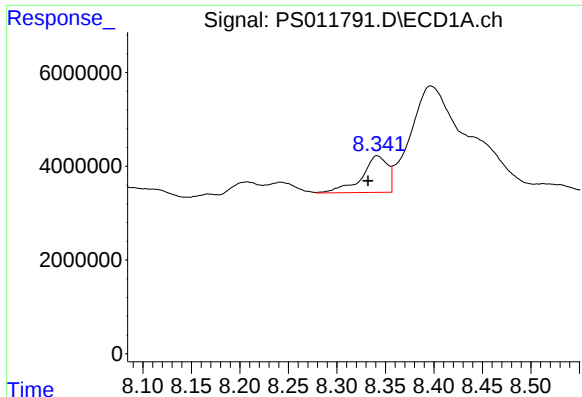

#9 2,4-D


R.T.: 8.342 min
Delta R.T.: 0.010 min
Response: 14533049
Conc: 12.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

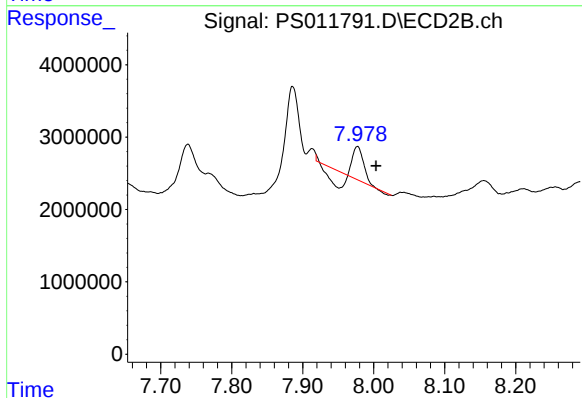


#9 2,4-D

R.T.: 7.977 min
Delta R.T.: -0.026 min
Response: 3012568
Conc: 4.10 ng/ml

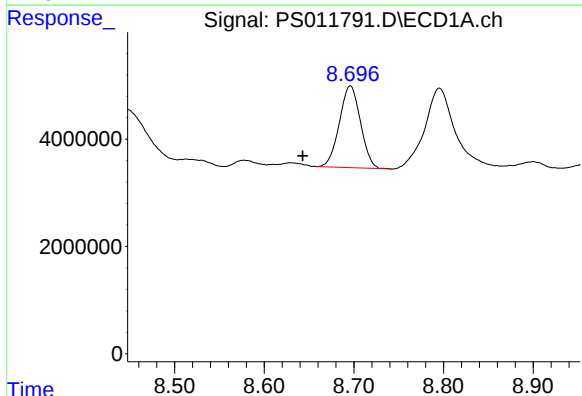


#10 Pentachlorophenol

R.T.: 8.696 min
Delta R.T.: 0.053 min
Response: 24951486
Conc: 1.73 ng/ml

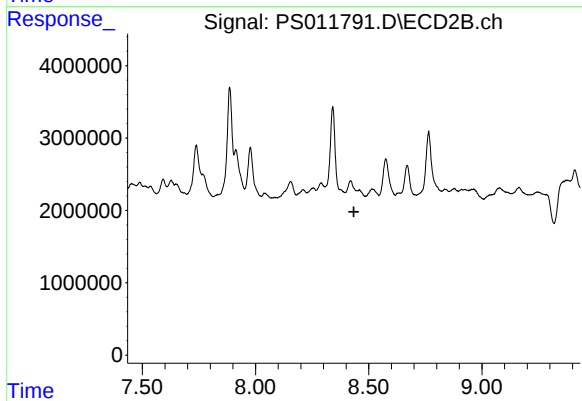

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 8.434 min
Response: 0
Conc: N.D.

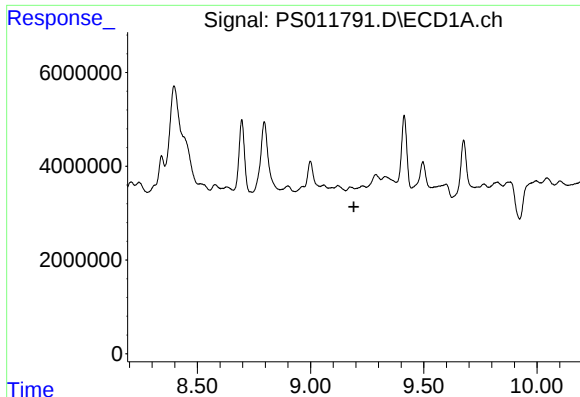

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.191 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

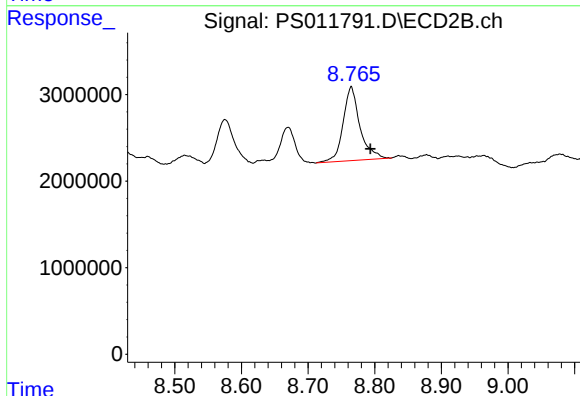


#11 2,4,5-TP (SILVEX)

R.T.: 8.765 min
Delta R.T.: -0.029 min
Response: 14977303
Conc: 5.12 ng/ml

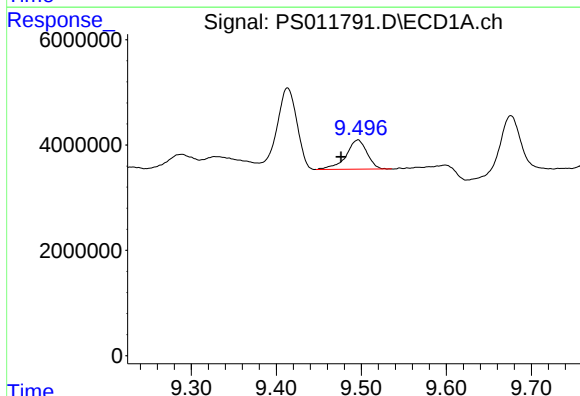


#12 2,4,5-T

R.T.: 9.496 min
Delta R.T.: 0.020 min
Response: 9548168
Conc: 1.61 ng/ml

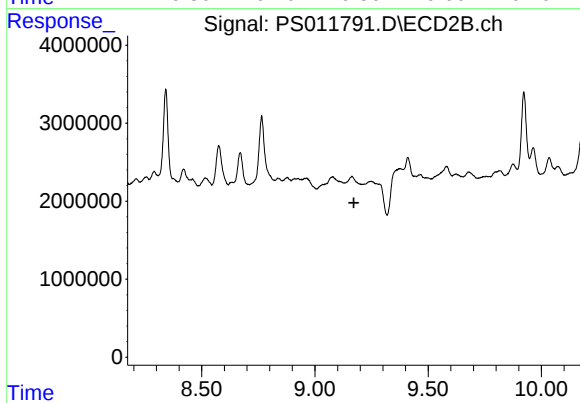

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.172 min
Response: 0
Conc: N.D.

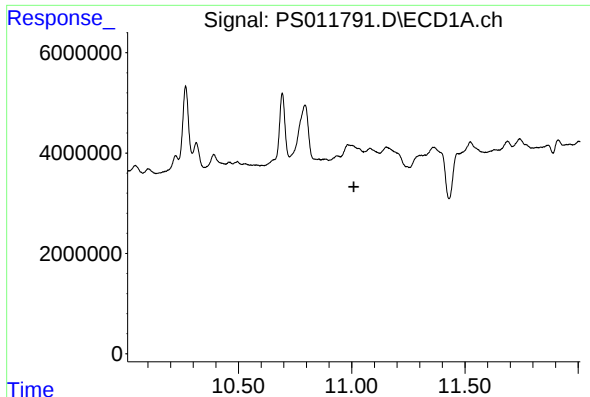

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.009 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

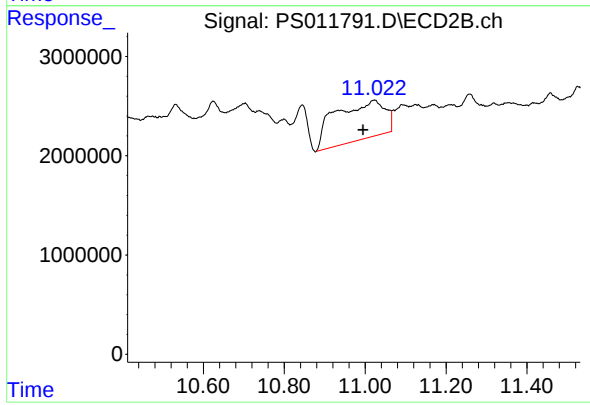

#15 Picloram

R.T.: 11.022 min
Delta R.T.: 0.027 min
Response: 33189396
Conc: 7.32 ng/ml