

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081420\
 Data File : PS011799.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2020 17:40
 Operator : DD\AJ
 Sample : PB130978TB
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 18:17:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 11 15:43:16 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.219	6.914	292.2E6	182.1E6	267.843	340.515 #
Target Compounds							
1) T	Dalapon	2.994	2.584	19579212	31037184	15.718	41.063 #
2) T	3,5-DICHL...	0.000	6.096	0	71450402	N.D.	86.857
3) T	4-Nitroph...	6.989	0.000	1577767	0	2.679	N.D. #
5) T	DICAMBA	7.397	7.049	8072493	13383824	1.971	6.195 #
6) T	MCPD	7.567	0.000	10976593	0	3.435	N.D. #
7) T	MCPA	7.685	7.396	101.6E6	17278084	22.347	6.306 #
8) T	DICHLORPROP	0.000	7.735	0	47032330	N.D.	83.297
9) T	2,4-D	8.399	0.000	113.2E6	0	100.271	N.D. #
10) T	Pentachlo...	8.696	0.000	12978564	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.761	0	12173534	N.D.	4.164
12) T	2,4,5-T	9.413	0.000	28548671	0	4.818	N.D. #
15) T	Picloram	11.006	11.011	13687832	1926476	1.751	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081420\
Data File : PS011799.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2020 17:40
Operator : DD\AJ
Sample : PB130978TB
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 18:17:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081120.M
Quant Title : 8080.M
QLast Update : Tue Aug 11 15:43:16 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

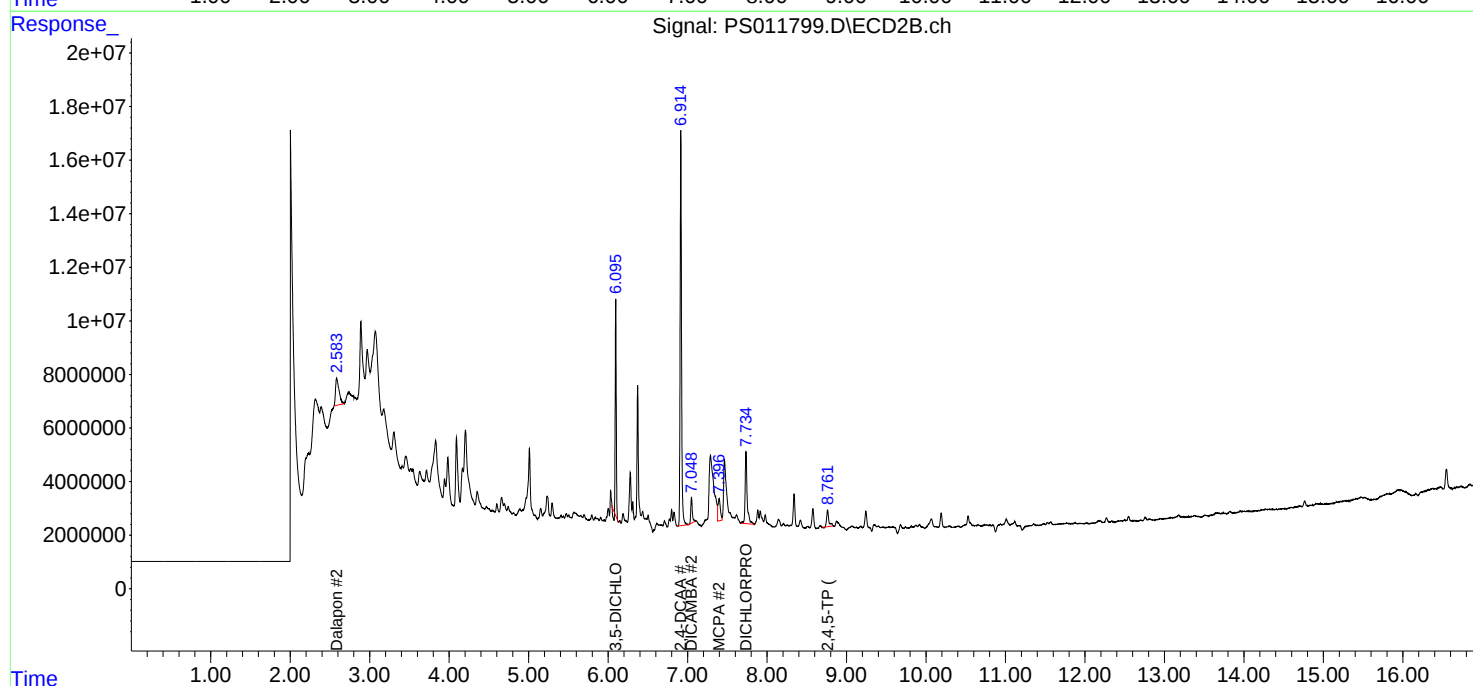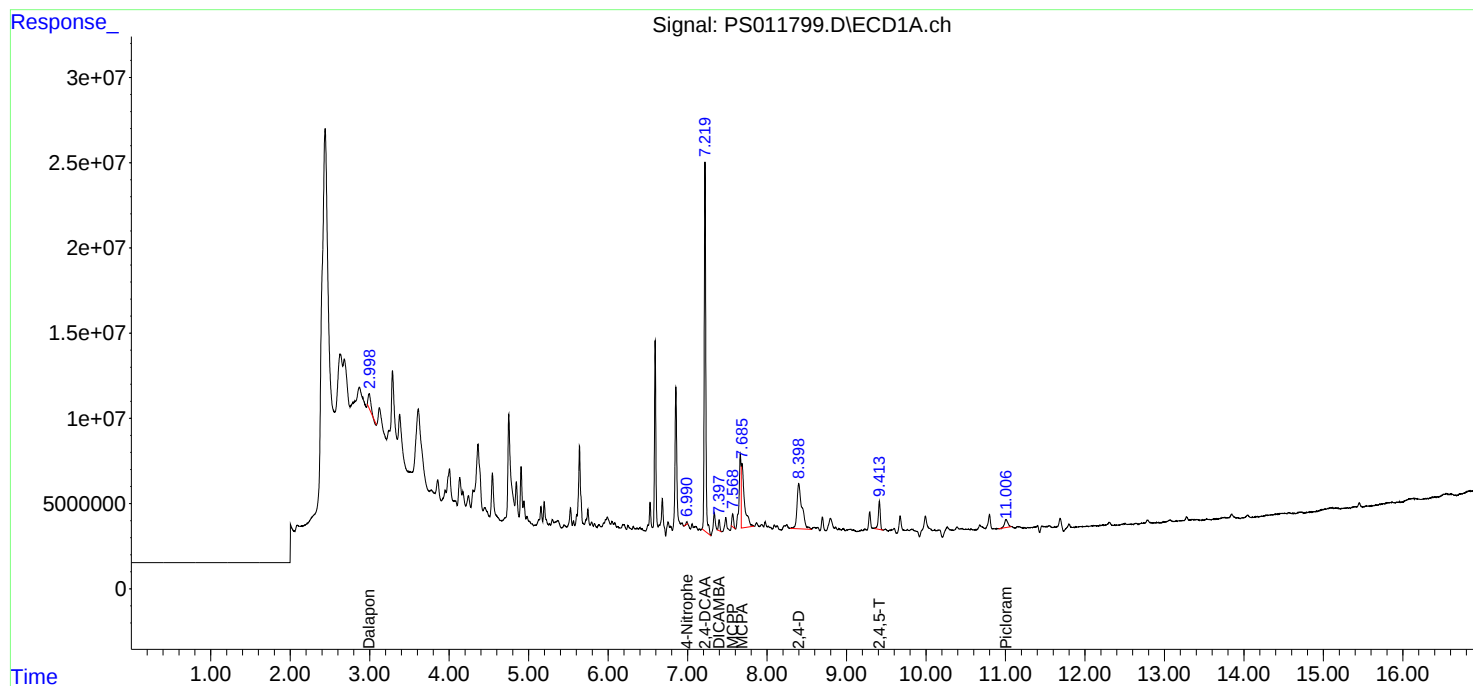


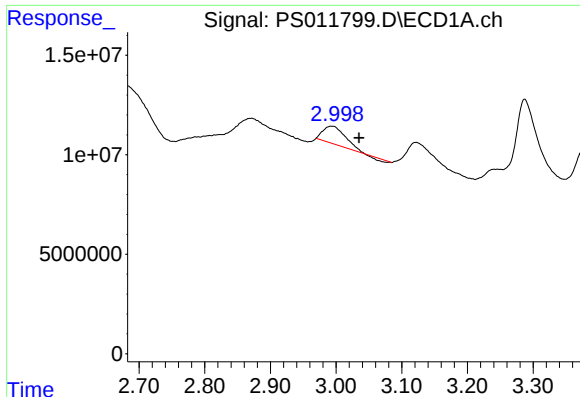

#1 Dalapon


R.T.: 2.994 min
Delta R.T.: -0.041 min
Response: 19579212
Conc: 15.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

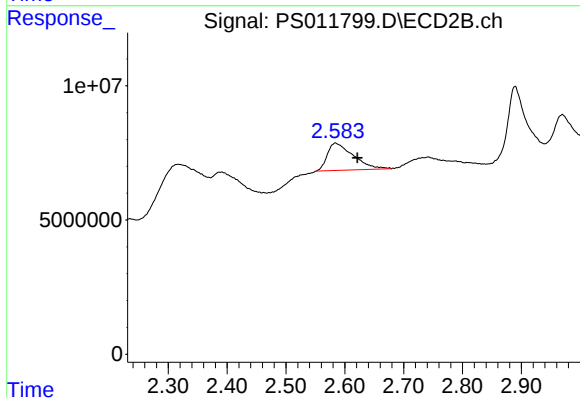


#1 Dalapon

R.T.: 2.584 min
Delta R.T.: -0.037 min
Response: 31037184
Conc: 41.06 ng/ml

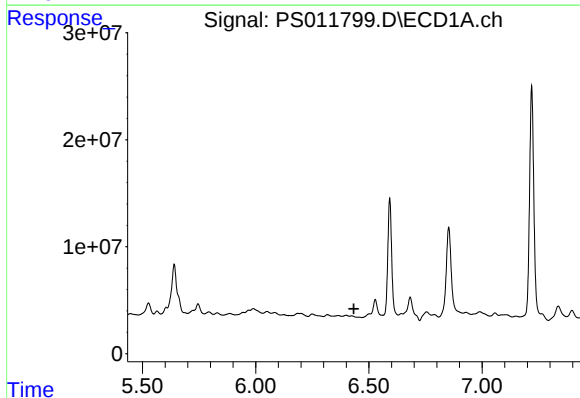


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.434 min
Response: 0
Conc: N.D.

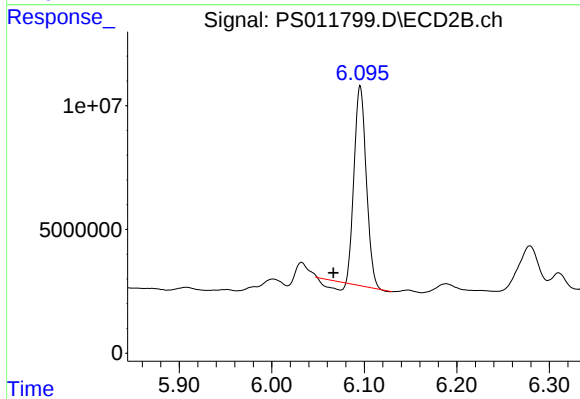

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.096 min
Delta R.T.: 0.029 min
Response: 71450402
Conc: 86.86 ng/ml

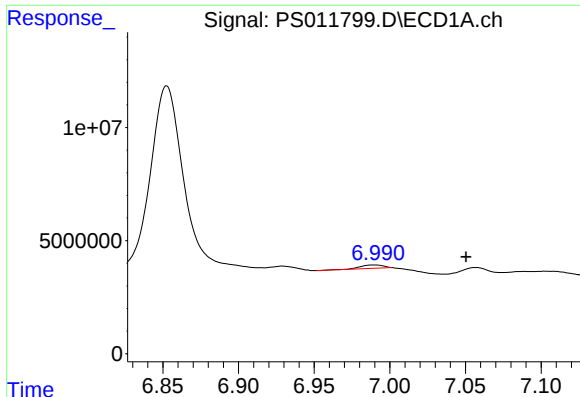

#3 4-Nitrophenol


R.T.: 6.989 min
Delta R.T.: -0.061 min
Response: 1577767
Conc: 2.68 ng/ml

Instrument :
ECD_S
ClientSampleId :

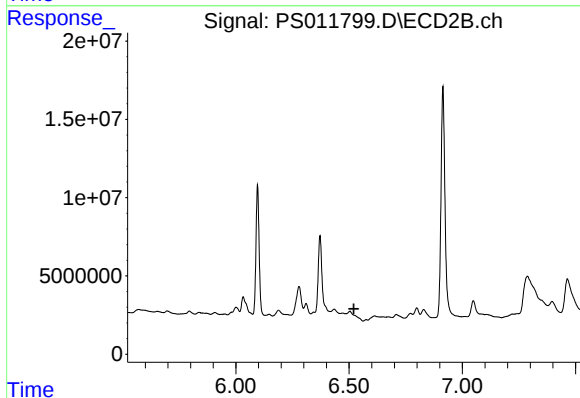


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.521 min
Response: 0
Conc: N.D.

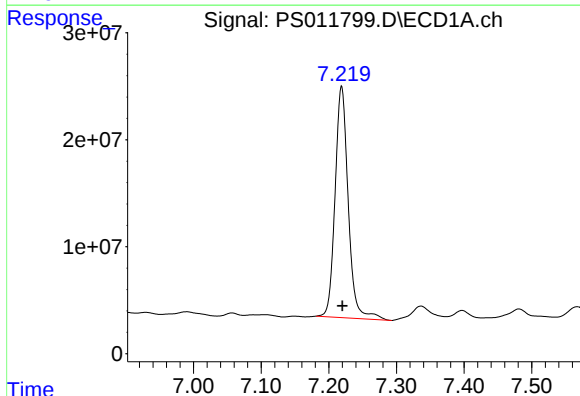


#4 2,4-DCAA

R.T.: 7.219 min
Delta R.T.: -0.001 min
Response: 292154792
Conc: 267.84 ng/ml

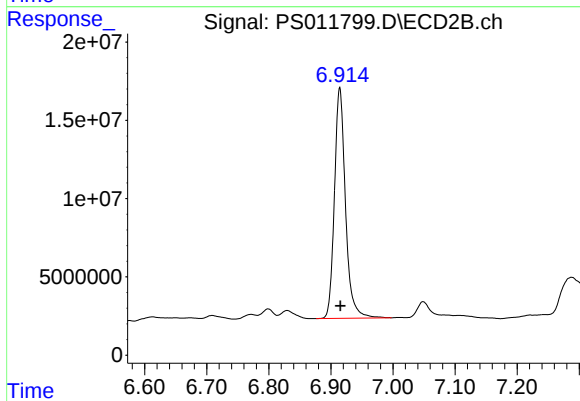

#4 2,4-DCAA


R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 182102945
Conc: 340.52 ng/ml

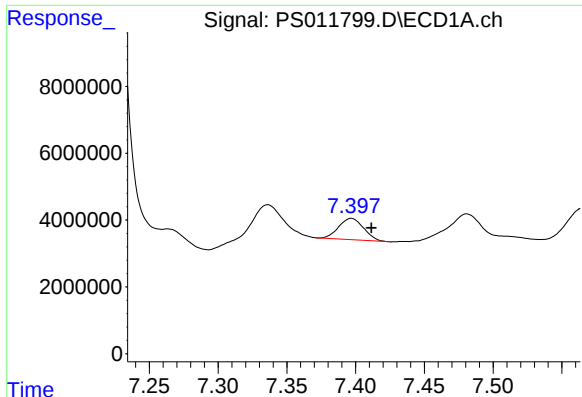

#5 DICAMBA


R.T.: 7.397 min
Delta R.T.: -0.015 min
Response: 8072493
Conc: 1.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

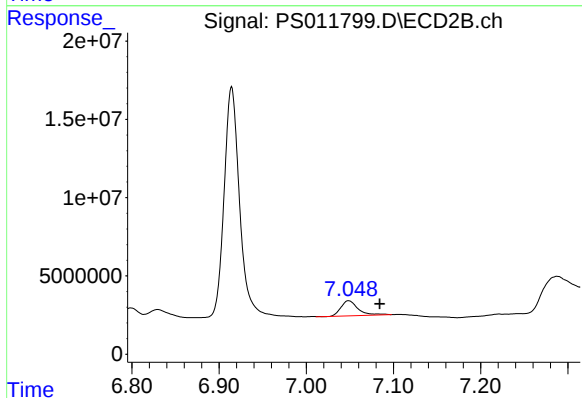


#5 DICAMBA

R.T.: 7.049 min
Delta R.T.: -0.035 min
Response: 13383824
Conc: 6.19 ng/ml

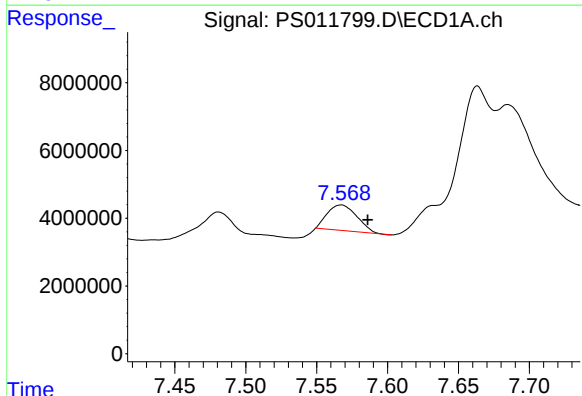


#6 MCP

R.T.: 7.567 min
Delta R.T.: -0.019 min
Response: 10976593
Conc: 3.44 ug/ml

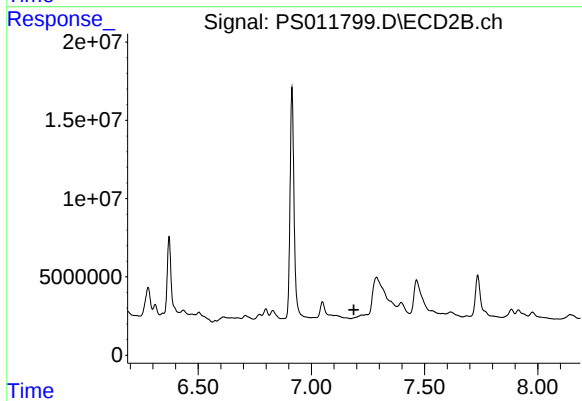

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.188 min
Response: 0
Conc: N.D.

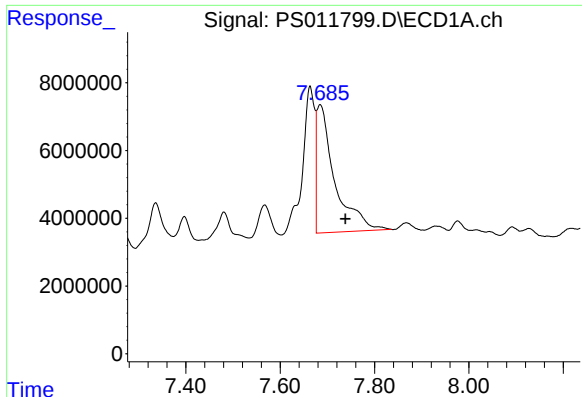

#7 MCPA


R.T.: 7.685 min
Delta R.T.: -0.054 min
Response: 101646581
Conc: 22.35 ug/ml

Instrument :
ECD_S
ClientSampleId :

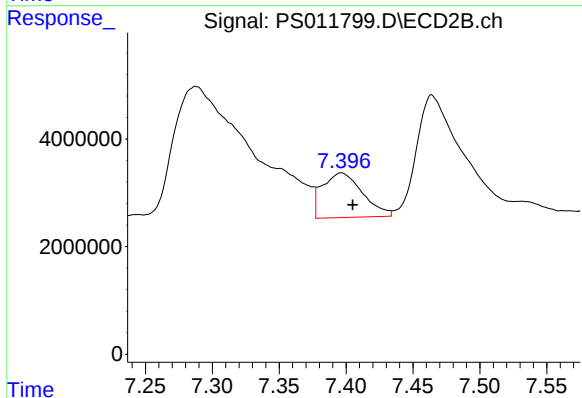


#7 MCPA

R.T.: 7.396 min
Delta R.T.: -0.009 min
Response: 17278084
Conc: 6.31 ug/ml

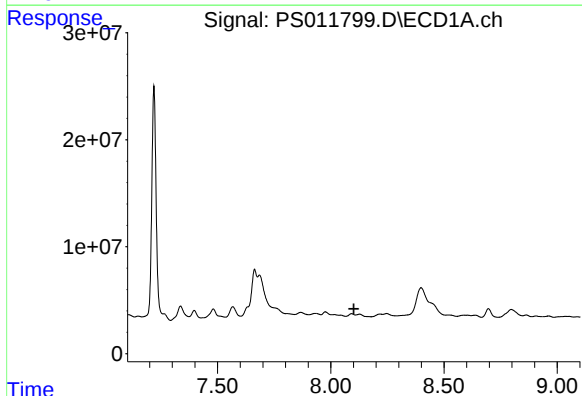


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.102 min
Response: 0
Conc: N.D.

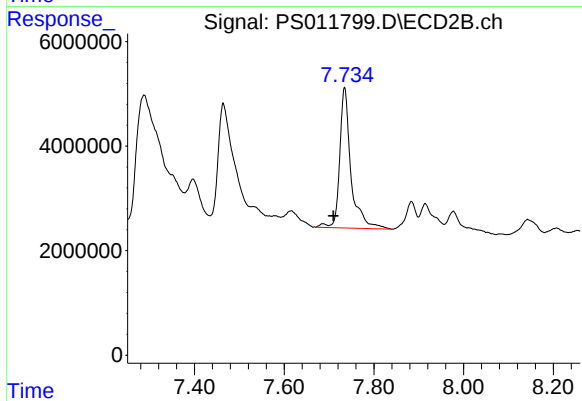

#8 DICHLORPROP


R.T.: 7.735 min
Delta R.T.: 0.025 min
Response: 47032330
Conc: 83.30 ng/ml

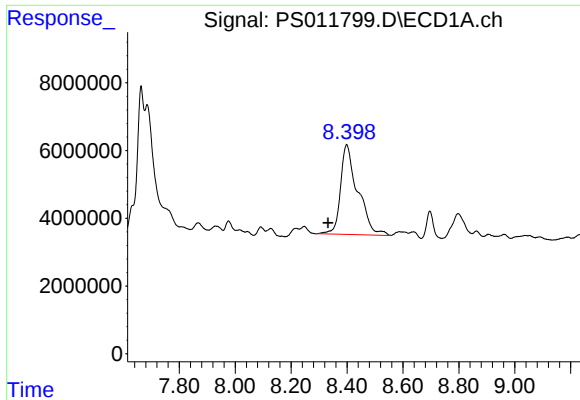

#9 2,4-D


R.T.: 8.399 min
Delta R.T.: 0.067 min
Response: 113215560
Conc: 100.27 ng/ml

Instrument :
ECD_S
ClientSampleId :

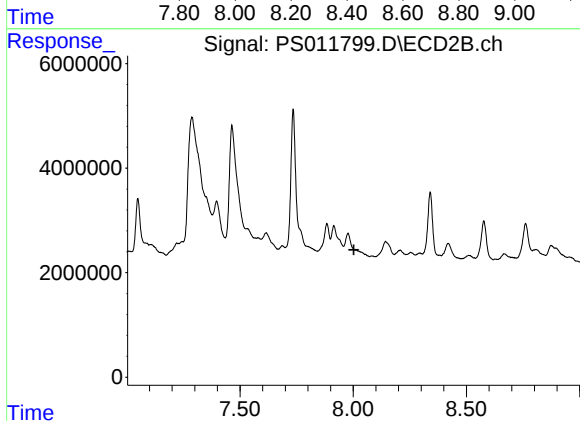


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.003 min
Response: 0
Conc: N.D.

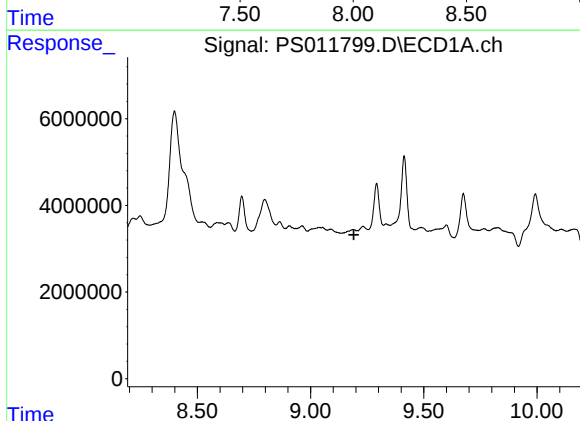


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.191 min
Response: 0
Conc: N.D.

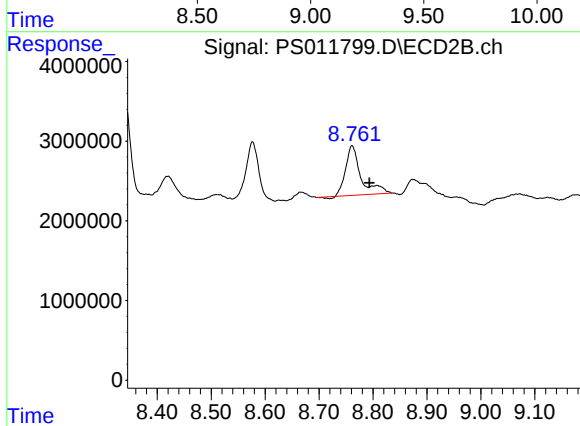

#11 2,4,5-TP (SILVEX)


R.T.: 8.761 min
Delta R.T.: -0.032 min
Response: 12173534
Conc: 4.16 ng/ml

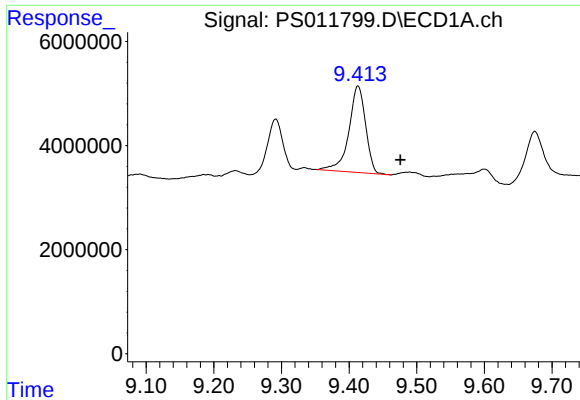

#12 2,4,5-T


R.T.: 9.413 min
Delta R.T.: -0.063 min
Response: 28548671
Conc: 4.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

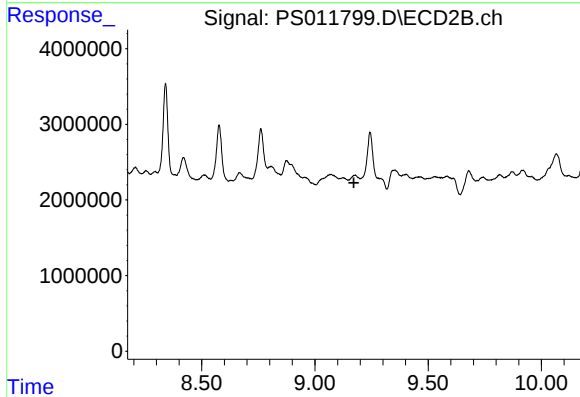


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.172 min
Response: 0
Conc: N.D.

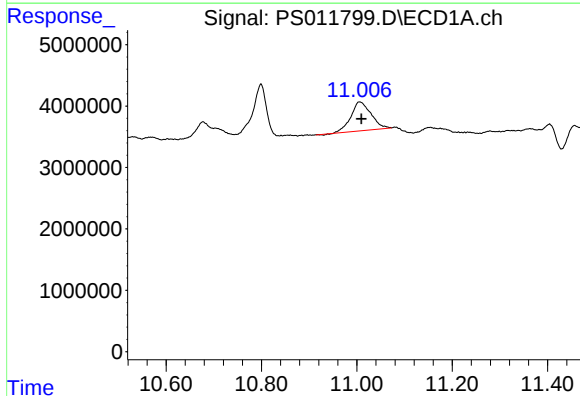

#15 Picloram

R.T.: 11.006 min
Delta R.T.: -0.003 min
Response: 13687832
Conc: 1.75 ng/ml

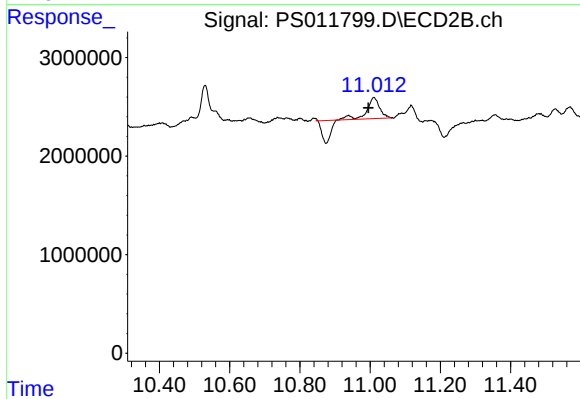

#15 Picloram

R.T.: 11.011 min
Delta R.T.: 0.015 min
Response: 1926476
Conc: N.D.