

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081423\
 Data File : PS024066.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Aug 2023 08:55
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 14 20:34:36 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080823.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 08 13:26:17 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.366	6.795	998.2E6	329.9E6	503.975	490.531
Target Compounds							
1) T	Dalapon	2.517	2.583	6844050	5016749	3.119	4.588 #
3) T	4-Nitroph...	6.208	0.000	6767557	0	6.114	N.D. #
5) T	DICAMBA	6.496	0.000	1323819	0	<MDL	N.D. #
6) T	MCP	6.686	0.000	502693	0	<MDL	N.D. #
7) T	MCPA	6.851f	0.000	474969	0	<MDL	N.D. #
8) T	DICHLORPROP	7.147f	7.589	688761	530658	<MDL	<MDL #
9) T	2,4-D	0.000	7.802f	0	487332	N.D.	<MDL #
11) T	2,4,5-TP ...	8.046	8.642	560740	402603	<MDL	<MDL #
12) T	2,4,5-T	8.302	9.058	737898	688833	<MDL	<MDL #
14) T	DINOSEB	9.856	0.000	735630	0	<MDL	N.D. #
15) T	Picloram	9.692	10.803	11806014	4802742	<MDL	<MDL #
16) T	DCPA	10.124	10.803	460261	4802742	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081423\
Data File : PS024066.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Aug 2023 08:55
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 14 20:34:36 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080823.M
Quant Title : 8080.M
QLast Update : Tue Aug 08 13:26:17 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

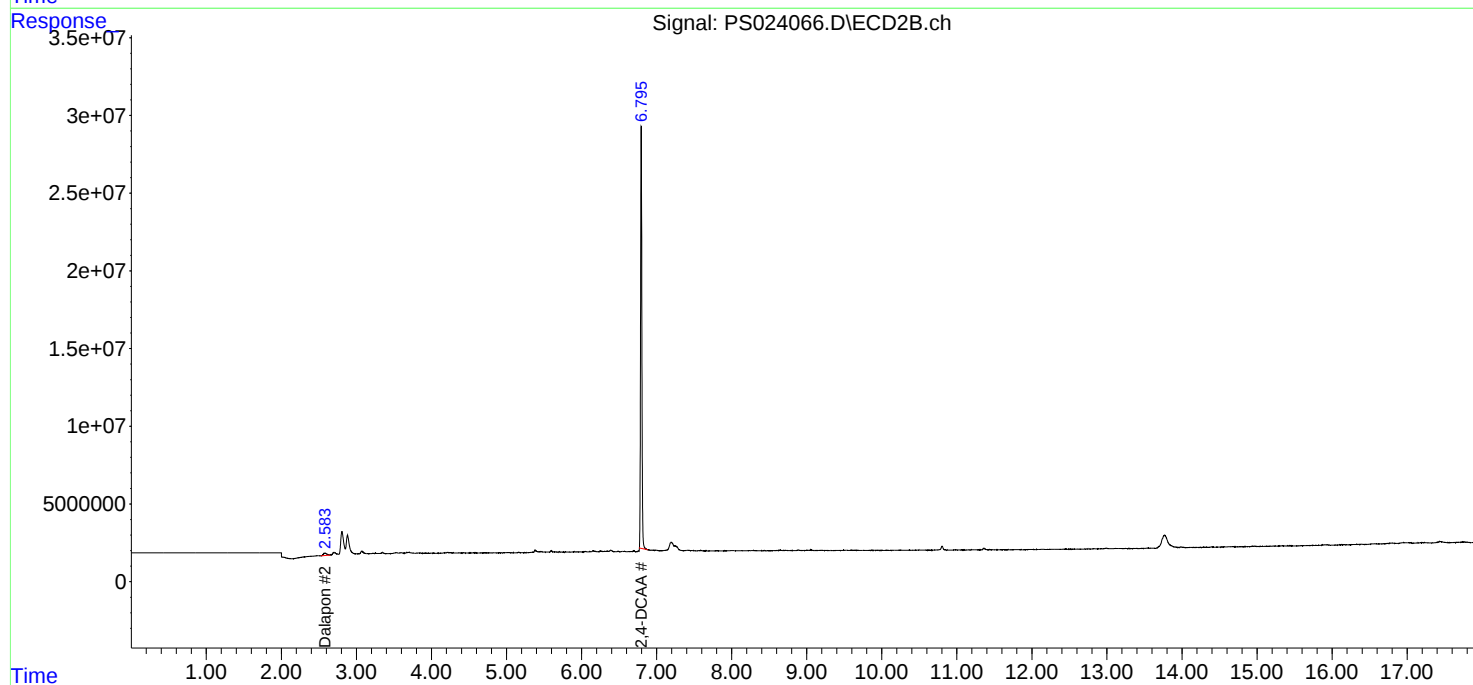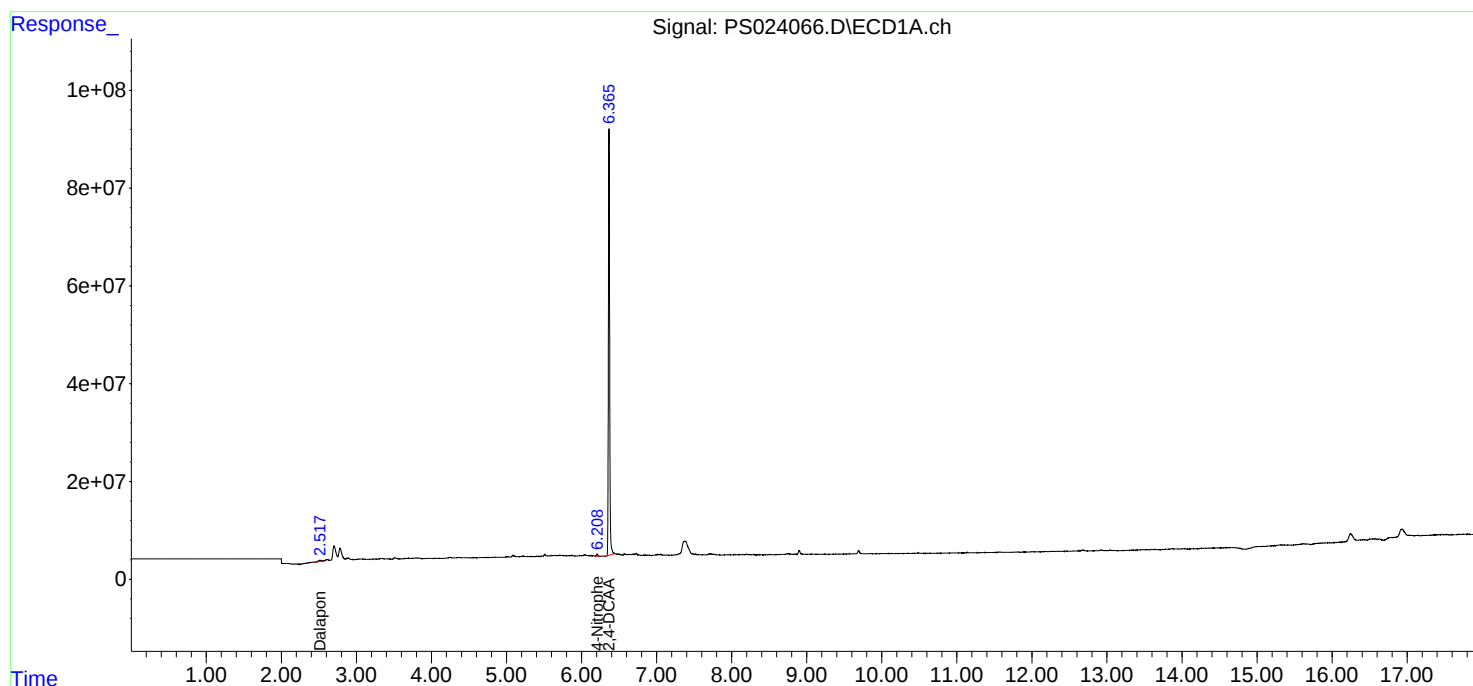


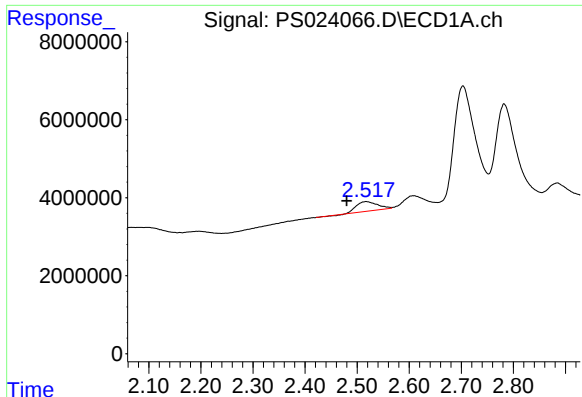

#1 Dalapon


R.T.: 2.517 min
Delta R.T.: 0.037 min
Response: 6844050
Conc: 3.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

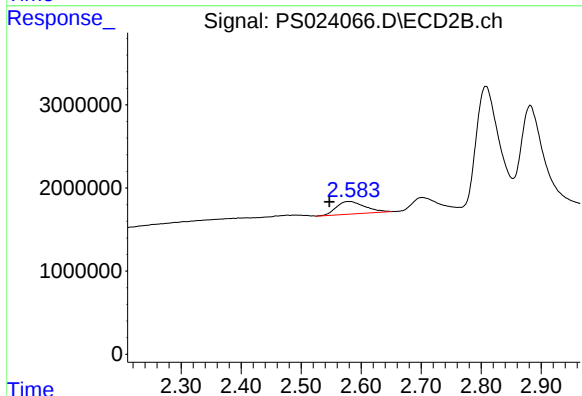


#1 Dalapon

R.T.: 2.583 min
Delta R.T.: 0.035 min
Response: 5016749
Conc: 4.59 ng/ml

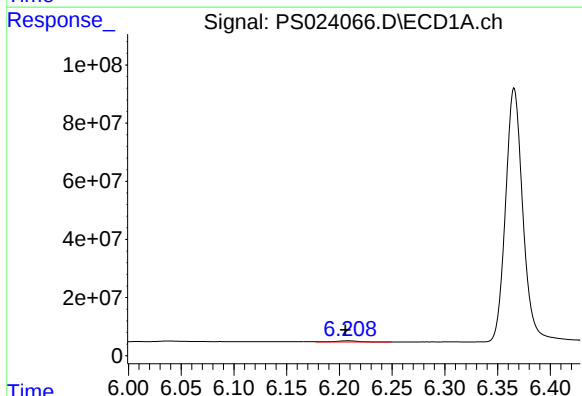


#3 4-Nitrophenol

R.T.: 6.208 min
Delta R.T.: 0.003 min
Response: 6767557
Conc: 6.11 ng/ml

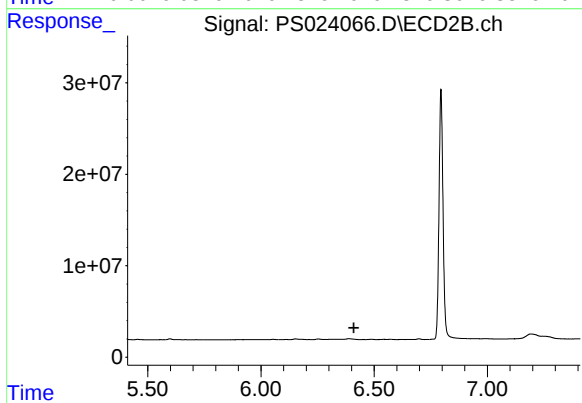

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.410 min
Response: 0
Conc: N.D.

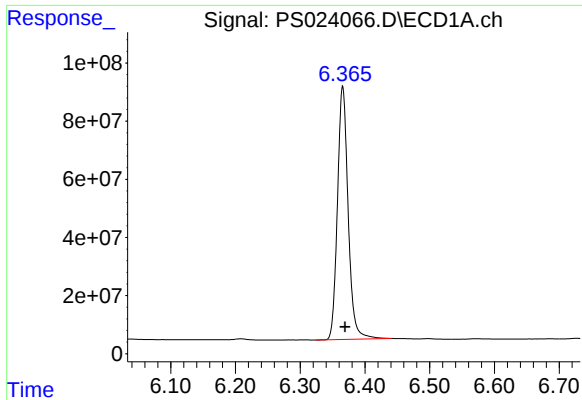

#4 2,4-DCAA

R.T.: 6.366 min
Delta R.T.: -0.003 min
Response: 998153295
Conc: 503.97 ng/ml

Instrument :
ECD_S
ClientSampleId :

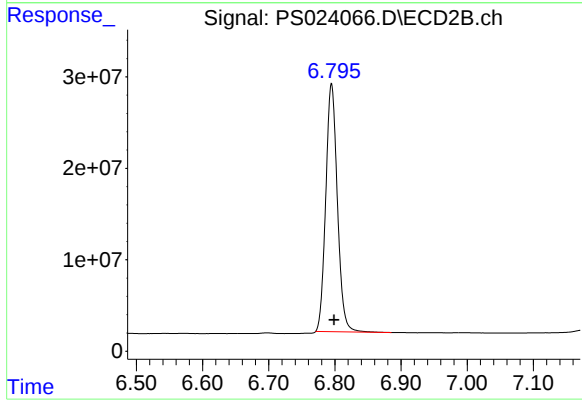

#4 2,4-DCAA

R.T.: 6.795 min
Delta R.T.: -0.004 min
Response: 329944795
Conc: 490.53 ng/ml