

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081518\
 Data File : PS001500.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2018 17:05
 Operator : UA
 Sample : J4454-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 17:39:07 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.620	11.030	96410930	88810650	519.596	488.306
Target Compounds							
1) T	Dalapon	2.965	2.409	2960696	264585	12.486	1.161 #
2) T	3,5-DICHL...	10.046	0.000	4003892	0	14.835	N.D. #
3) T	4-Nitroph...	0.000	10.188	0	6675214	N.D.	65.482 #
5) T	DICAMBA	0.000	11.273	0	5256042	N.D.	7.669 #
6) T	MCP	12.313	0.000	7056020	0	14.039	N.D. #
12) T	2,4,5-T	0.000	14.657	0	2396994	N.D.	2.595 #
13) T	2,4-DB	15.824	0.000	1922289	0	13.353	N.D. #
15) T	Picloram	17.154	16.970	5220444	13275410	3.303	9.630 #
16) T	DCPA	17.754	16.970	5073011	13275410	3.758	9.192 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081518\
Data File : PS001500.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2018 17:05
Operator : UA
Sample : J4454-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 17:39:07 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

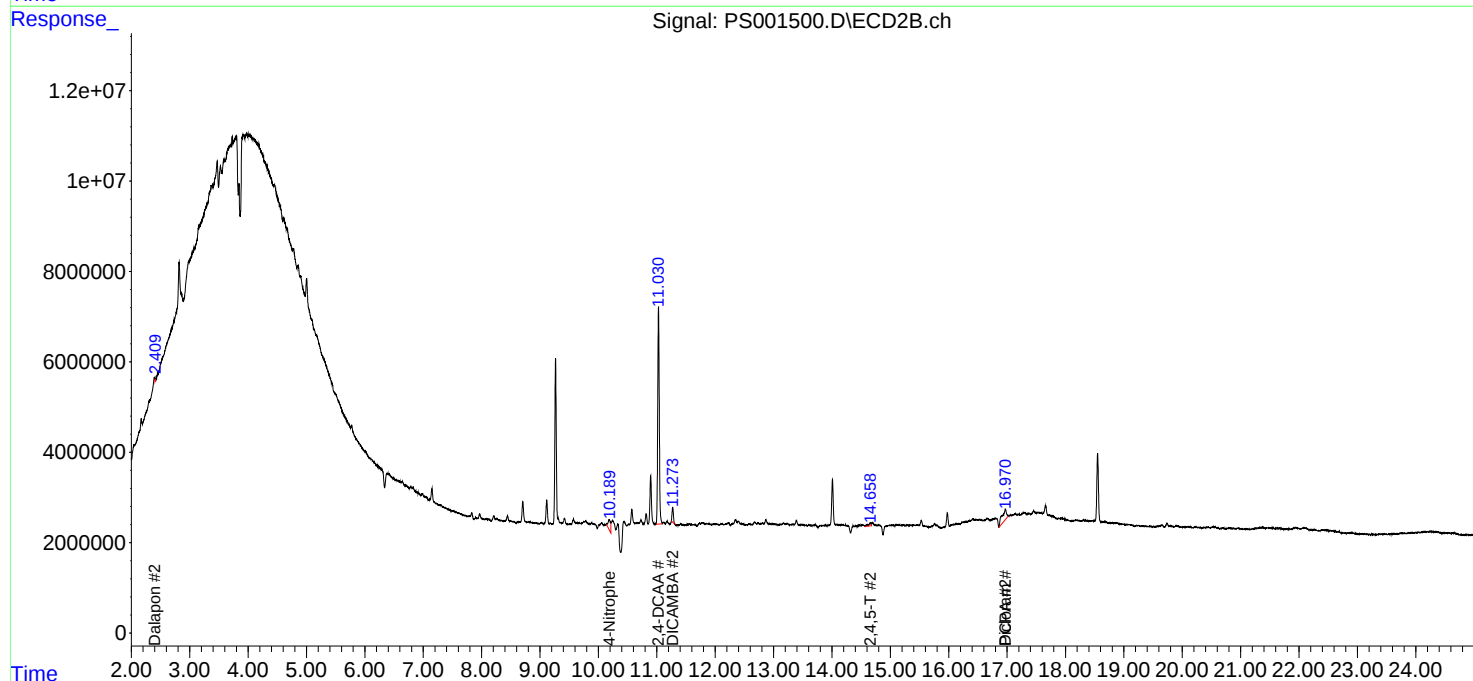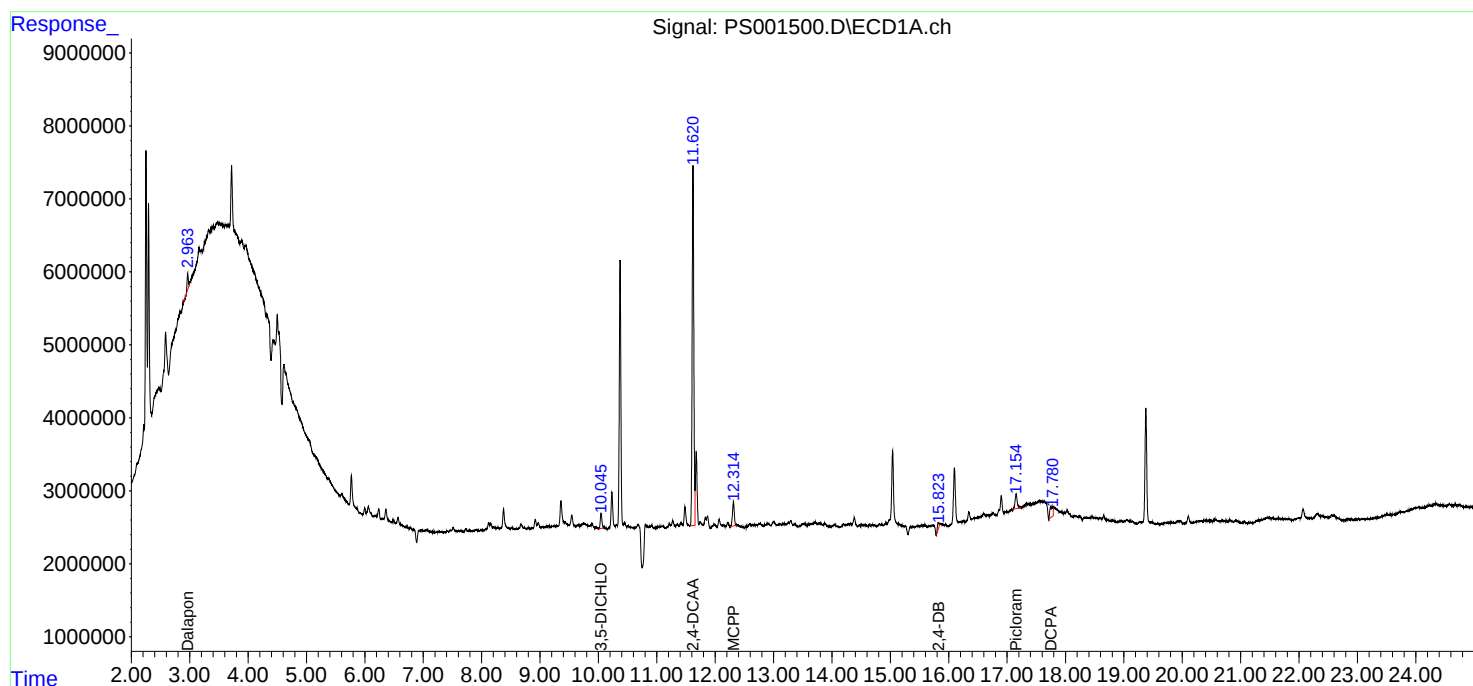


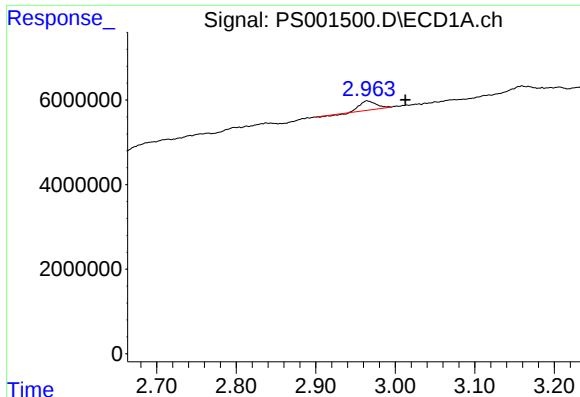

#1 Dalapon


R.T.: 2.965 min
Delta R.T.: -0.048 min
Response: 2960696
Conc: 12.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

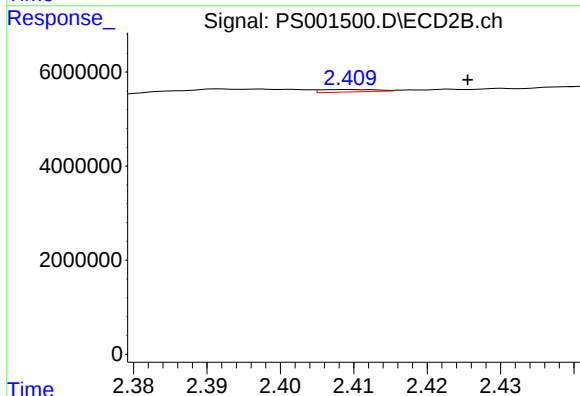


#1 Dalapon

R.T.: 2.409 min
Delta R.T.: -0.016 min
Response: 264585
Conc: 1.16 ng/ml

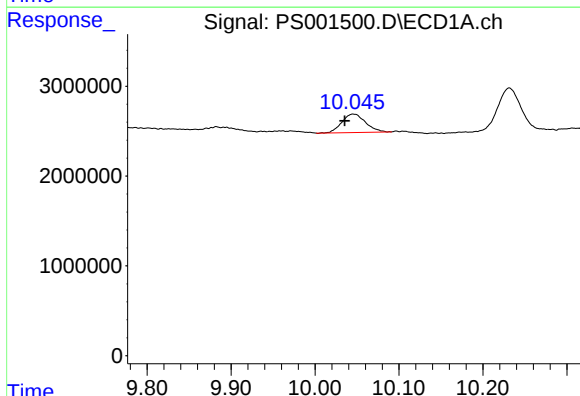


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 10.046 min
Delta R.T.: 0.010 min
Response: 4003892
Conc: 14.83 ng/ml

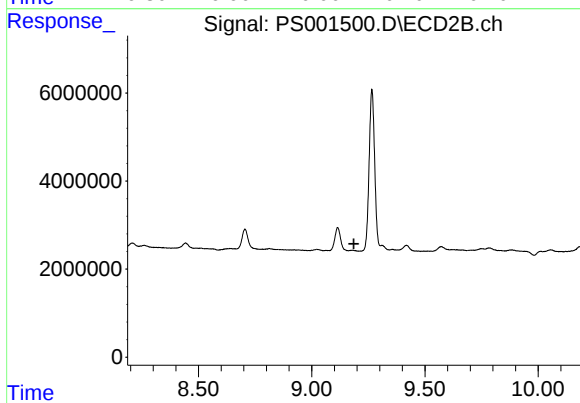

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.186 min
Response: 0
Conc: N.D.

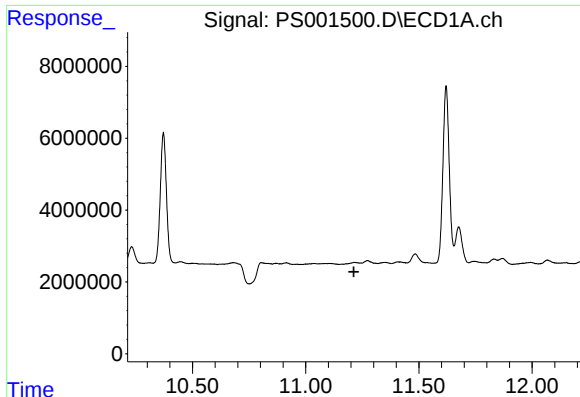

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 11.213 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

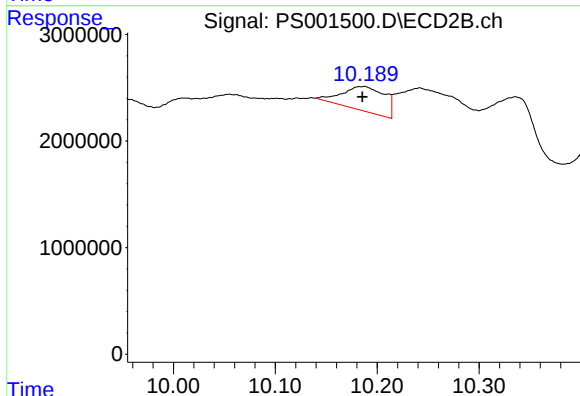


#3 4-Nitrophenol

R.T.: 10.188 min
Delta R.T.: 0.002 min
Response: 6675214
Conc: 65.48 ng/ml

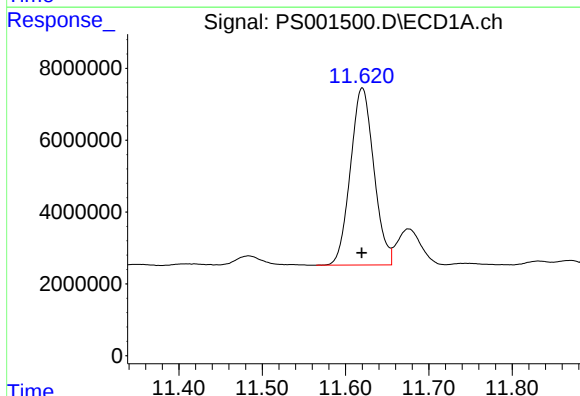


#4 2,4-DCAA

R.T.: 11.620 min
Delta R.T.: 0.000 min
Response: 96410930
Conc: 519.60 ng/ml

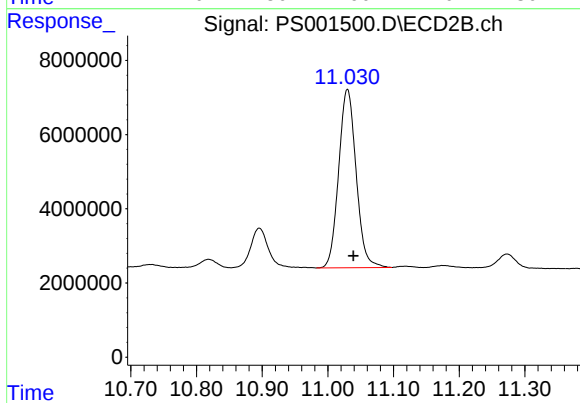

#4 2,4-DCAA


R.T.: 11.030 min
Delta R.T.: -0.009 min
Response: 88810650
Conc: 488.31 ng/ml

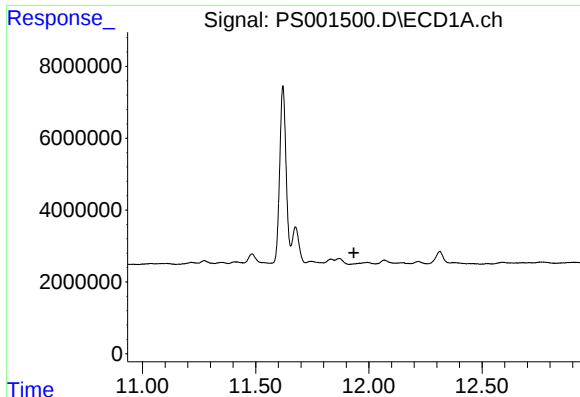

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.934 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

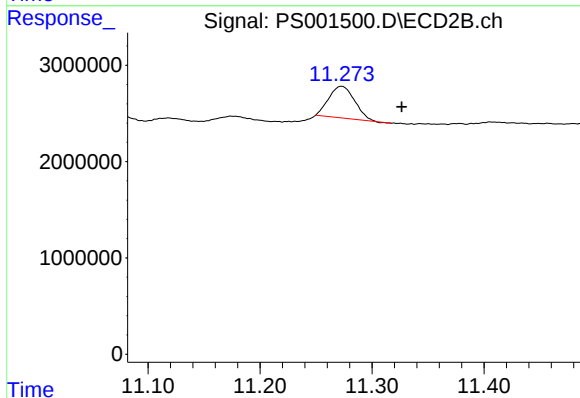


#5 DICAMBA

R.T.: 11.273 min
Delta R.T.: -0.054 min
Response: 5256042
Conc: 7.67 ng/ml

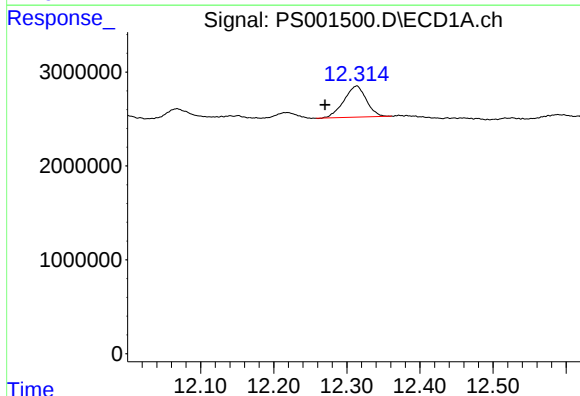


#6 MCP

R.T.: 12.313 min
Delta R.T.: 0.043 min
Response: 7056020
Conc: 14.04 ug/ml

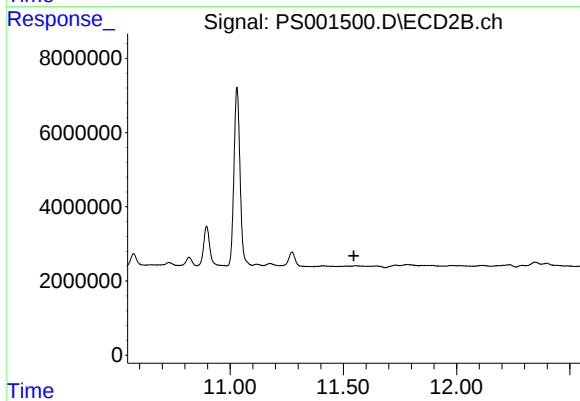

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.546 min
Response: 0
Conc: N.D.

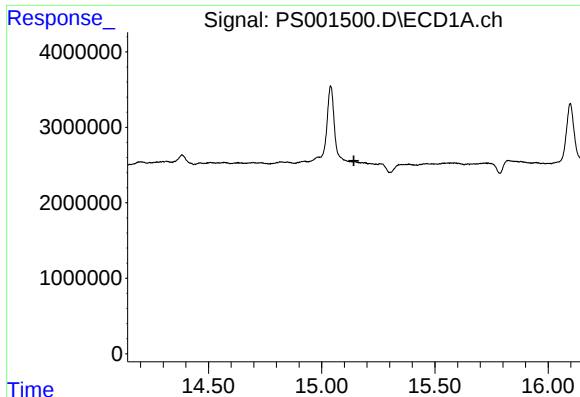

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.142 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

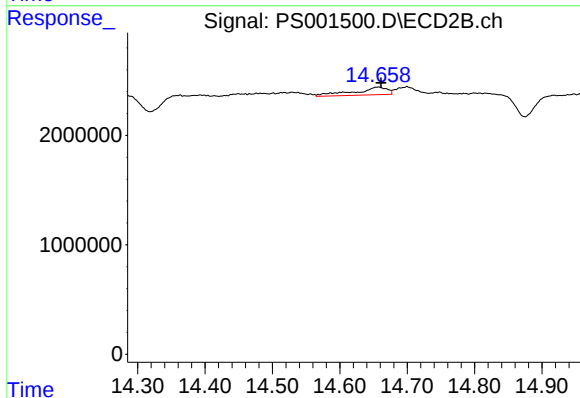


#12 2,4,5-T

R.T.: 14.657 min
Delta R.T.: -0.005 min
Response: 2396994
Conc: 2.59 ng/ml

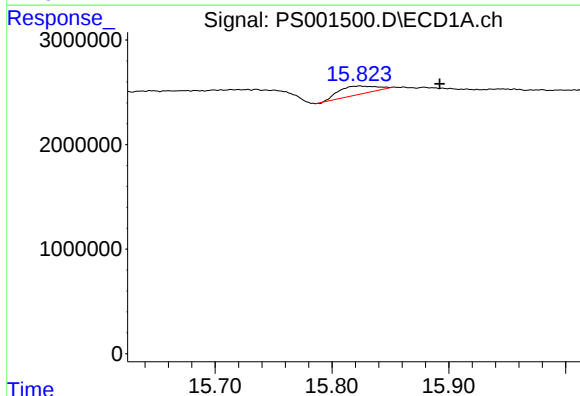


#13 2,4-DB

R.T.: 15.824 min
Delta R.T.: -0.068 min
Response: 1922289
Conc: 13.35 ng/ml

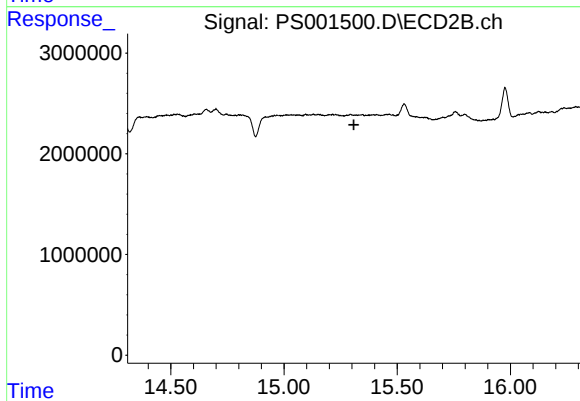

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.308 min
Response: 0
Conc: N.D.

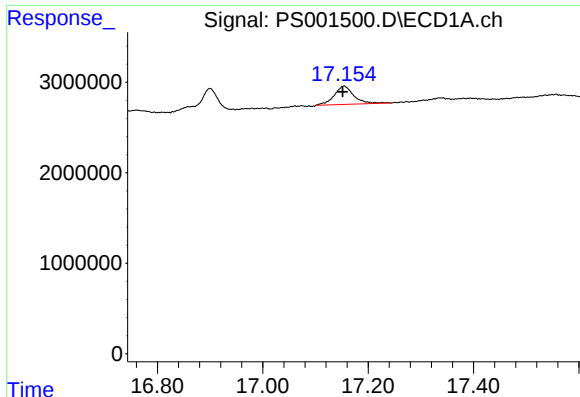

#15 Picloram


R.T.: 17.154 min
Delta R.T.: 0.002 min
Response: 5220444
Conc: 3.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

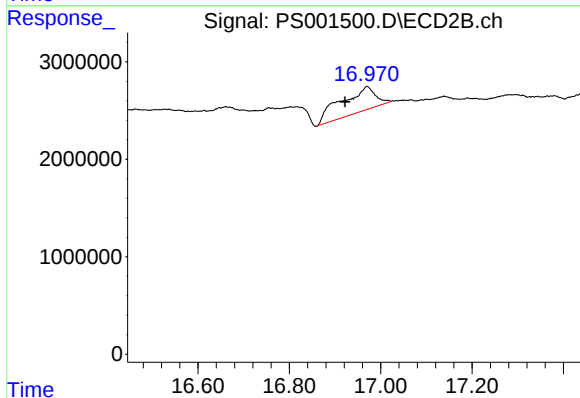


#15 Picloram

R.T.: 16.970 min
Delta R.T.: 0.048 min
Response: 13275410
Conc: 9.63 ng/ml

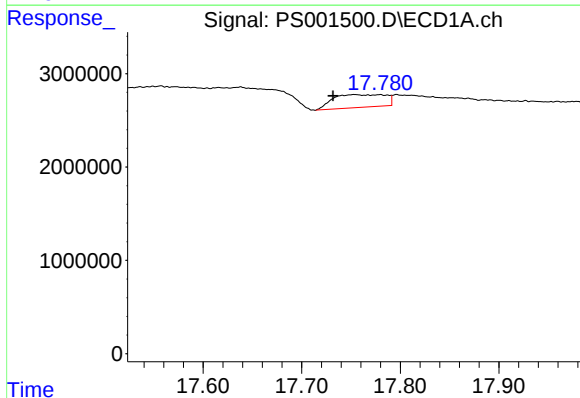

#16 DCPA

R.T.: 17.754 min
Delta R.T.: 0.022 min
Response: 5073011
Conc: 3.76 ng/ml

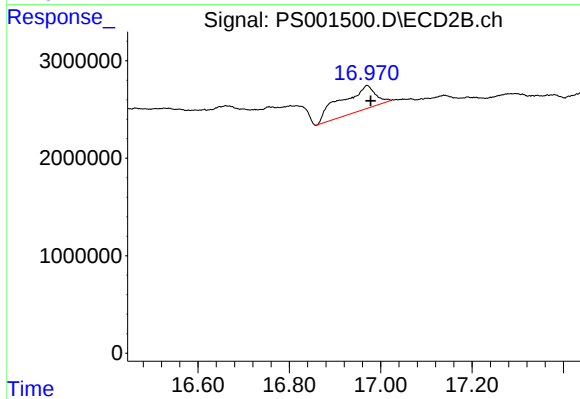

#16 DCPA

R.T.: 16.970 min
Delta R.T.: -0.008 min
Response: 13275410
Conc: 9.19 ng/ml