

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081518\
 Data File : PS001503.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2018 18:38
 Operator : UA
 Sample : PB112067BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 04:33:41 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.612	11.034	98972730	83073688	533.402	456.763
Target Compounds							
1) T	Dalapon	2.960	2.401	5266075	4846855	22.208	21.270
2) T	3,5-DICHL...	0.000	9.121	0	69866	N.D.	0.274 #
5) T	DICAMBA	0.000	11.277	0	5580924	N.D.	8.143 #
6) T	MCP	12.305	0.000	7483558	0	14.889	N.D. #
7) T	MCPA	12.581	0.000	8249573	0	10.461	N.D. #
12) T	2,4,5-T	0.000	14.659	0	2973238	N.D.	3.219 #
14) T	DINOSEB	0.000	15.728	0	9316147	N.D.	13.106 #
15) T	Picloram	0.000	16.976	0	22303206	N.D.	16.179 #
16) T	DCPA	0.000	16.976	0	22303206	N.D.	15.442 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081518\
Data File : PS001503.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2018 18:38
Operator : UA
Sample : PB112067BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 04:33:41 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

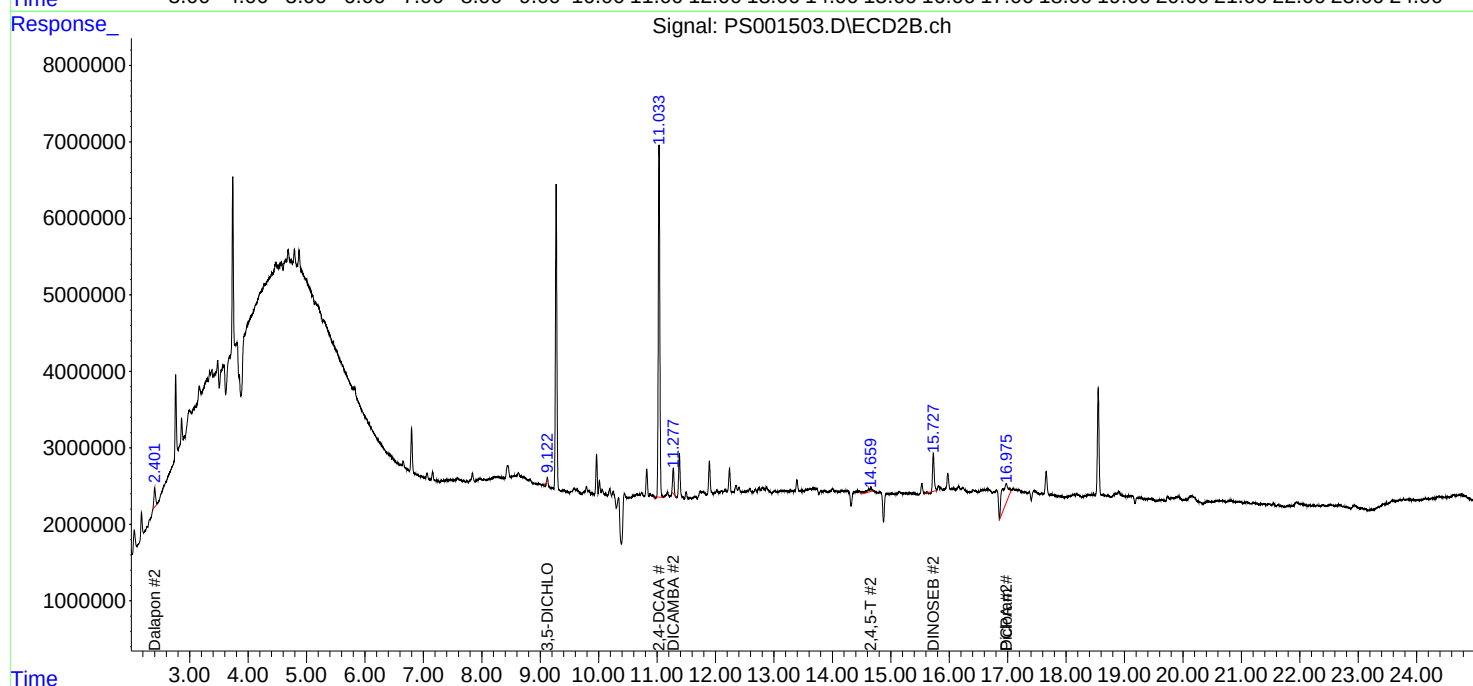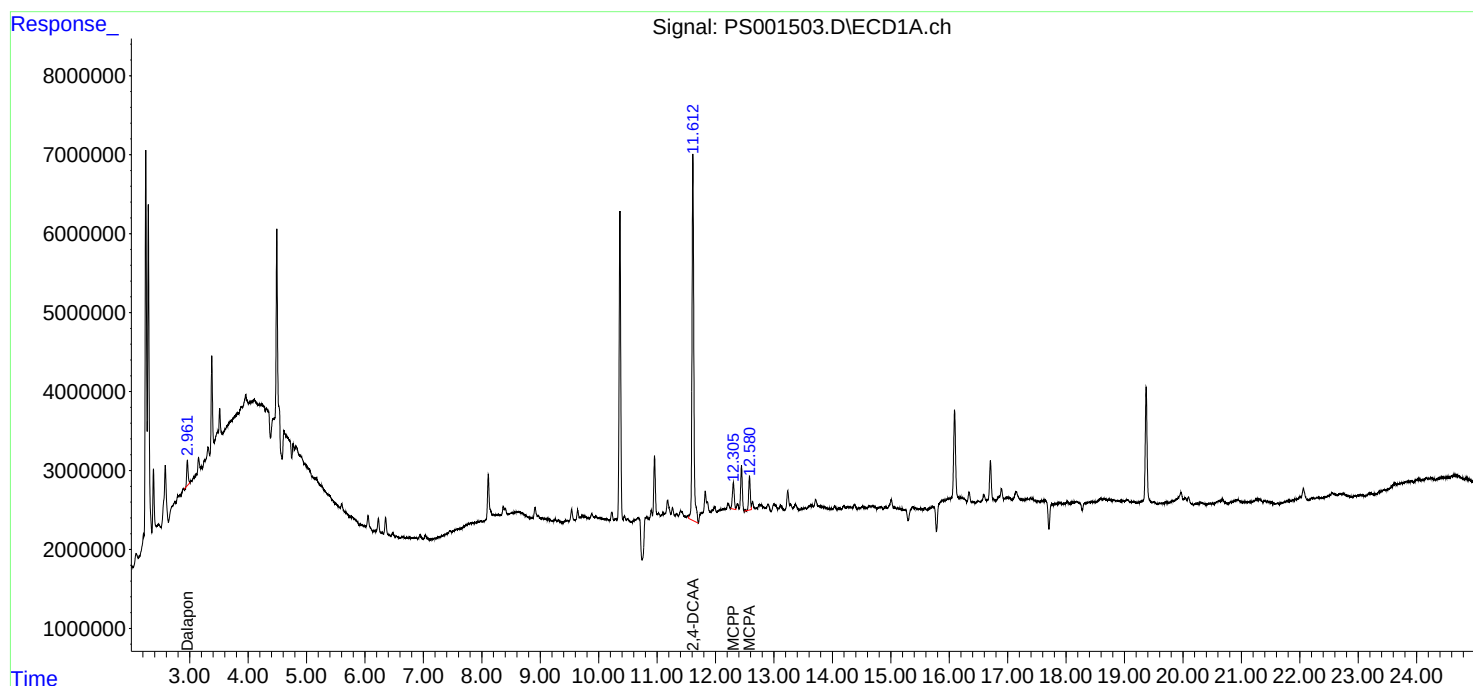


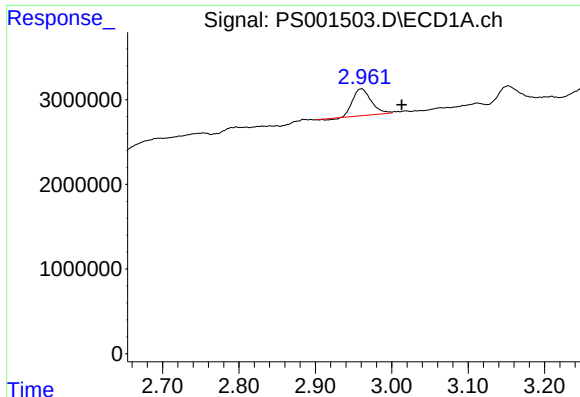

#1 Dalapon


R.T.: 2.960 min
Delta R.T.: -0.053 min
Response: 5266075
Conc: 22.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

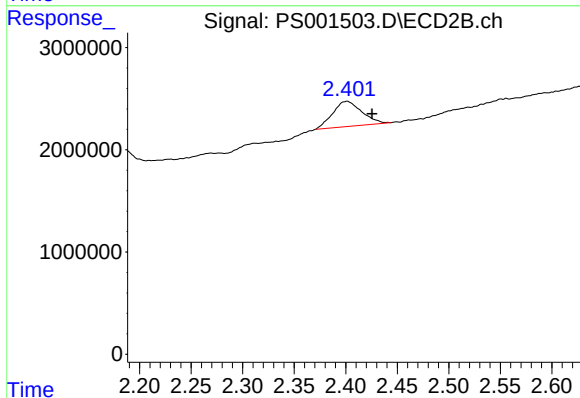


#1 Dalapon

R.T.: 2.401 min
Delta R.T.: -0.024 min
Response: 4846855
Conc: 21.27 ng/ml

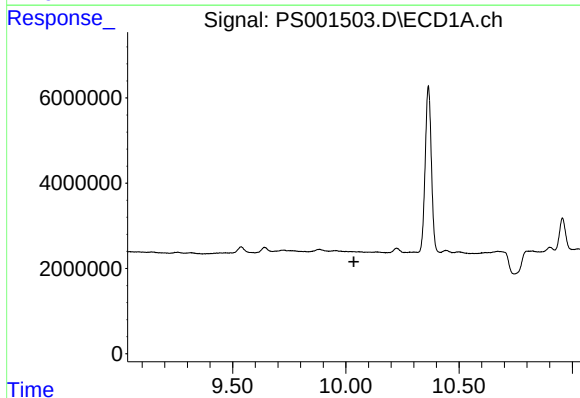


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 10.035 min
Response: 0
Conc: N.D.

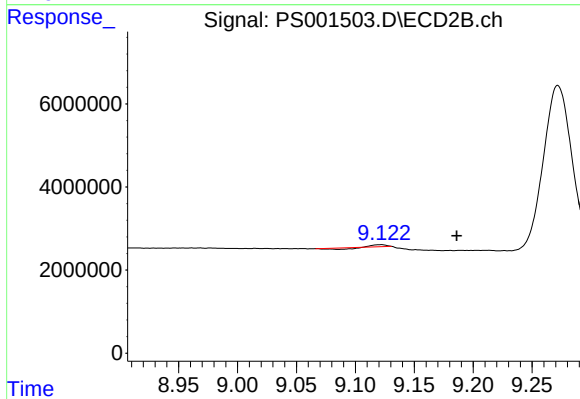

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.121 min
Delta R.T.: -0.065 min
Response: 69866
Conc: 0.27 ng/ml

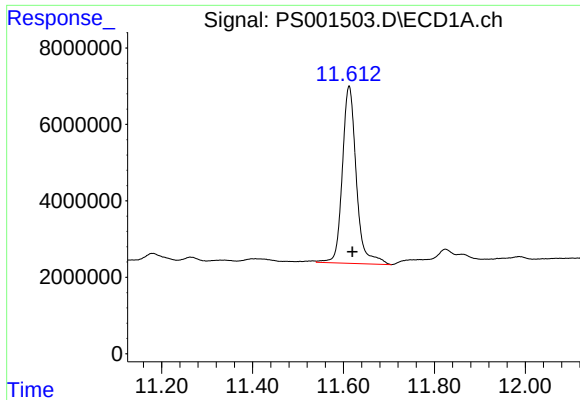

#4 2,4-DCAA


R.T.: 11.612 min
Delta R.T.: -0.007 min
Response: 98972730
Conc: 533.40 ng/ml

Instrument :
ECD_S
ClientSampleId :

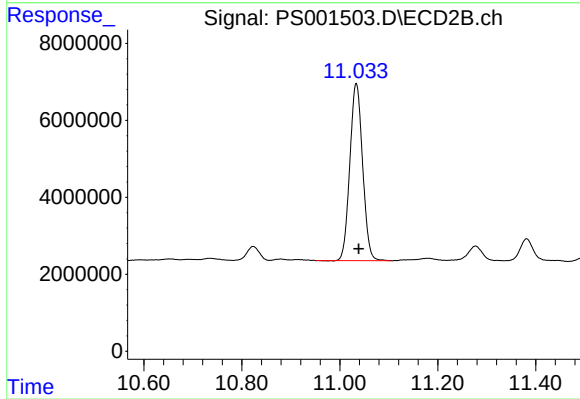


#4 2,4-DCAA

R.T.: 11.034 min
Delta R.T.: -0.005 min
Response: 83073688
Conc: 456.76 ng/ml

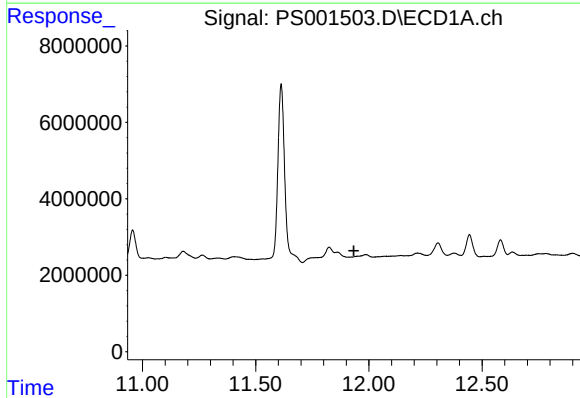


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.934 min
Response: 0
Conc: N.D.

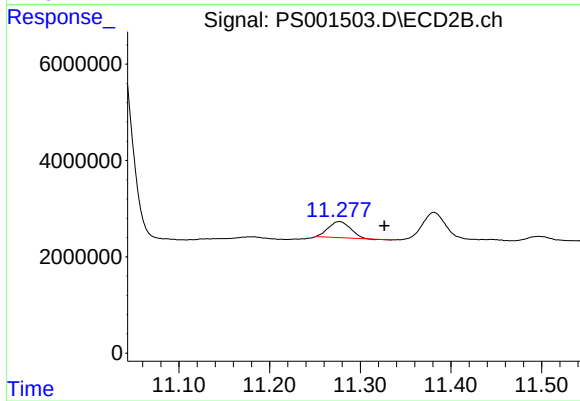

#5 DICAMBA


R.T.: 11.277 min
Delta R.T.: -0.049 min
Response: 5580924
Conc: 8.14 ng/ml

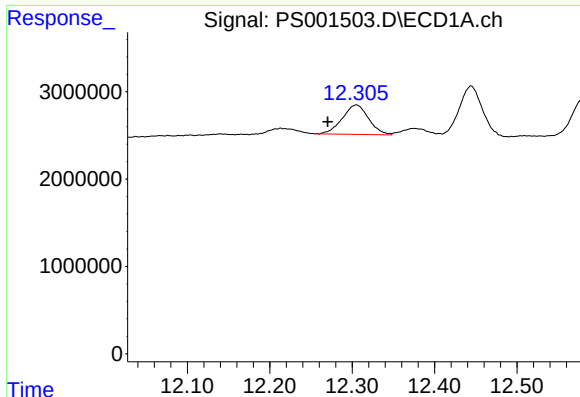

#6 MCPP


R.T.: 12.305 min
Delta R.T.: 0.035 min
Response: 7483558
Conc: 14.89 ug/ml

Instrument :
ECD_S
ClientSampleId :

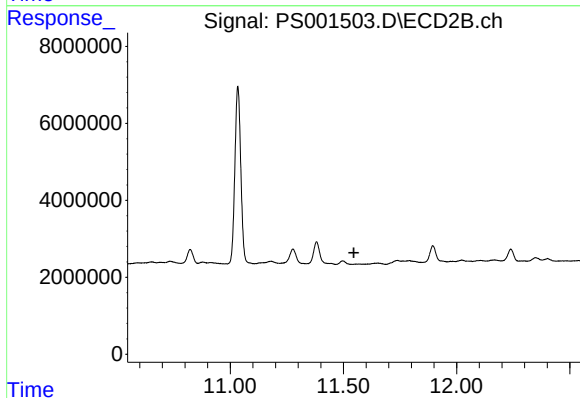


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.546 min
Response: 0
Conc: N.D.

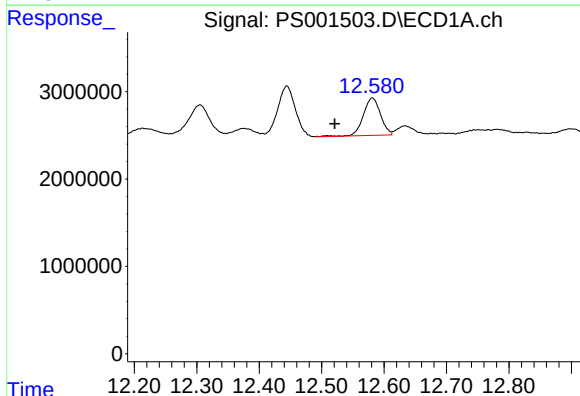


#7 MCPA

R.T.: 12.581 min
Delta R.T.: 0.060 min
Response: 8249573
Conc: 10.46 ug/ml

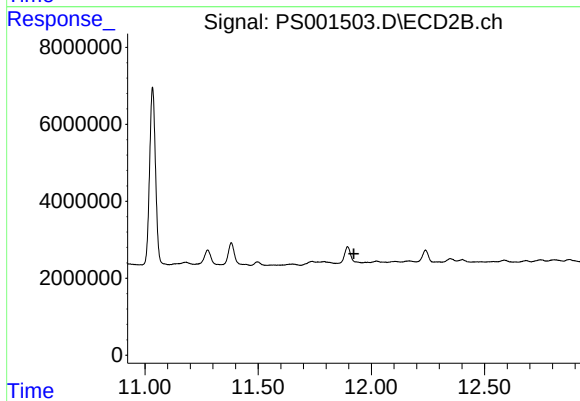

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 11.922 min
Response: 0
Conc: N.D.

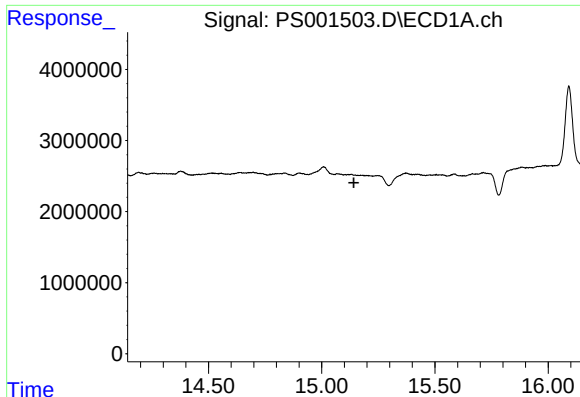

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T. : 15.142 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

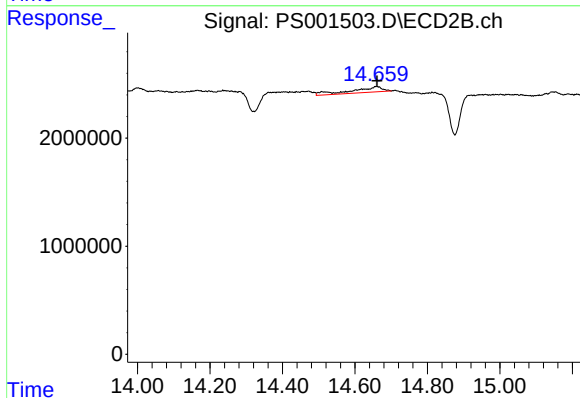


#12 2,4,5-T

R.T.: 14.659 min
Delta R.T.: -0.003 min
Response: 2973238
Conc: 3.22 ng/ml

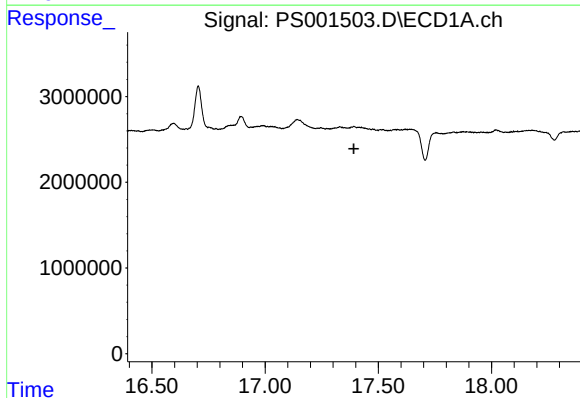


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 17.392 min
Response: 0
Conc: N.D.

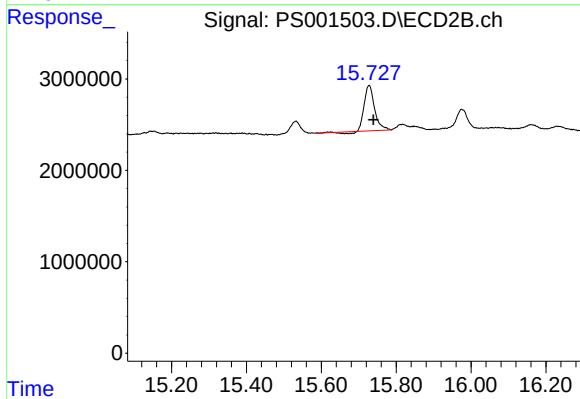

#14 DINOSEB


R.T.: 15.728 min
Delta R.T.: -0.012 min
Response: 9316147
Conc: 13.11 ng/ml

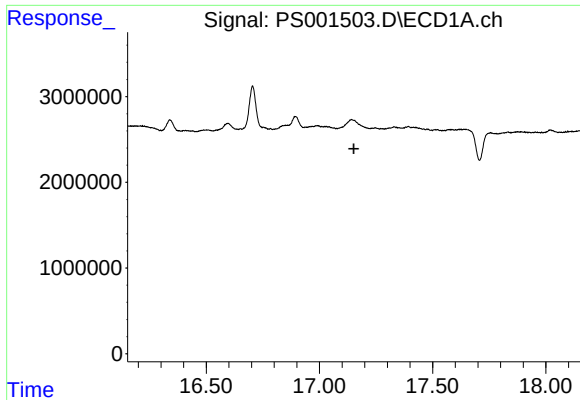

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 17.152 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

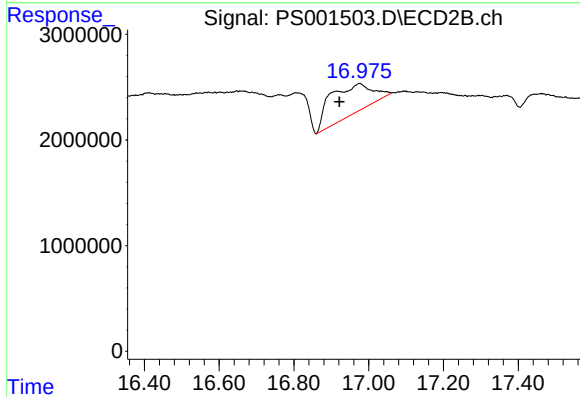


#15 Picloram

R.T.: 16.976 min
Delta R.T.: 0.054 min
Response: 22303206
Conc: 16.18 ng/ml

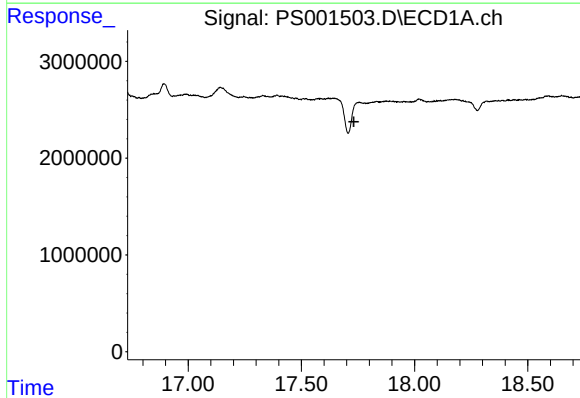

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.732 min
Response: 0
Conc: N.D.

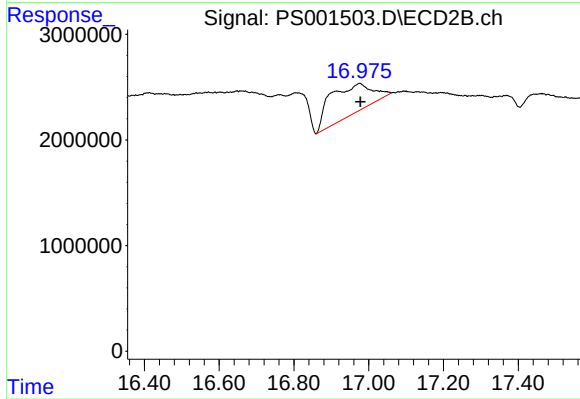

#16 DCPA

R.T.: 16.976 min
Delta R.T.: -0.002 min
Response: 22303206
Conc: 15.44 ng/ml