

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081518\
 Data File : PS001511.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2018 22:47
 Operator : UA
 Sample : J4471-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 04:36:33 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.632	11.053	86708774	81758664	467.307	449.533
Target Compounds							
1) T	Dalapon	2.981	2.422	3950855	4660440	16.661	20.452
2) T	3,5-DICHL...	10.058	9.141	4678149	1030636	17.333	4.046 #
5) T	DICAMBA	0.000	11.296	0	7049549	N.D.	10.286 #
6) T	MCP	12.324	0.000	7983311	0	15.884	N.D. #
11) T	2,4,5-TP ...	0.000	14.029	0	11364847	N.D.	10.394 #
12) T	2,4,5-T	0.000	14.678	0	2077332	N.D.	2.249 #
15) T	Picloram	17.167	16.990	6489367	11130156	4.106	8.074 #
16) T	DCPA	0.000	16.990	0	11130156	N.D.	7.706 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081518\
Data File : PS001511.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2018 22:47
Operator : UA
Sample : J4471-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 04:36:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

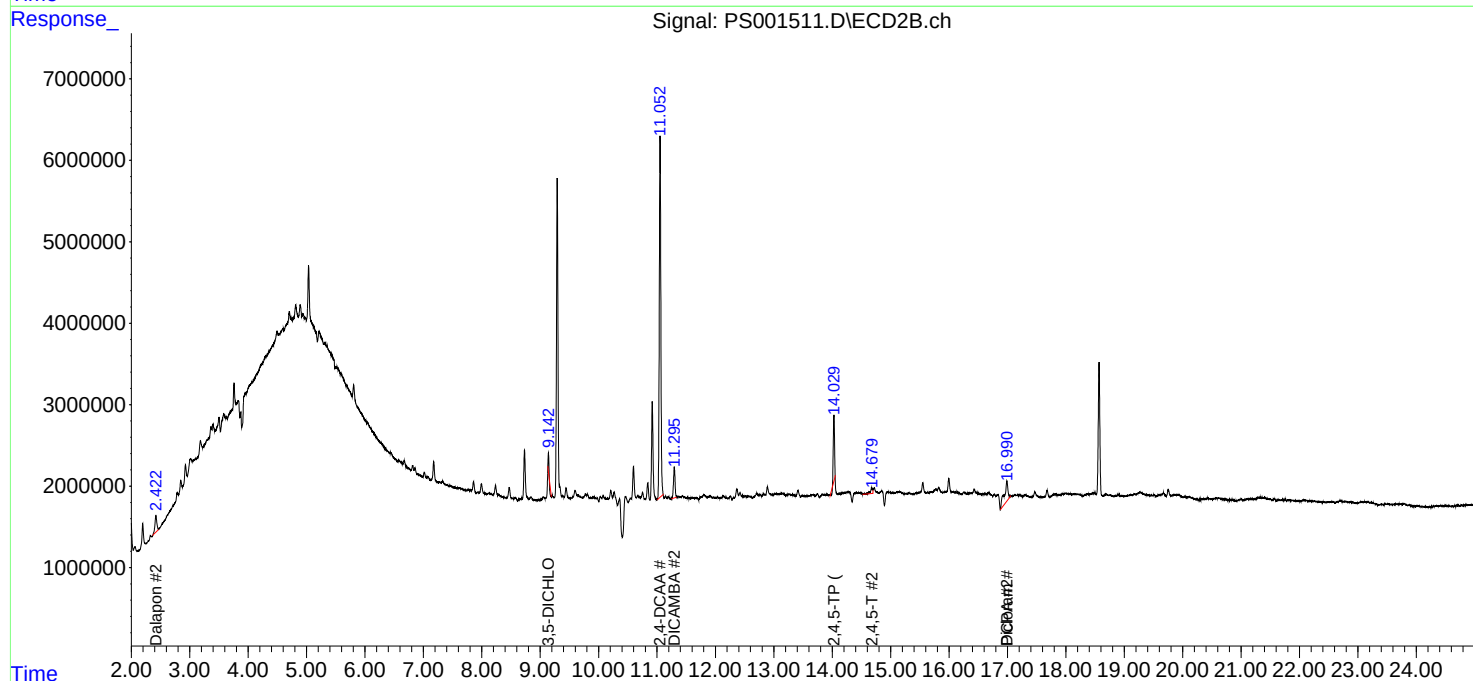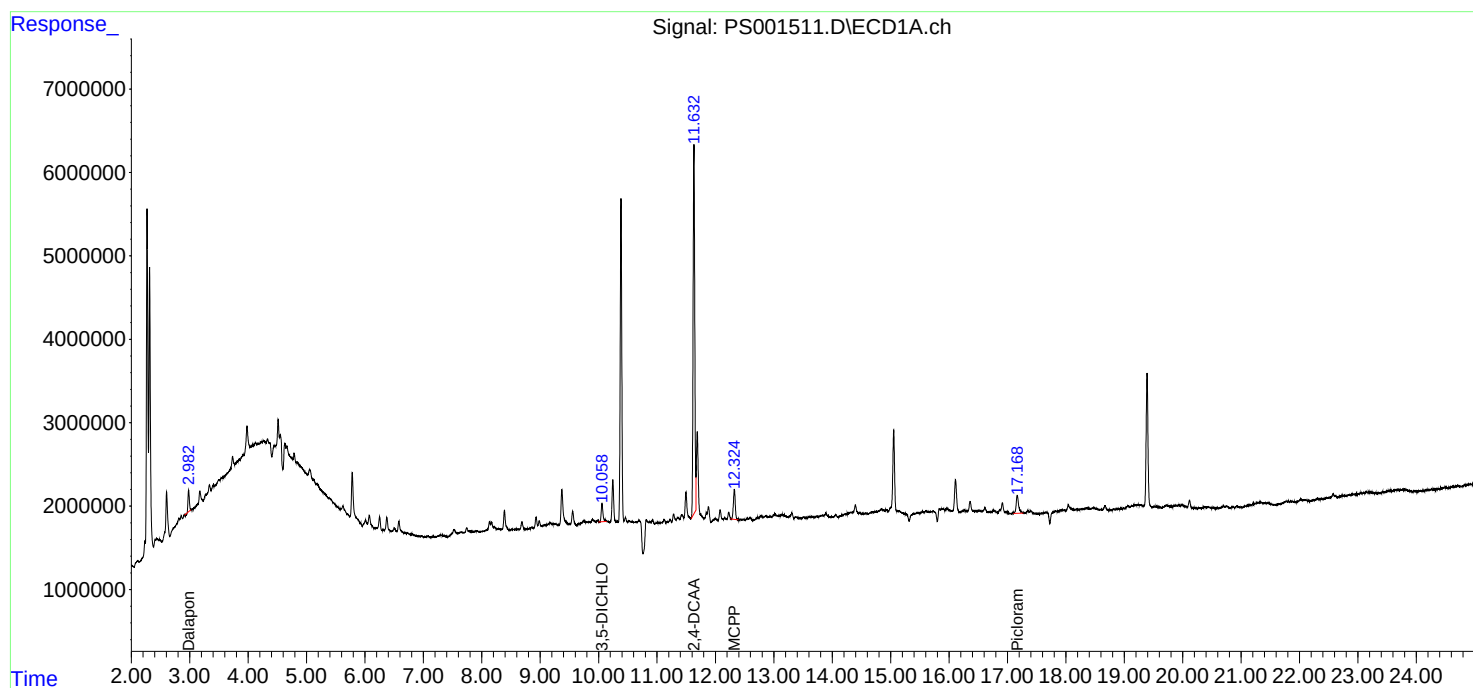


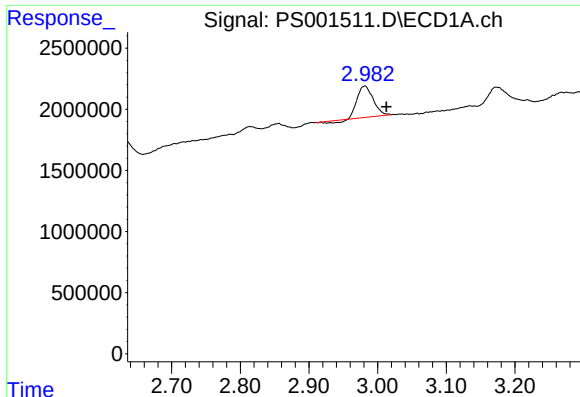

#1 Dalapon


R.T.: 2.981 min
Delta R.T.: -0.032 min
Response: 3950855
Conc: 16.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

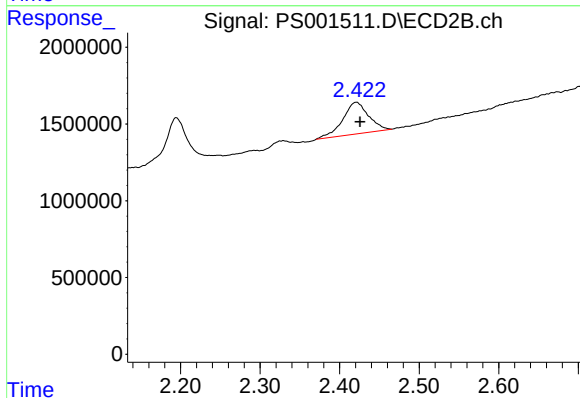


#1 Dalapon

R.T.: 2.422 min
Delta R.T.: -0.004 min
Response: 4660440
Conc: 20.45 ng/ml

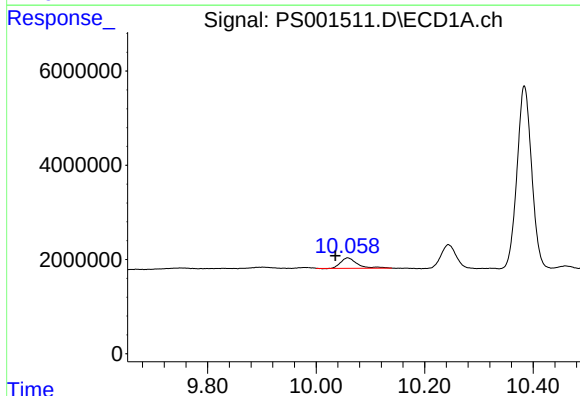


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 10.058 min
Delta R.T.: 0.023 min
Response: 4678149
Conc: 17.33 ng/ml

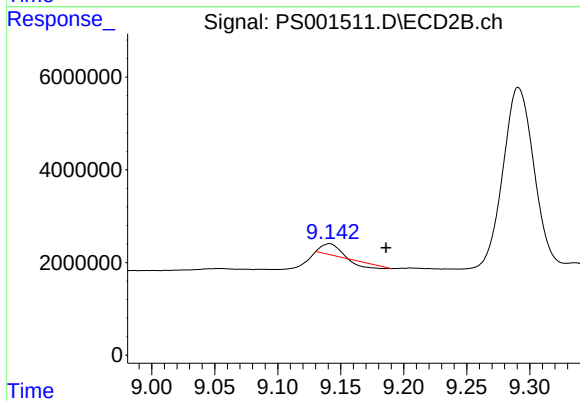

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 9.141 min
Delta R.T.: -0.045 min
Response: 1030636
Conc: 4.05 ng/ml

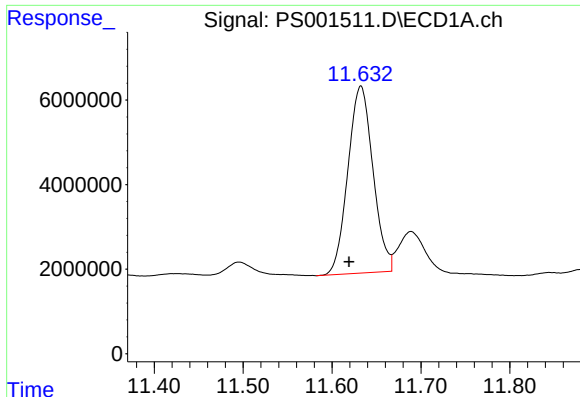

#4 2,4-DCAA


R.T.: 11.632 min
Delta R.T.: 0.013 min
Response: 86708774
Conc: 467.31 ng/ml

Instrument :
ECD_S
ClientSampleId :

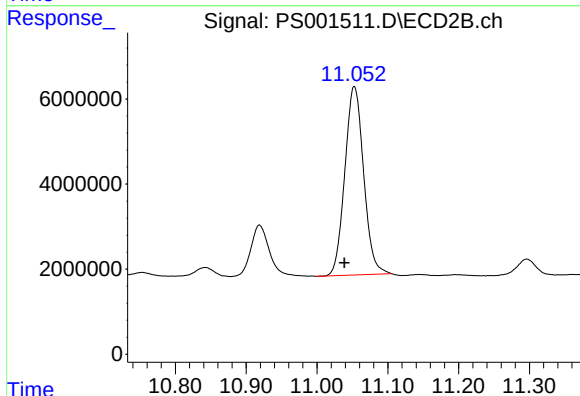


#4 2,4-DCAA

R.T.: 11.053 min
Delta R.T.: 0.014 min
Response: 81758664
Conc: 449.53 ng/ml

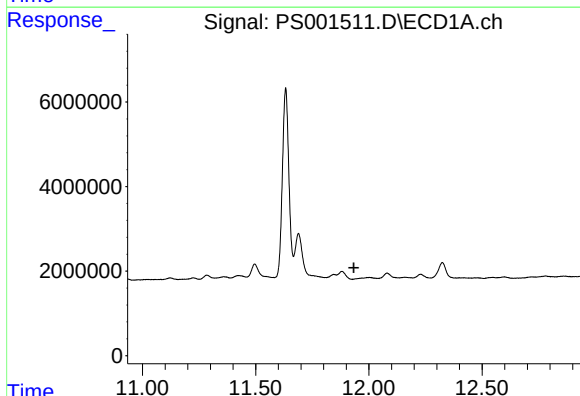


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.934 min
Response: 0
Conc: N.D.

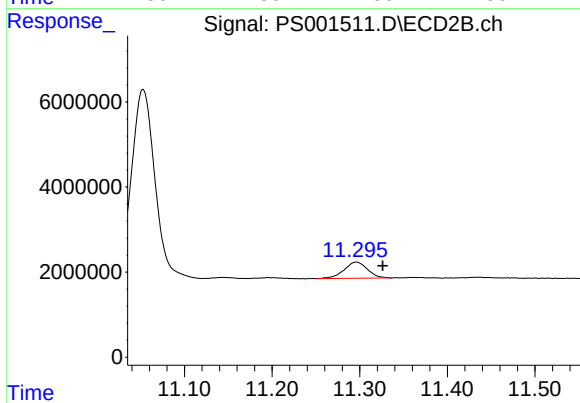

#5 DICAMBA


R.T.: 11.296 min
Delta R.T.: -0.030 min
Response: 7049549
Conc: 10.29 ng/ml

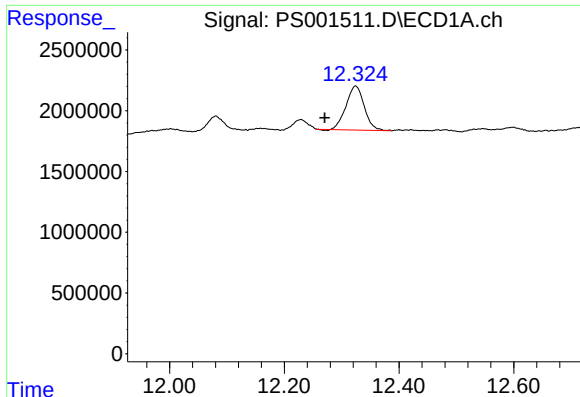

#6 MCP


R.T.: 12.324 min
Delta R.T.: 0.054 min
Response: 7983311
Conc: 15.88 ug/ml

Instrument :
ECD_S
ClientSampleId :

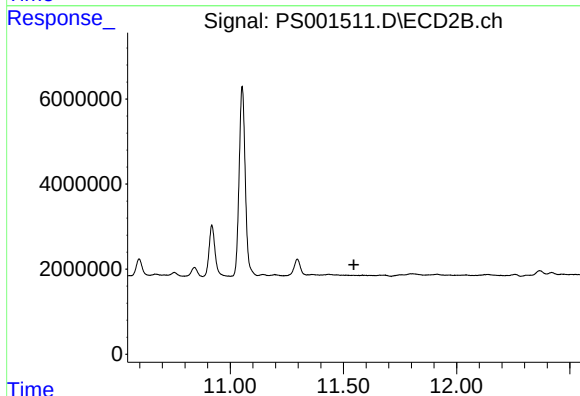


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.546 min
Response: 0
Conc: N.D.

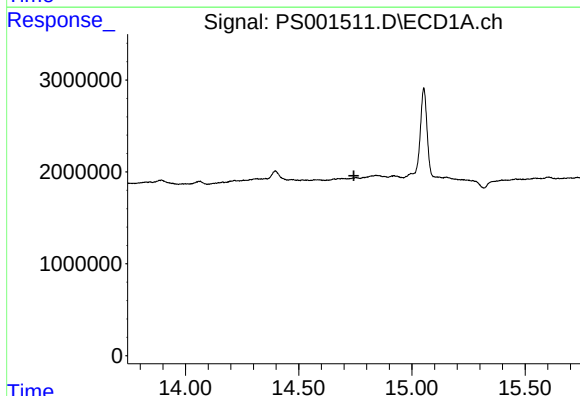


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.743 min
Response: 0
Conc: N.D.

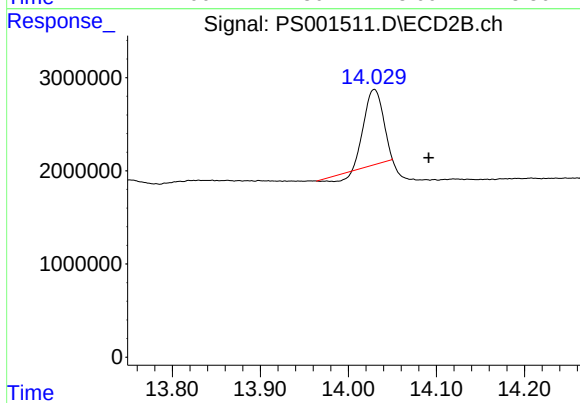

#11 2,4,5-TP (SILVEX)


R.T.: 14.029 min
Delta R.T.: -0.062 min
Response: 11364847
Conc: 10.39 ng/ml

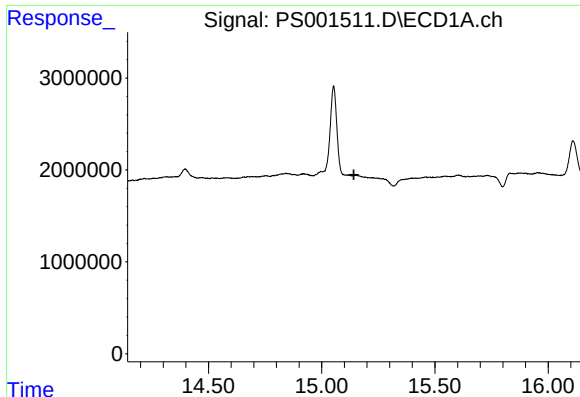

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.142 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

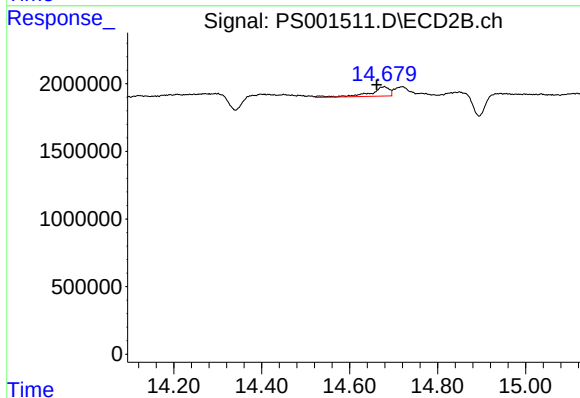


#12 2,4,5-T

R.T.: 14.678 min
Delta R.T.: 0.017 min
Response: 2077332
Conc: 2.25 ng/ml

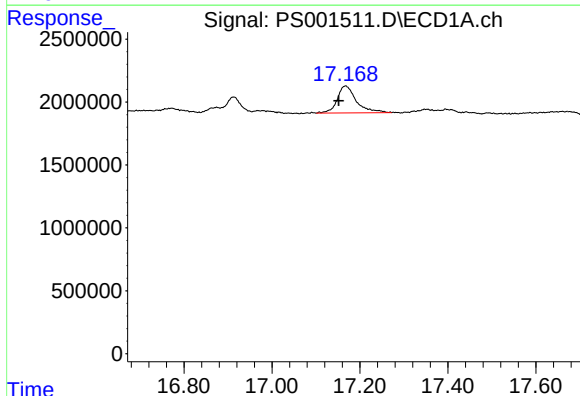


#15 Picloram

R.T.: 17.167 min
Delta R.T.: 0.015 min
Response: 6489367
Conc: 4.11 ng/ml

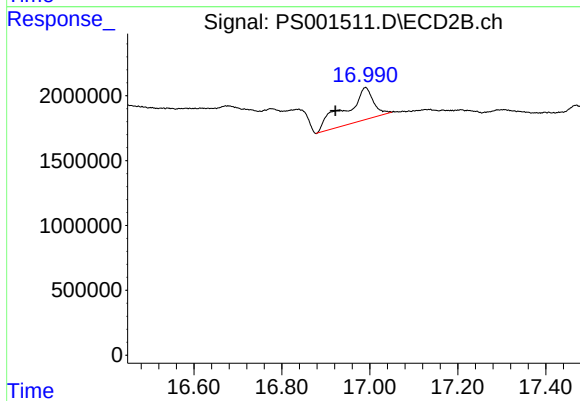

#15 Picloram


R.T.: 16.990 min
Delta R.T.: 0.068 min
Response: 11130156
Conc: 8.07 ng/ml

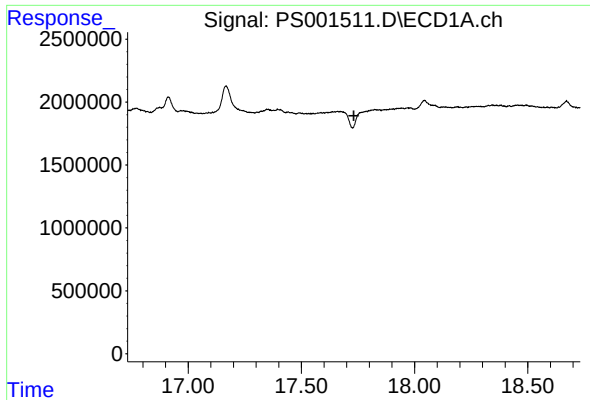

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.732 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

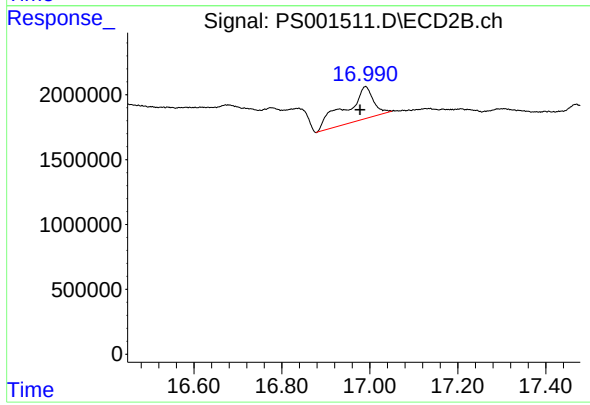

#16 DCPA

R.T.: 16.990 min
Delta R.T.: 0.012 min
Response: 11130156
Conc: 7.71 ng/ml