

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081518\
 Data File : PS001512.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2018 23:18
 Operator : UA
 Sample : J4471-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 04:36:53 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
 Quant Title : 8080.M
 QLast Update : Sat Jul 21 01:18:58 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.607	11.027	91617055	84689683	493.760	465.648
Target Compounds							
1) T	Dalapon	2.956	2.395	6427850	5373358	27.107	23.581
2) T	3,5-DICHL...	10.034	0.000	3402012	0	12.605	N.D. #
5) T	DICAMBA	0.000	11.271	0	3662117	N.D.	5.343 #
6) T	MCP	12.300	0.000	6165825	0	12.268	N.D. #
9) T	2,4-D	0.000	12.865	0	1750489	N.D.	7.377 #
15) T	Picloram	0.000	16.970	0	89455	N.D.	0.065 #
16) T	DCPA	0.000	16.970	0	89455	N.D.	0.062 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081518\
Data File : PS001512.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2018 23:18
Operator : UA
Sample : J4471-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 04:36:53 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS072118.M
Quant Title : 8080.M
QLast Update : Sat Jul 21 01:18:58 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

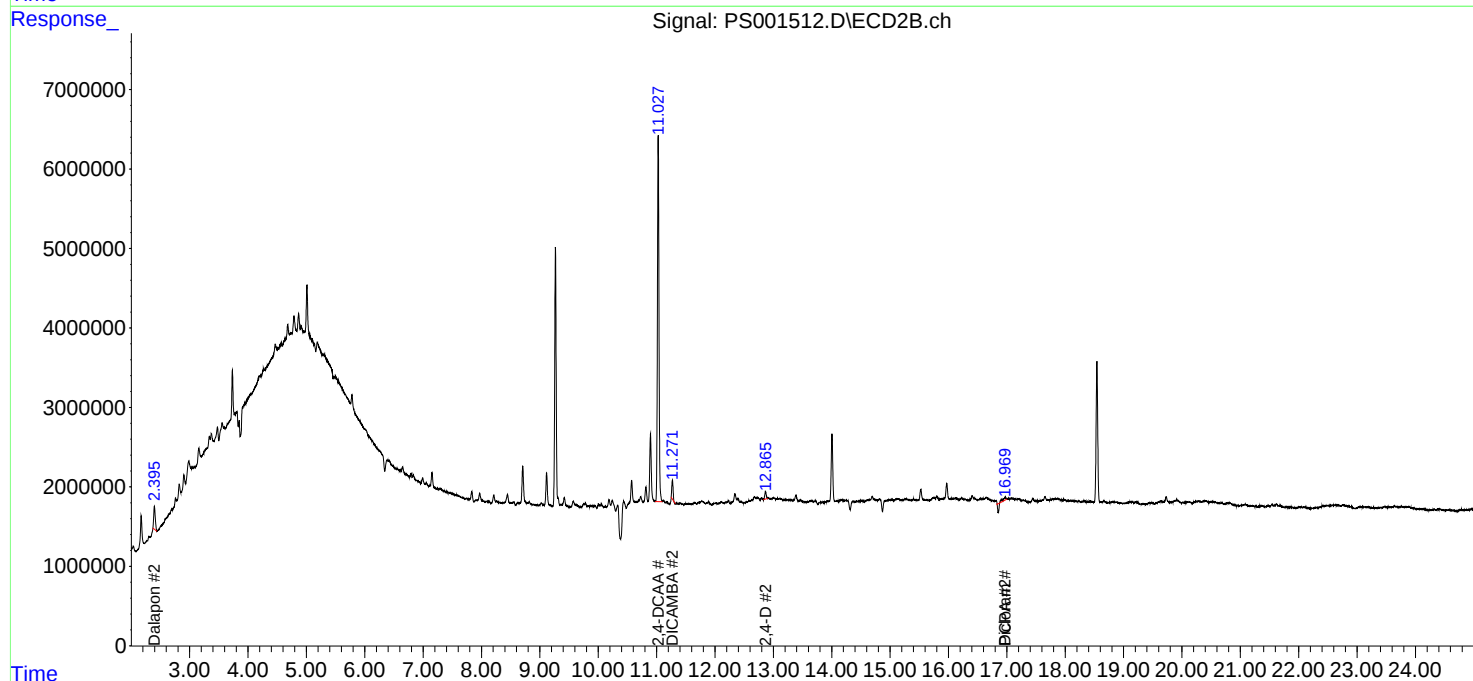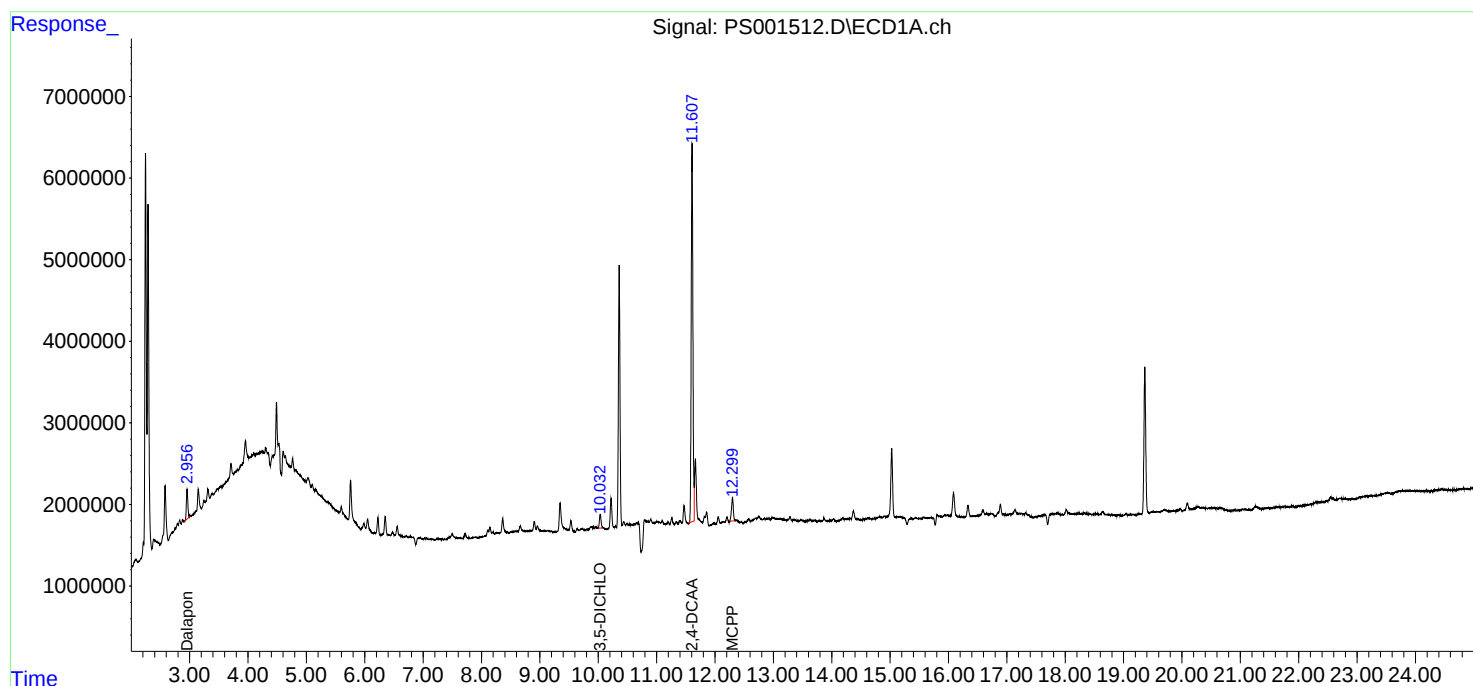


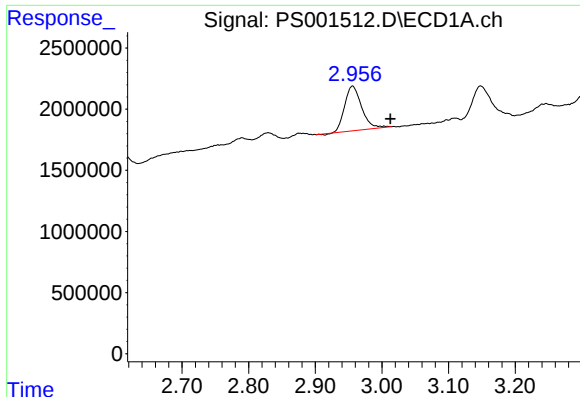

#1 Dalapon


R.T.: 2.956 min
Delta R.T.: -0.057 min
Response: 6427850
Conc: 27.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

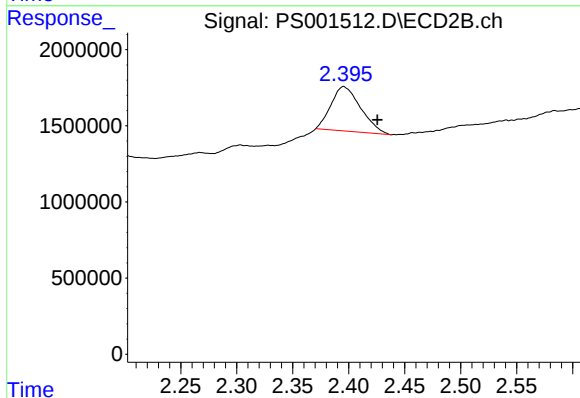


#1 Dalapon

R.T.: 2.395 min
Delta R.T.: -0.030 min
Response: 5373358
Conc: 23.58 ng/ml

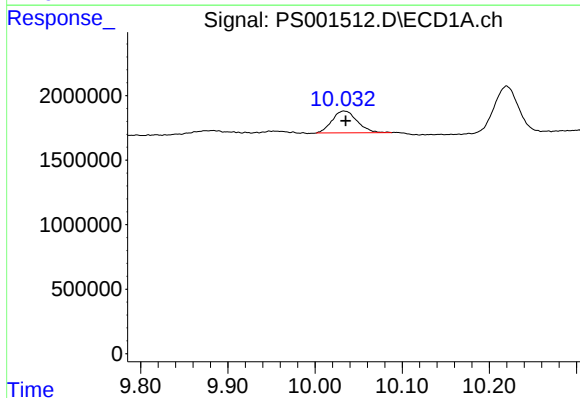


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 10.034 min
Delta R.T.: -0.002 min
Response: 3402012
Conc: 12.60 ng/ml

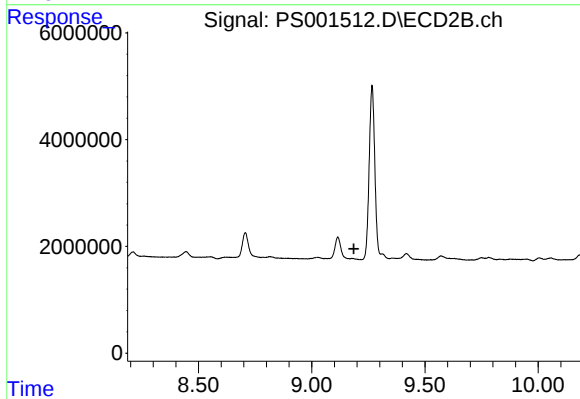

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T. : 9.186 min
Response: 0
Conc: N.D.

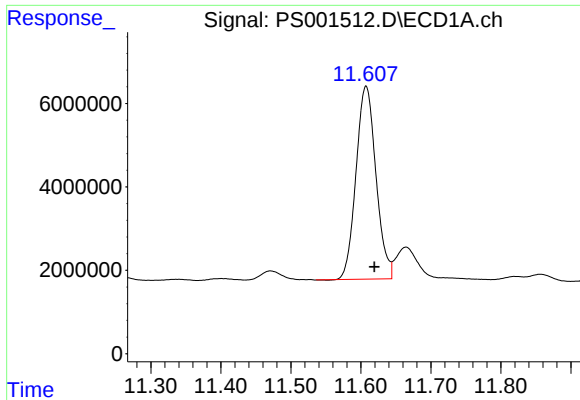

#4 2,4-DCAA


R.T.: 11.607 min
Delta R.T.: -0.012 min
Response: 91617055
Conc: 493.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

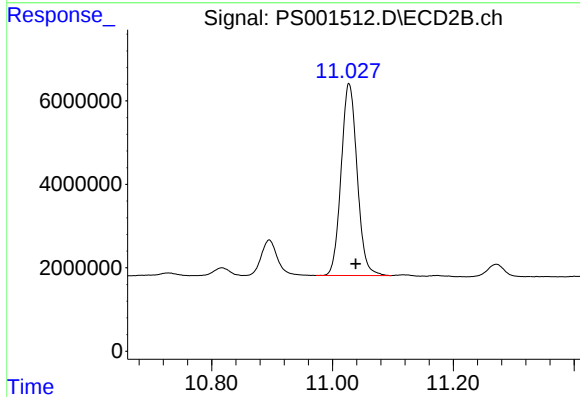


#4 2,4-DCAA

R.T.: 11.027 min
Delta R.T.: -0.011 min
Response: 84689683
Conc: 465.65 ng/ml

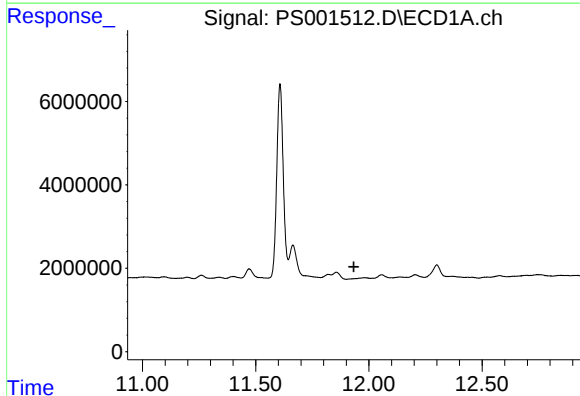


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.934 min
Response: 0
Conc: N.D.

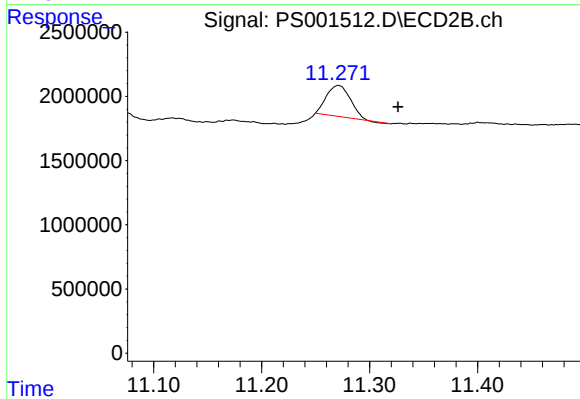

#5 DICAMBA


R.T.: 11.271 min
Delta R.T.: -0.055 min
Response: 3662117
Conc: 5.34 ng/ml

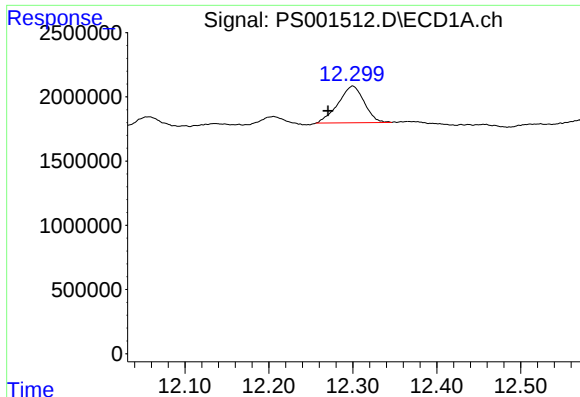

#6 MCP


R.T.: 12.300 min
Delta R.T.: 0.029 min
Response: 6165825
Conc: 12.27 ug/ml

Instrument :
ECD_S
ClientSampleId :

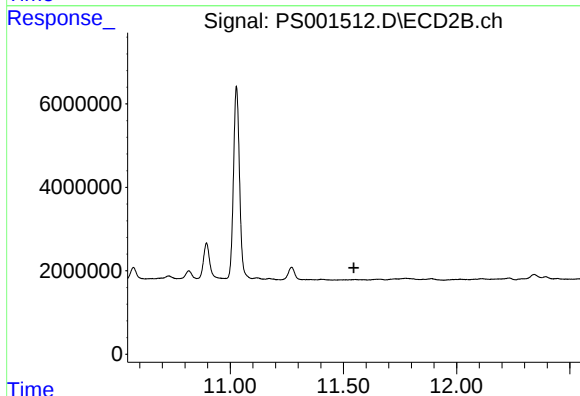


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.546 min
Response: 0
Conc: N.D.

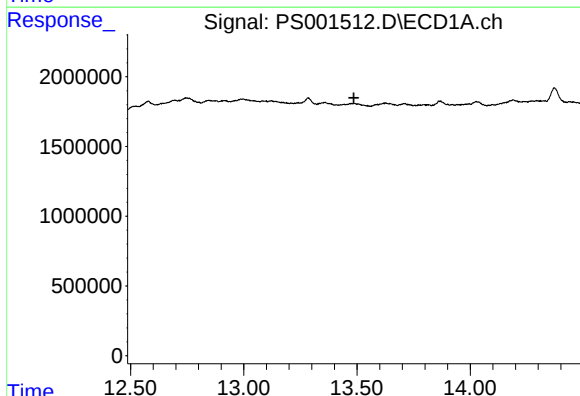


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.486 min
Response: 0
Conc: N.D.

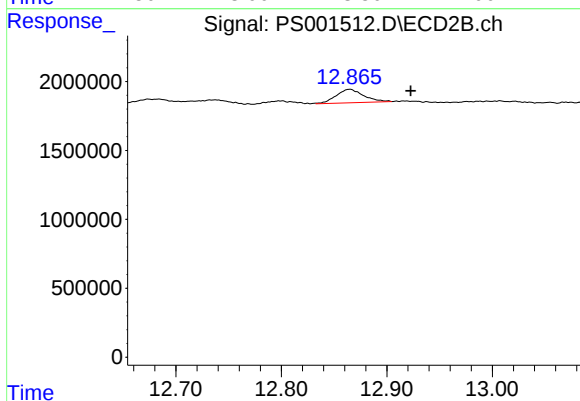

#9 2,4-D


R.T.: 12.865 min
Delta R.T.: -0.058 min
Response: 1750489
Conc: 7.38 ng/ml

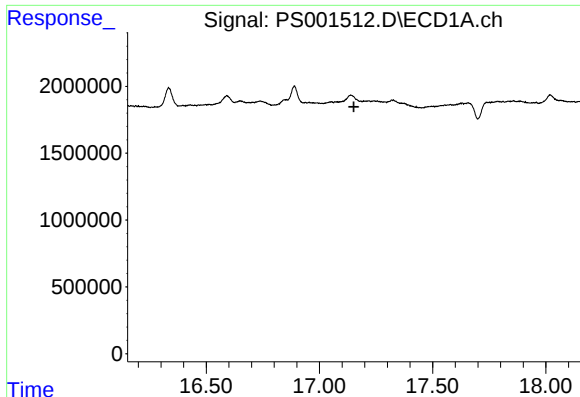

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 17.152 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

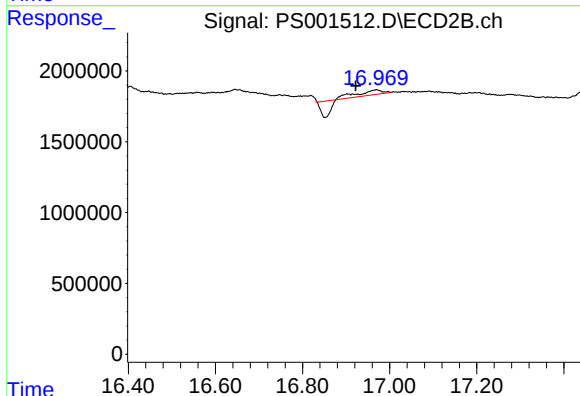


#15 Picloram

R.T.: 16.970 min
Delta R.T.: 0.048 min
Response: 89455
Conc: 0.06 ng/ml

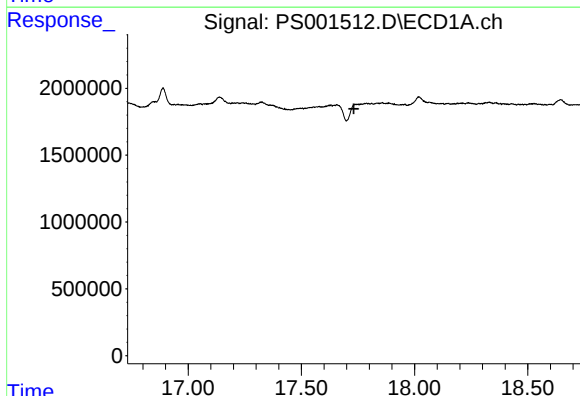

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.732 min
Response: 0
Conc: N.D.

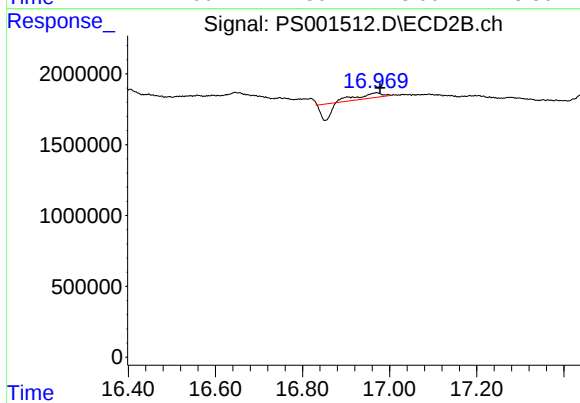

#16 DCPA

R.T.: 16.970 min
Delta R.T.: -0.008 min
Response: 89455
Conc: 0.06 ng/ml