

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081519\
 Data File : PS006103.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2019 09:30
 Operator : SM\AJ
 Sample : PB121288BL
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 15 13:43:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.480	5.225	296.5E6	180.5E6	343.433	367.007
Target Compounds							
9) T	2,4-D	6.540	0.000	192.6E6	0	236.371	N.D. #
10) T	Pentachlo...	6.744	0.000	19950313	0	1.688	N.D. #
12) T	2,4,5-T	0.000	7.320	0	36550668	N.D.	14.702
14) T	DINOSEB	9.163	0.000	31078302	0	8.490	N.D. #
15) T	Picloram	9.057	9.011	106.0E6	87433951	14.247	19.383 #
16) T	DCPA	0.000	9.011	0	87433951	N.D.	25.073



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081519\
Data File : PS006103.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2019 09:30
Operator : SM\AJ
Sample : PB121288BL
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 15 13:43:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

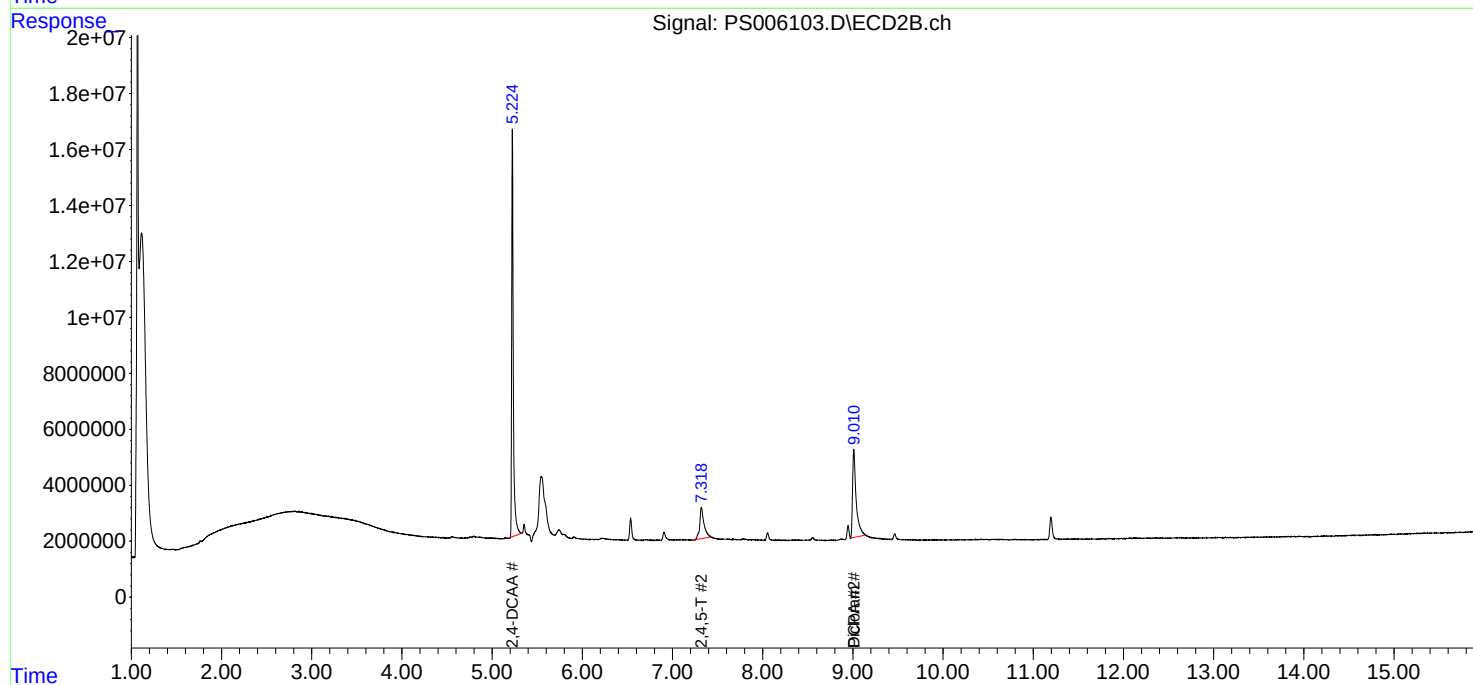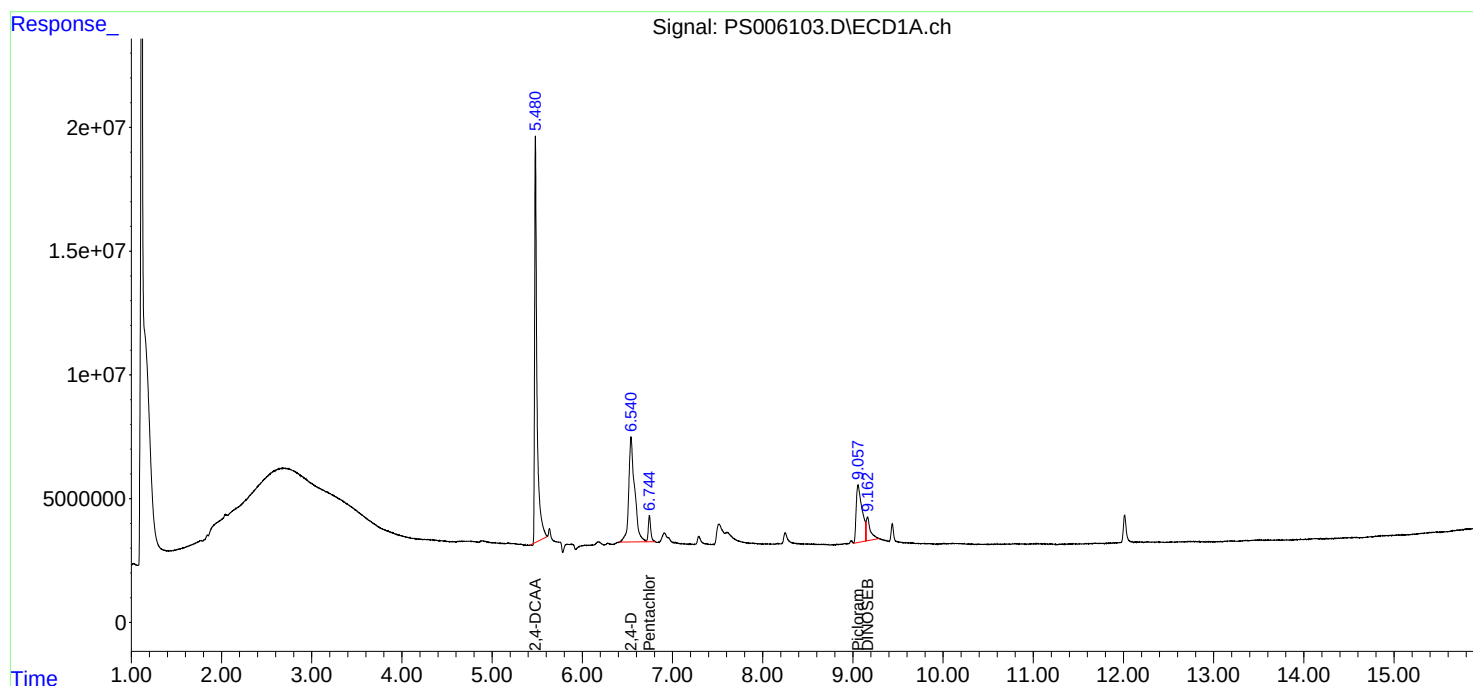


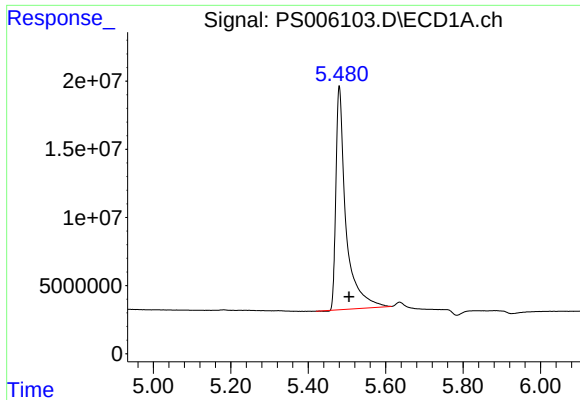

#4 2,4-DCAA


R.T.: 5.480 min
Delta R.T.: -0.025 min
Response: 296451275
Conc: 343.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

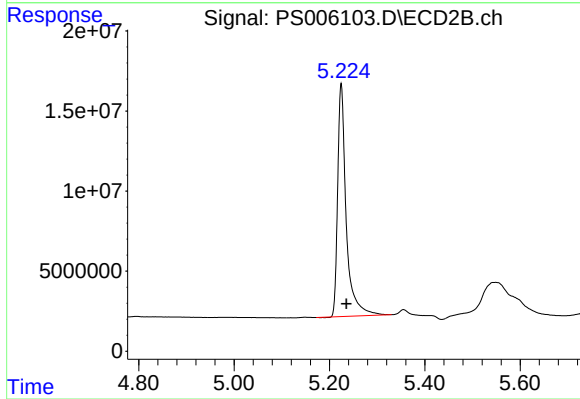


#4 2,4-DCAA

R.T.: 5.225 min
Delta R.T.: -0.011 min
Response: 180513302
Conc: 367.01 ng/ml

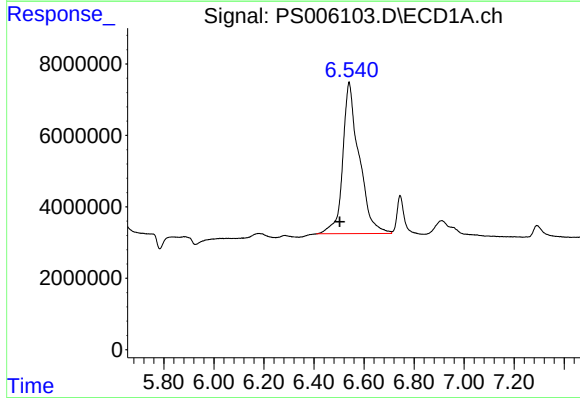


#9 2,4-D

R.T.: 6.540 min
Delta R.T.: 0.038 min
Response: 192591066
Conc: 236.37 ng/ml

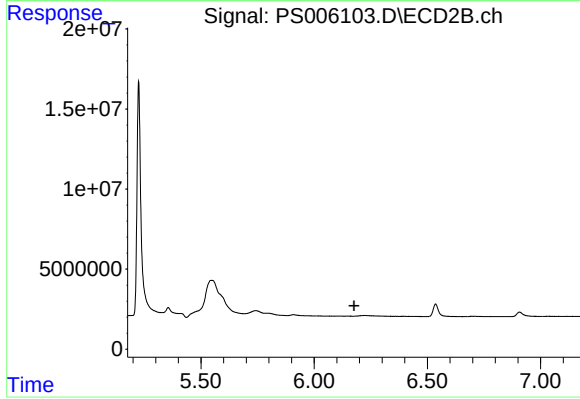

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.176 min
Response: 0
Conc: N.D.

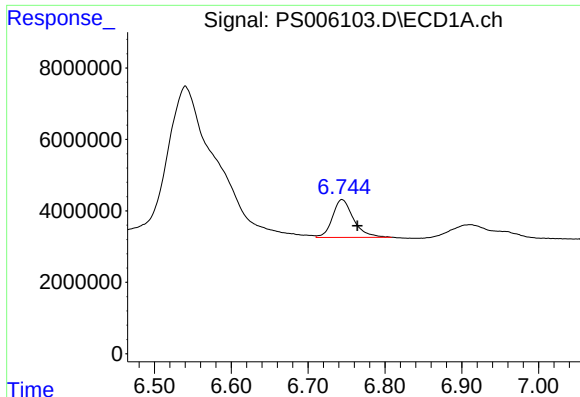

#10 Pentachlorophenol


R.T.: 6.744 min
Delta R.T.: -0.020 min
Response: 19950313
Conc: 1.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

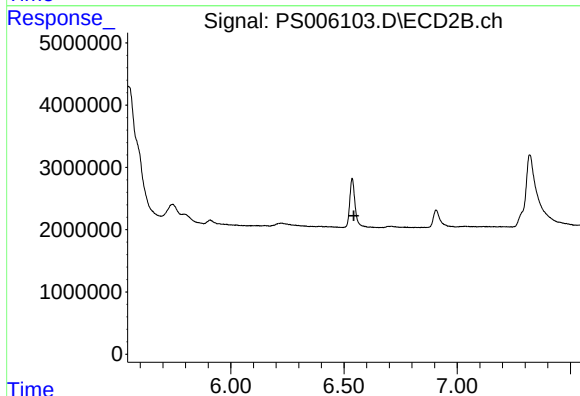


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 6.544 min
Response: 0
Conc: N.D.

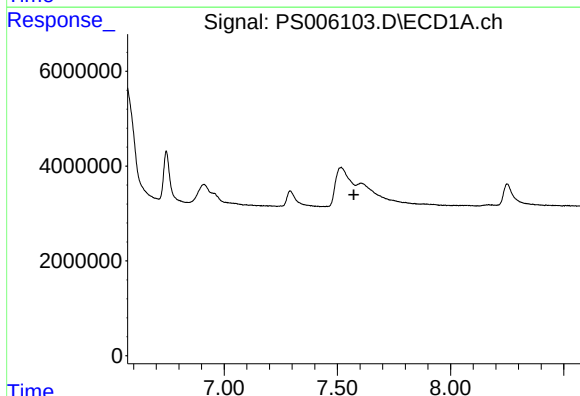


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 7.573 min
Response: 0
Conc: N.D.

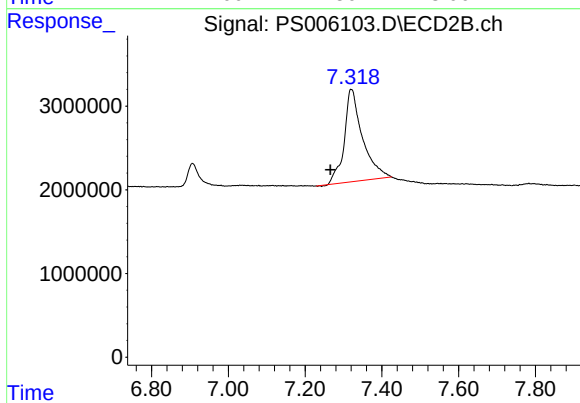

#12 2,4,5-T


R.T.: 7.320 min
Delta R.T.: 0.054 min
Response: 36550668
Conc: 14.70 ng/ml

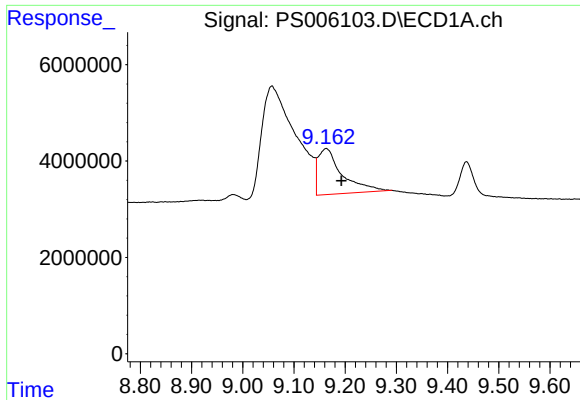

#14 DINOSEB


R.T.: 9.163 min
Delta R.T.: -0.029 min
Response: 31078302
Conc: 8.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

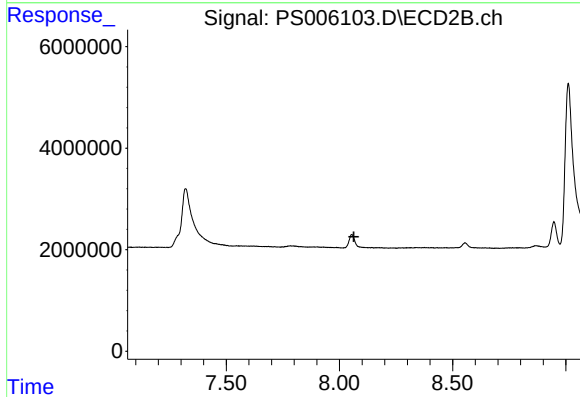


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 8.064 min
Response: 0
Conc: N.D.

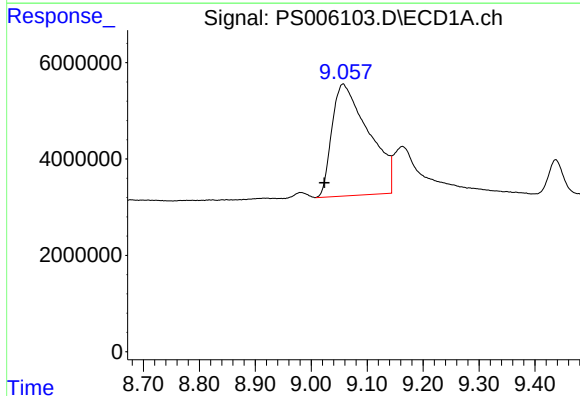


#15 Picloram

R.T.: 9.057 min
Delta R.T.: 0.033 min
Response: 106003599
Conc: 14.25 ng/ml

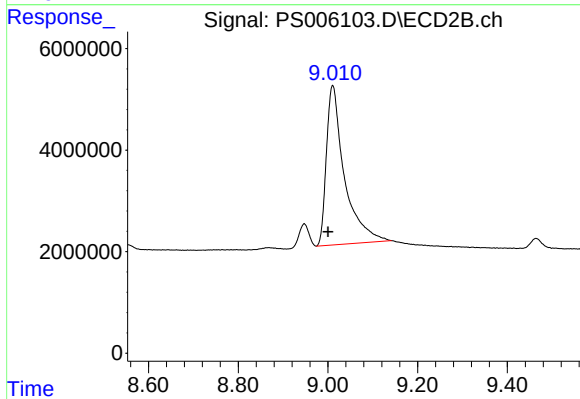

#15 Picloram


R.T.: 9.011 min
Delta R.T.: 0.011 min
Response: 87433951
Conc: 19.38 ng/ml

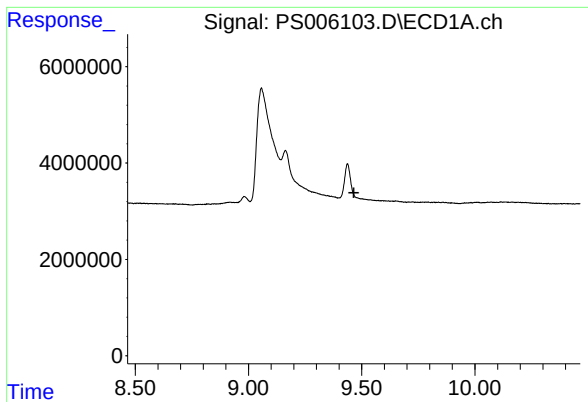

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

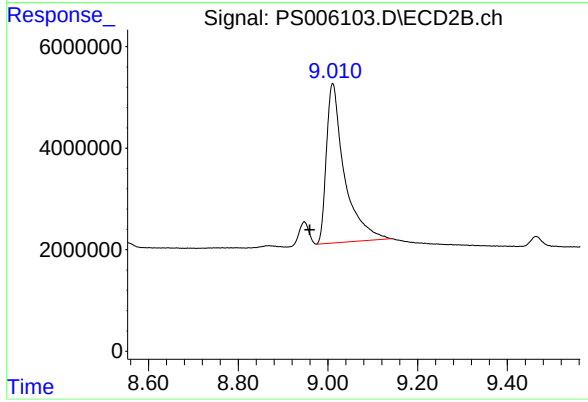

#16 DCPA

R.T.: 9.011 min
Delta R.T.: 0.051 min
Response: 87433951
Conc: 25.07 ng/ml