

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081519\
 Data File : PS006113.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2019 13:14
 Operator : SM\AJ
 Sample : K4322-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 03:50:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.504	5.234	408.1E6	256.5E6	472.743	521.432
Target Compounds							
1) T	Dalapon	2.045	1.759	76397572	69758111	70.114	111.170 #
2) T	3,5-DICHL...	0.000	4.563	0	49588410	N.D.	81.869
9) T	2,4-D	6.568	0.000	202.3E6	0	248.253	N.D. #
15) T	Picloram	9.064	9.016	89739530	51182972	12.061	11.347
16) T	DCPA	0.000	9.016	0	51182972	N.D.	14.678



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081519\
Data File : PS006113.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2019 13:14
Operator : SM\AJ
Sample : K4322-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 03:50:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

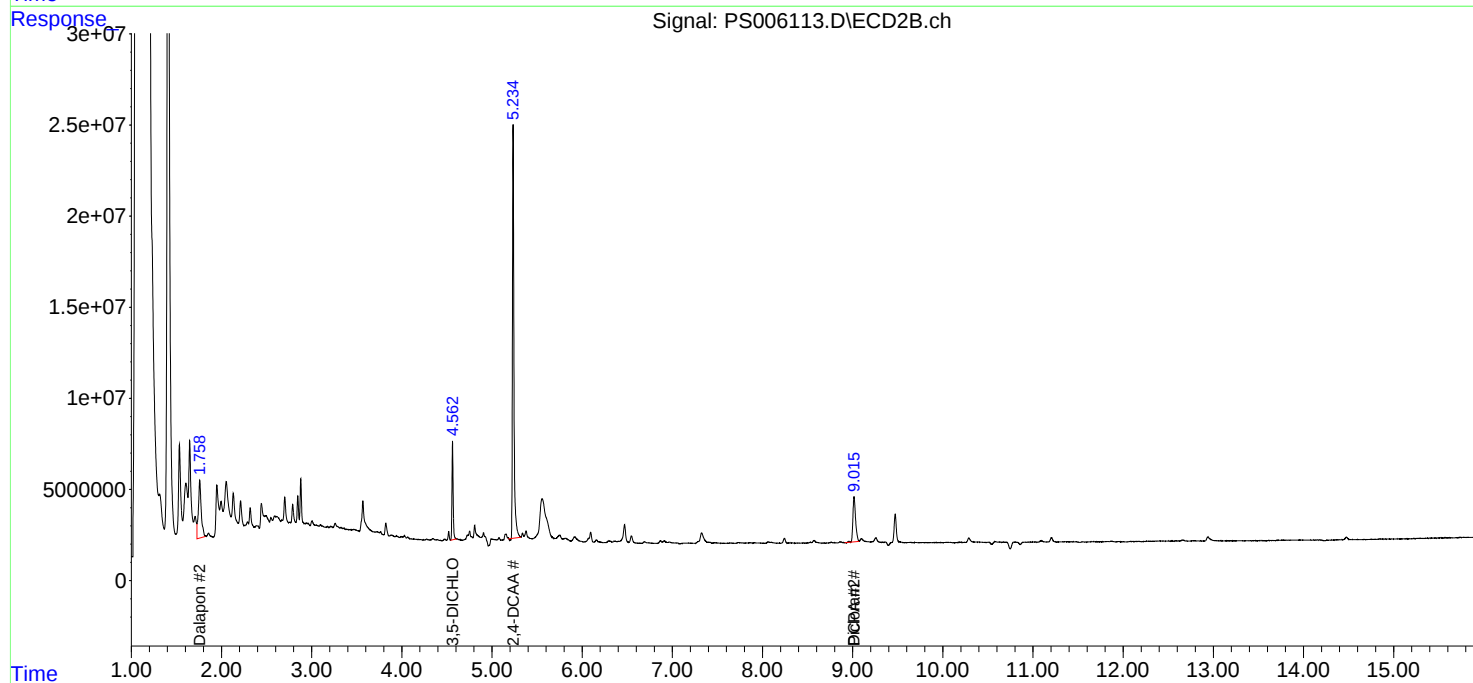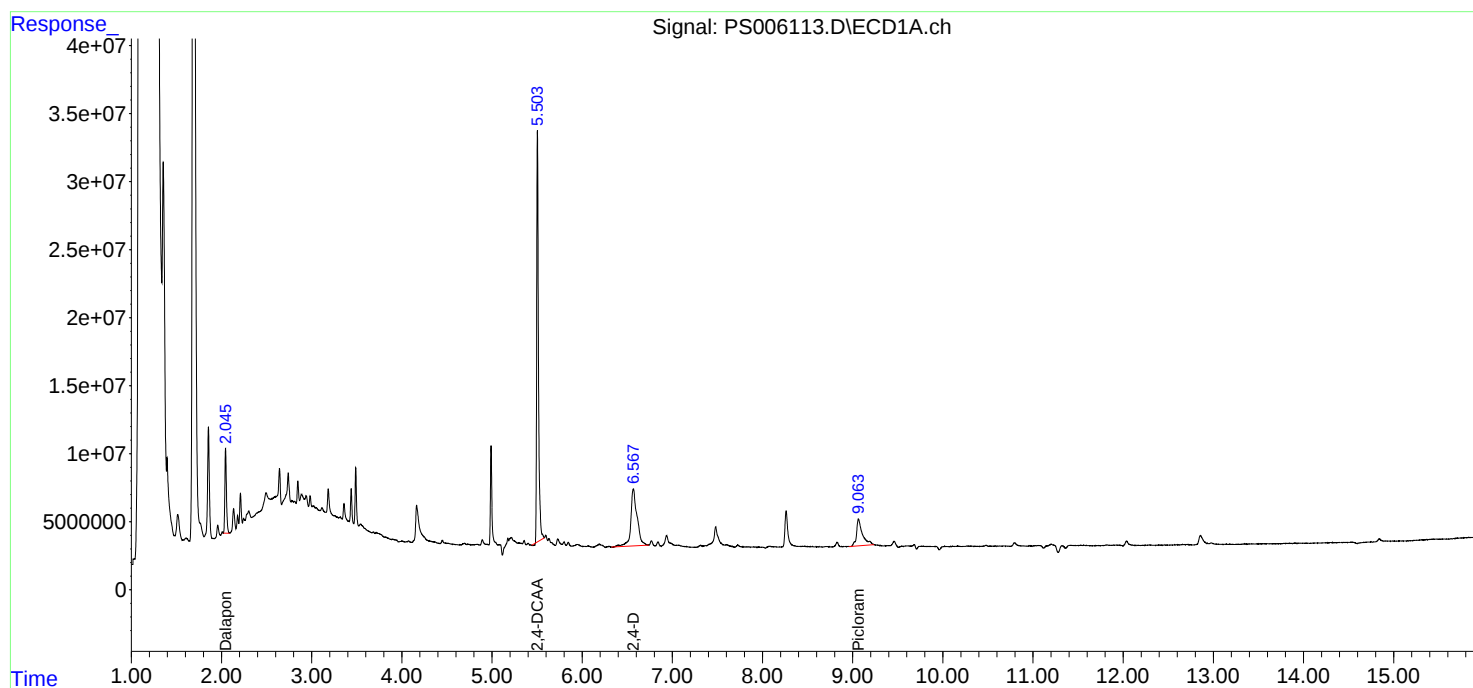


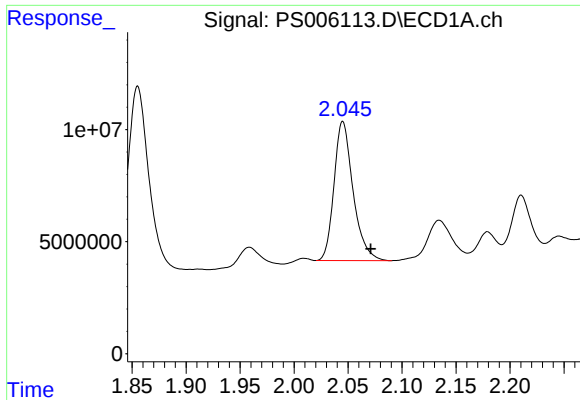

#1 Dalapon


R.T.: 2.045 min
Delta R.T.: -0.026 min
Response: 76397572
Conc: 70.11 ng/ml

Instrument :
ECD_S
ClientSampleId :

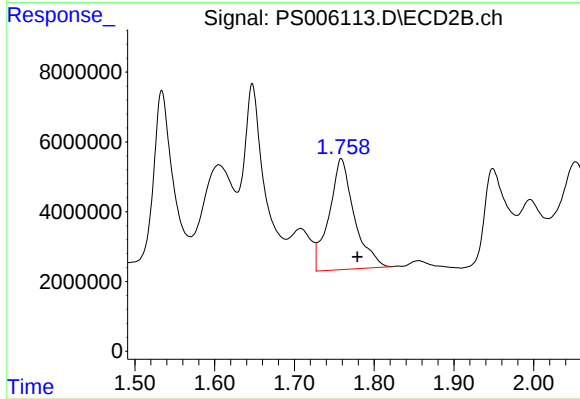


#1 Dalapon

R.T.: 1.759 min
Delta R.T.: -0.020 min
Response: 69758111
Conc: 111.17 ng/ml

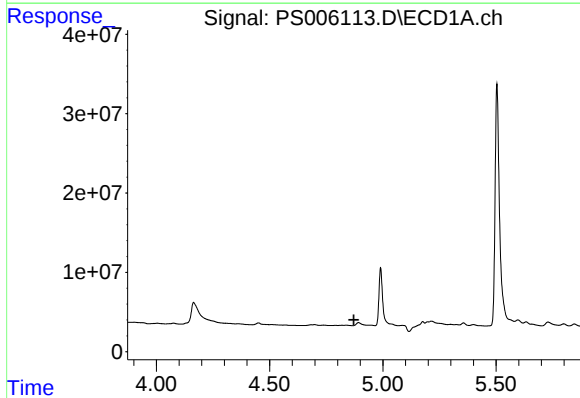


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.872 min
Response: 0
Conc: N.D.

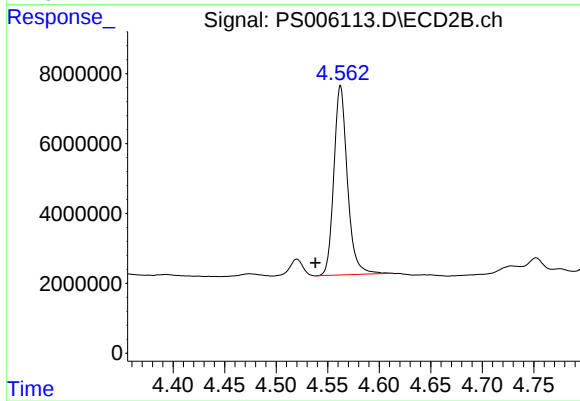

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.563 min
Delta R.T.: 0.025 min
Response: 49588410
Conc: 81.87 ng/ml

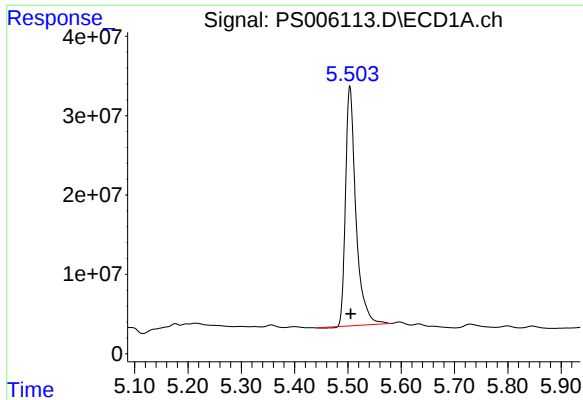

#4 2,4-DCAA


R.T.: 5.504 min
Delta R.T.: -0.001 min
Response: 408071974
Conc: 472.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

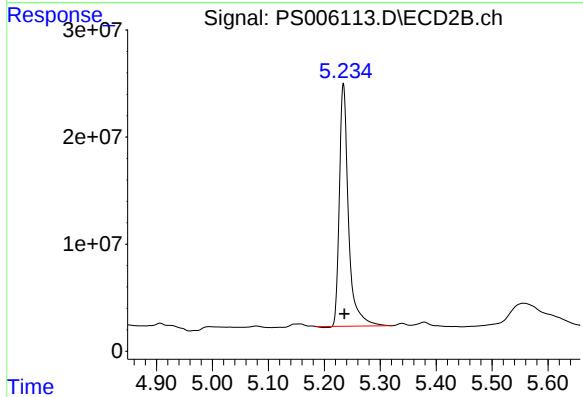


#4 2,4-DCAA

R.T.: 5.234 min
Delta R.T.: -0.001 min
Response: 256467438
Conc: 521.43 ng/ml

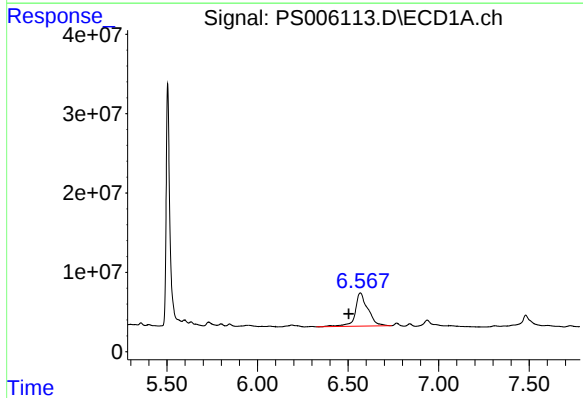


#9 2,4-D

R.T.: 6.568 min
Delta R.T.: 0.065 min
Response: 202272434
Conc: 248.25 ng/ml

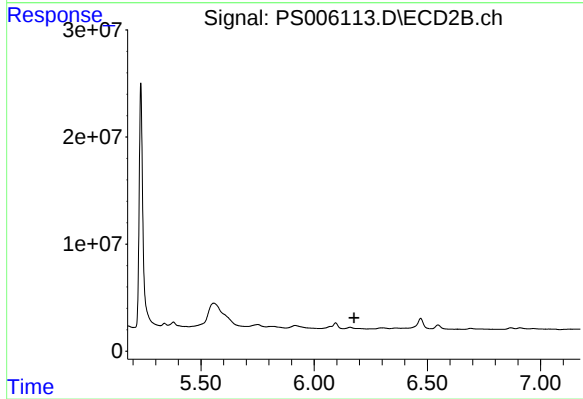

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.176 min
Response: 0
Conc: N.D.

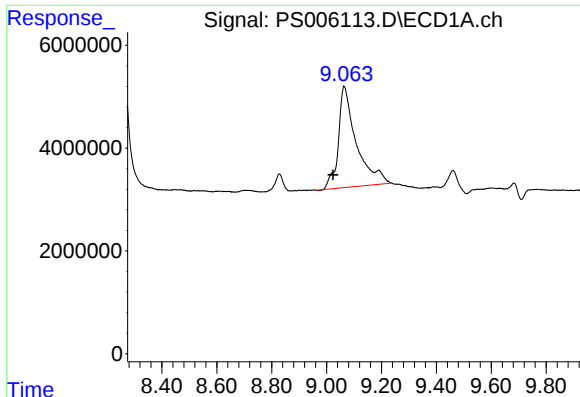

#15 Picloram


R.T.: 9.064 min
Delta R.T.: 0.041 min
Response: 89739530
Conc: 12.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

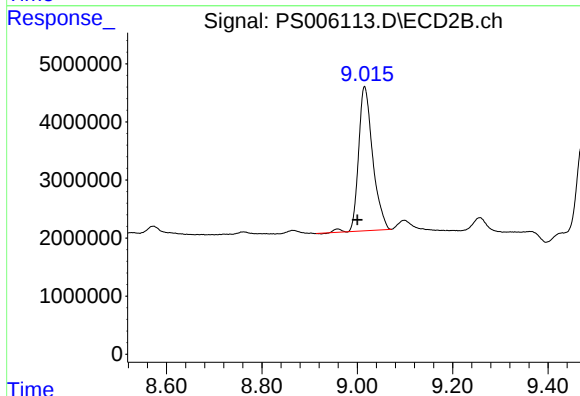


#15 Picloram

R.T.: 9.016 min
Delta R.T.: 0.015 min
Response: 51182972
Conc: 11.35 ng/ml

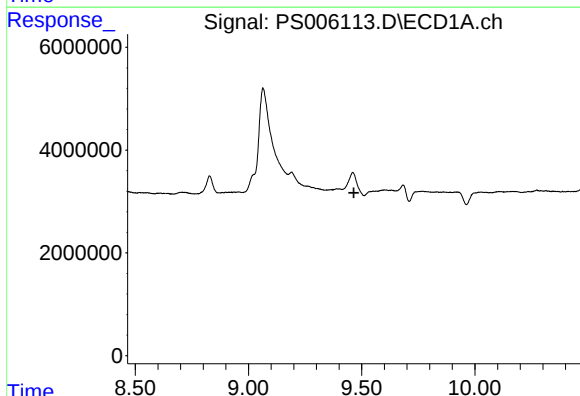

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.465 min
Response: 0
Conc: N.D.

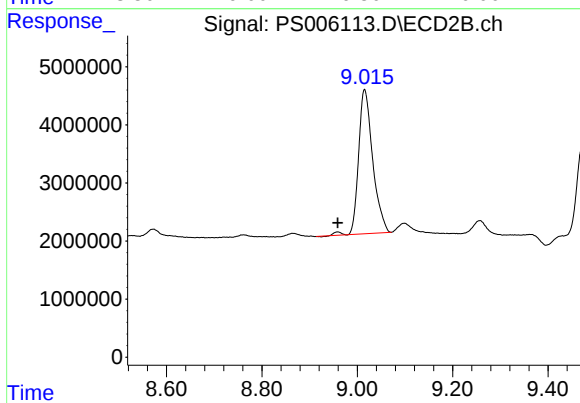

#16 DCPA

R.T.: 9.016 min
Delta R.T.: 0.056 min
Response: 51182972
Conc: 14.68 ng/ml