

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081519\
 Data File : PS006131.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2019 19:56
 Operator : SM\AJ
 Sample : IDOC WATER BL
 Misc : FOR DHAVAL DAVE
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 03:58:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.508	5.235	312.9E6	181.8E6	362.520	369.698
Target Compounds							
9) T	2,4-D	6.567	0.000	220.4E6	0	270.470	N.D. #
12) T	2,4,5-T	7.547	7.333	44268998	46146765	8.953	18.562 #
15) T	Picloram	9.078	9.017	328.7E6	210.6E6	44.174	46.684
16) T	DCPA	0.000	9.017	0	210.6E6	N.D.	60.389



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081519\
Data File : PS006131.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2019 19:56
Operator : SM\AJ
Sample : IDOC WATER BL
Misc : FOR DHAVAL DAVE
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 03:58:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

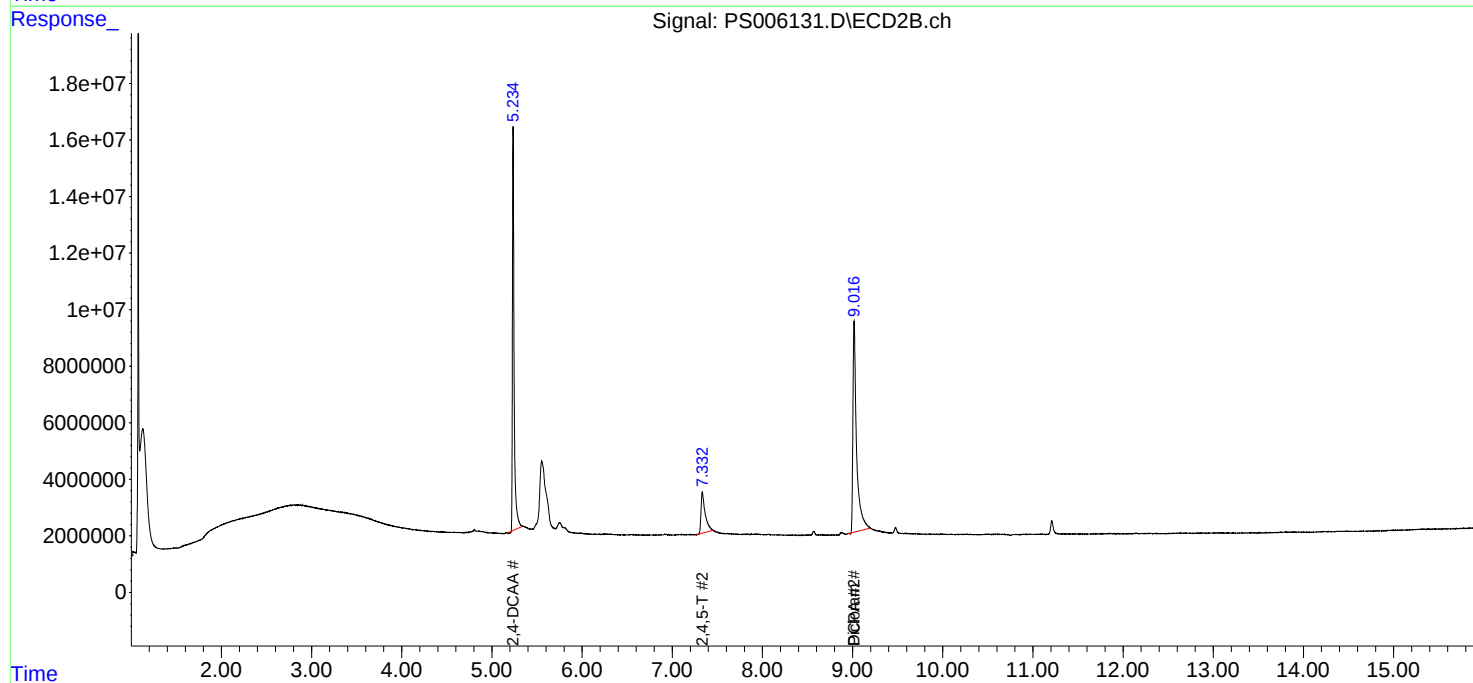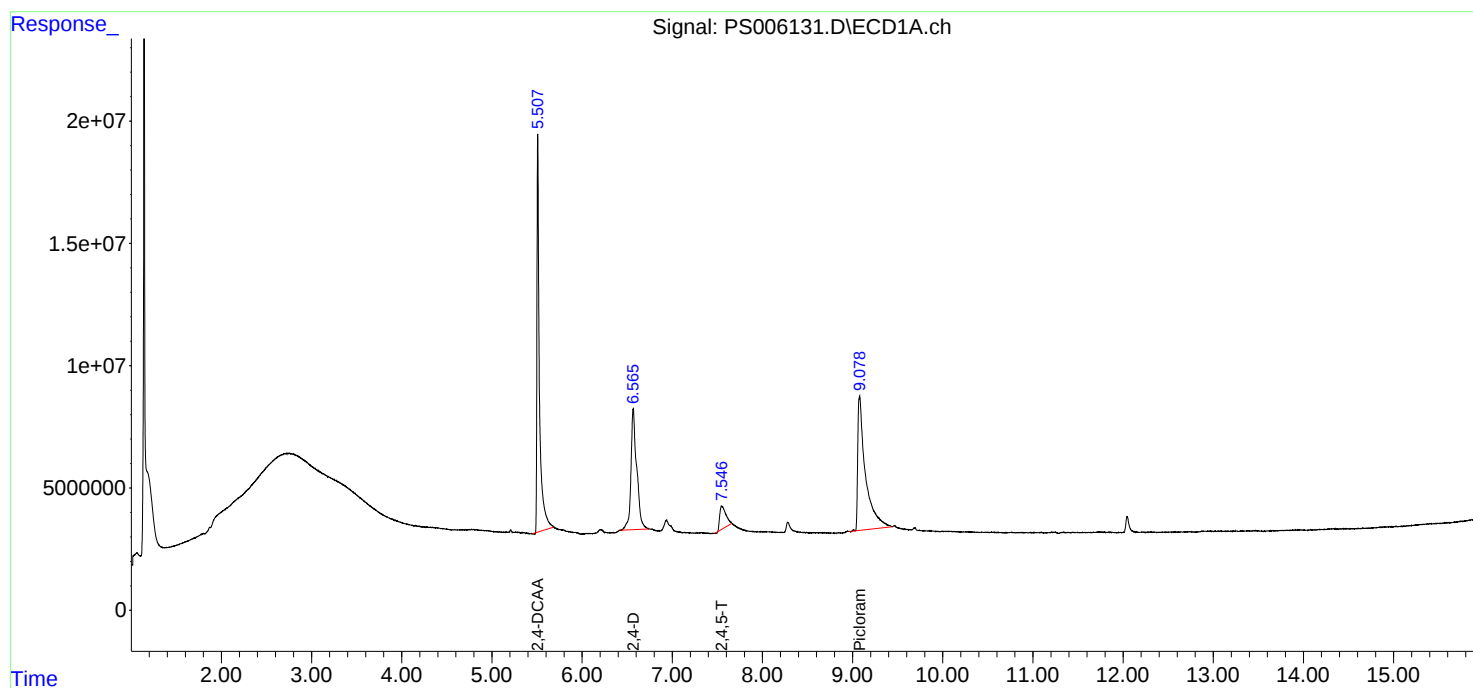


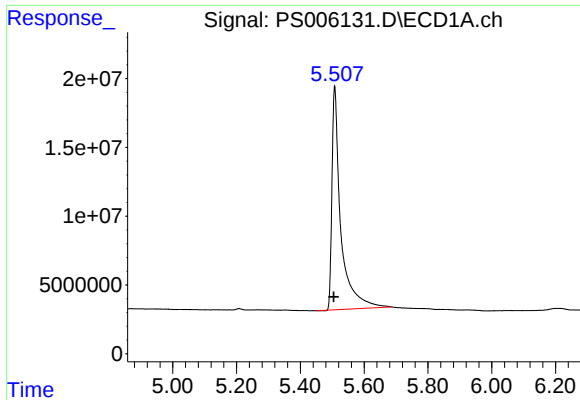

#4 2,4-DCAA


R.T.: 5.508 min
Delta R.T.: 0.003 min
Response: 312927795
Conc: 362.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

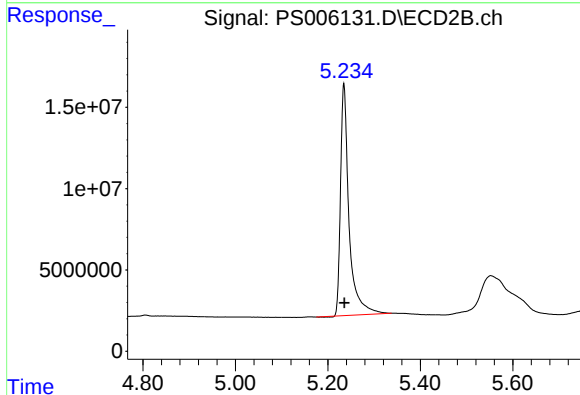


#4 2,4-DCAA

R.T.: 5.235 min
Delta R.T.: 0.000 min
Response: 181836888
Conc: 369.70 ng/ml

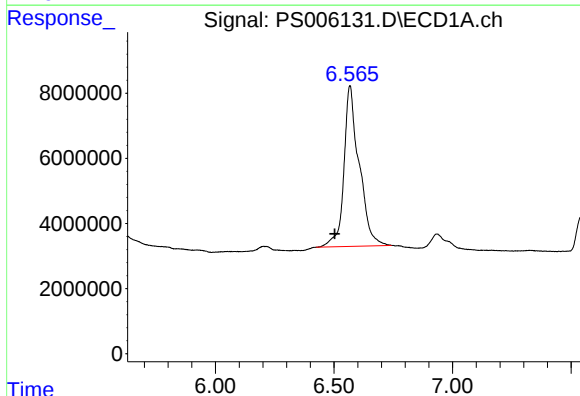


#9 2,4-D

R.T.: 6.567 min
Delta R.T.: 0.064 min
Response: 220375101
Conc: 270.47 ng/ml

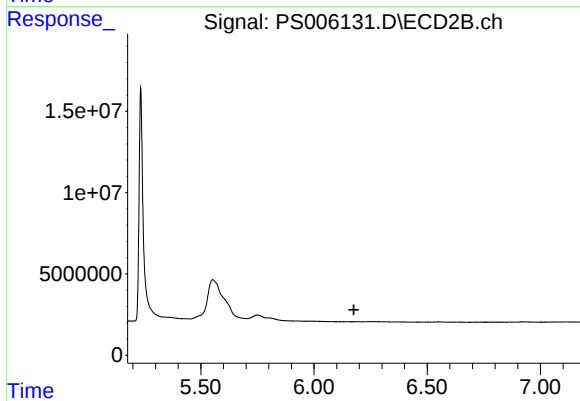

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.176 min
Response: 0
Conc: N.D.

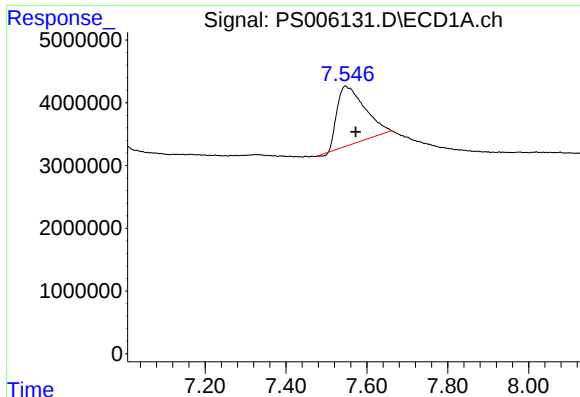

#12 2,4,5-T


R.T.: 7.547 min
Delta R.T.: -0.026 min
Response: 44268998
Conc: 8.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

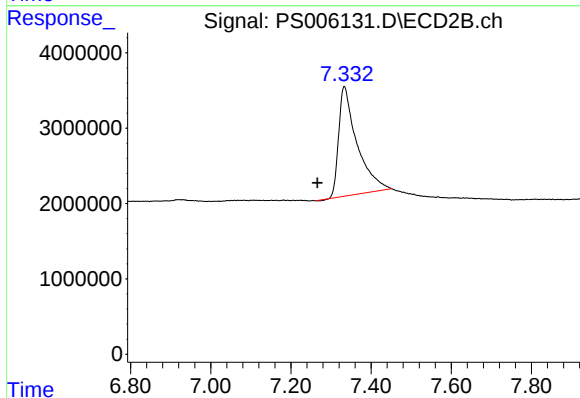


#12 2,4,5-T

R.T.: 7.333 min
Delta R.T.: 0.067 min
Response: 46146765
Conc: 18.56 ng/ml

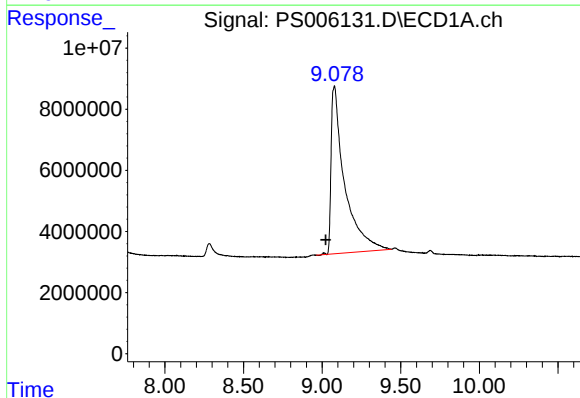


#15 Picloram

R.T.: 9.078 min
Delta R.T.: 0.054 min
Response: 328680942
Conc: 44.17 ng/ml

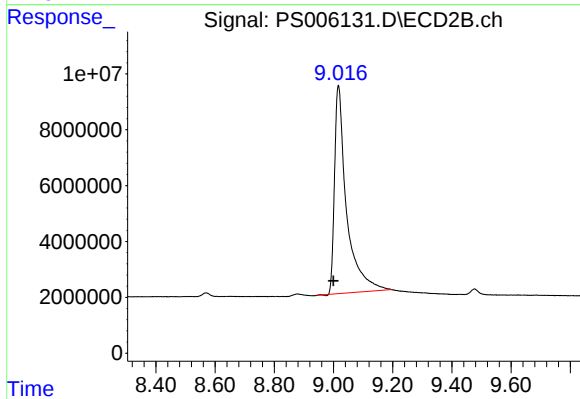

#15 Picloram


R.T.: 9.017 min
Delta R.T.: 0.017 min
Response: 210584305
Conc: 46.68 ng/ml

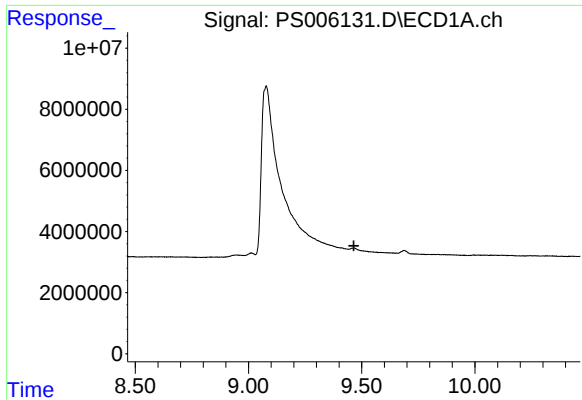

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

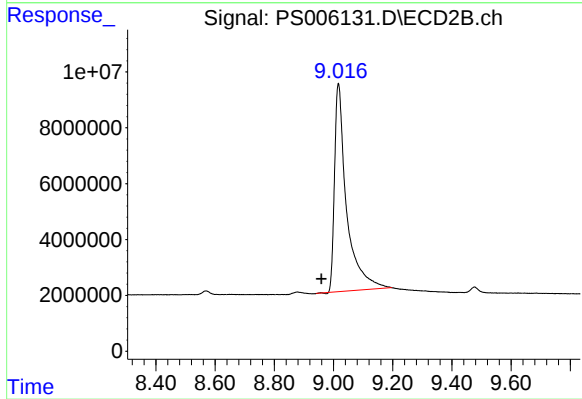

#16 DCPA

R.T.: 9.017 min
Delta R.T.: 0.057 min
Response: 210584305
Conc: 60.39 ng/ml