

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081519\
 Data File : PS006132.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2019 20:18
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 03:58:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.491	5.218	338.0E6	194.3E6	391.578	394.956
Target Compounds							
9) T	2,4-D	6.550	0.000	225.0E6	0	276.179	N.D. #
12) T	2,4,5-T	7.534	7.318	32601673	37861062	6.593	15.229 #
15) T	Picloram	9.057	8.999	335.9E6	205.6E6	45.143	45.583
16) T	DCPA	0.000	8.999	0	205.6E6	N.D.	58.965



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081519\
Data File : PS006132.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2019 20:18
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 03:58:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

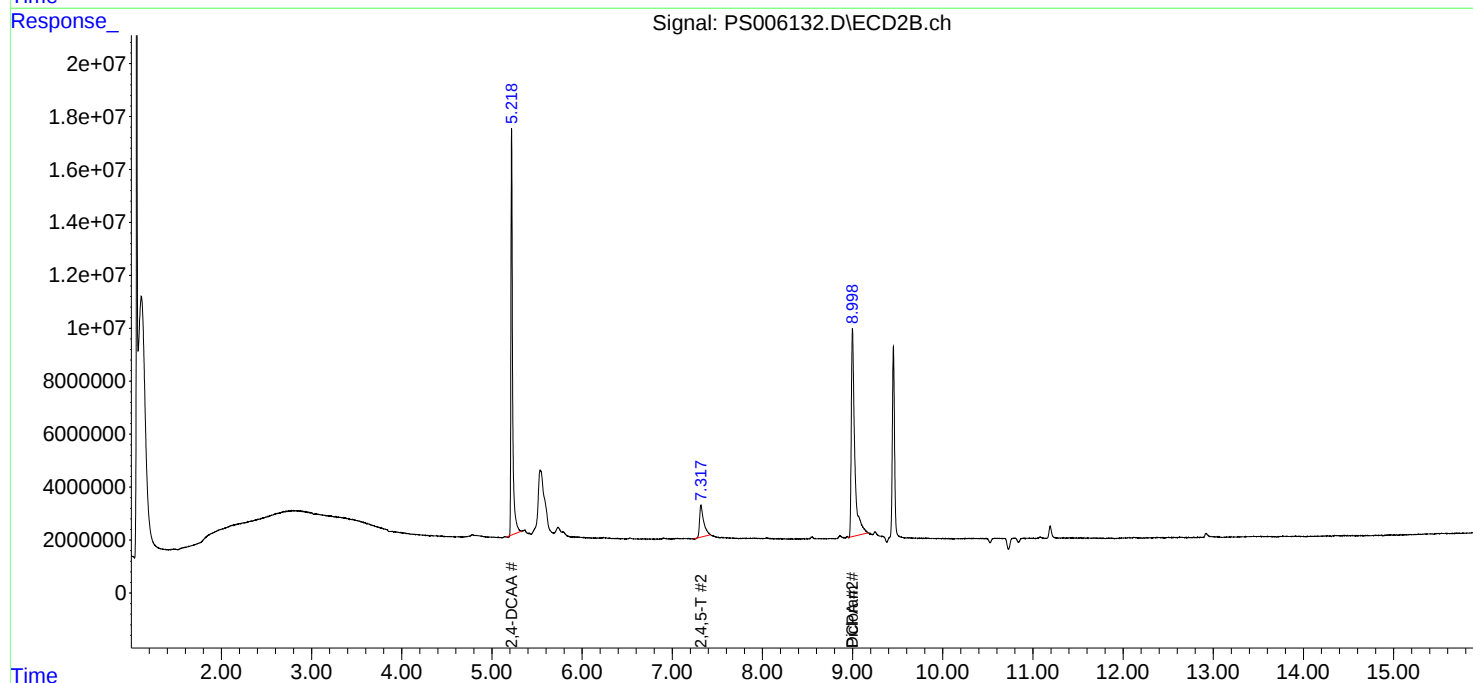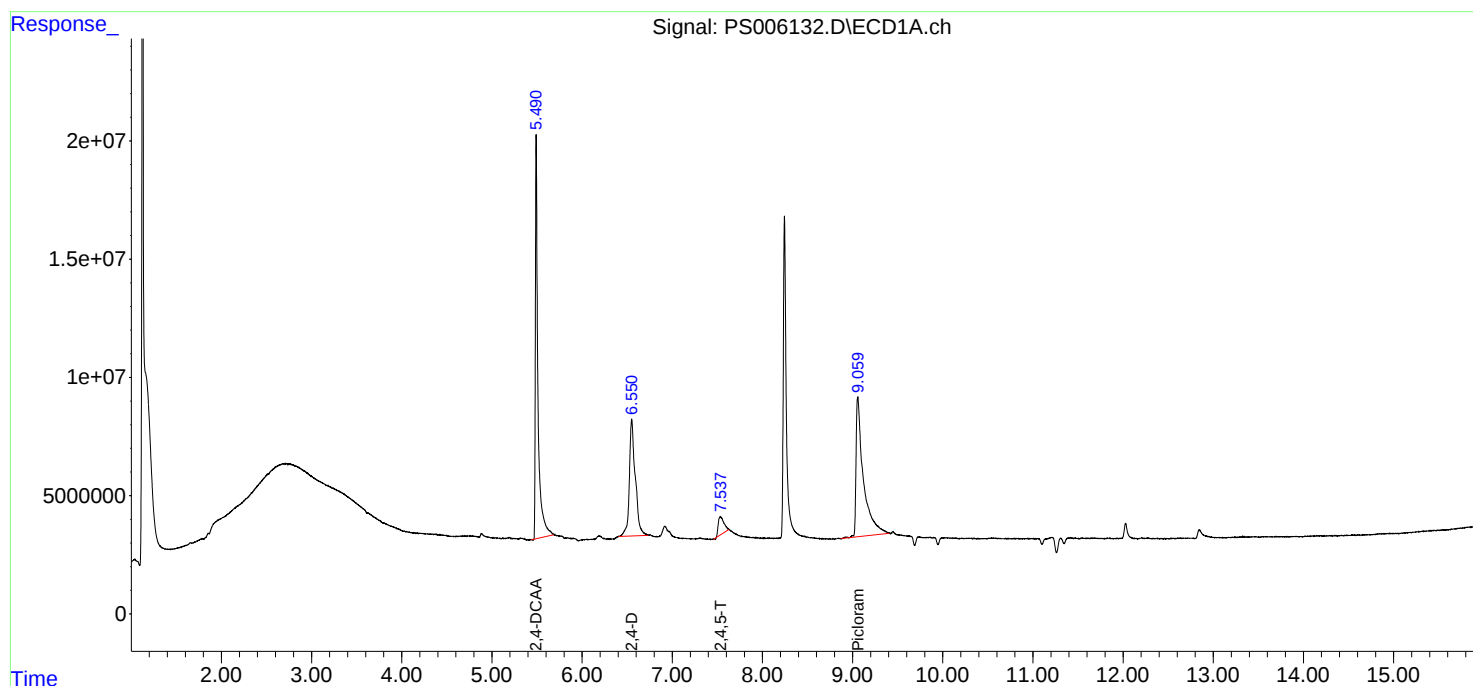


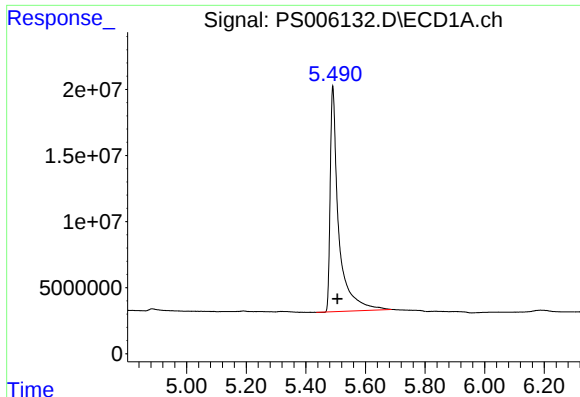

#4 2,4-DCAA


R.T.: 5.491 min
Delta R.T.: -0.014 min
Response: 338010610
Conc: 391.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

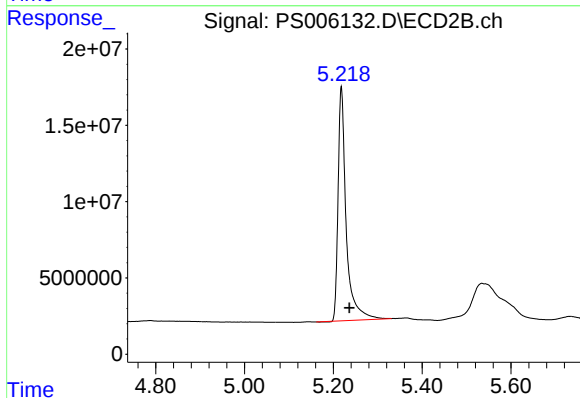


#4 2,4-DCAA

R.T.: 5.218 min
Delta R.T.: -0.017 min
Response: 194259774
Conc: 394.96 ng/ml

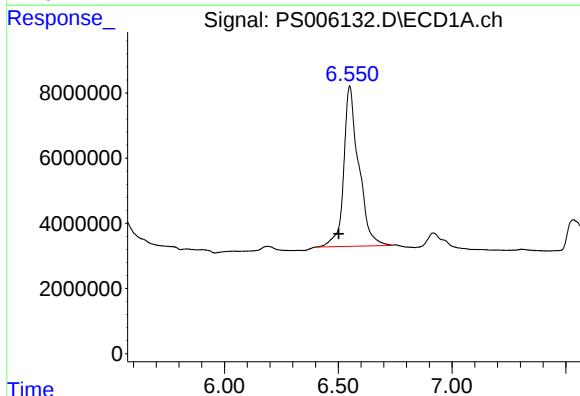


#9 2,4-D

R.T.: 6.550 min
Delta R.T.: 0.047 min
Response: 225026585
Conc: 276.18 ng/ml

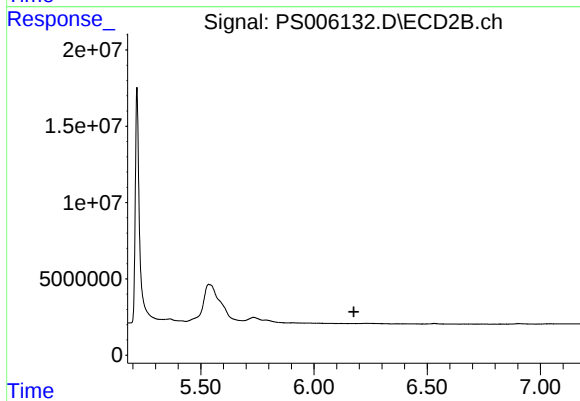

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.176 min
Response: 0
Conc: N.D.

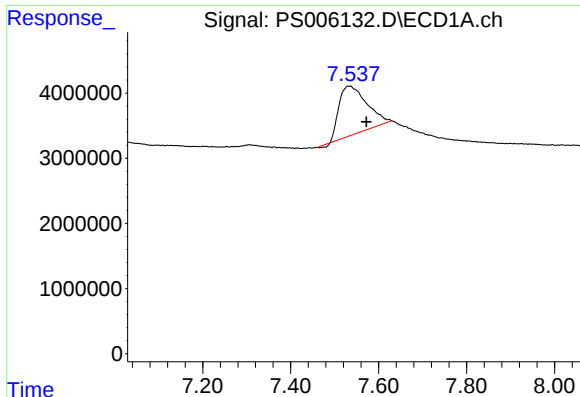

#12 2,4,5-T


R.T.: 7.534 min
Delta R.T.: -0.039 min
Response: 32601673
Conc: 6.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

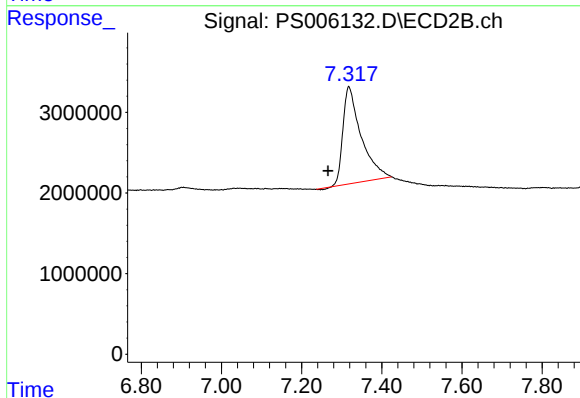


#12 2,4,5-T

R.T.: 7.318 min
Delta R.T.: 0.052 min
Response: 37861062
Conc: 15.23 ng/ml

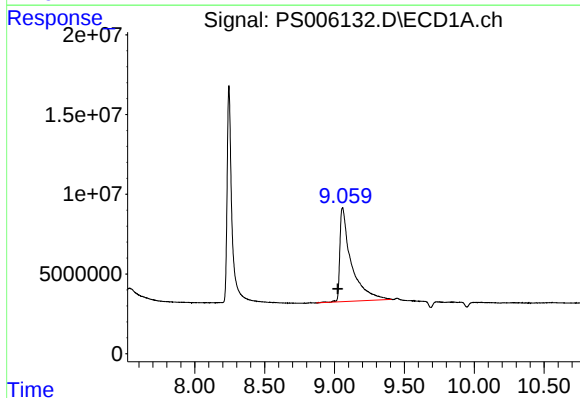


#15 Picloram

R.T.: 9.057 min
Delta R.T.: 0.033 min
Response: 335891566
Conc: 45.14 ng/ml

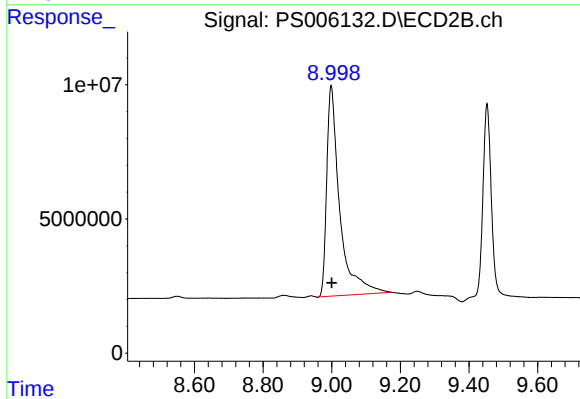

#15 Picloram


R.T.: 8.999 min
Delta R.T.: -0.002 min
Response: 205618510
Conc: 45.58 ng/ml

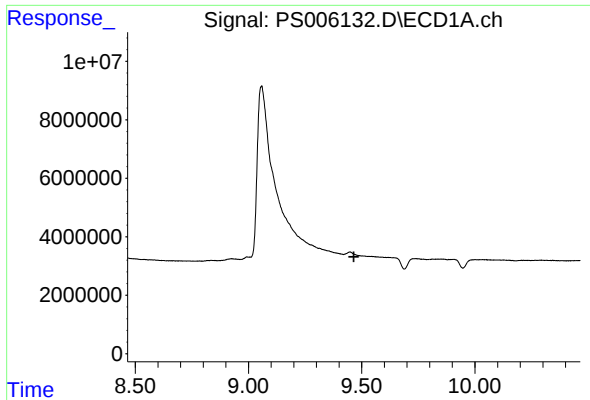

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

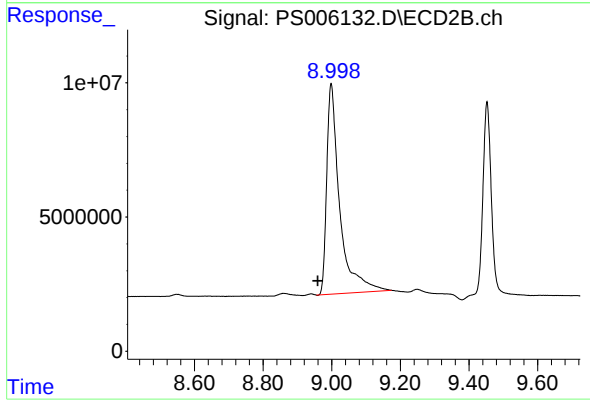

#16 DCPA

R.T.: 8.999 min
Delta R.T.: 0.039 min
Response: 205618510
Conc: 58.96 ng/ml