

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081523\
 Data File : PS024071.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2023 13:50
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 16 00:03:29 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080823.M
 Quant Title : 8080.M
 QLast Update : Tue Aug 08 13:26:17 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

1) T	Dalapon	2.514	2.574	7444423	4927605	3.393	4.506 #
2) T	3,5-DICHL...	5.738	5.981	104549	831112	<MDL	<MDL #
3) T	4-Nitroph...	6.208	6.387	18747935	1245562	16.939	3.147 #
5) T	DICAMBA	0.000	6.978	0	4447053	N.D.	1.516
6) T	MCP	0.000	7.093	0	665172	N.D.	<MDL
7) T	MCPA	6.776	7.205f	3488327	10956349	<MDL	3.745 #
8) T	DICHLORPROP	7.112	0.000	12231503	0	5.436	N.D. #
9) T	2,4-D	7.299	7.800f	19381109	555382	7.821	<MDL #
11) T	2,4,5-TP ...	8.049	8.714f	478873	206375	<MDL	<MDL #
12) T	2,4,5-T	8.311	9.055	955850	1484148	<MDL	<MDL #
14) T	DINOSEB	9.878	9.844	167952	281471	<MDL	<MDL #
15) T	Picloram	9.698	10.803	15929438	5570575	1.232	1.118
16) T	DCPA	0.000	10.803	0	5570575	N.D.	1.084



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081523\
Data File : PS024071.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2023 13:50
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 16 00:03:29 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080823.M
Quant Title : 8080.M
QLast Update : Tue Aug 08 13:26:17 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

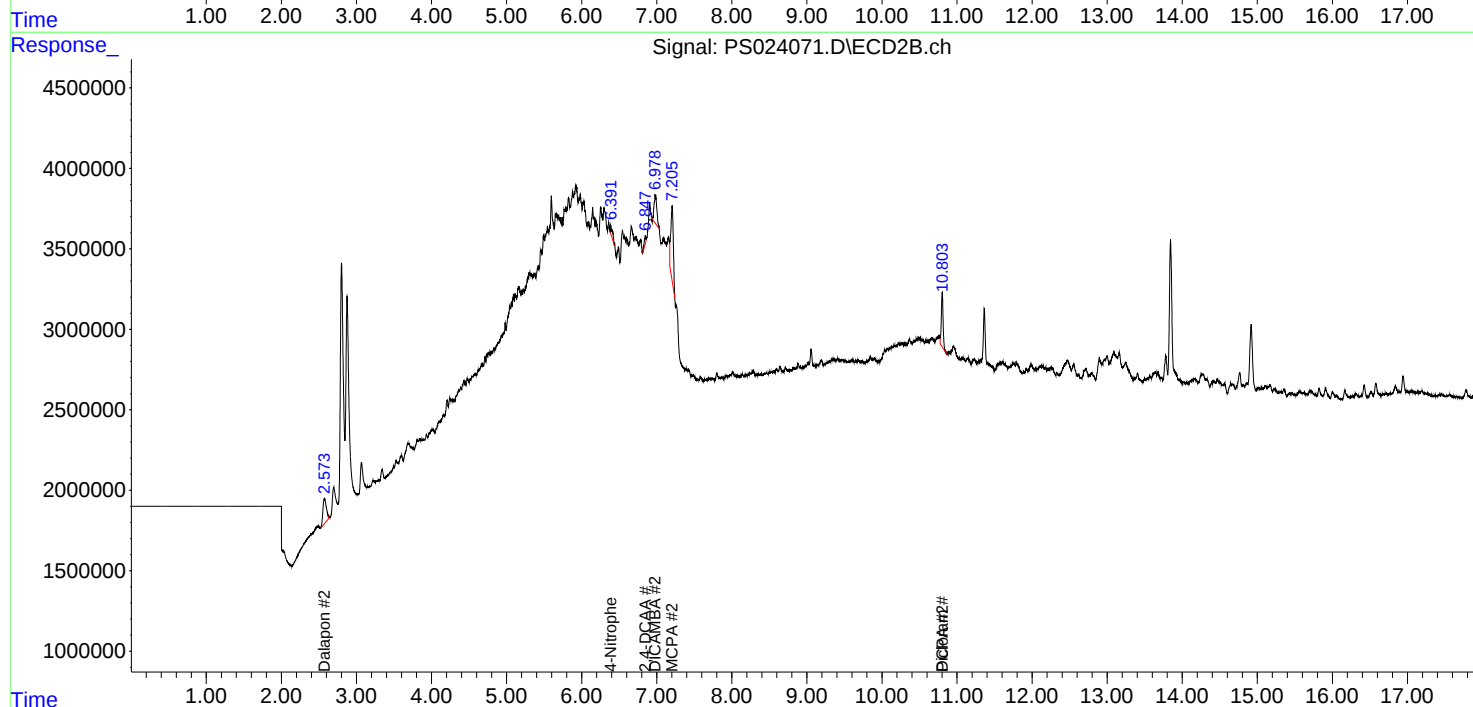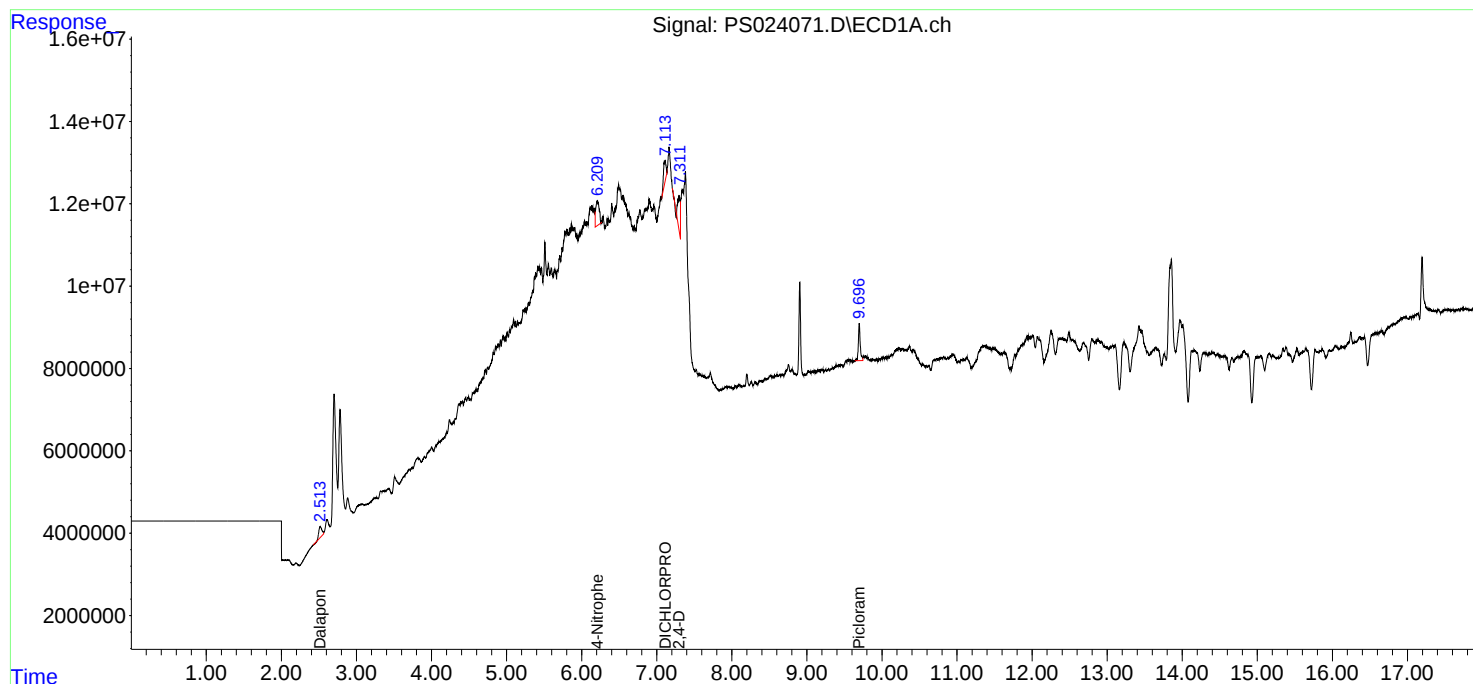


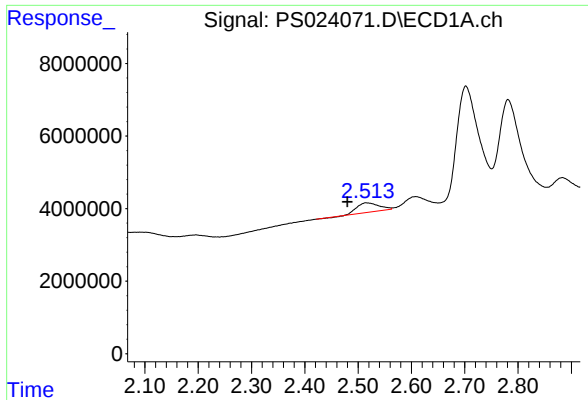

#1 Dalapon


R.T.: 2.514 min
Delta R.T.: 0.034 min
Response: 7444423
Conc: 3.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

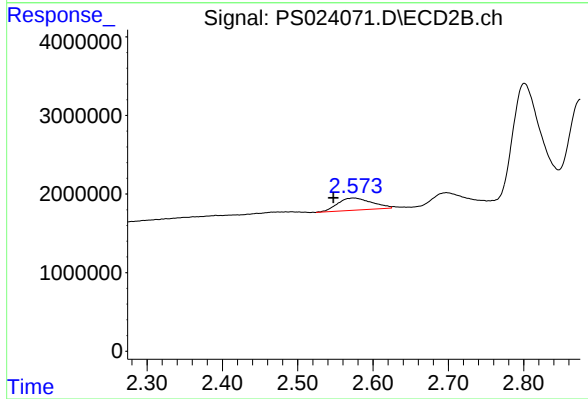


#1 Dalapon

R.T.: 2.574 min
Delta R.T.: 0.026 min
Response: 4927605
Conc: 4.51 ng/ml

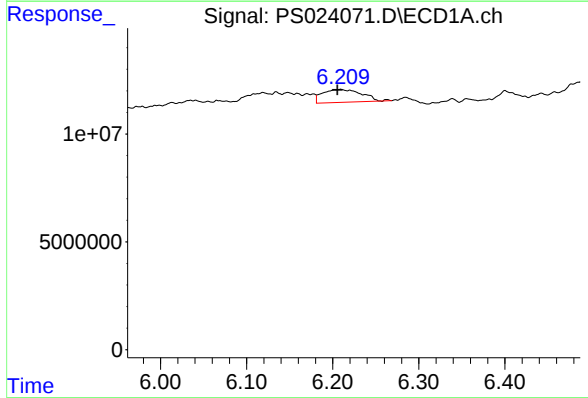


#3 4-Nitrophenol

R.T.: 6.208 min
Delta R.T.: 0.002 min
Response: 18747935
Conc: 16.94 ng/ml

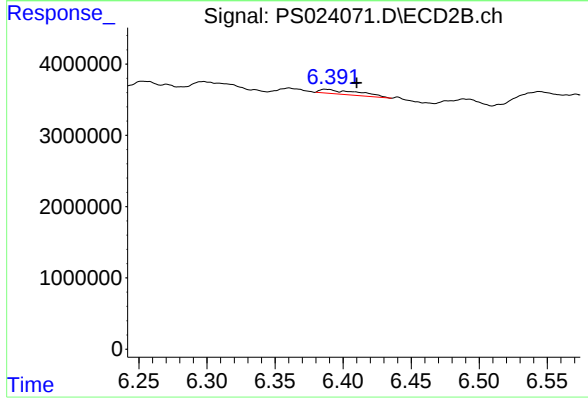

#3 4-Nitrophenol


R.T.: 6.387 min
Delta R.T.: -0.023 min
Response: 1245562
Conc: 3.15 ng/ml

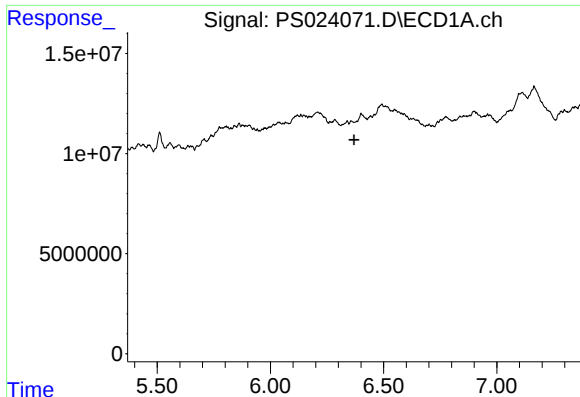

#4 2,4-DCAA


R.T.: 6.339 min
Delta R.T.: -0.030 min
Response: -2498732
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

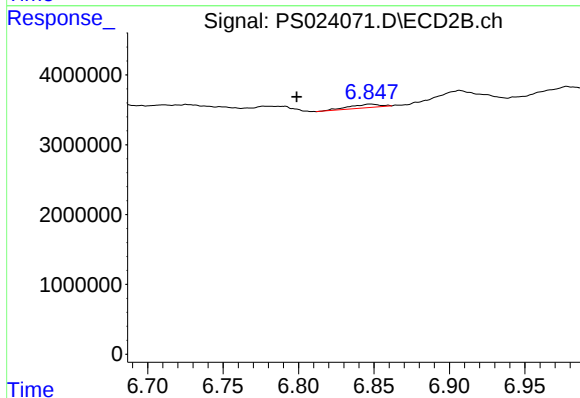


#4 2,4-DCAA

R.T.: 6.848 min
Delta R.T.: 0.049 min
Response: 724685
Conc: 1.08 ng/ml

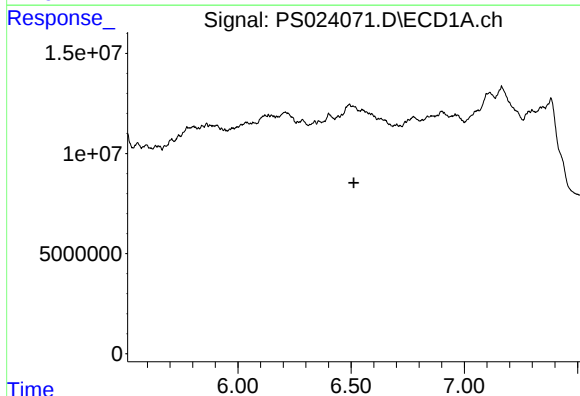


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.512 min
Response: 0
Conc: N.D.

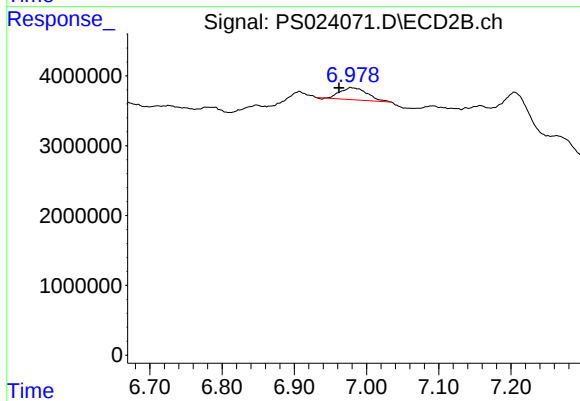

#5 DICAMBA


R.T.: 6.978 min
Delta R.T.: 0.016 min
Response: 4447053
Conc: 1.52 ng/ml

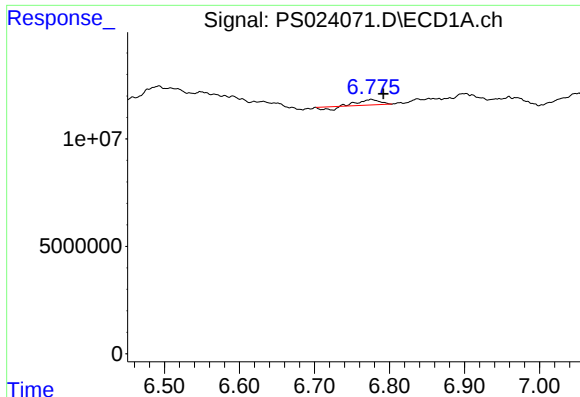

#7 MCPA


R.T.: 6.776 min
Delta R.T.: -0.016 min
Response: 3488327
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

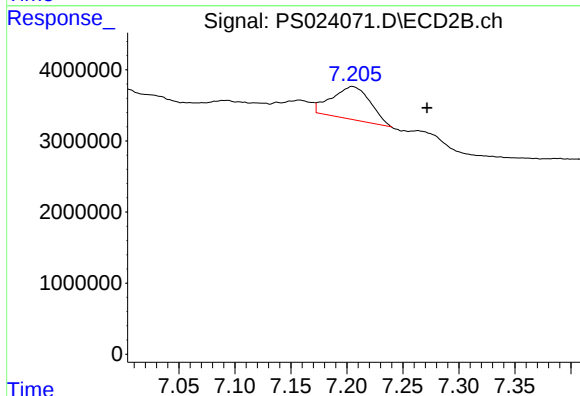


#7 MCPA

R.T.: 7.205 min
Delta R.T.: -0.067 min
Response: 10956349
Conc: 3.75 ug/ml

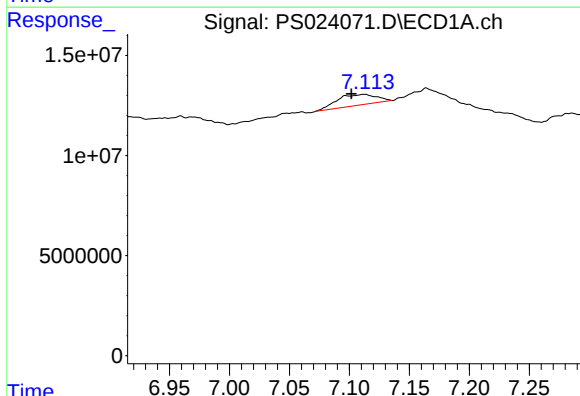


#8 DICHLORPROP

R.T.: 7.112 min
Delta R.T.: 0.010 min
Response: 12231503
Conc: 5.44 ng/ml

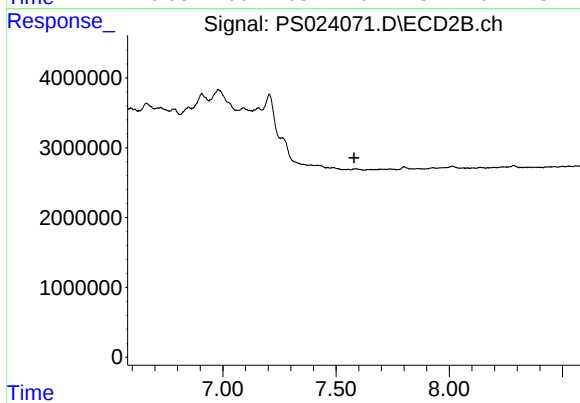

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.579 min
Response: 0
Conc: N.D.

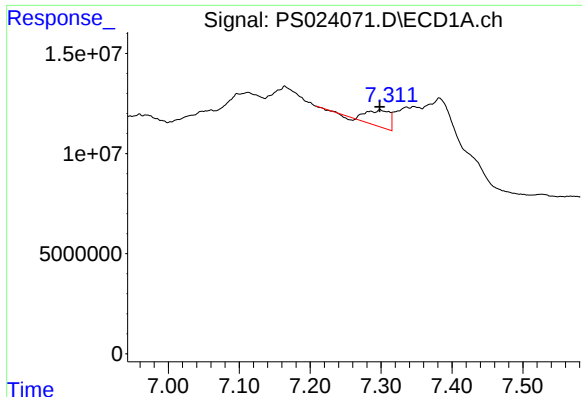

#9 2,4-D


R.T.: 7.299 min
Delta R.T.: 0.001 min
Response: 19381109
Conc: 7.82 ng/ml

Instrument :
ECD_S
ClientSampleId :

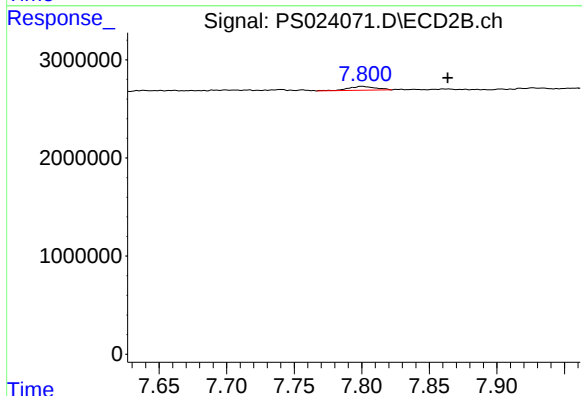


#9 2,4-D

R.T.: 7.800 min
Delta R.T.: -0.063 min
Response: 555382
Conc: N.D.

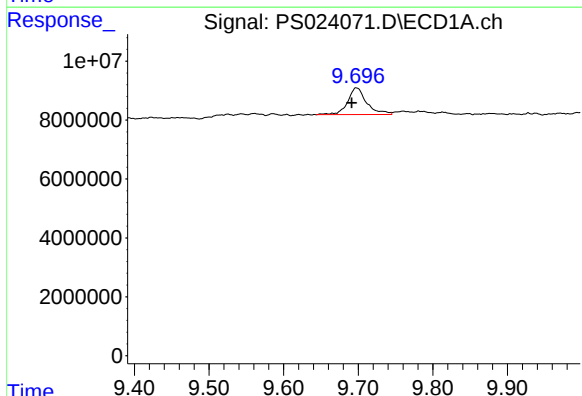


#15 Picloram

R.T.: 9.698 min
Delta R.T.: 0.007 min
Response: 15929438
Conc: 1.23 ng/ml

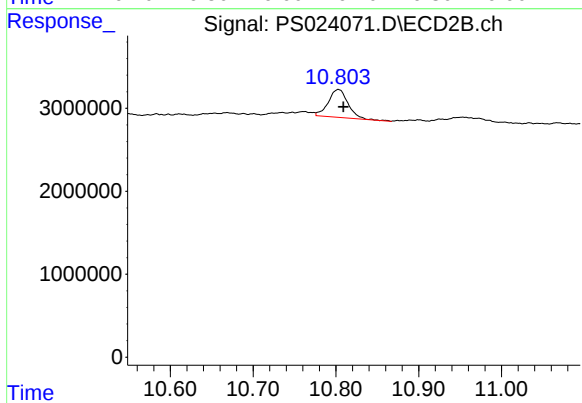

#15 Picloram


R.T.: 10.803 min
Delta R.T.: -0.006 min
Response: 5570575
Conc: 1.12 ng/ml

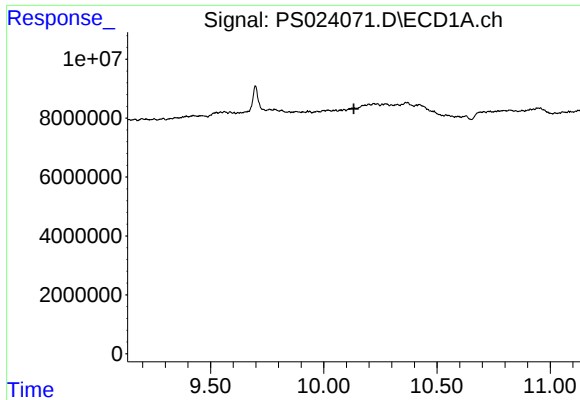

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

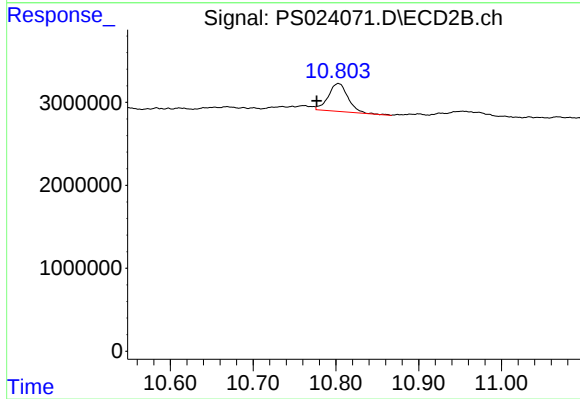

#16 DCPA

R.T.: 10.803 min
Delta R.T.: 0.026 min
Response: 5570575
Conc: 1.08 ng/ml