

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081525\
 Data File : PS031453.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2025 10:32
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 03:46:09 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
 Quant Title : 8080.M
 QLast Update : Fri Aug 08 03:17:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.291	7.745	1605.2E6	456.8E6	505.736	540.322
Target Compounds							
1) T	Dalapon	0.000	2.659f	0	51087179	N.D.	19.198
2) T	3,5-DICHL...	6.445	0.000	3916206	0	<MDL	N.D. #
6) T	MCP	7.623f	8.057	998621	785709	<MDL	<MDL #
7) T	MCPA	0.000	8.248f	0	41438114	N.D.	14.770
8) T	DICHLORPROP	8.184	0.000	3247736	0	1.024	N.D. #
10) T	Pentachlo...	8.715	9.513	6756087	9157349	<MDL	<MDL #
11) T	2,4,5-TP ...	9.297	9.903	4459597	6675110	<MDL	<MDL #
12) T	2,4,5-T	9.564f	10.374f	8174804	21275228	<MDL	1.797 #
13) T	2,4-DB	10.178	0.000	555846	0	<MDL	N.D. #
14) T	DINOSEB	11.369	0.000	3590584	0	<MDL	N.D. #
15) T	Picloram	11.172	12.436f	5760077	11876154	<MDL	<MDL #
16) T	DCPA	11.666	12.324	5811148	-2744930	<MDL	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081525\
Data File : PS031453.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2025 10:32
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 03:46:09 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
Quant Title : 8080.M
QLast Update : Fri Aug 08 03:17:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

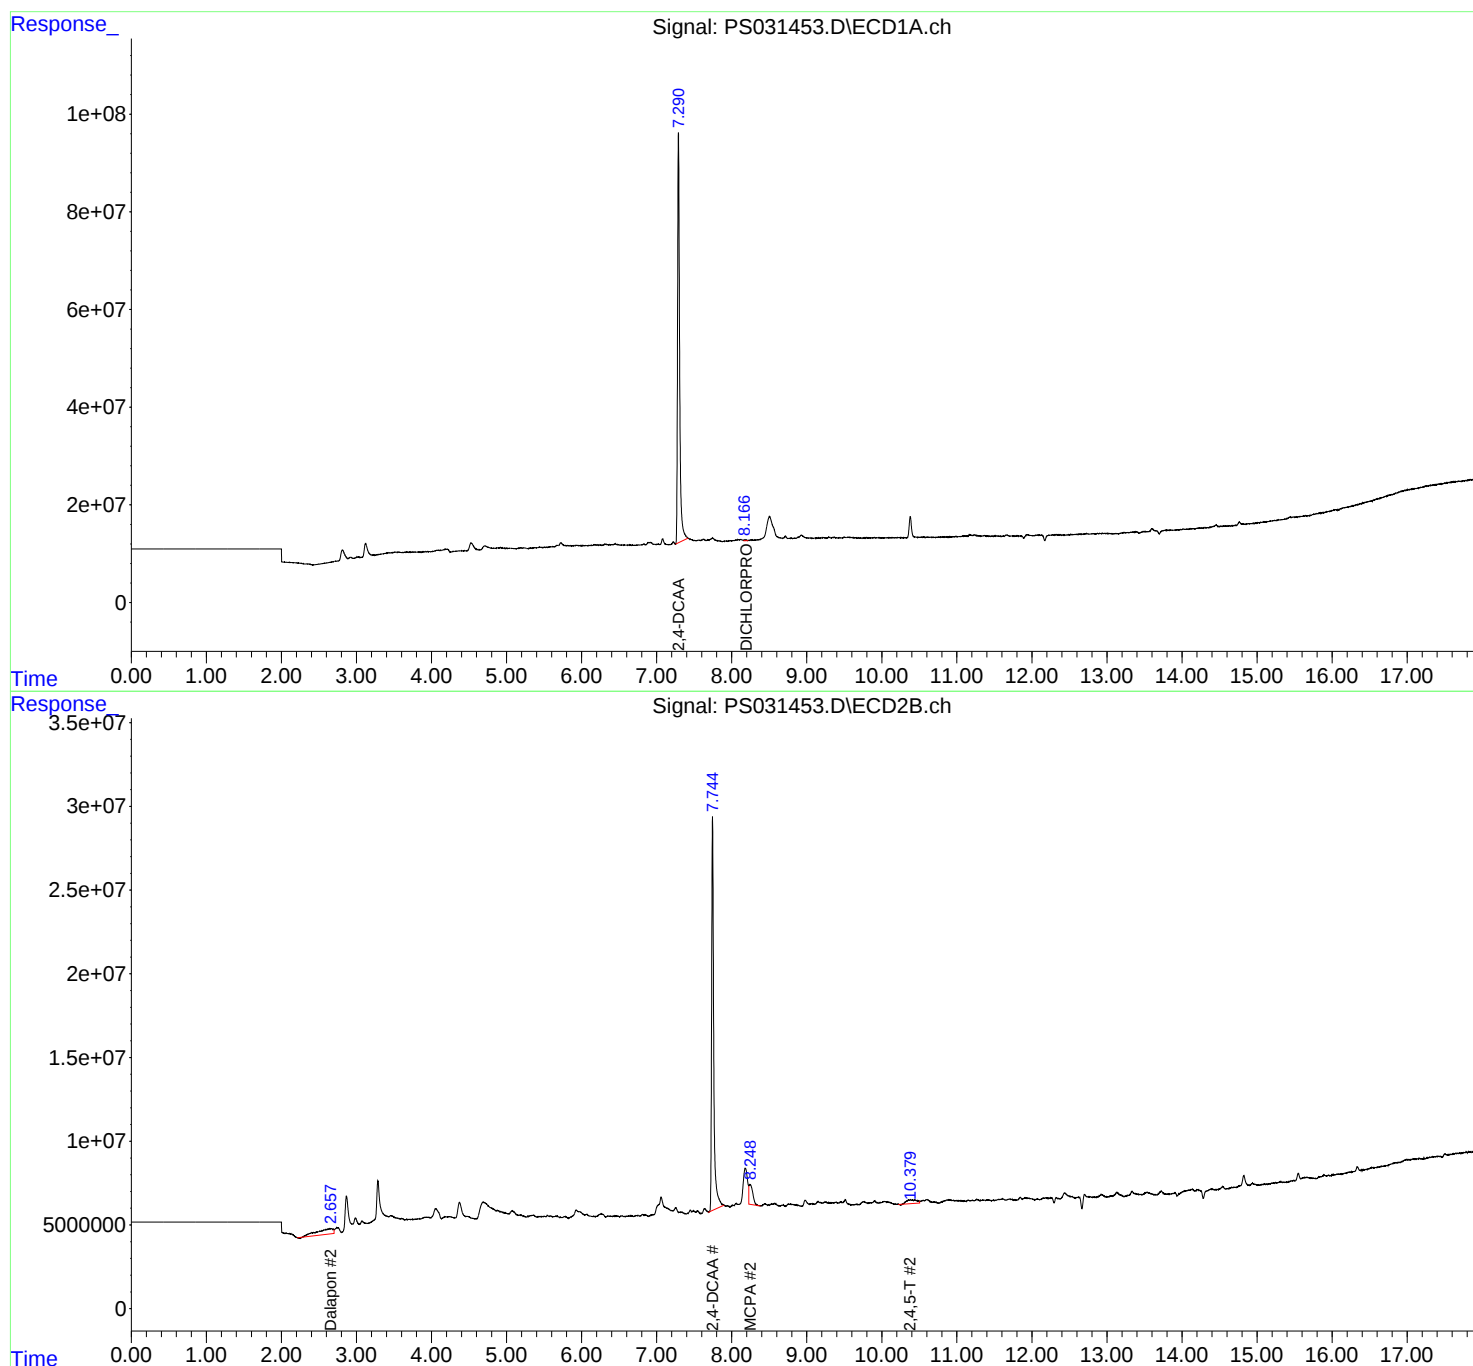


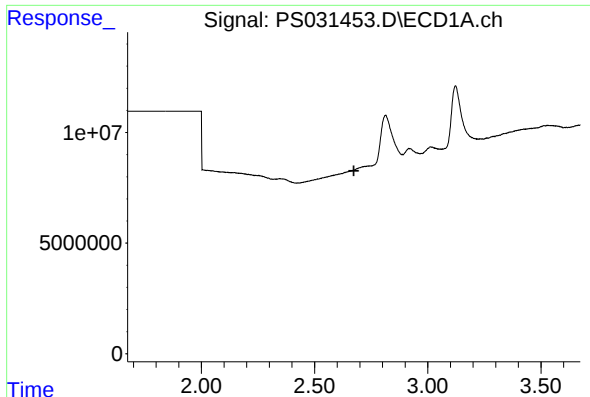

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

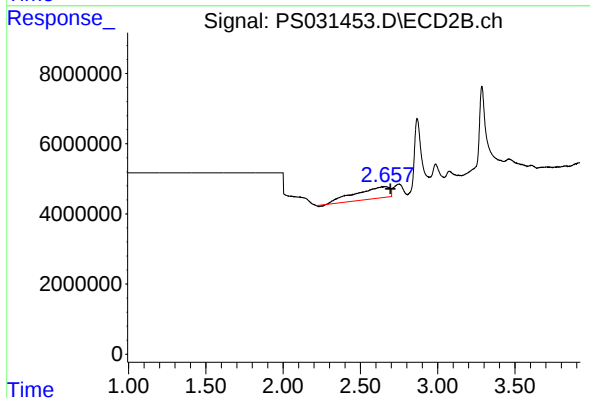


#1 Dalapon

R.T.: 2.659 min
Delta R.T.: -0.036 min
Response: 51087179
Conc: 19.20 ng/ml

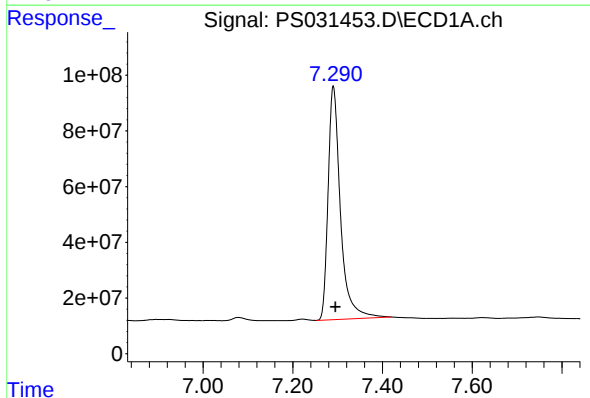


#4 2,4-DCAA

R.T.: 7.291 min
Delta R.T.: -0.004 min
Response: 1605198763
Conc: 505.74 ng/ml

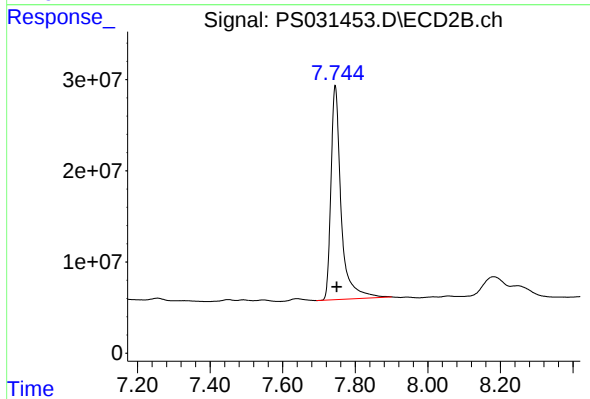

#4 2,4-DCAA


R.T.: 7.745 min
Delta R.T.: -0.004 min
Response: 456755586
Conc: 540.32 ng/ml

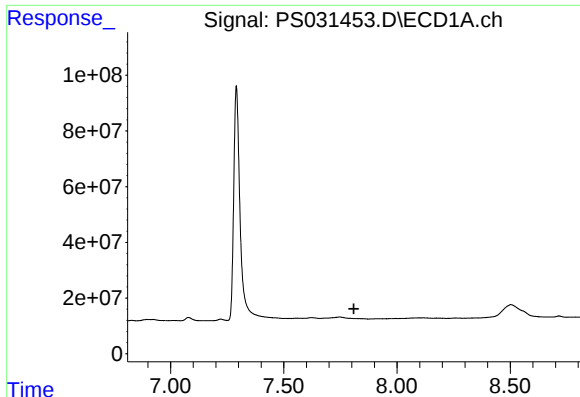

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.809 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

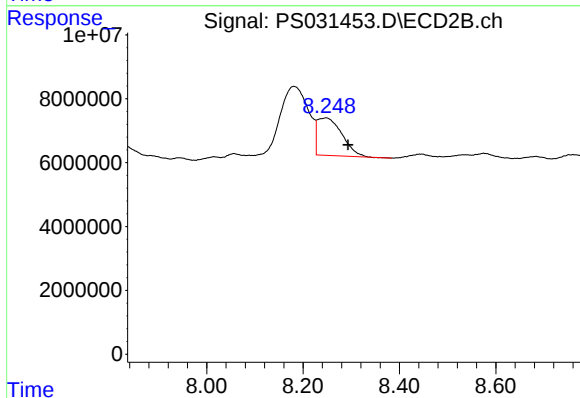


#7 MCPA

R.T.: 8.248 min
Delta R.T.: -0.046 min
Response: 41438114
Conc: 14.77 ug/ml

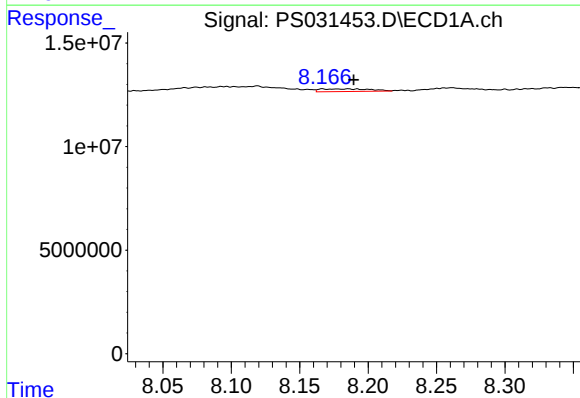


#8 DICHLORPROP

R.T.: 8.184 min
Delta R.T.: -0.005 min
Response: 3247736
Conc: 1.02 ng/ml

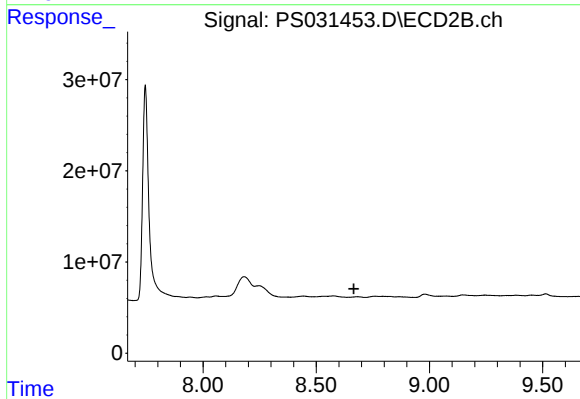

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.666 min
Response: 0
Conc: N.D.

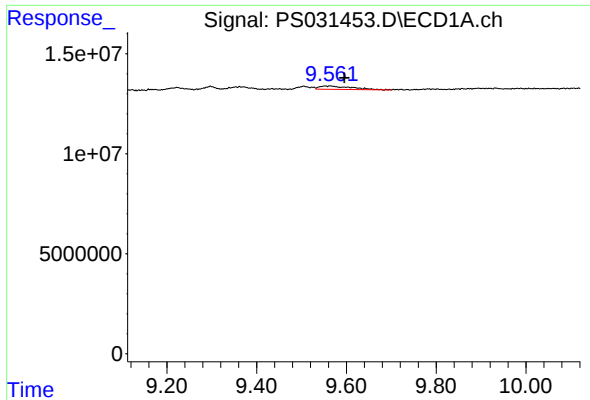

#12 2,4,5-T

R.T.: 9.564 min
Delta R.T.: -0.031 min
Response: 8174804
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

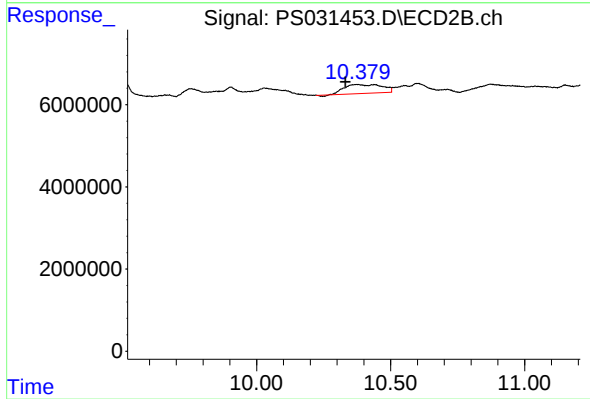

#12 2,4,5-T

R.T.: 10.374 min
Delta R.T.: 0.043 min
Response: 21275228
Conc: 1.80 ng/ml