

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081525\
 Data File : PS031460.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Aug 2025 19:05
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 03:48:30 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
 Quant Title : 8080.M
 QLast Update : Fri Aug 08 03:17:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.290	7.746	1639.0E6	468.5E6	516.376	554.207
Target Compounds							
1) T	Dalapon	2.714f	2.645f	2580221	56166817	<MDL	21.107 #
2) T	3,5-DICHL...	6.443	0.000	5461193	0	1.157	N.D. #
6) T	MCP	7.683	8.058	667555	2399150	<MDL	1.357 #
7) T	MCPA	7.823	0.000	220983	0	<MDL	N.D. #
8) T	DICHLORPROP	8.172	0.000	3241800	0	1.022	N.D. #
10) T	Pentachlo...	8.716	9.516	7085149	9841450	<MDL	<MDL #
11) T	2,4,5-TP ...	9.293	9.905	6068912	2809571	<MDL	<MDL #
12) T	2,4,5-T	9.575	10.379f	804782	13954644	<MDL	1.179 #
13) T	2,4-DB	10.166	0.000	676138	0	<MDL	N.D. #
14) T	DINOSEB	11.369	0.000	2916863	0	<MDL	N.D. #
15) T	Picloram	11.176	0.000	3364156	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081525\
Data File : PS031460.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Aug 2025 19:05
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 03:48:30 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
Quant Title : 8080.M
QLast Update : Fri Aug 08 03:17:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

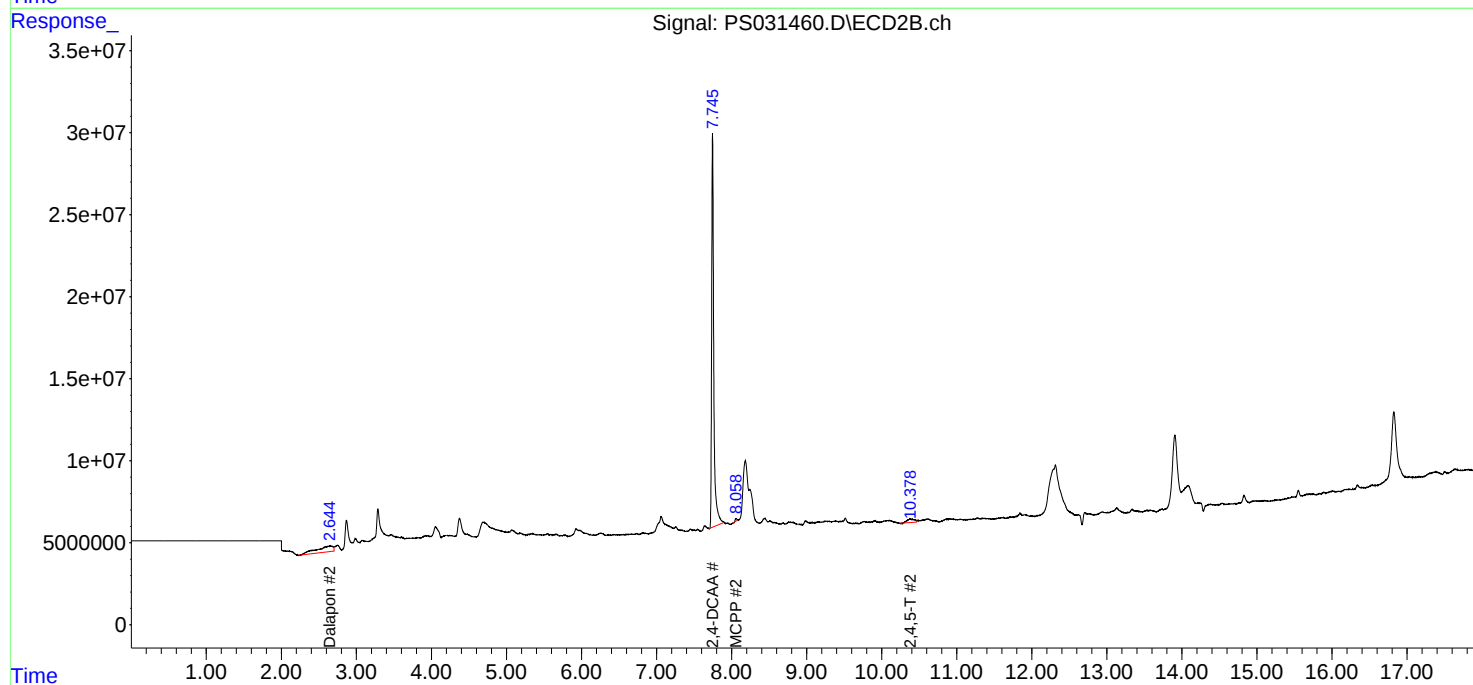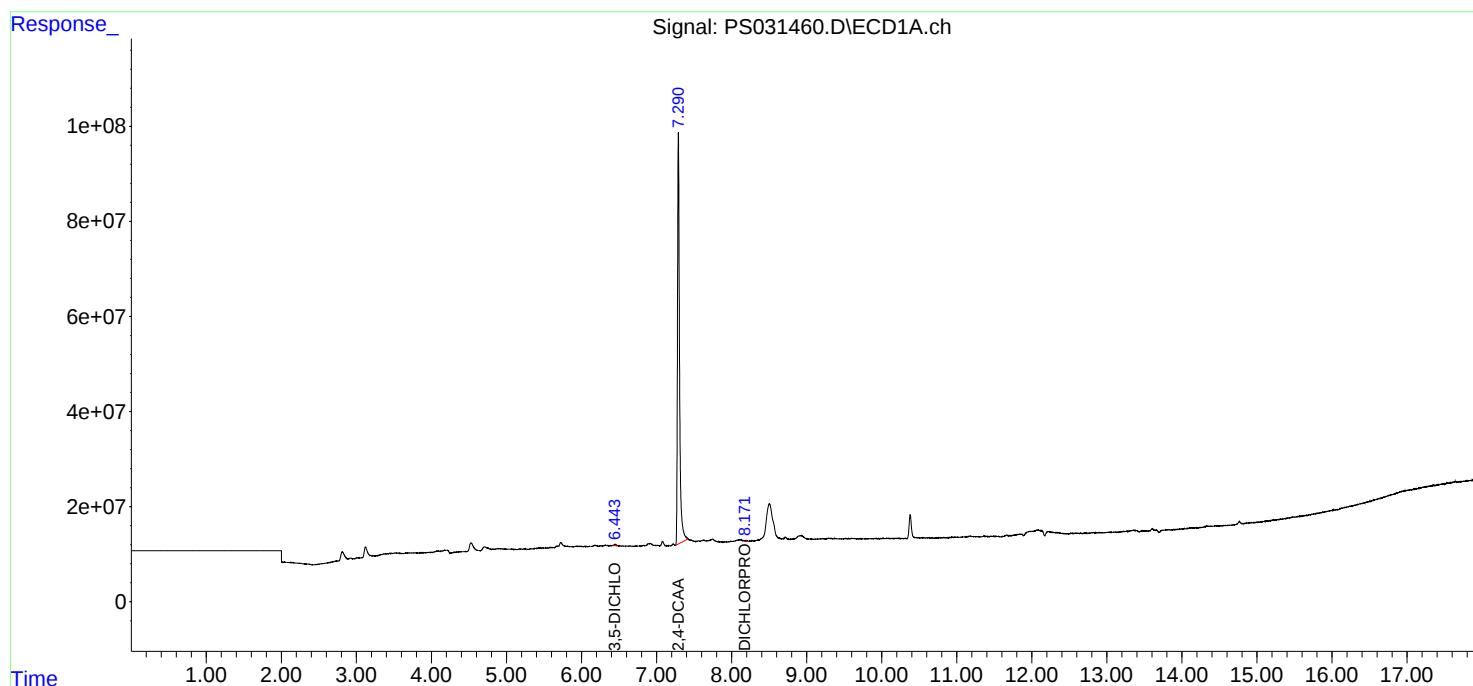


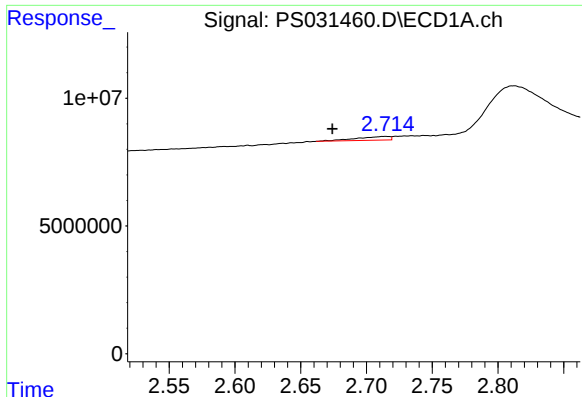

#1 Dalapon


R.T.: 2.714 min
Delta R.T.: 0.040 min
Response: 2580221
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

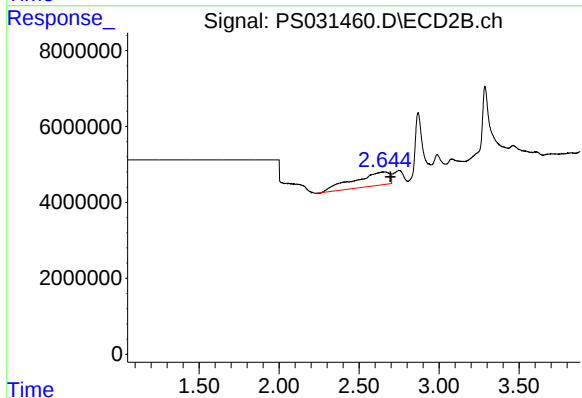


#1 Dalapon

R.T.: 2.645 min
Delta R.T.: -0.050 min
Response: 56166817
Conc: 21.11 ng/ml

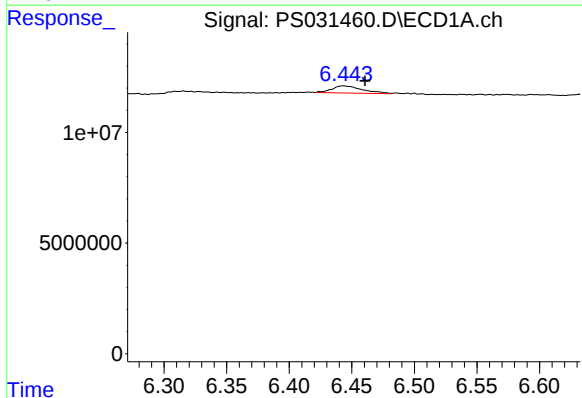


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.443 min
Delta R.T.: -0.017 min
Response: 5461193
Conc: 1.16 ng/ml

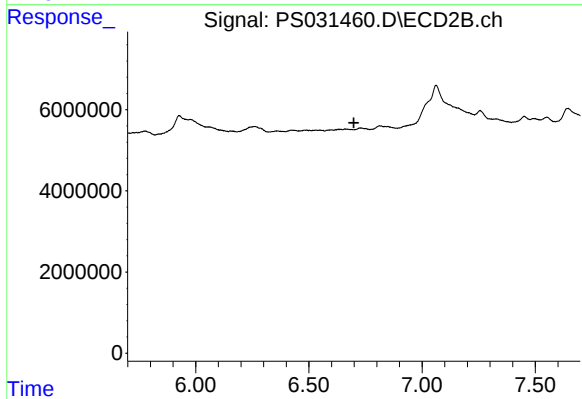

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.699 min
Response: 0
Conc: N.D.

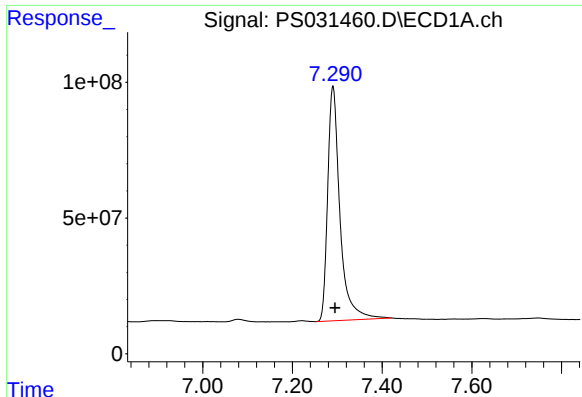

#4 2,4-DCAA


R.T.: 7.290 min
Delta R.T.: -0.005 min
Response: 1638972636
Conc: 516.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

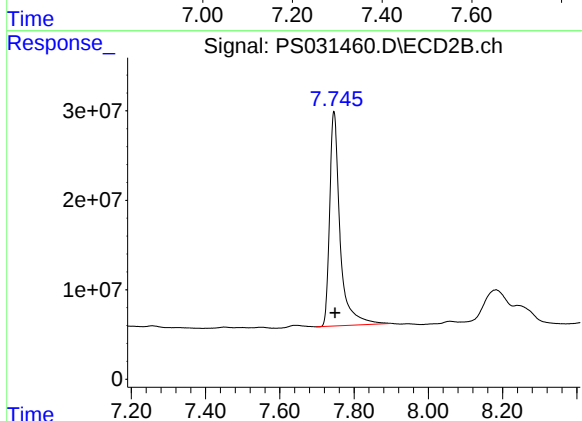


#4 2,4-DCAA

R.T.: 7.746 min
Delta R.T.: -0.003 min
Response: 468493420
Conc: 554.21 ng/ml

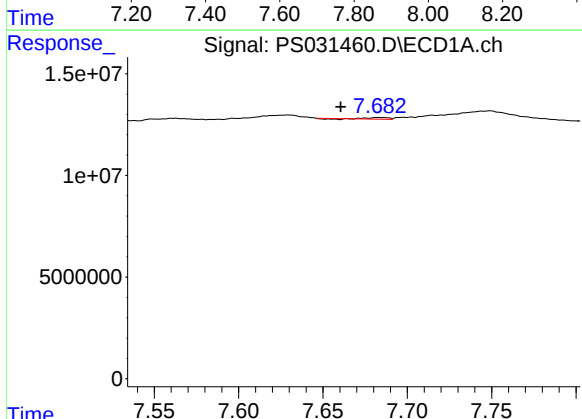


#6 MCP

R.T.: 7.683 min
Delta R.T.: 0.022 min
Response: 667555
Conc: N.D.

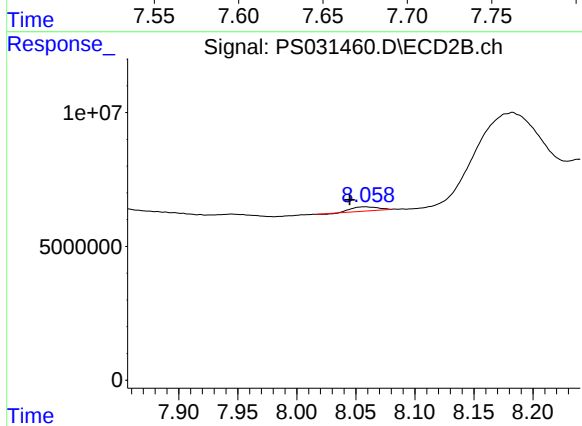

#6 MCP


R.T.: 8.058 min
Delta R.T.: 0.013 min
Response: 2399150
Conc: 1.36 ug/ml

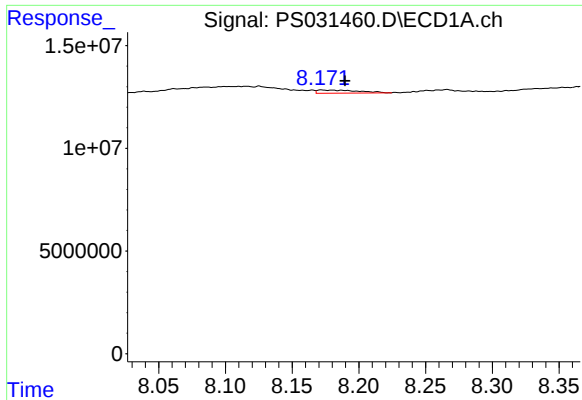

#8 DICHLORPROP


R.T.: 8.172 min
Delta R.T.: -0.017 min
Response: 3241800
Conc: 1.02 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

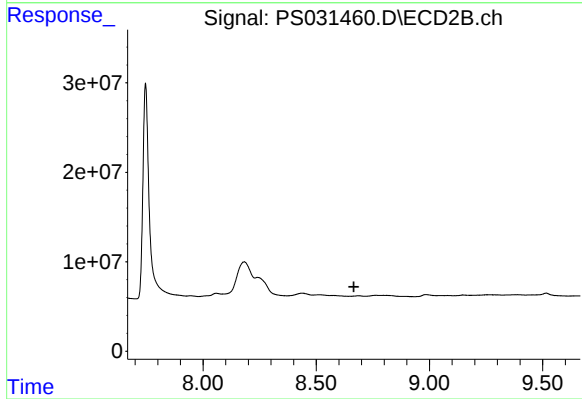


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.666 min
Response: 0
Conc: N.D.

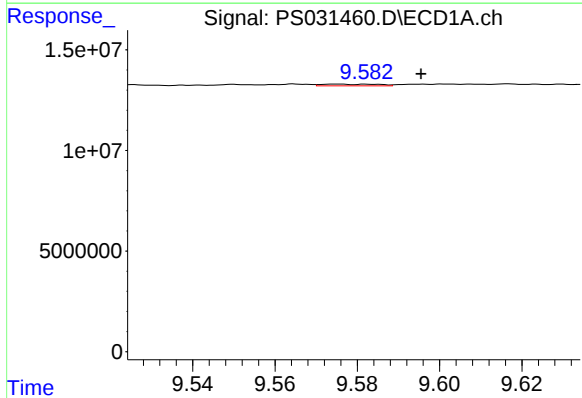

#12 2,4,5-T

R.T.: 9.575 min
Delta R.T.: -0.021 min
Response: 804782
Conc: N.D.

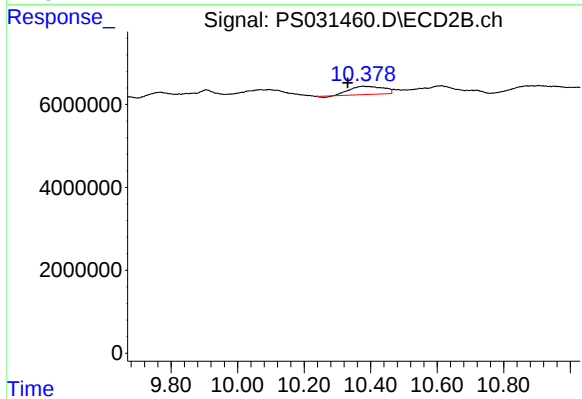

#12 2,4,5-T

R.T.: 10.379 min
Delta R.T.: 0.048 min
Response: 13954644
Conc: 1.18 ng/ml