

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081525\
 Data File : PS031472.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2025 00:43
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 03:52:31 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
 Quant Title : 8080.M
 QLast Update : Fri Aug 08 03:17:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.290	7.745	1653.6E6	480.4E6	520.997	568.300
Target Compounds							
1) T	Dalapon	0.000	2.656f	0	55031899	N.D.	20.681
2) T	3,5-DICHL...	6.444	0.000	8347793	0	1.769	N.D. #
6) T	MCP	7.685	8.054	-220008	4791041	N.D.	2.710
7) T	MCPA	0.000	8.245f	0	44619155	N.D.	15.904
8) T	DICHLORPROP	8.177	0.000	3146782	0	<MDL	N.D. #
10) T	Pentachlo...	8.716	9.515	7490404	7239613	<MDL	<MDL #
11) T	2,4,5-TP ...	9.295	9.908	5838922	5594140	<MDL	<MDL #
12) T	2,4,5-T	9.615	10.377f	2767602	7653038	<MDL	<MDL #
13) T	2,4-DB	10.186	0.000	1460453	0	<MDL	N.D. #
14) T	DINOSEB	11.366	0.000	2554862	0	<MDL	N.D. #
15) T	Picloram	11.176	0.000	3850352	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081525\
Data File : PS031472.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2025 00:43
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 18 03:52:31 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080725.M
Quant Title : 8080.M
QLast Update : Fri Aug 08 03:17:54 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

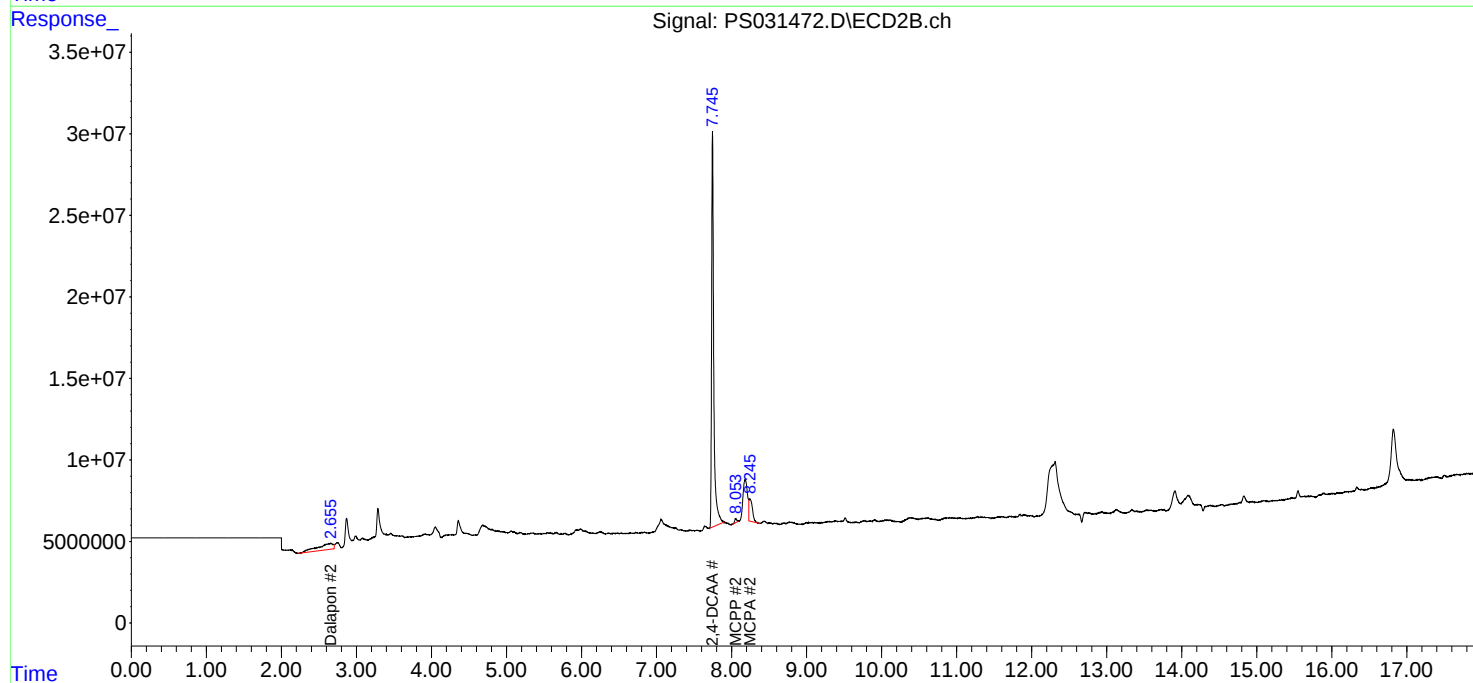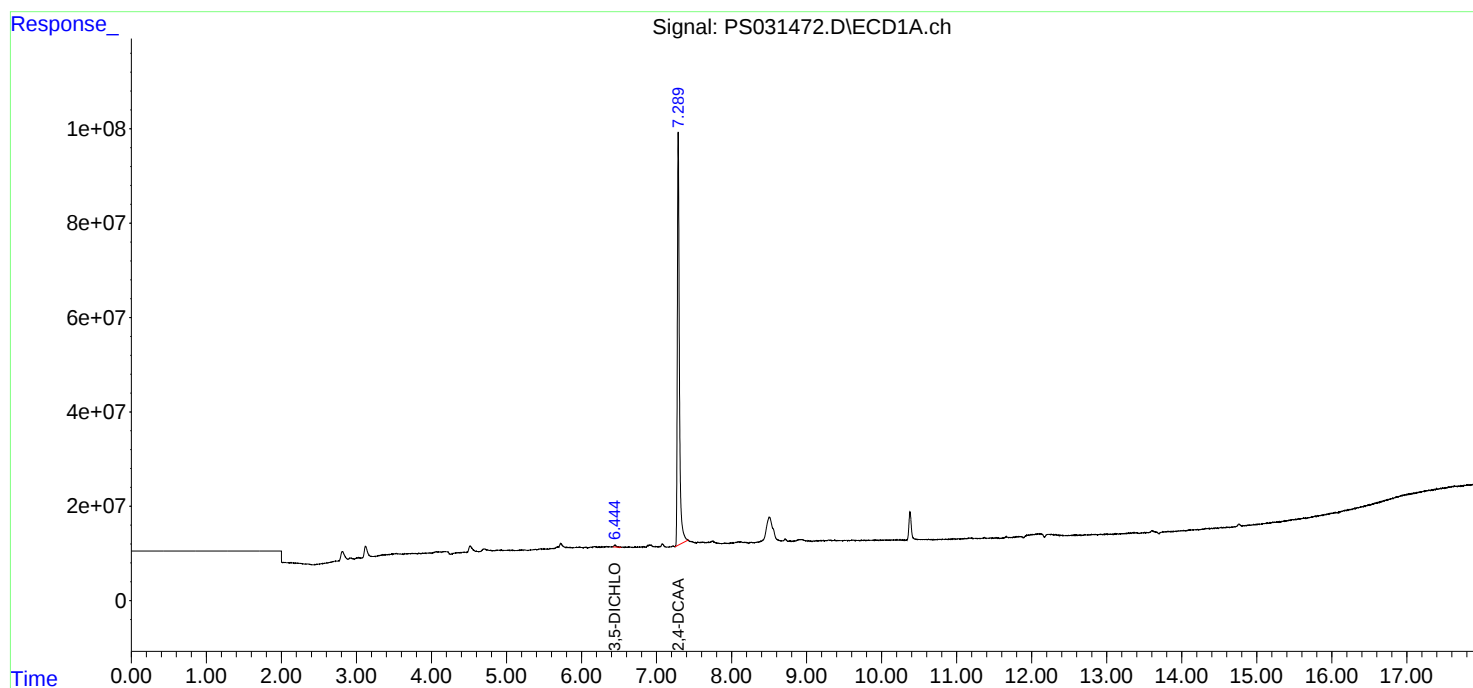


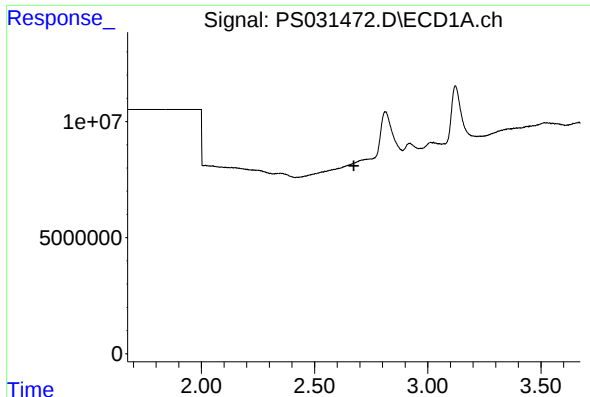

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.674 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

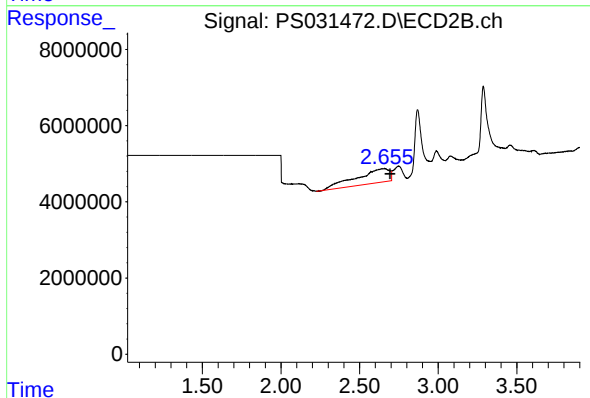


#1 Dalapon

R.T.: 2.656 min
Delta R.T.: -0.039 min
Response: 55031899
Conc: 20.68 ng/ml

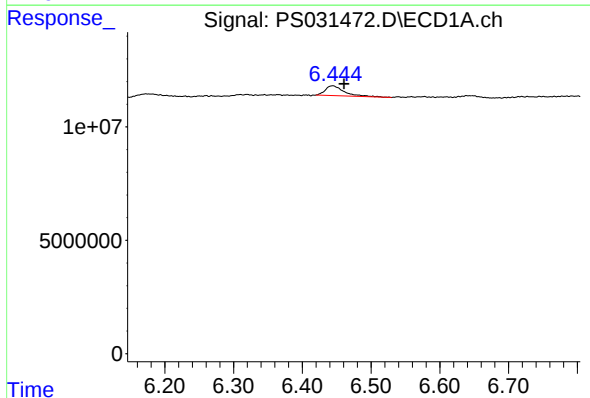


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.444 min
Delta R.T.: -0.016 min
Response: 8347793
Conc: 1.77 ng/ml

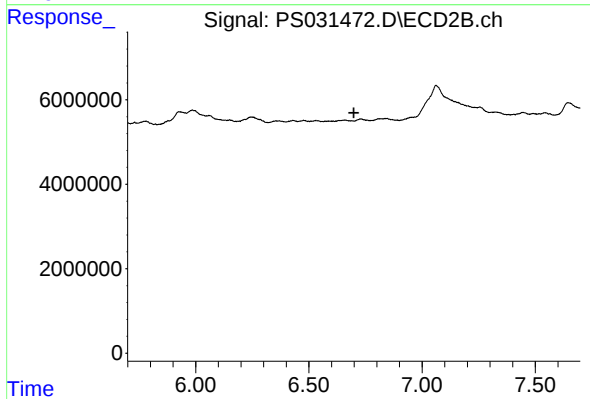

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.699 min
Response: 0
Conc: N.D.

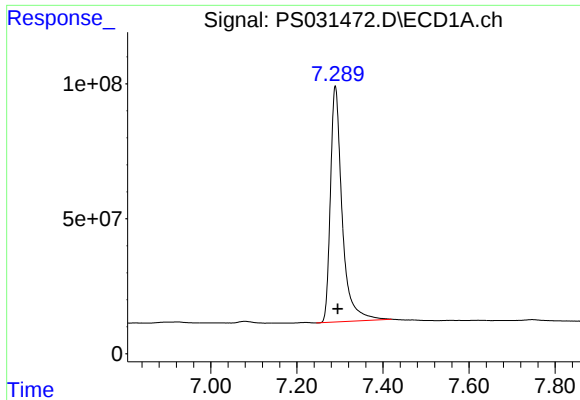

#4 2,4-DCAA


R.T.: 7.290 min
Delta R.T.: -0.005 min
Response: 1653636951
Conc: 521.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

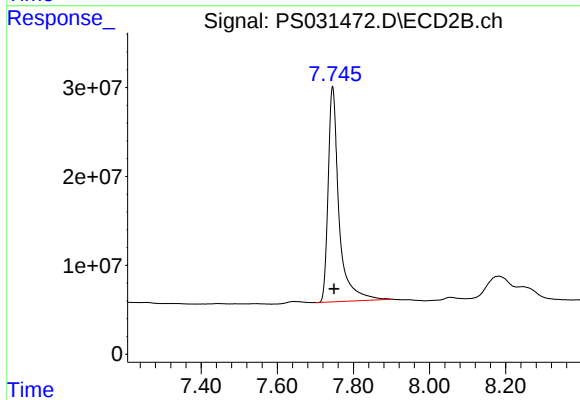


#4 2,4-DCAA

R.T.: 7.745 min
Delta R.T.: -0.004 min
Response: 480406289
Conc: 568.30 ng/ml

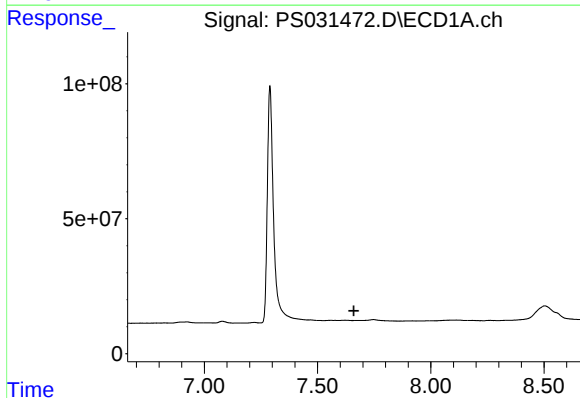


#6 MCP

R.T.: 7.685 min
Delta R.T.: 0.024 min
Response: -220008
Conc: N.D.

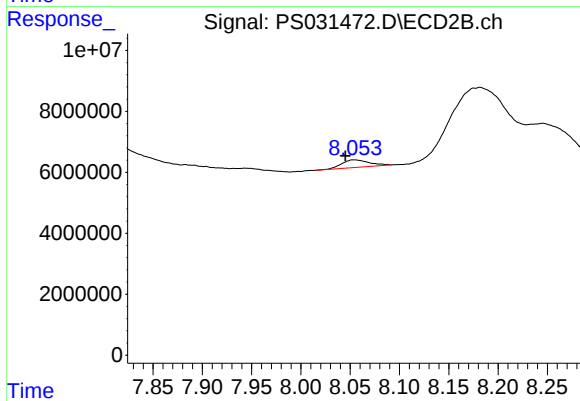

#6 MCP


R.T.: 8.054 min
Delta R.T.: 0.009 min
Response: 4791041
Conc: 2.71 ug/ml

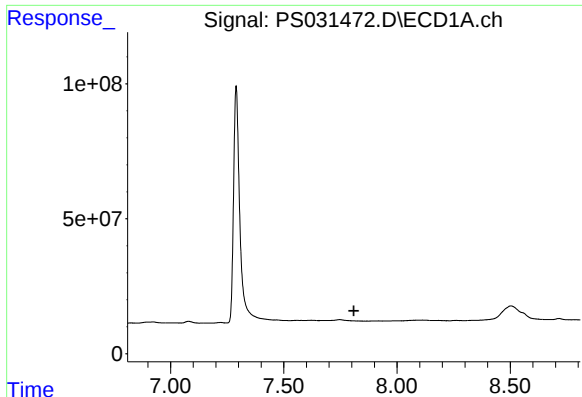

#7 MCPA

R.T.: 0.000 min
Exp R.T.: 7.809 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

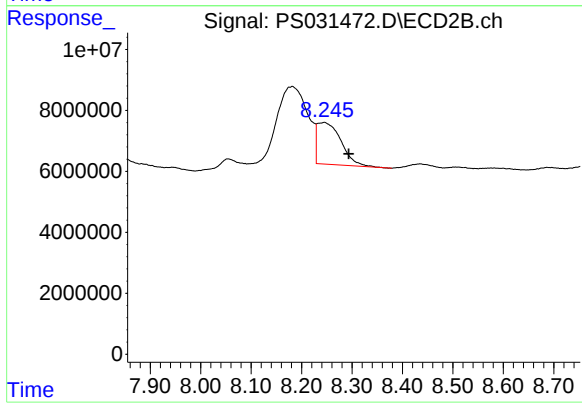

#7 MCPA

R.T.: 8.245 min
Delta R.T.: -0.048 min
Response: 44619155
Conc: 15.90 ug/ml