

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081619\
 Data File : PS006139.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2019 10:08
 Operator : SM\AJ
 Sample : PB121337BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 01:26:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.501	5.224	322.4E6	175.7E6	373.459	357.309
Target Compounds							
6) T	MCP	0.000	5.467	0	285.5E6	N.D.	230.766
9) T	2,4-D	6.510	0.000	620.5E6	0	761.590	N.D. #
15) T	Picloram	9.080	9.011	143.5E6	89349077	19.291	19.808
16) T	DCPA	0.000	9.011	0	89349077	N.D.	25.622



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081619\
Data File : PS006139.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2019 10:08
Operator : SM\AJ
Sample : PB121337BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 01:26:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

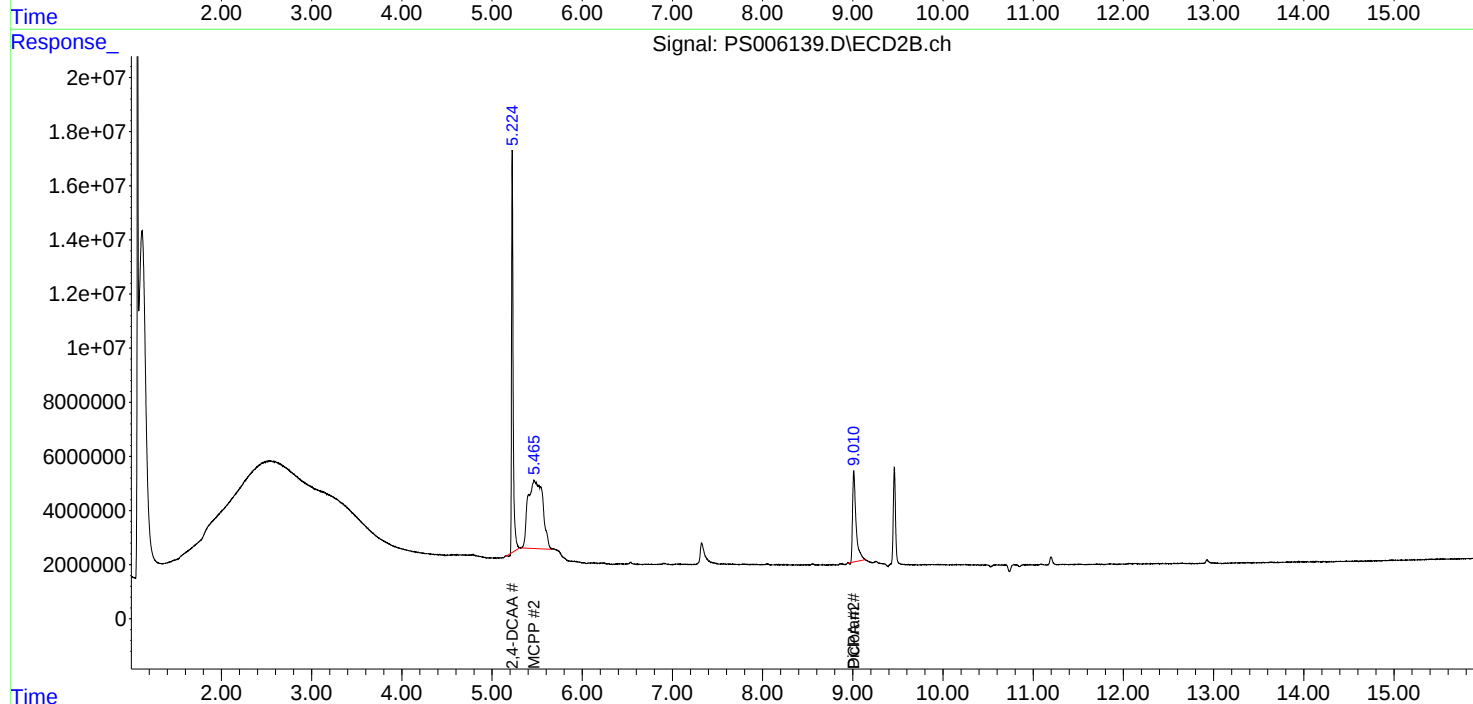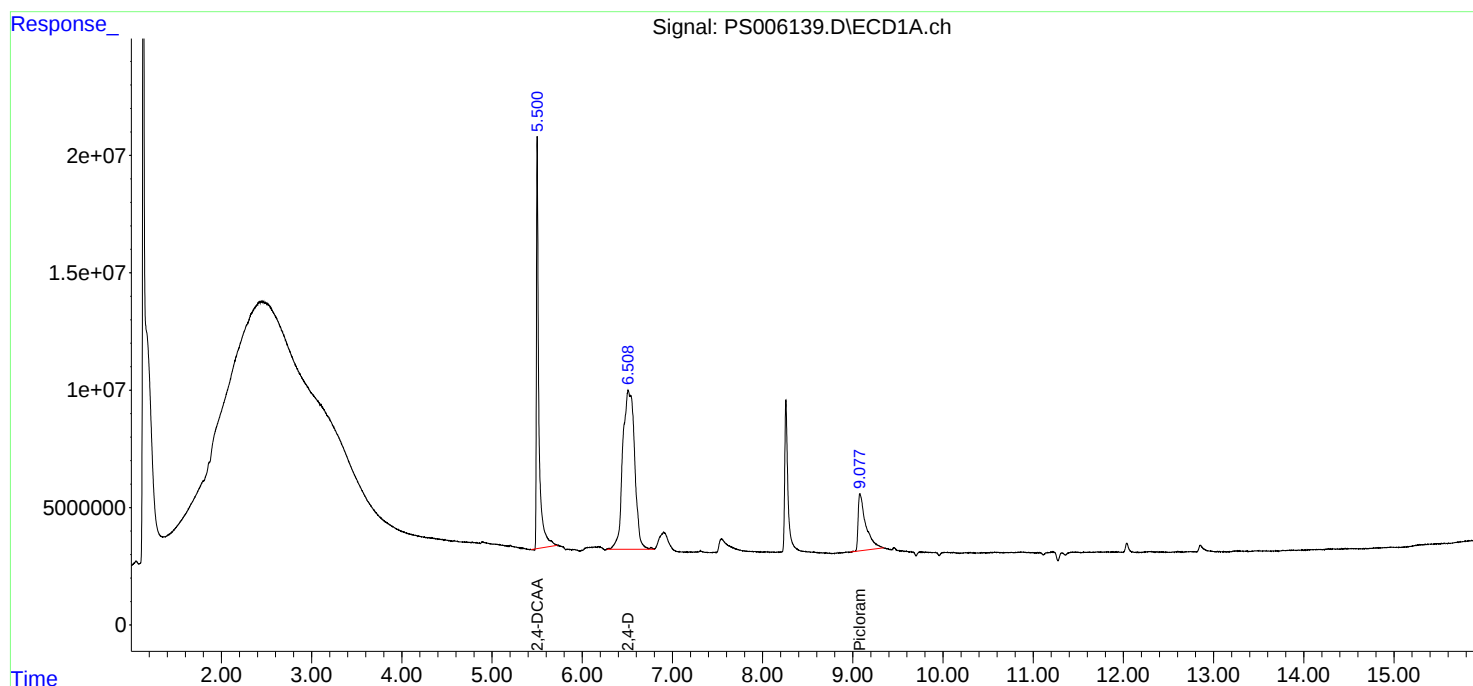


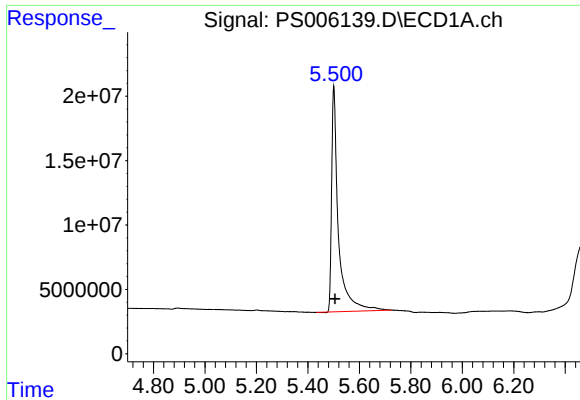

#4 2,4-DCAA


R.T.: 5.501 min
Delta R.T.: -0.004 min
Response: 322369884
Conc: 373.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

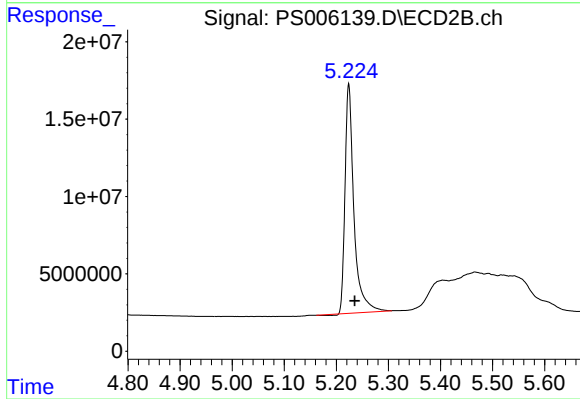


#4 2,4-DCAA

R.T.: 5.224 min
Delta R.T.: -0.012 min
Response: 175742926
Conc: 357.31 ng/ml

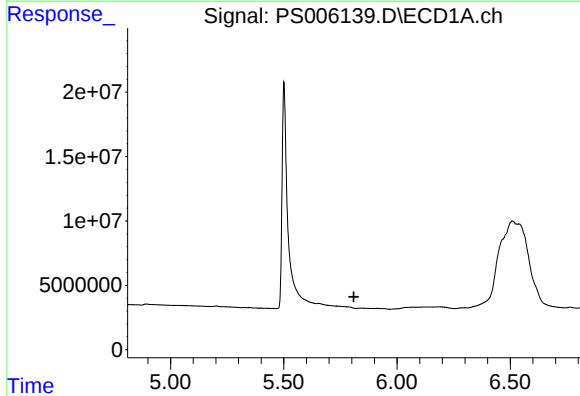


#6 MCP

R.T.: 0.000 min
Exp R.T. : 5.810 min
Response: 0
Conc: N.D.

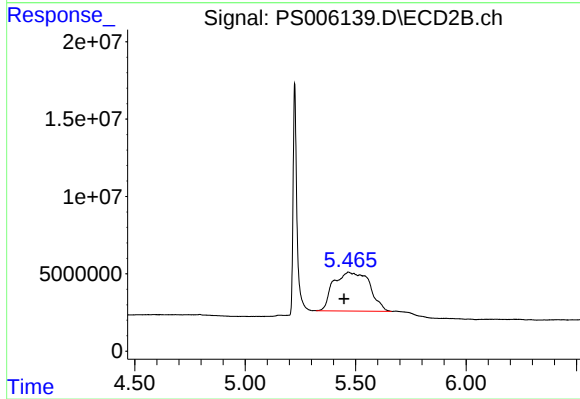

#6 MCP


R.T.: 5.467 min
Delta R.T.: 0.019 min
Response: 285480731
Conc: 230.77 ug/ml

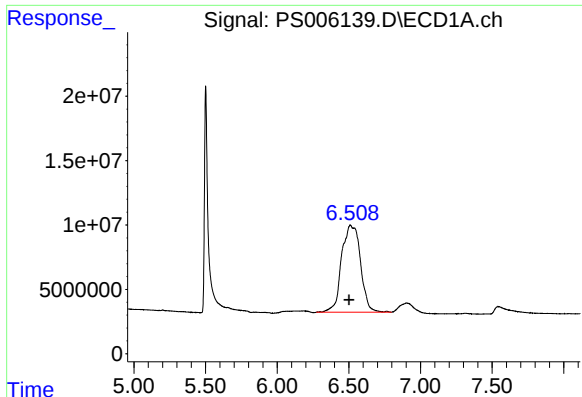

#9 2,4-D


R.T.: 6.510 min
Delta R.T.: 0.007 min
Response: 620531642
Conc: 761.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

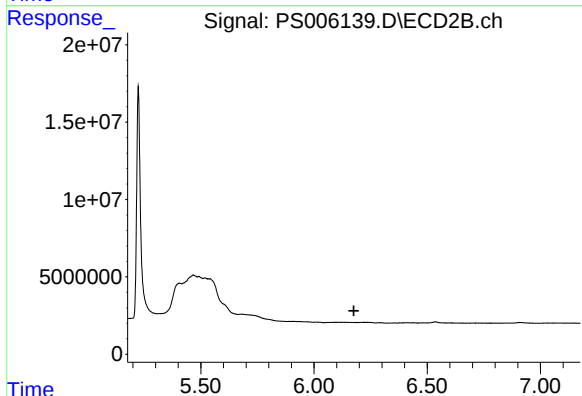


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.

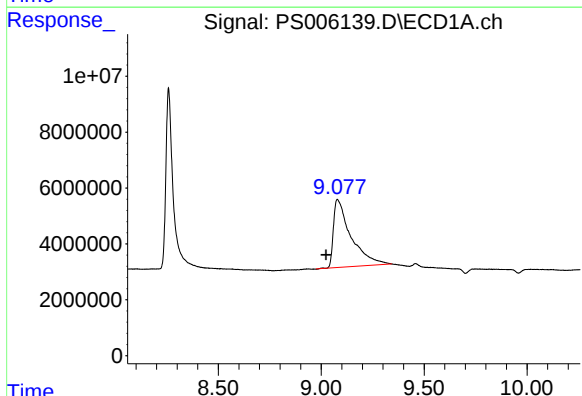


#15 Picloram

R.T.: 9.080 min
Delta R.T.: 0.057 min
Response: 143536415
Conc: 19.29 ng/ml

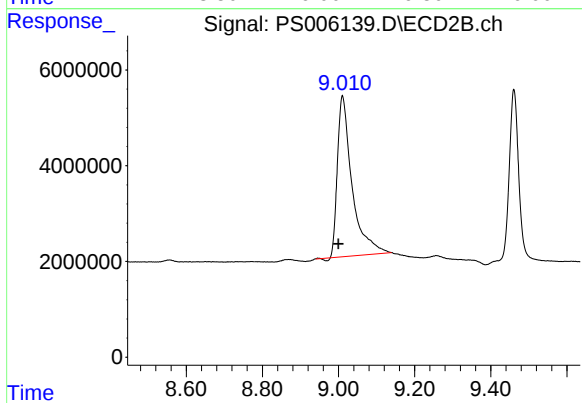

#15 Picloram


R.T.: 9.011 min
Delta R.T.: 0.011 min
Response: 89349077
Conc: 19.81 ng/ml

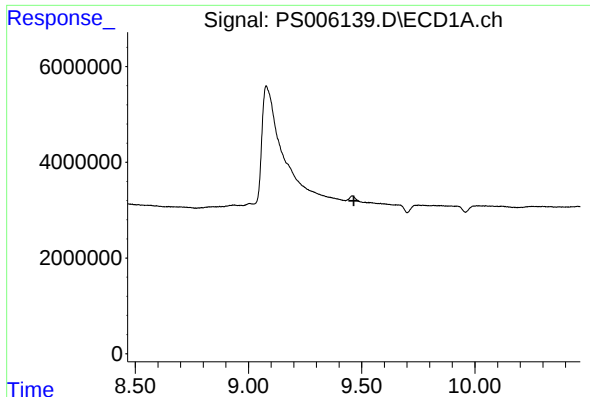

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

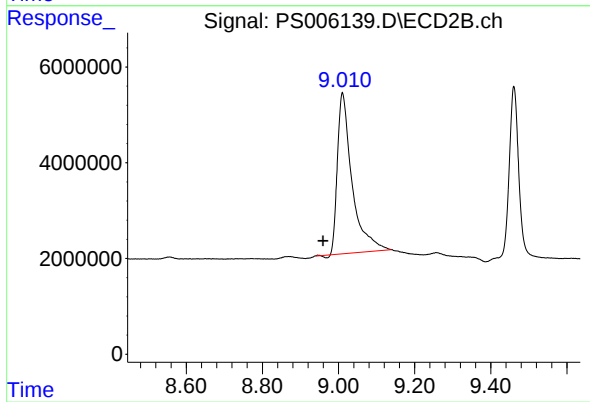

#16 DCPA

R.T.: 9.011 min
Delta R.T.: 0.051 min
Response: 89349077
Conc: 25.62 ng/ml