

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081619\
 Data File : PS006141.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2019 10:53
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 01:27:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.491	5.218	341.1E6	194.5E6	395.196	395.511
Target Compounds							
9) T	2,4-D	6.549	0.000	191.3E6	0	234.750	N.D. #
15) T	Picloram	9.075	9.007	118.9E6	80061268	15.976	17.749
16) T	DCPA	0.000	9.007	0	80061268	N.D.	22.959



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081619\
Data File : PS006141.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2019 10:53
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 01:27:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

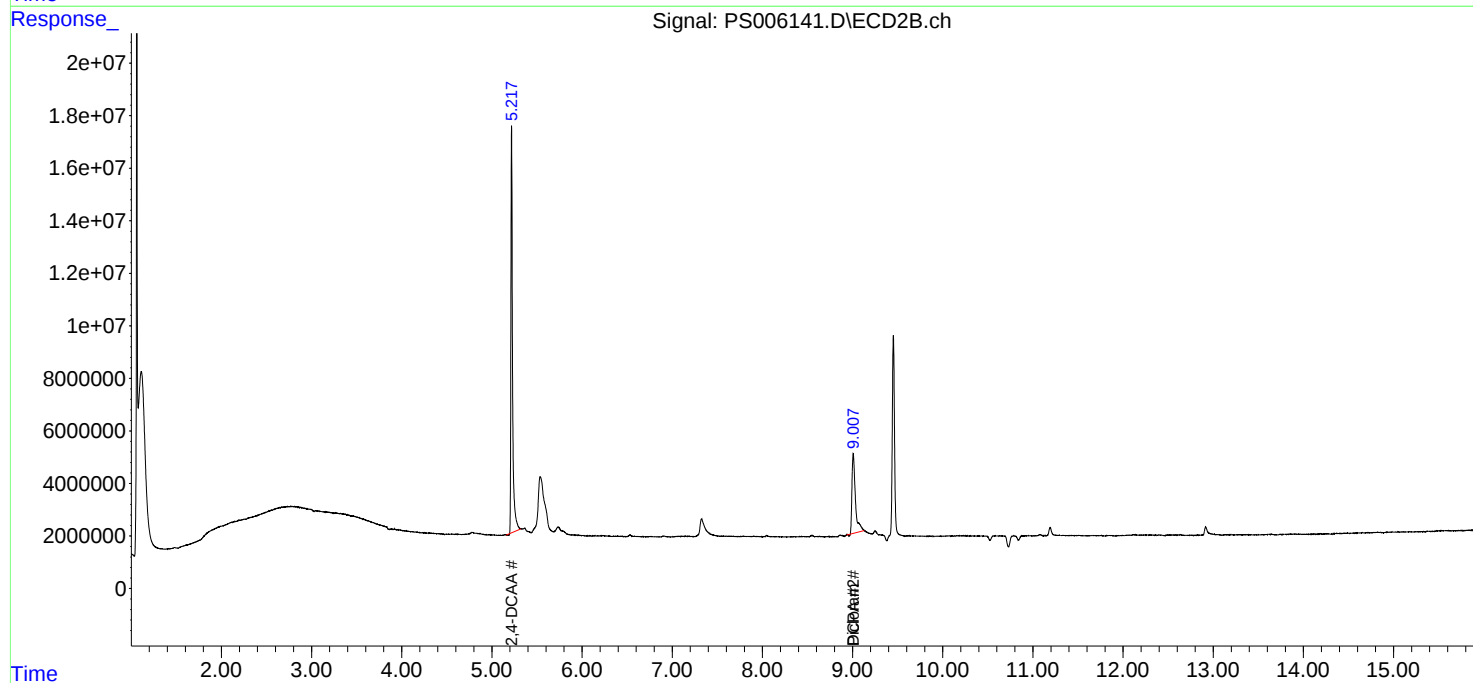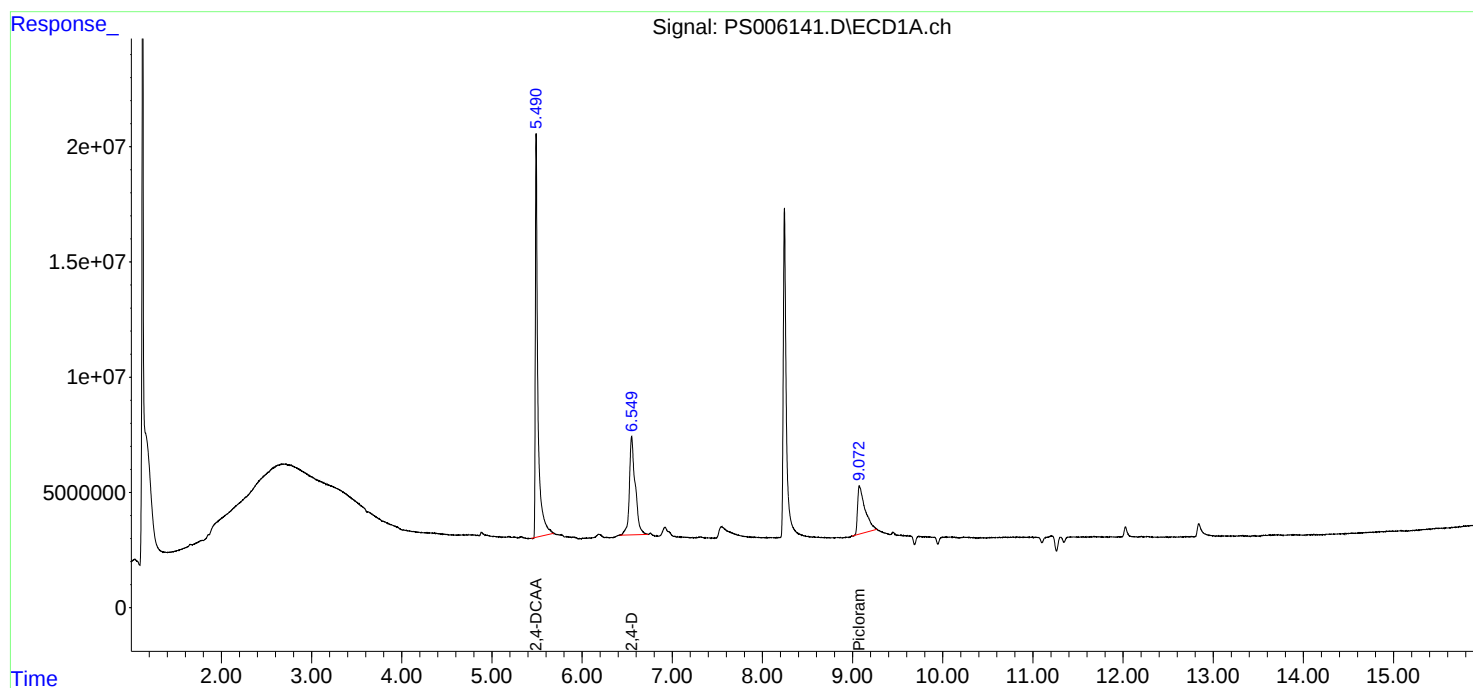


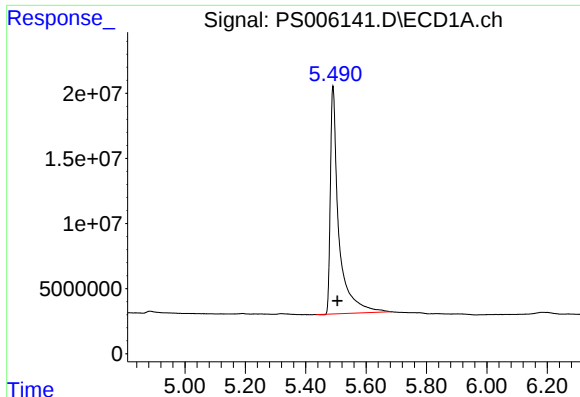

#4 2,4-DCAA


R.T.: 5.491 min
Delta R.T.: -0.015 min
Response: 341133766
Conc: 395.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

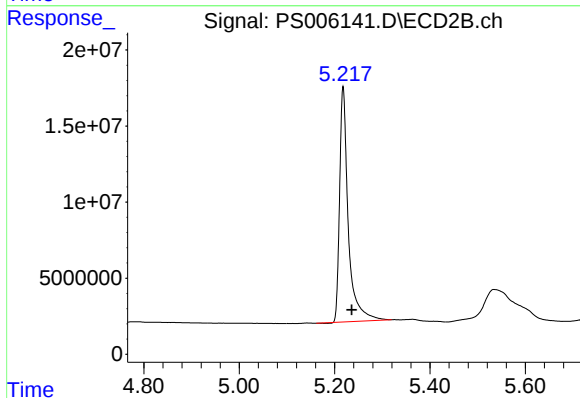


#4 2,4-DCAA

R.T.: 5.218 min
Delta R.T.: -0.018 min
Response: 194532697
Conc: 395.51 ng/ml

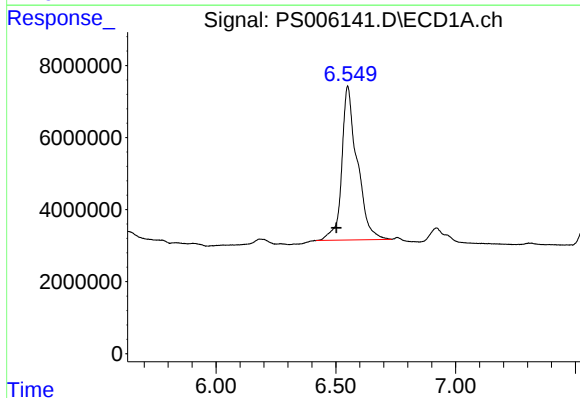


#9 2,4-D

R.T.: 6.549 min
Delta R.T.: 0.047 min
Response: 191270626
Conc: 234.75 ng/ml

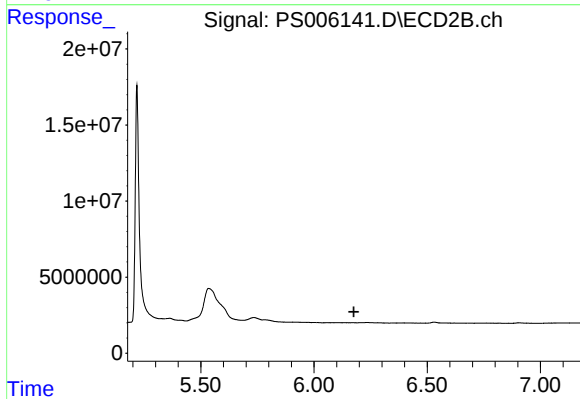

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.176 min
Response: 0
Conc: N.D.

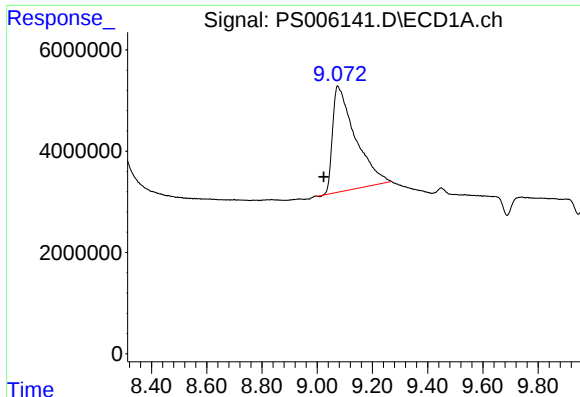

#15 Picloram


R.T.: 9.075 min
Delta R.T.: 0.051 min
Response: 118870999
Conc: 15.98 ng/ml

Instrument :
ECD_S
ClientSampleId :

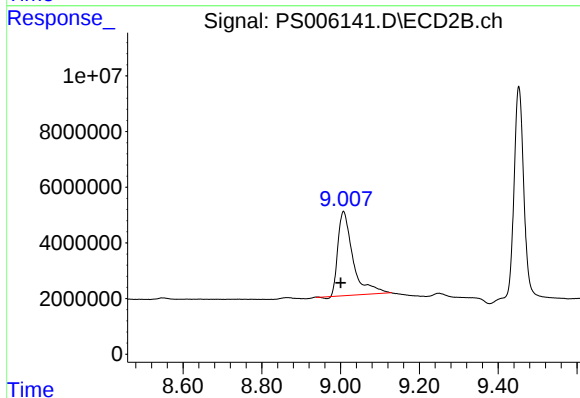


#15 Picloram

R.T.: 9.007 min
Delta R.T.: 0.007 min
Response: 80061268
Conc: 17.75 ng/ml

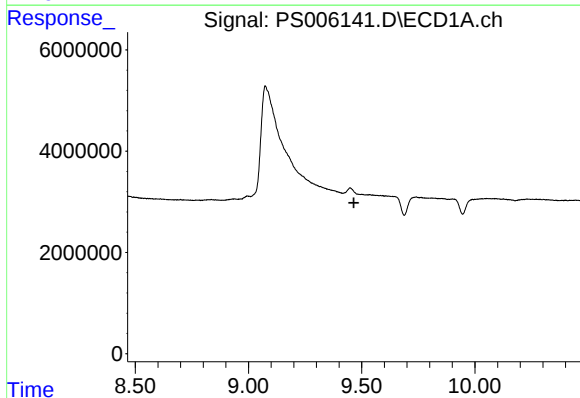

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 9.465 min
Response: 0
Conc: N.D.

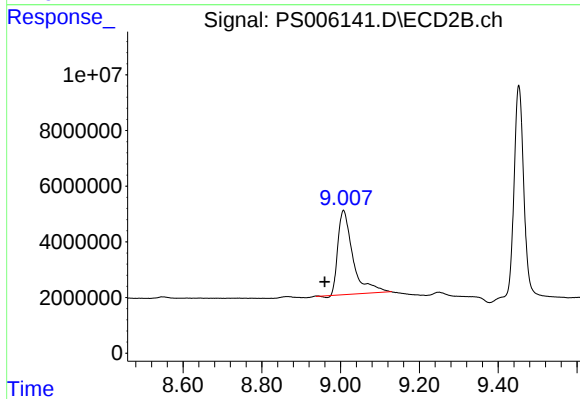

#16 DCPA

R.T.: 9.007 min
Delta R.T.: 0.048 min
Response: 80061268
Conc: 22.96 ng/ml