

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081619\
 Data File : PS006143.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2019 11:37
 Operator : SM\AJ
 Sample : PB122311BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 01:28:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.488	5.218	410.6E6	261.8E6	475.641	532.250
Target Compounds							
1) T	Dalapon	2.117	1.743	2292692	64460741	2.104	102.727 #
2) T	3,5-DICHL...	0.000	4.546	0	42193268	N.D.	69.660
3) T	4-Nitroph...	5.298	0.000	5654196	0	15.061	N.D. #
7) T	MCPA	5.963	5.595	20851446	30226197	6.605	14.790 #
9) T	2,4-D	6.551	0.000	184.0E6	0	225.851	N.D. #
12) T	2,4,5-T	0.000	7.309	0	50640327	N.D.	20.370
15) T	Picloram	9.052	9.000	186.7E6	137.0E6	25.094	30.374
16) T	DCPA	0.000	9.000	0	137.0E6	N.D.	39.290



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081619\
Data File : PS006143.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2019 11:37
Operator : SM\AJ
Sample : PB122311BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 01:28:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

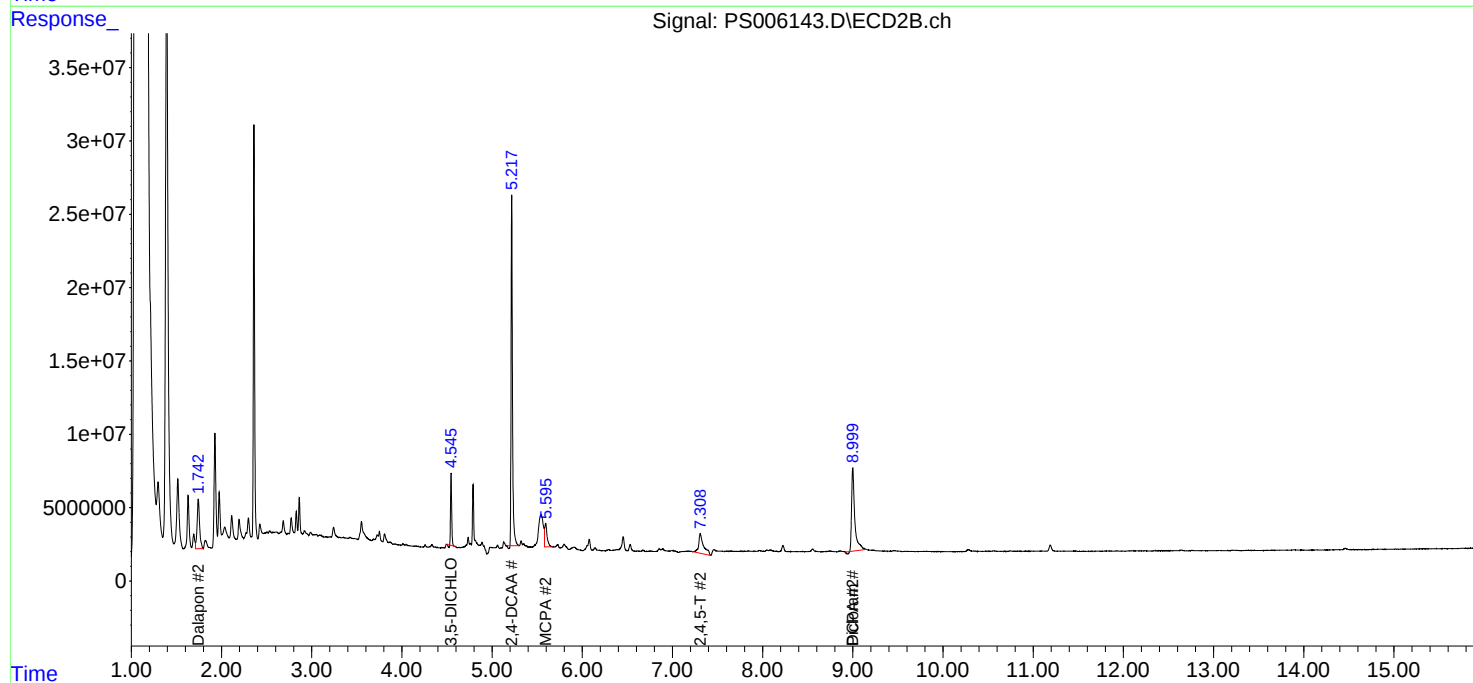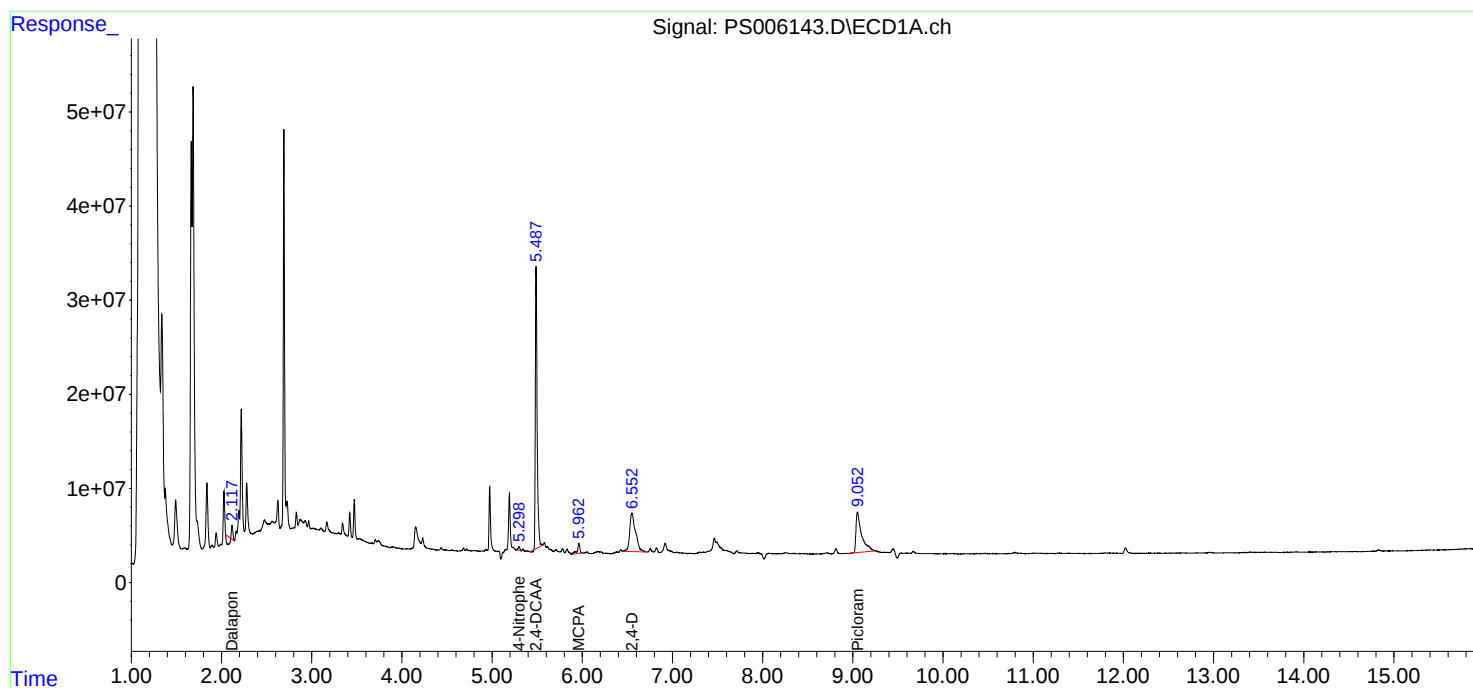


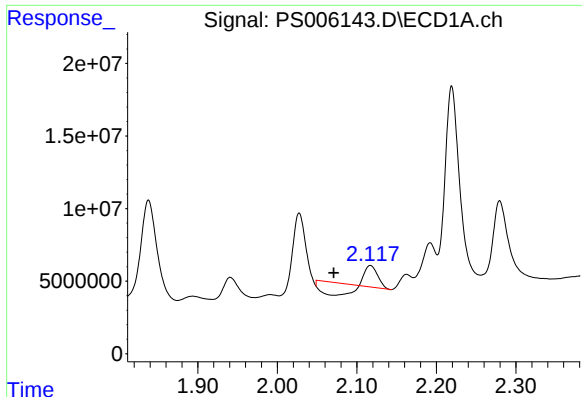

#1 Dalapon


R.T.: 2.117 min
Delta R.T.: 0.046 min
Response: 2292692
Conc: 2.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

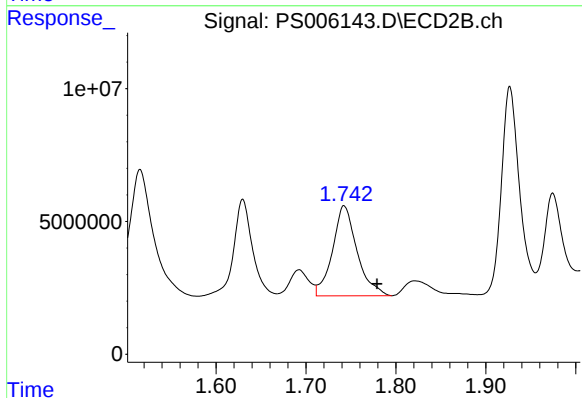


#1 Dalapon

R.T.: 1.743 min
Delta R.T.: -0.036 min
Response: 64460741
Conc: 102.73 ng/ml

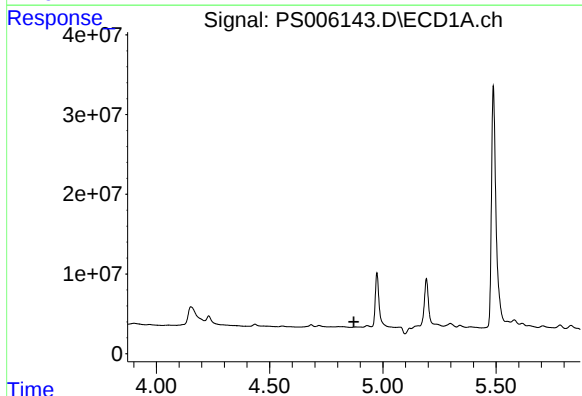


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.872 min
Response: 0
Conc: N.D.

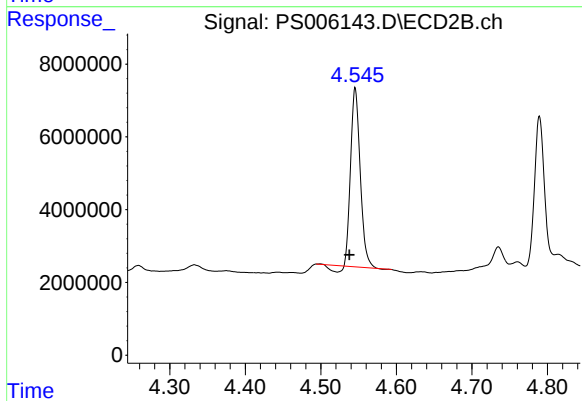

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.546 min
Delta R.T.: 0.008 min
Response: 42193268
Conc: 69.66 ng/ml

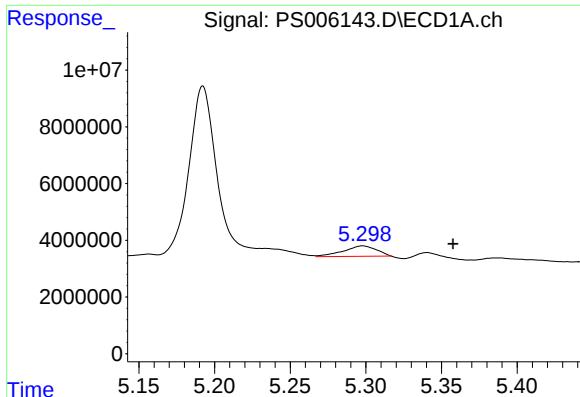

#3 4-Nitrophenol


R.T.: 5.298 min
Delta R.T.: -0.060 min
Response: 5654196
Conc: 15.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

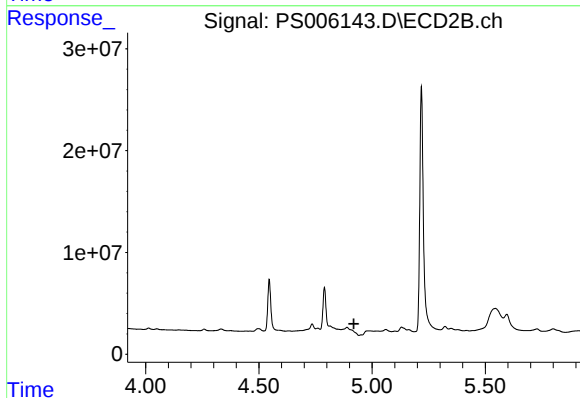


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 4.920 min
Response: 0
Conc: N.D.

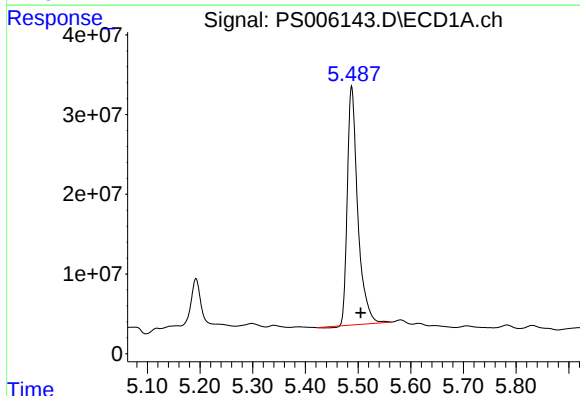


#4 2,4-DCAA

R.T.: 5.488 min
Delta R.T.: -0.017 min
Response: 410574072
Conc: 475.64 ng/ml

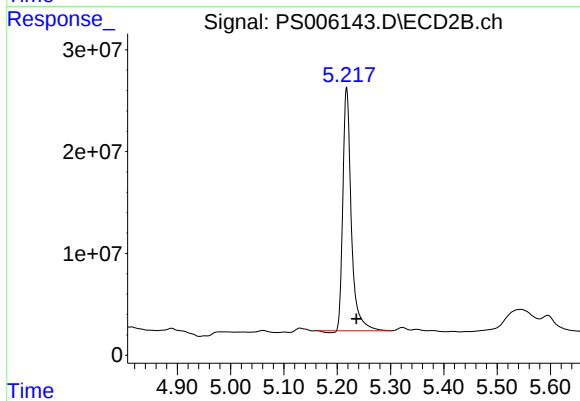

#4 2,4-DCAA


R.T.: 5.218 min
Delta R.T.: -0.018 min
Response: 261788160
Conc: 532.25 ng/ml

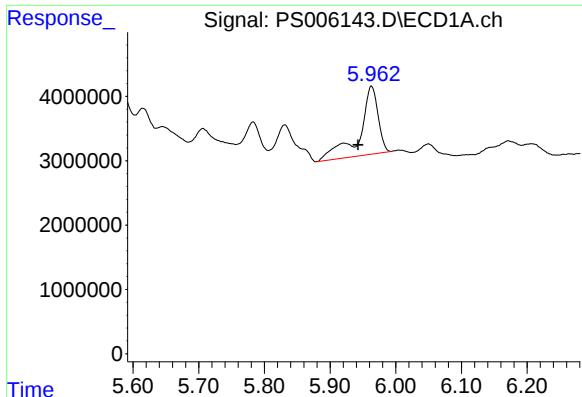

#7 MCPA


R.T.: 5.963 min
Delta R.T.: 0.021 min
Response: 20851446
Conc: 6.60 ug/ml

Instrument :
ECD_S
ClientSampleId :

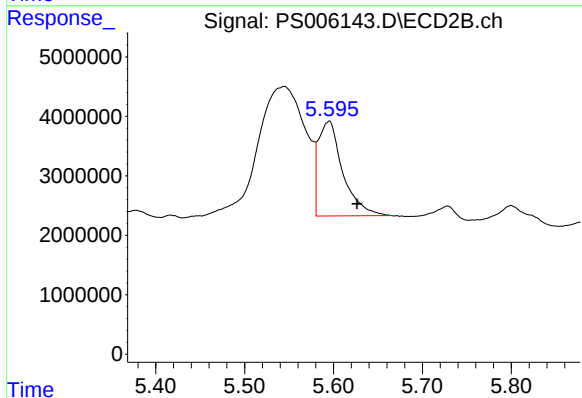


#7 MCPA

R.T.: 5.595 min
Delta R.T.: -0.032 min
Response: 30226197
Conc: 14.79 ug/ml

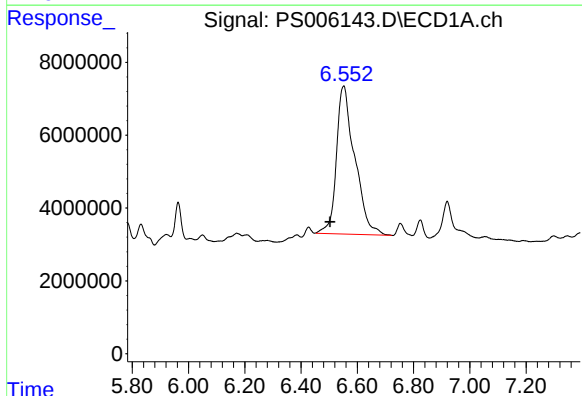


#9 2,4-D

R.T.: 6.551 min
Delta R.T.: 0.048 min
Response: 184019573
Conc: 225.85 ng/ml

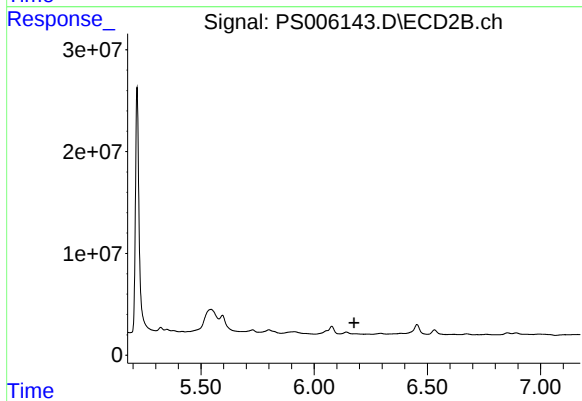

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.176 min
Response: 0
Conc: N.D.

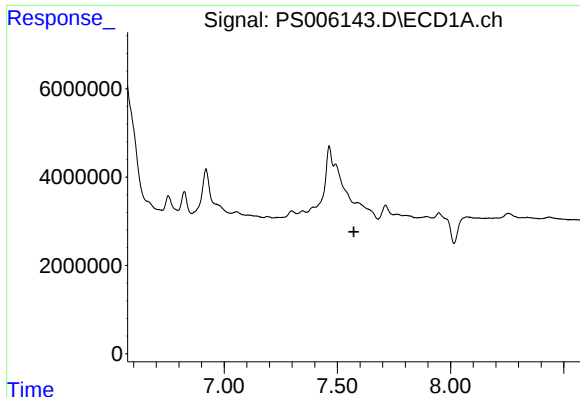

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 7.573 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

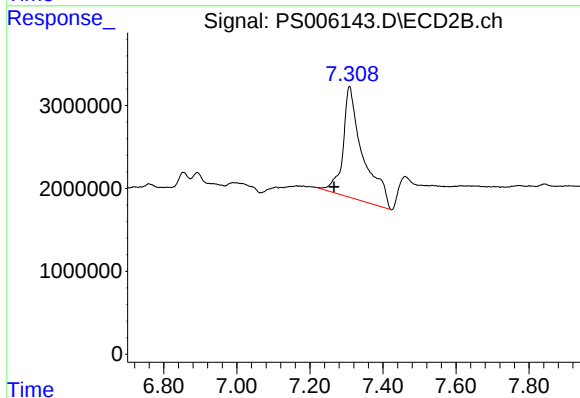


#12 2,4,5-T

R.T.: 7.309 min
Delta R.T.: 0.042 min
Response: 50640327
Conc: 20.37 ng/ml

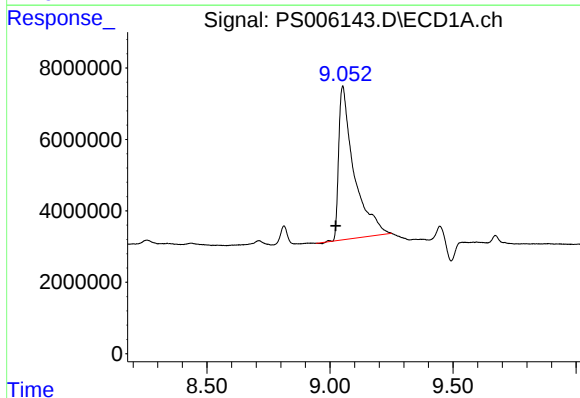


#15 Picloram

R.T.: 9.052 min
Delta R.T.: 0.028 min
Response: 186717871
Conc: 25.09 ng/ml

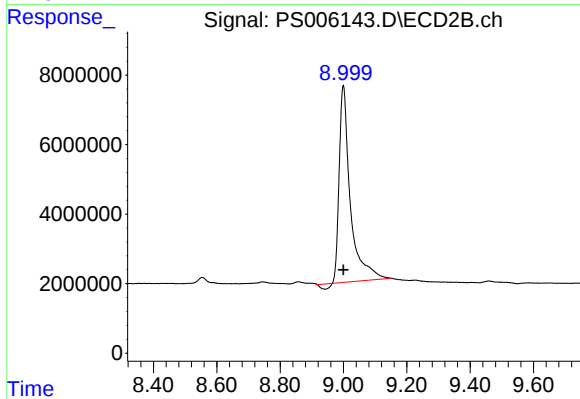

#15 Picloram


R.T.: 9.000 min
Delta R.T.: 0.000 min
Response: 137011877
Conc: 30.37 ng/ml

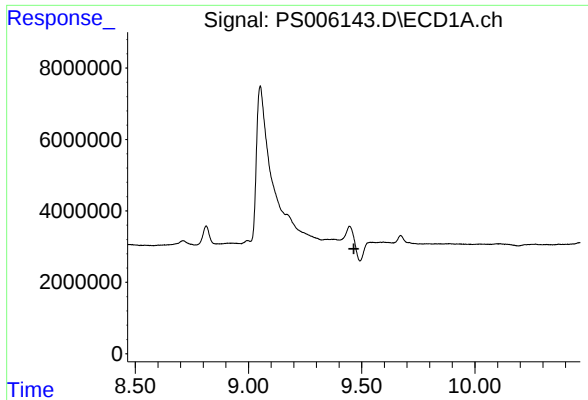

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 9.465 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

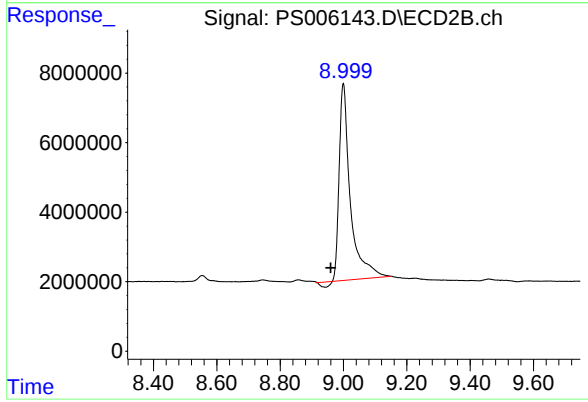

#16 DCPA

R.T.: 9.000 min
Delta R.T.: 0.040 min
Response: 137011877
Conc: 39.29 ng/ml