

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081619\
 Data File : PS006181.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2019 01:37
 Operator : SM\AJ
 Sample : K4321-05
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 02:12:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.515	5.246	228.2E6	136.4E6	264.348	277.228
Target Compounds							
1) T	Dalapon	2.057	1.772	65957893	217.0E6	60.533	345.877 #
2) T	3,5-DICHL...	4.898	4.574	79394455	57278514	73.641	94.565 #
5) T	DICAMBA	5.609	5.388	22615025	58006666	7.042	31.448 #
6) T	MCP	0.000	5.388	0	58006666	N.D.	46.889
7) T	MCPA	5.991	5.623	10969987	32437030	3.475	15.872 #
8) T	DICHLORPROP	6.345	0.000	68575080	0	90.424	N.D. #
9) T	2,4-D	6.537	0.000	95096884	0	116.714	N.D. #
10) T	Pentachlo...	0.000	6.482	0	45860628	N.D.	6.784
13) T	2,4-DB	8.127	0.000	29467878	0	47.316	N.D. #
14) T	DINOSEB	0.000	8.098	0	17298004	N.D.	9.006
15) T	Picloram	9.061	0.000	22595540	0	3.037	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081619\
Data File : PS006181.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2019 01:37
Operator : SM\AJ
Sample : K4321-05
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 02:12:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

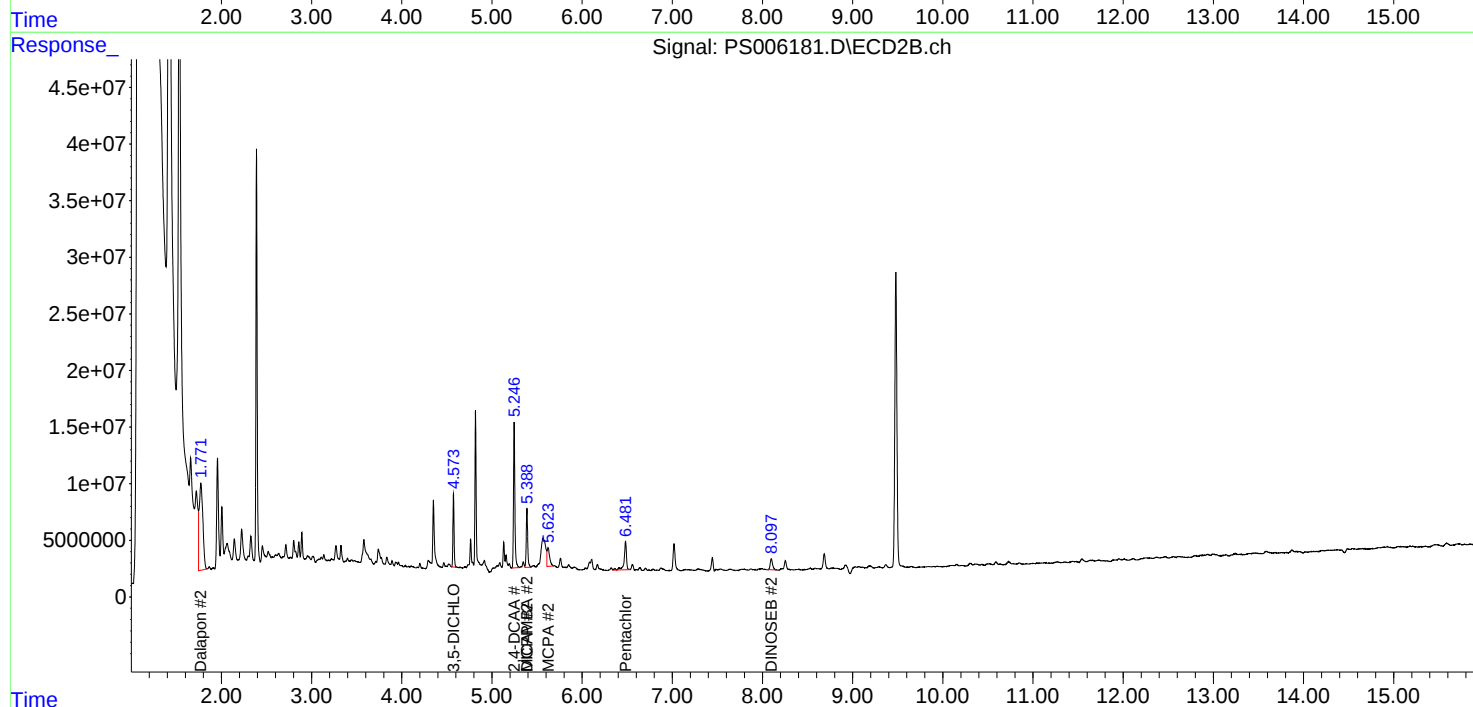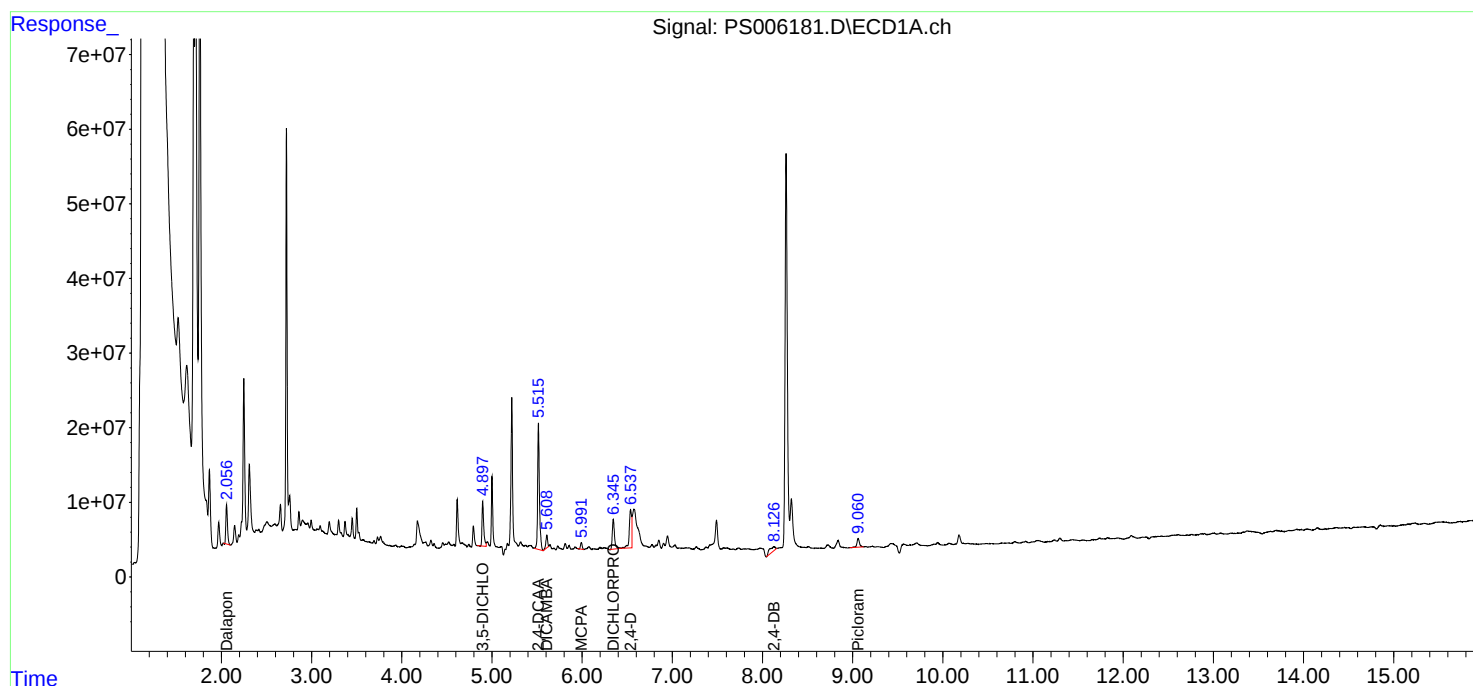


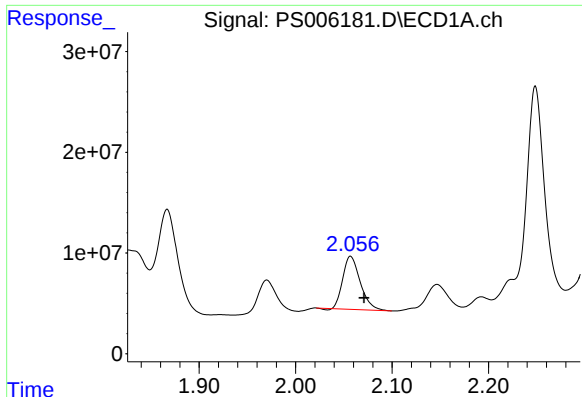

#1 Dalapon


R.T.: 2.057 min
Delta R.T.: -0.014 min
Response: 65957893
Conc: 60.53 ng/ml

Instrument :
ECD_S
ClientSampleId :

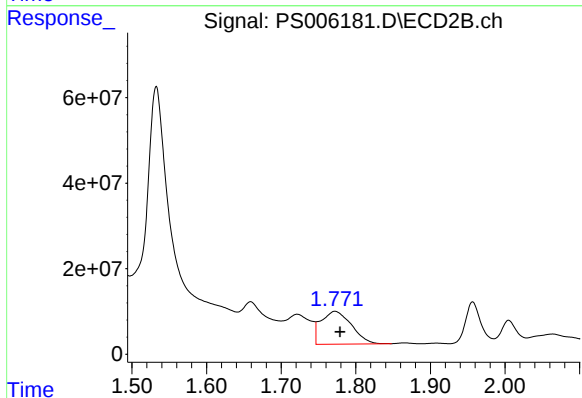


#1 Dalapon

R.T.: 1.772 min
Delta R.T.: -0.007 min
Response: 217035255
Conc: 345.88 ng/ml

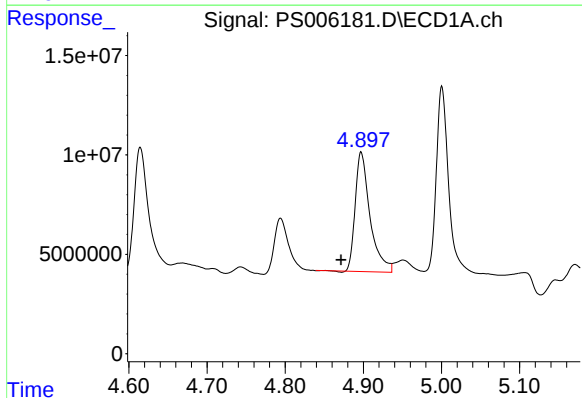


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 4.898 min
Delta R.T.: 0.026 min
Response: 79394455
Conc: 73.64 ng/ml

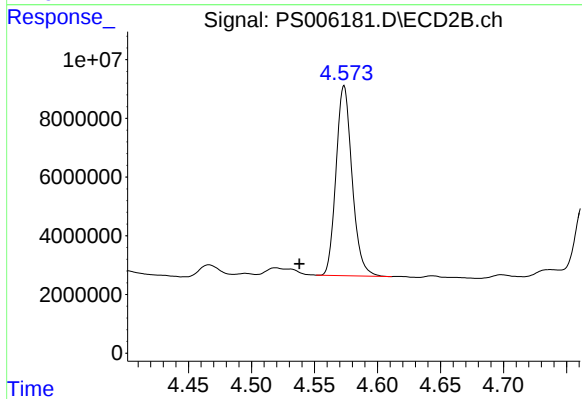

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.574 min
Delta R.T.: 0.036 min
Response: 57278514
Conc: 94.56 ng/ml

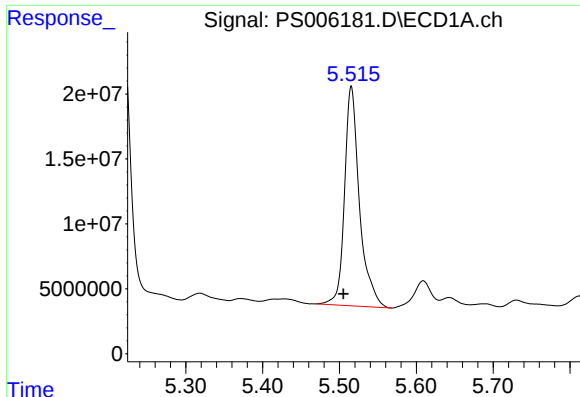

#4 2,4-DCAA


R.T.: 5.515 min
Delta R.T.: 0.010 min
Response: 228185698
Conc: 264.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

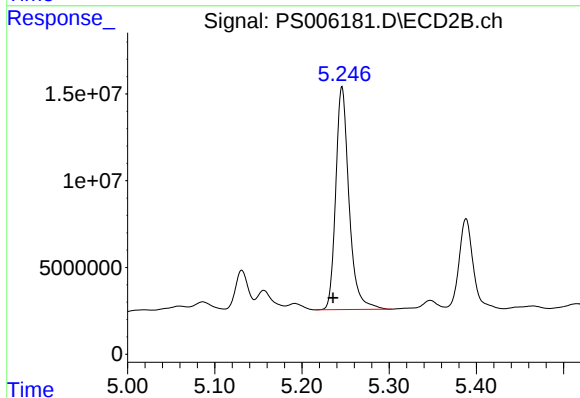


#4 2,4-DCAA

R.T.: 5.246 min
Delta R.T.: 0.010 min
Response: 136354882
Conc: 277.23 ng/ml

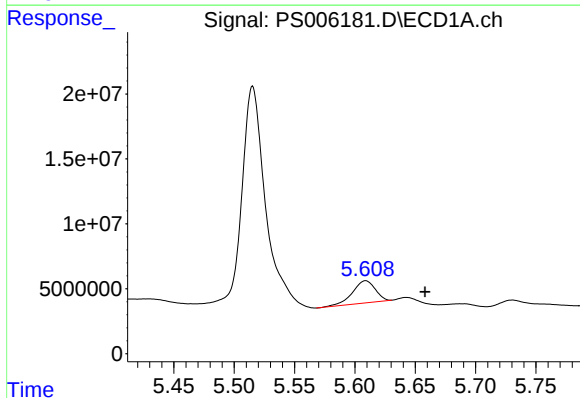


#5 DICAMBA

R.T.: 5.609 min
Delta R.T.: -0.049 min
Response: 22615025
Conc: 7.04 ng/ml

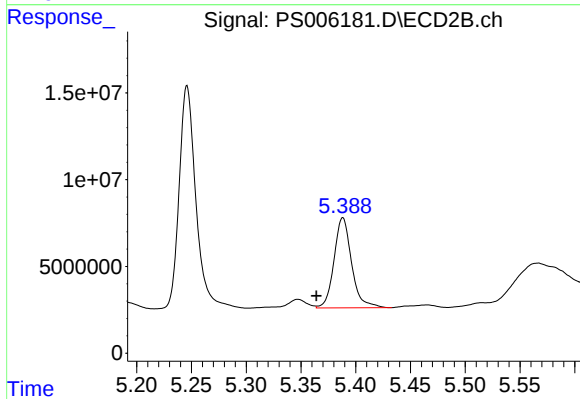

#5 DICAMBA


R.T.: 5.388 min
Delta R.T.: 0.024 min
Response: 58006666
Conc: 31.45 ng/ml

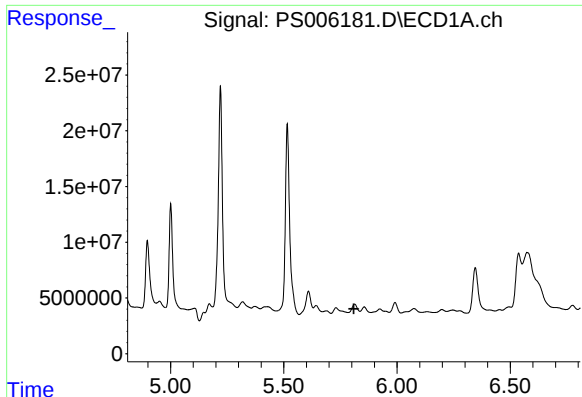

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 5.810 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

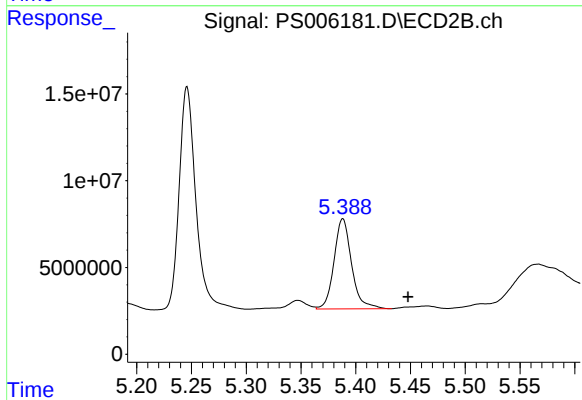


#6 MCPP

R.T.: 5.388 min
Delta R.T.: -0.060 min
Response: 58006666
Conc: 46.89 ug/ml

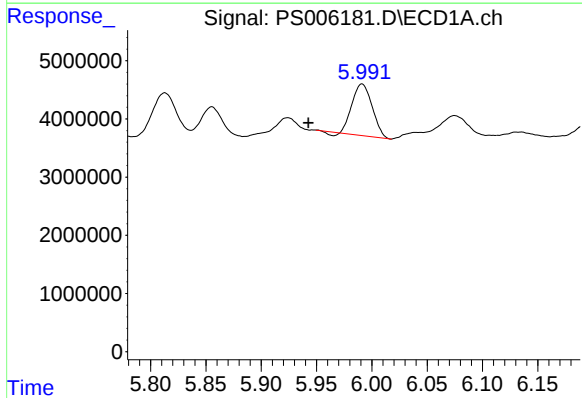


#7 MCPA

R.T.: 5.991 min
Delta R.T.: 0.048 min
Response: 10969987
Conc: 3.47 ug/ml

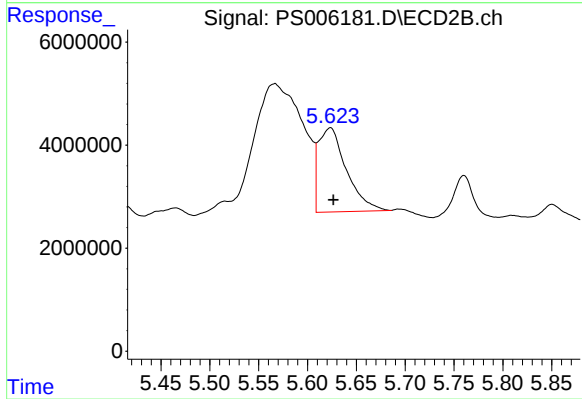

#7 MCPA


R.T.: 5.623 min
Delta R.T.: -0.003 min
Response: 32437030
Conc: 15.87 ug/ml

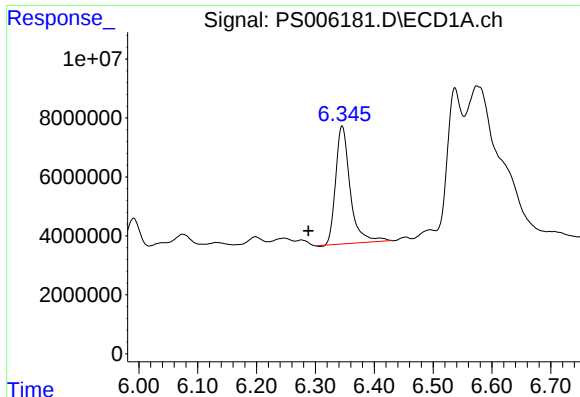

#8 DICHLORPROP


R.T.: 6.345 min
Delta R.T.: 0.058 min
Response: 68575080
Conc: 90.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

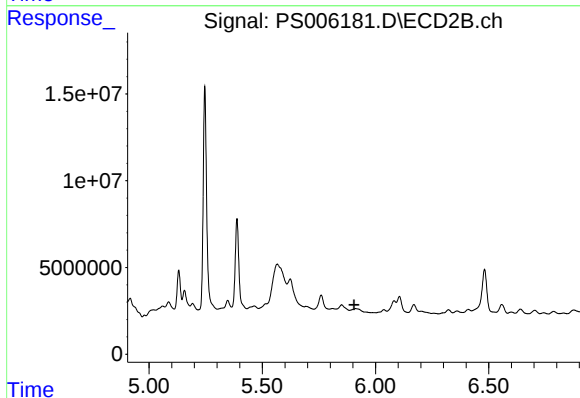


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 5.905 min
Response: 0
Conc: N.D.

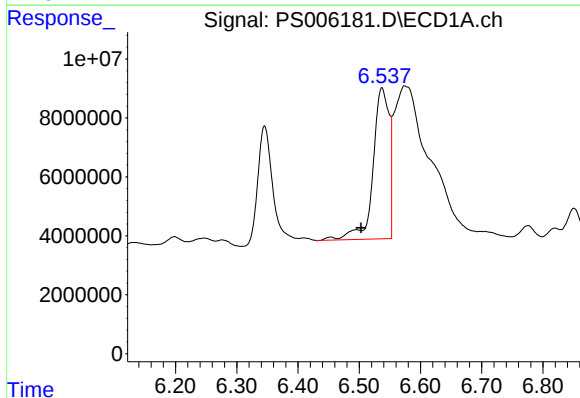


#9 2,4-D

R.T.: 6.537 min
Delta R.T.: 0.034 min
Response: 95096884
Conc: 116.71 ng/ml

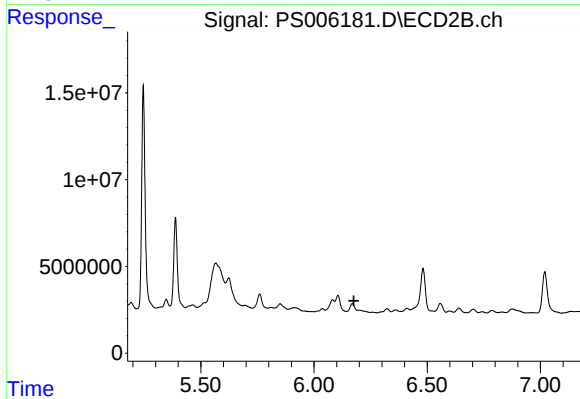

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 6.176 min
Response: 0
Conc: N.D.

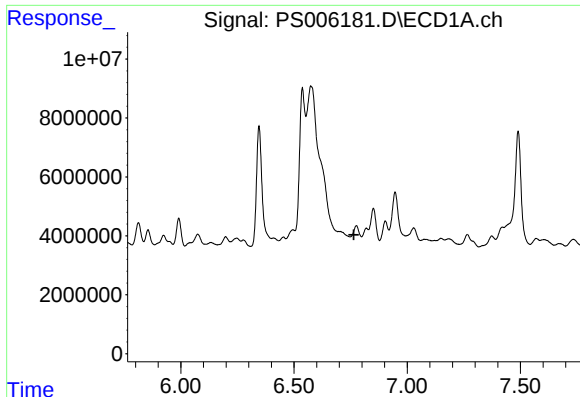

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.764 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

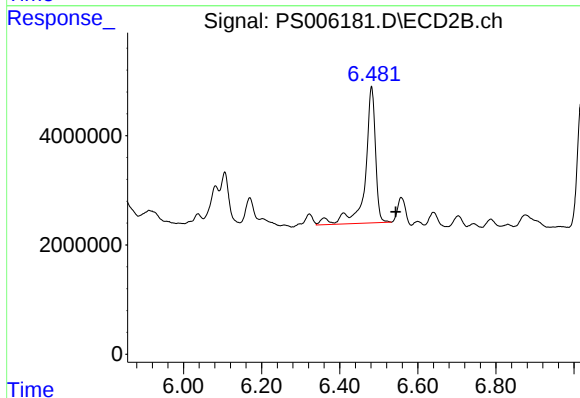


#10 Pentachlorophenol

R.T.: 6.482 min
Delta R.T.: -0.062 min
Response: 45860628
Conc: 6.78 ng/ml

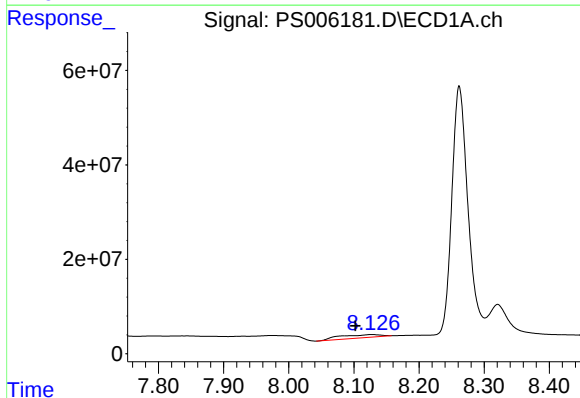


#13 2,4-DB

R.T.: 8.127 min
Delta R.T.: 0.025 min
Response: 29467878
Conc: 47.32 ng/ml

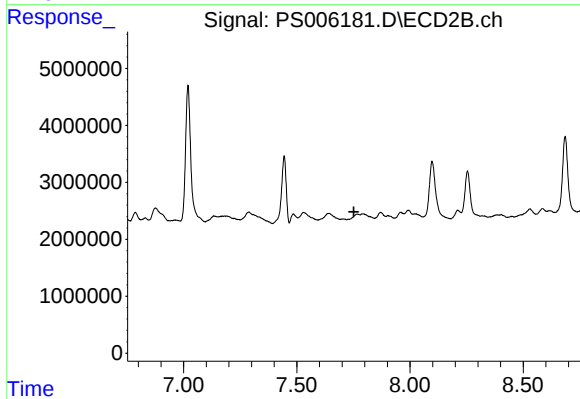

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 7.752 min
Response: 0
Conc: N.D.

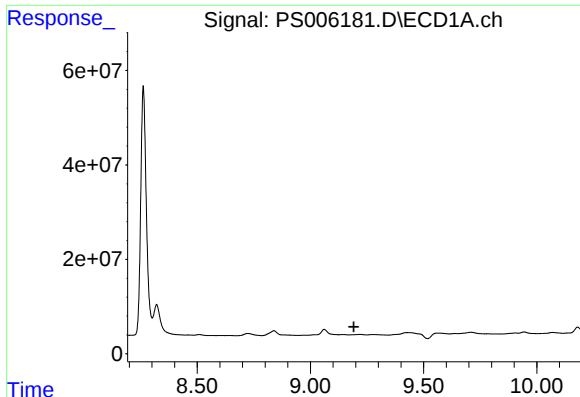

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 9.192 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

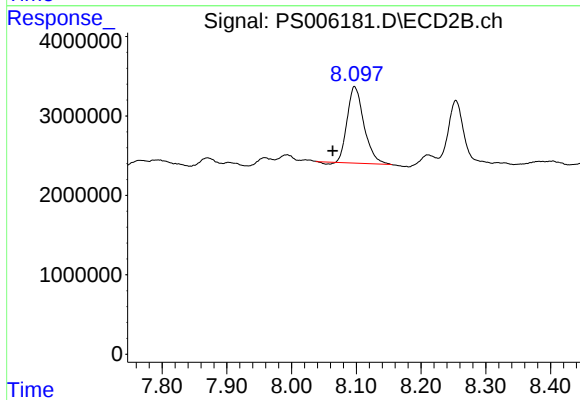


#14 DINOSEB

R.T.: 8.098 min
Delta R.T.: 0.034 min
Response: 17298004
Conc: 9.01 ng/ml

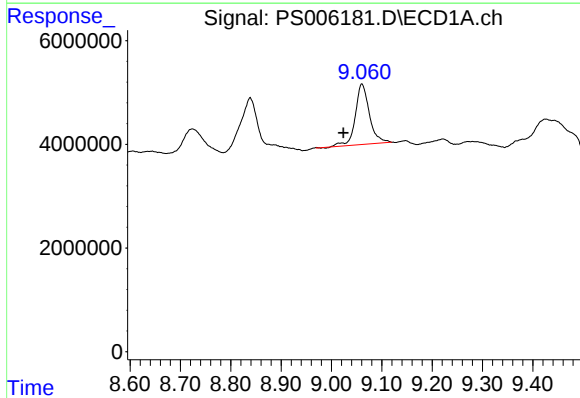

#15 Picloram

R.T.: 9.061 min
Delta R.T.: 0.037 min
Response: 22595540
Conc: 3.04 ng/ml

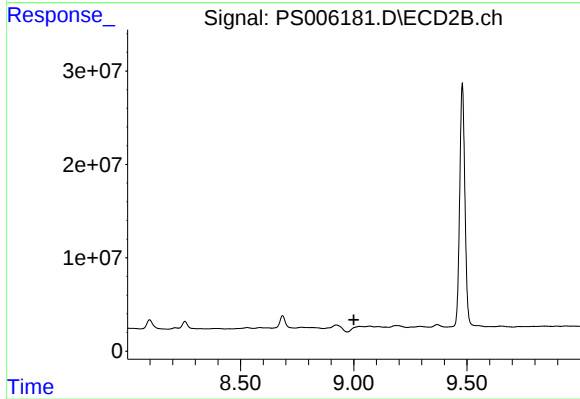

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 9.000 min
Response: 0
Conc: N.D.