

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081619\
 Data File : PS006183.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Aug 2019 02:22
 Operator : SM\AJ
 Sample : K4355-01
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 03:13:32 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
 Quant Title : 8080.M
 QLast Update : Wed Aug 14 15:09:52 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.509	5.247	101.7E6	60002906	117.828	121.994
Target Compounds							
1) T	Dalapon	2.052	1.771	69043057	205.2E6	63.364	327.076 #
5) T	DICAMBA	5.604	0.000	16146087	0	5.027	N.D. #
6) T	MCPD	0.000	5.465	0	16254476	N.D.	13.139
7) T	MCPA	5.985	5.621	16831065	31443205	5.331	15.385 #
10) T	Pentachlo...	6.769	6.554	837.8E6	482.2E6	70.876	71.325
13) T	2,4-DB	8.114	0.000	33244174	0	53.380	N.D. #
14) T	DINOSEB	0.000	8.102	0	35812323	N.D.	18.644
15) T	Picloram	8.964	0.000	22988618	0	3.090	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081619\
Data File : PS006183.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Aug 2019 02:22
Operator : SM\AJ
Sample : K4355-01
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 03:13:32 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS081419.M
Quant Title : 8080.M
QLast Update : Wed Aug 14 15:09:52 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

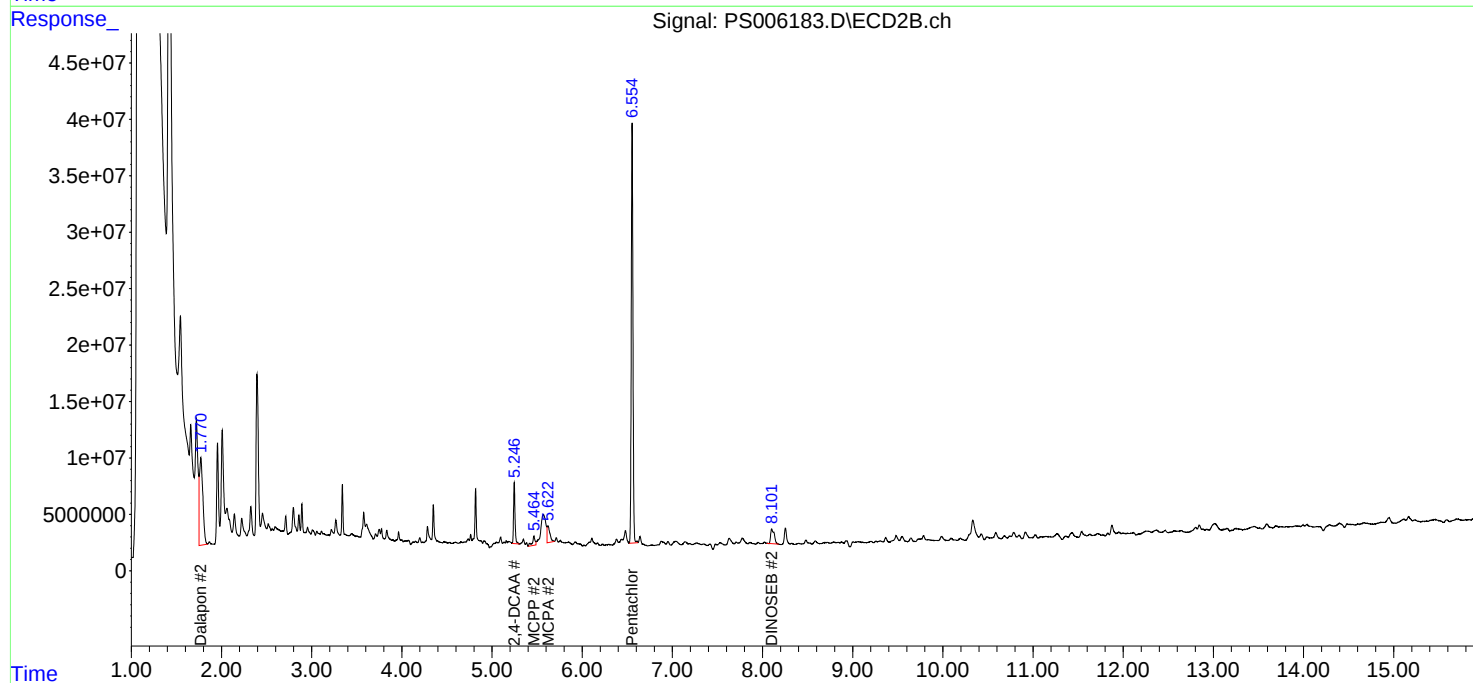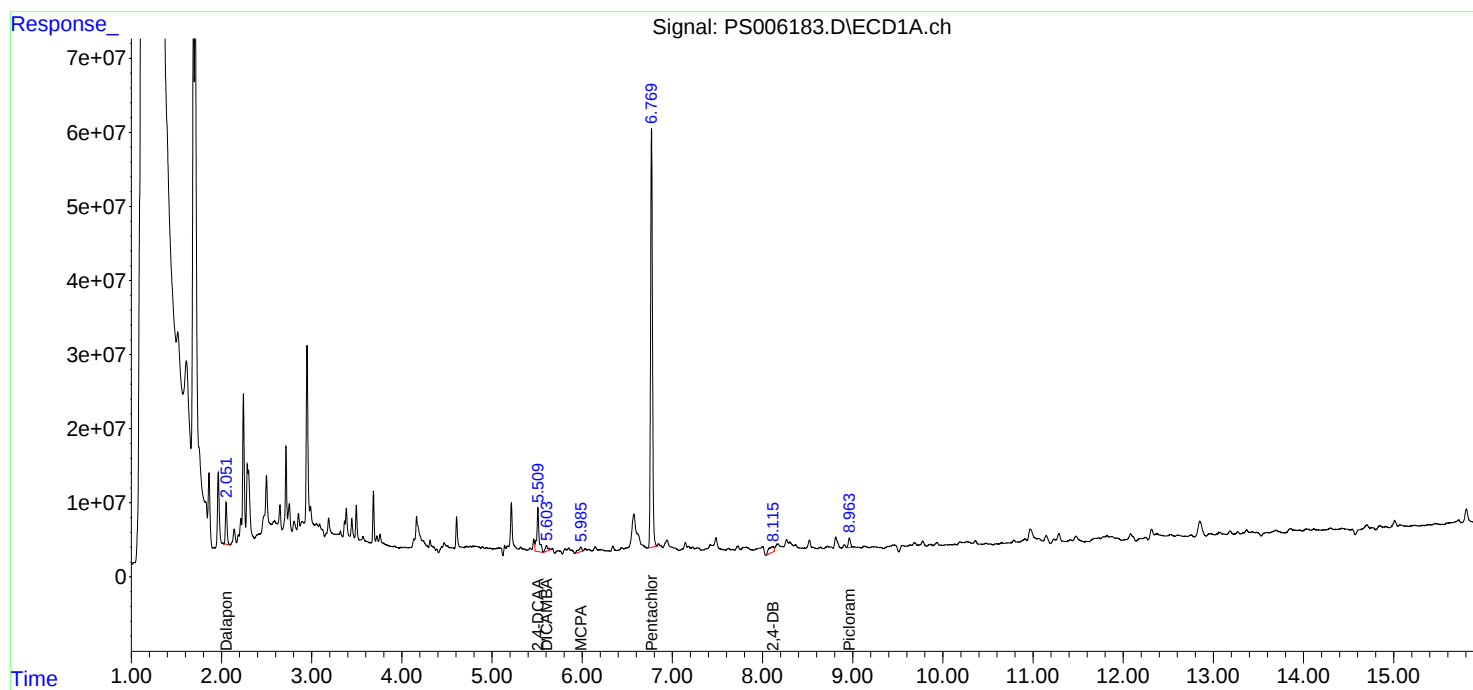


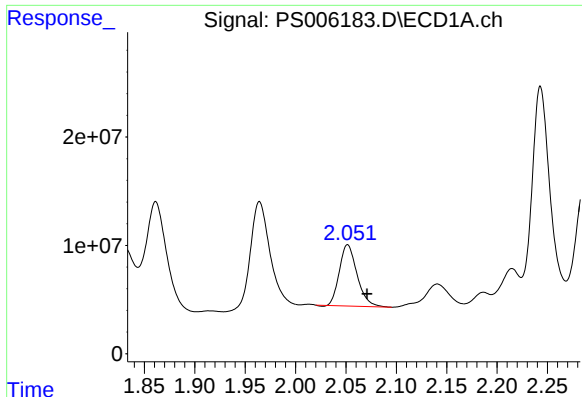

#1 Dalapon


R.T.: 2.052 min
Delta R.T.: -0.019 min
Response: 69043057
Conc: 63.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

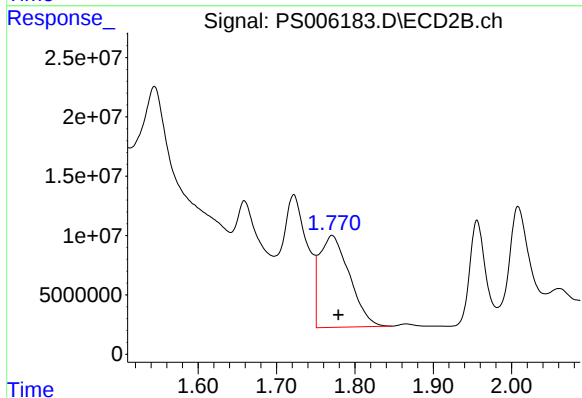


#1 Dalapon

R.T.: 1.771 min
Delta R.T.: -0.008 min
Response: 205237962
Conc: 327.08 ng/ml

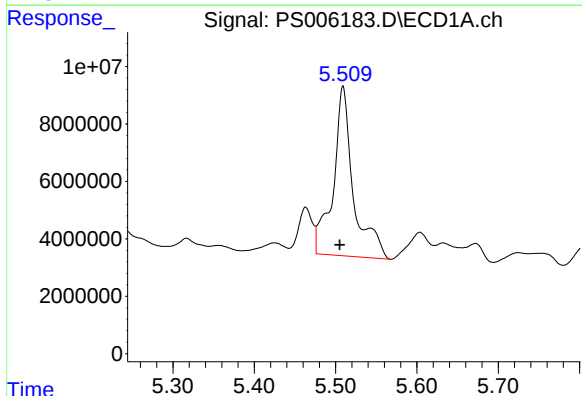


#4 2,4-DCAA

R.T.: 5.509 min
Delta R.T.: 0.004 min
Response: 101708986
Conc: 117.83 ng/ml

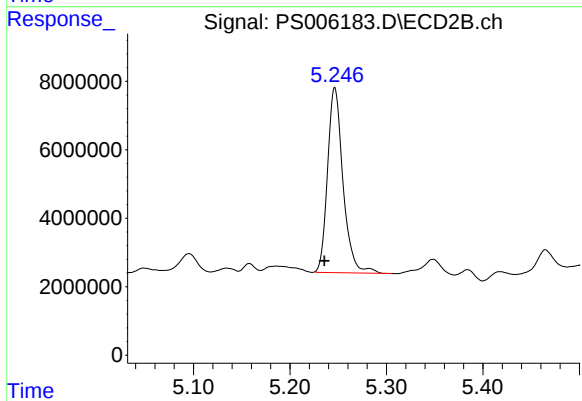

#4 2,4-DCAA


R.T.: 5.247 min
Delta R.T.: 0.011 min
Response: 60002906
Conc: 121.99 ng/ml

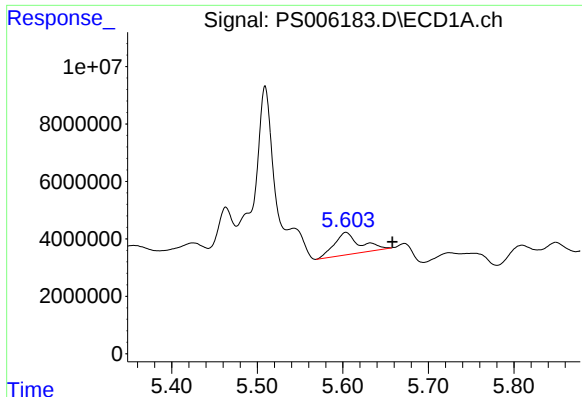

#5 DICAMBA


R.T.: 5.604 min
Delta R.T.: -0.054 min
Response: 16146087
Conc: 5.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

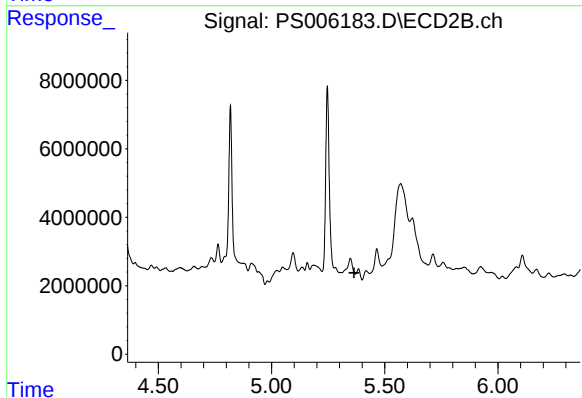


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.364 min
Response: 0
Conc: N.D.

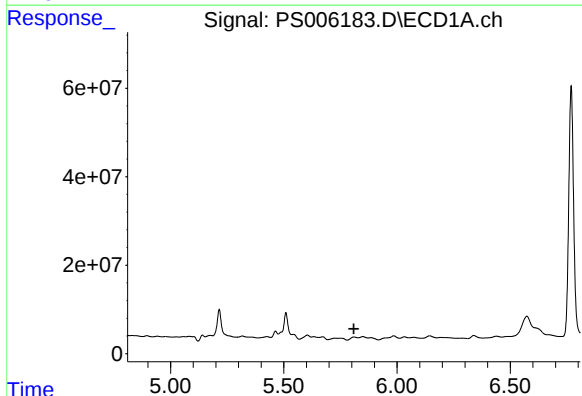


#6 MCP

R.T.: 0.000 min
Exp R.T. : 5.810 min
Response: 0
Conc: N.D.

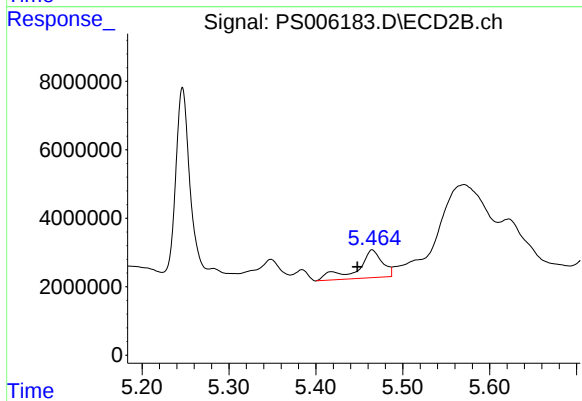

#6 MCP


R.T.: 5.465 min
Delta R.T.: 0.017 min
Response: 16254476
Conc: 13.14 ug/ml

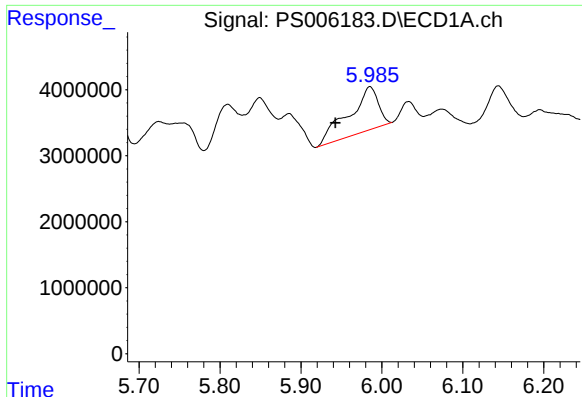

#7 MCPA


R.T.: 5.985 min
Delta R.T.: 0.043 min
Response: 16831065
Conc: 5.33 ug/ml

Instrument :
ECD_S
ClientSampleId :

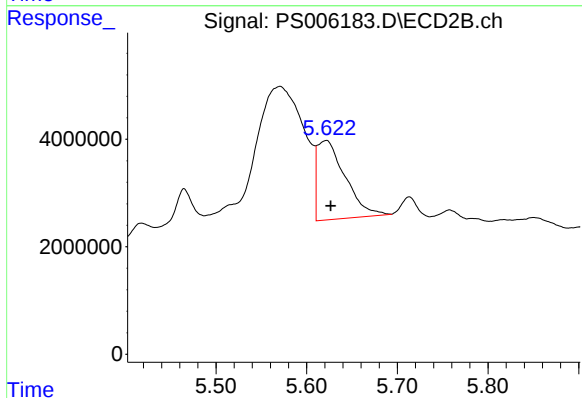


#7 MCPA

R.T.: 5.621 min
Delta R.T.: -0.005 min
Response: 31443205
Conc: 15.39 ug/ml

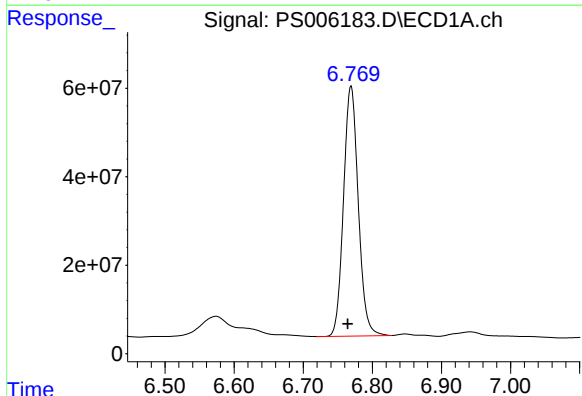


#10 Pentachlorophenol

R.T.: 6.769 min
Delta R.T.: 0.005 min
Response: 837818139
Conc: 70.88 ng/ml

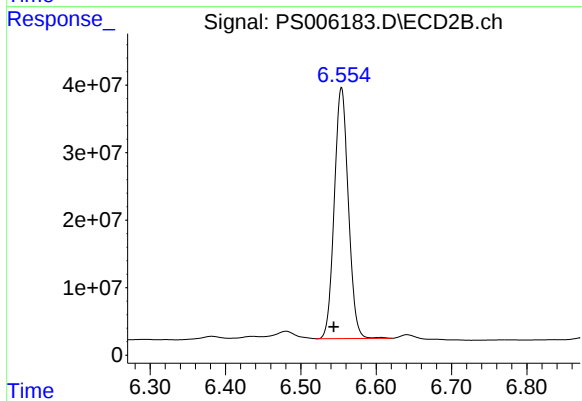

#10 Pentachlorophenol


R.T.: 6.554 min
Delta R.T.: 0.010 min
Response: 482151542
Conc: 71.32 ng/ml

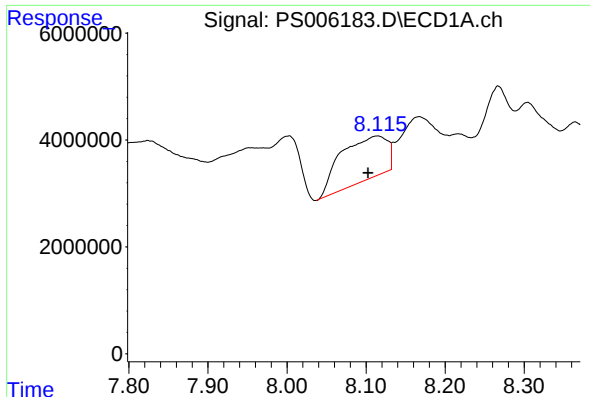

#13 2,4-DB


R.T.: 8.114 min
Delta R.T.: 0.012 min
Response: 33244174
Conc: 53.38 ng/ml

Instrument :
ECD_S
ClientSampleId :

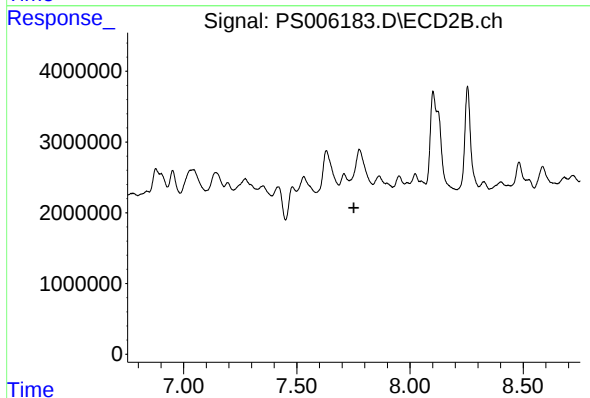


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 7.752 min
Response: 0
Conc: N.D.

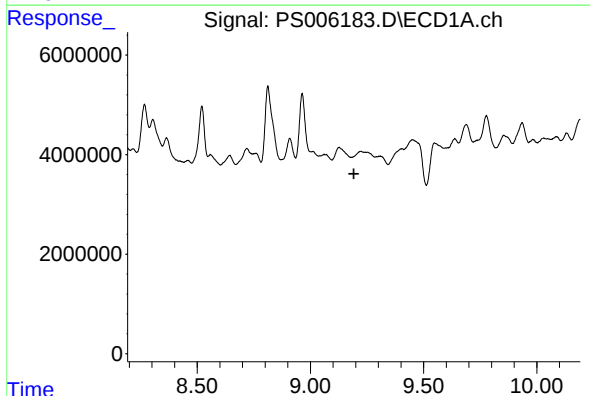


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 9.192 min
Response: 0
Conc: N.D.

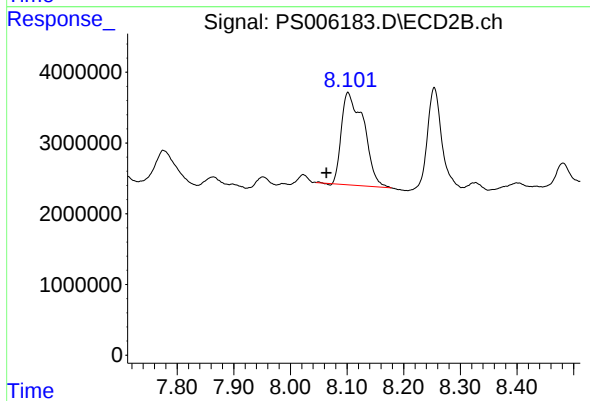

#14 DINOSEB


R.T.: 8.102 min
Delta R.T.: 0.038 min
Response: 35812323
Conc: 18.64 ng/ml

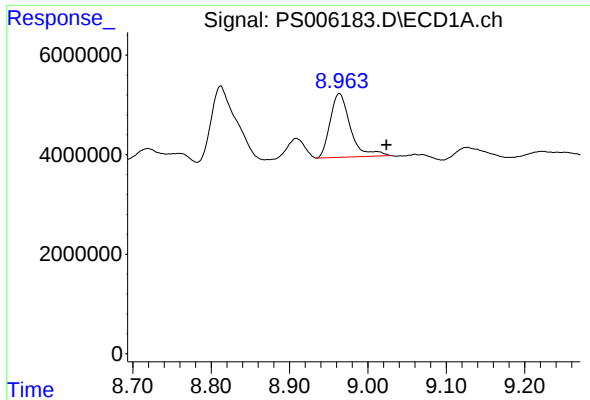

#15 Picloram

R.T.: 8.964 min
Delta R.T.: -0.060 min
Response: 22988618
Conc: 3.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

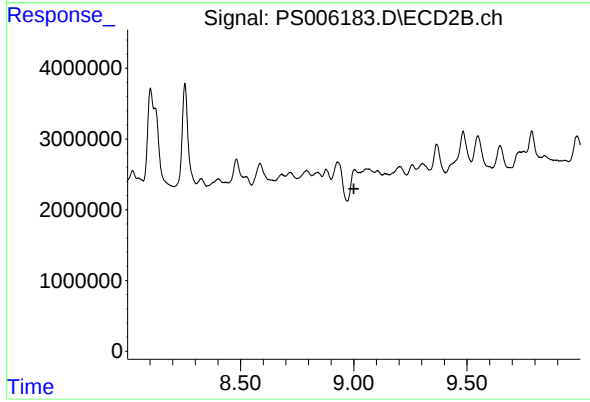

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.000 min
Response: 0
Conc: N.D.