

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081621\
 Data File : PS016390.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Aug 2021 08:45
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 17 06:20:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
 Quant Title : 8080.M
 QLast Update : Mon Aug 02 14:10:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
2) T	3,5-DICHL...	0.000	5.888f	0	68556	N.D. <MDL
5) T	DICAMBA	0.000	6.926	0	1828388	N.D. <MDL
10) T	Pentachlo...	8.606	8.262	6990743	3352326	<MDL <MDL #
11) T	2,4,5-TP ...	0.000	8.625	0	2572771	N.D. <MDL
12) T	2,4,5-T	9.444	9.003	8447604	3001128	1.108 1.036
14) T	DINOSEB	0.000	9.834	0	2291638	N.D. 1.125
15) T	Picloram	10.975	10.816	75475470	32882611	7.562 8.166
16) T	DCPA	11.416	10.764	9568286	4720291	<MDL 1.050 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS081621\
Data File : PS016390.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Aug 2021 08:45
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 17 06:20:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS080221.M
Quant Title : 8080.M
QLast Update : Mon Aug 02 14:10:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

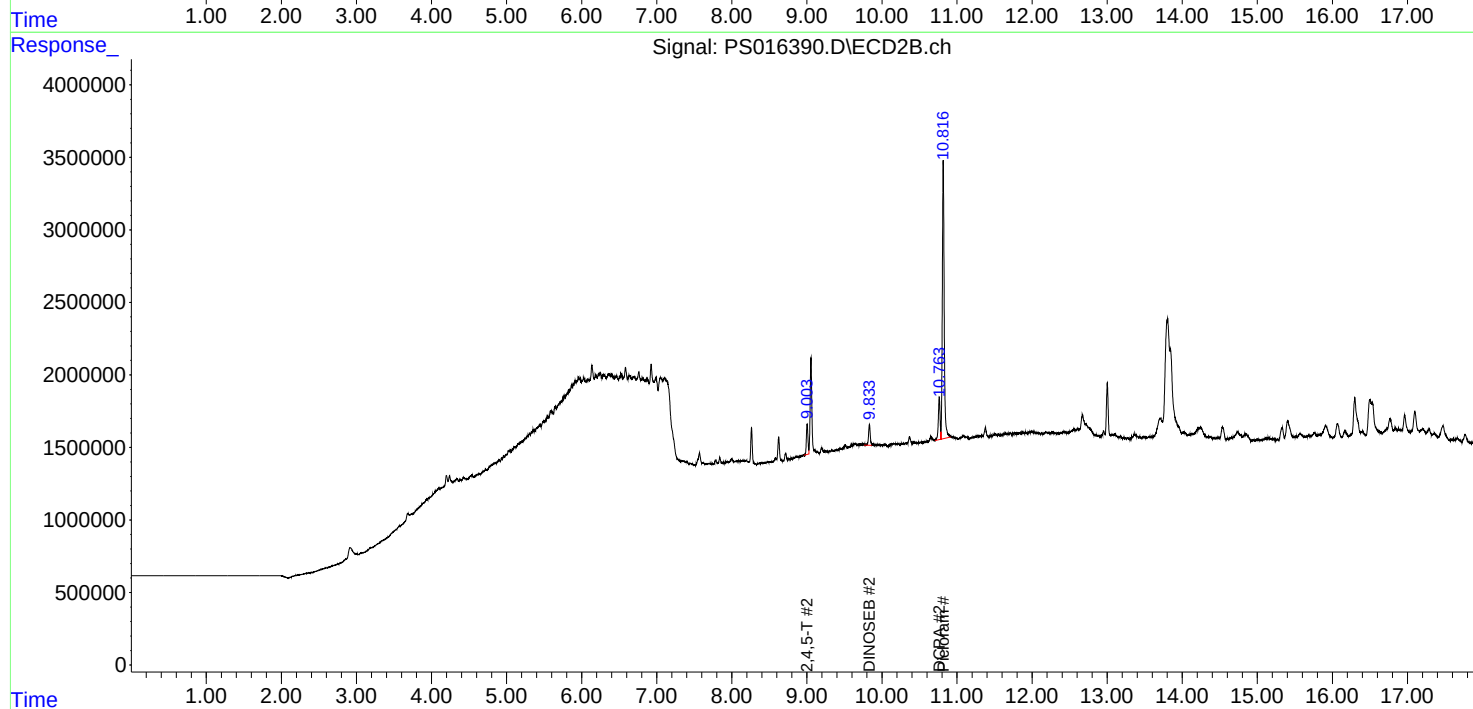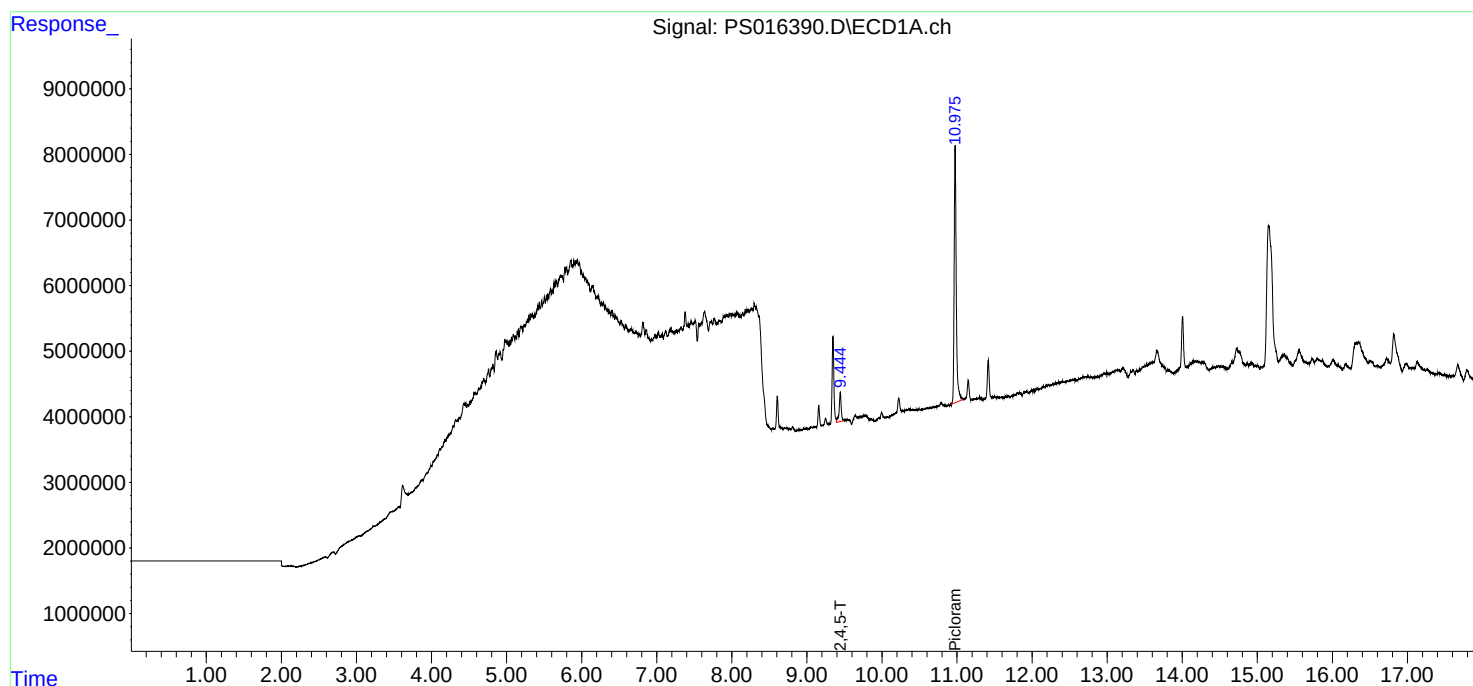


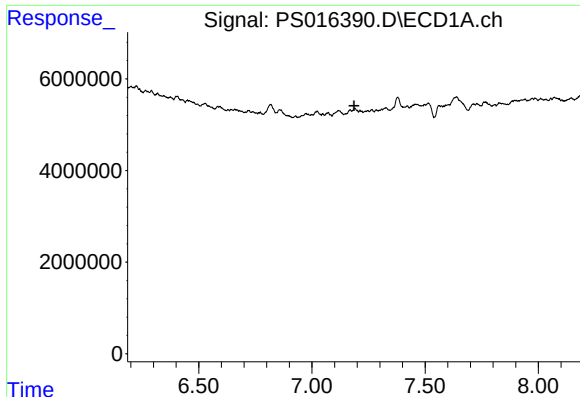

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.186 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

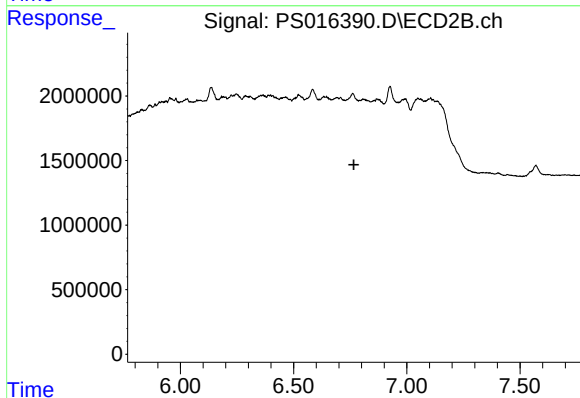


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 6.766 min
Response: 0
Conc: N.D.

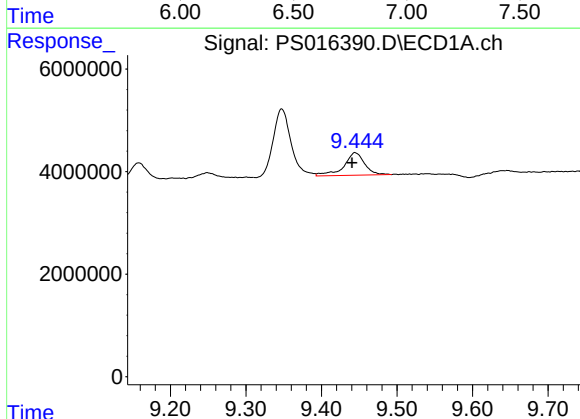


#12 2,4,5-T

R.T.: 9.444 min
Delta R.T.: 0.004 min
Response: 8447604
Conc: 1.11 ng/ml

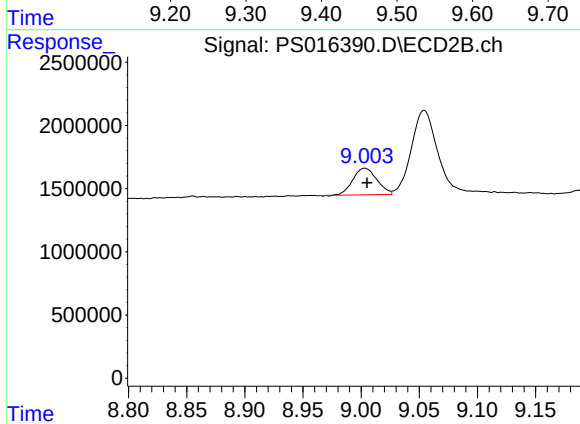

#12 2,4,5-T


R.T.: 9.003 min
Delta R.T.: -0.002 min
Response: 3001128
Conc: 1.04 ng/ml

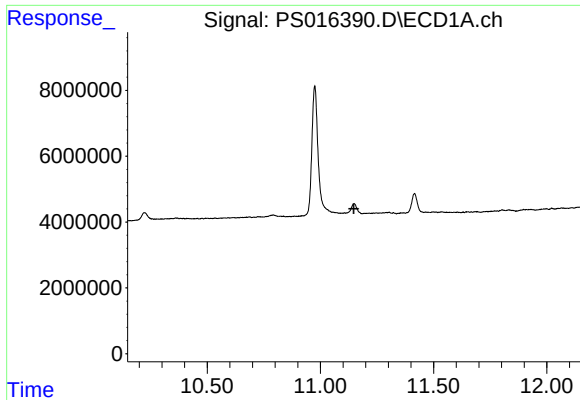

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.148 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

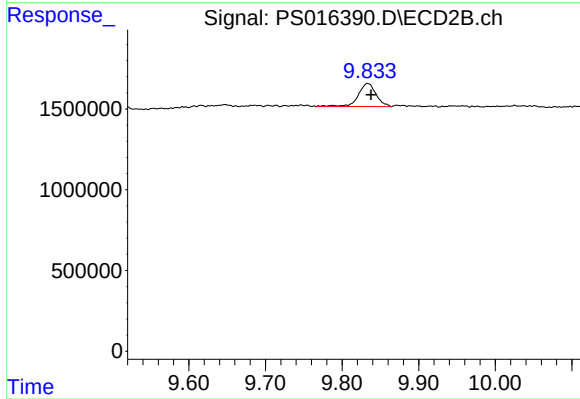


#14 DINOSEB

R.T.: 9.834 min
Delta R.T.: -0.004 min
Response: 2291638
Conc: 1.12 ng/ml

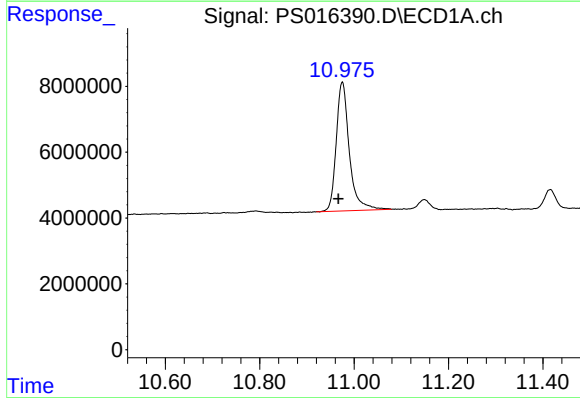


#15 Picloram

R.T.: 10.975 min
Delta R.T.: 0.008 min
Response: 75475470
Conc: 7.56 ng/ml

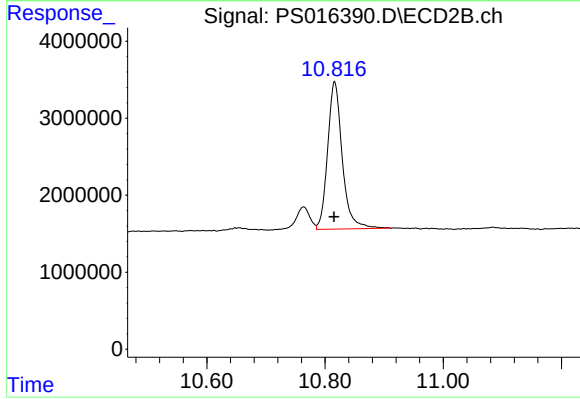

#15 Picloram


R.T.: 10.816 min
Delta R.T.: 0.000 min
Response: 32882611
Conc: 8.17 ng/ml

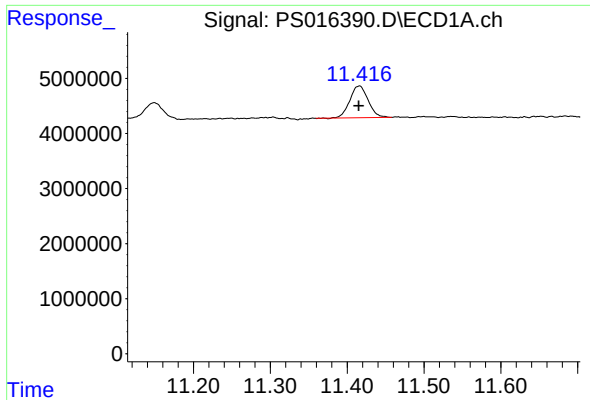

#16 DCPA

R.T.: 11.416 min
Delta R.T.: 0.000 min
Response: 9568286
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

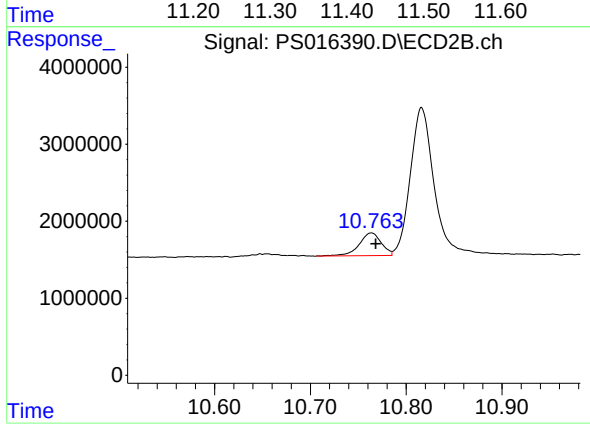

#16 DCPA

R.T.: 10.764 min
Delta R.T.: -0.005 min
Response: 4720291
Conc: 1.05 ng/ml